


Chloroethane


Response Ratio

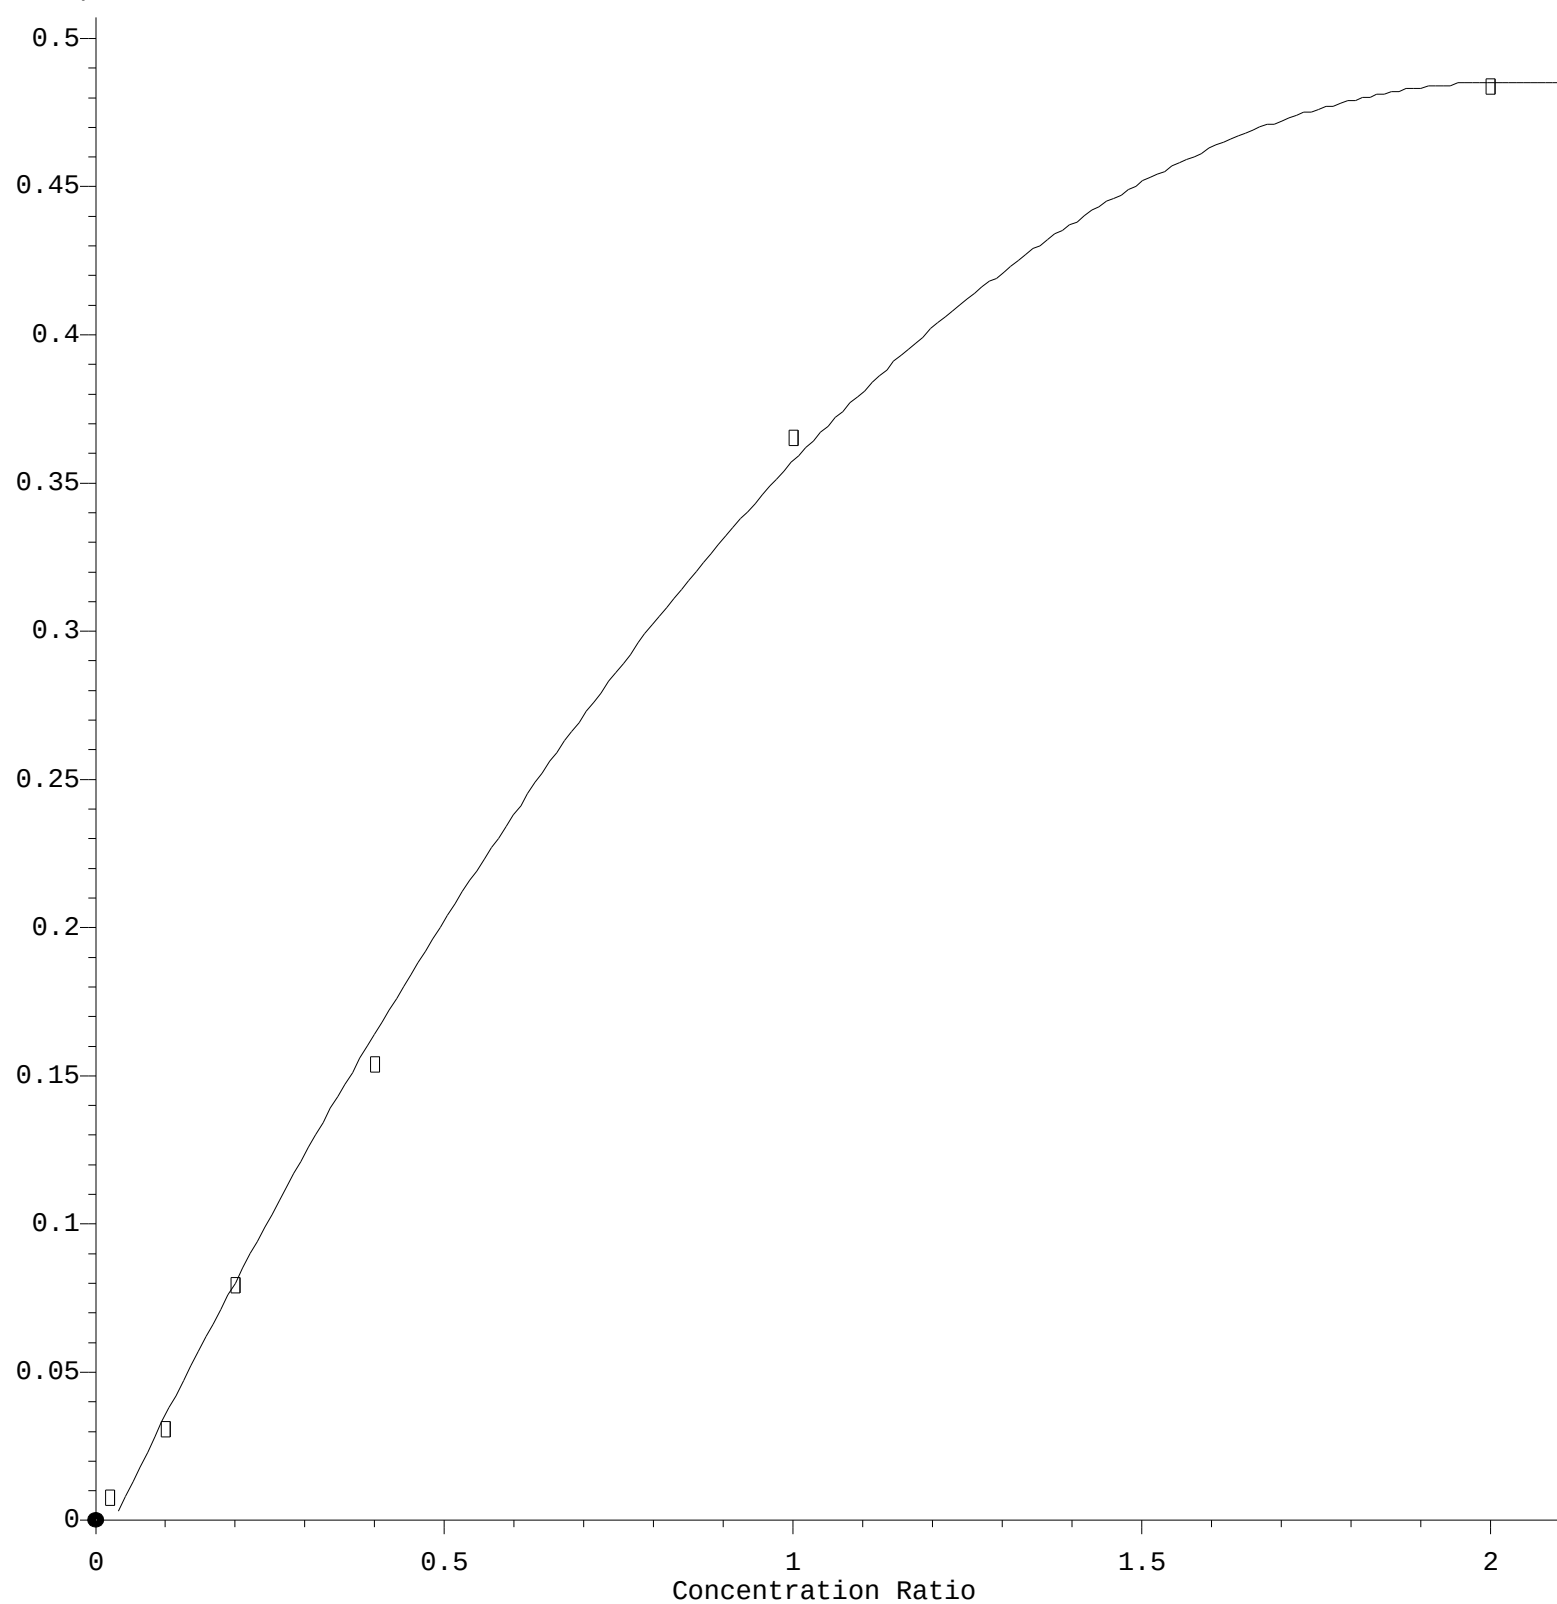

$R = -1.209e-001 A^2 + 4.908e-001 A - 1.261e-002$
 Coef of Det (r^2) = 0.998357 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Calibration Table Last Updated: Mon Jun 20 01:31:01 2022

Methyl Iodide

Response Ratio

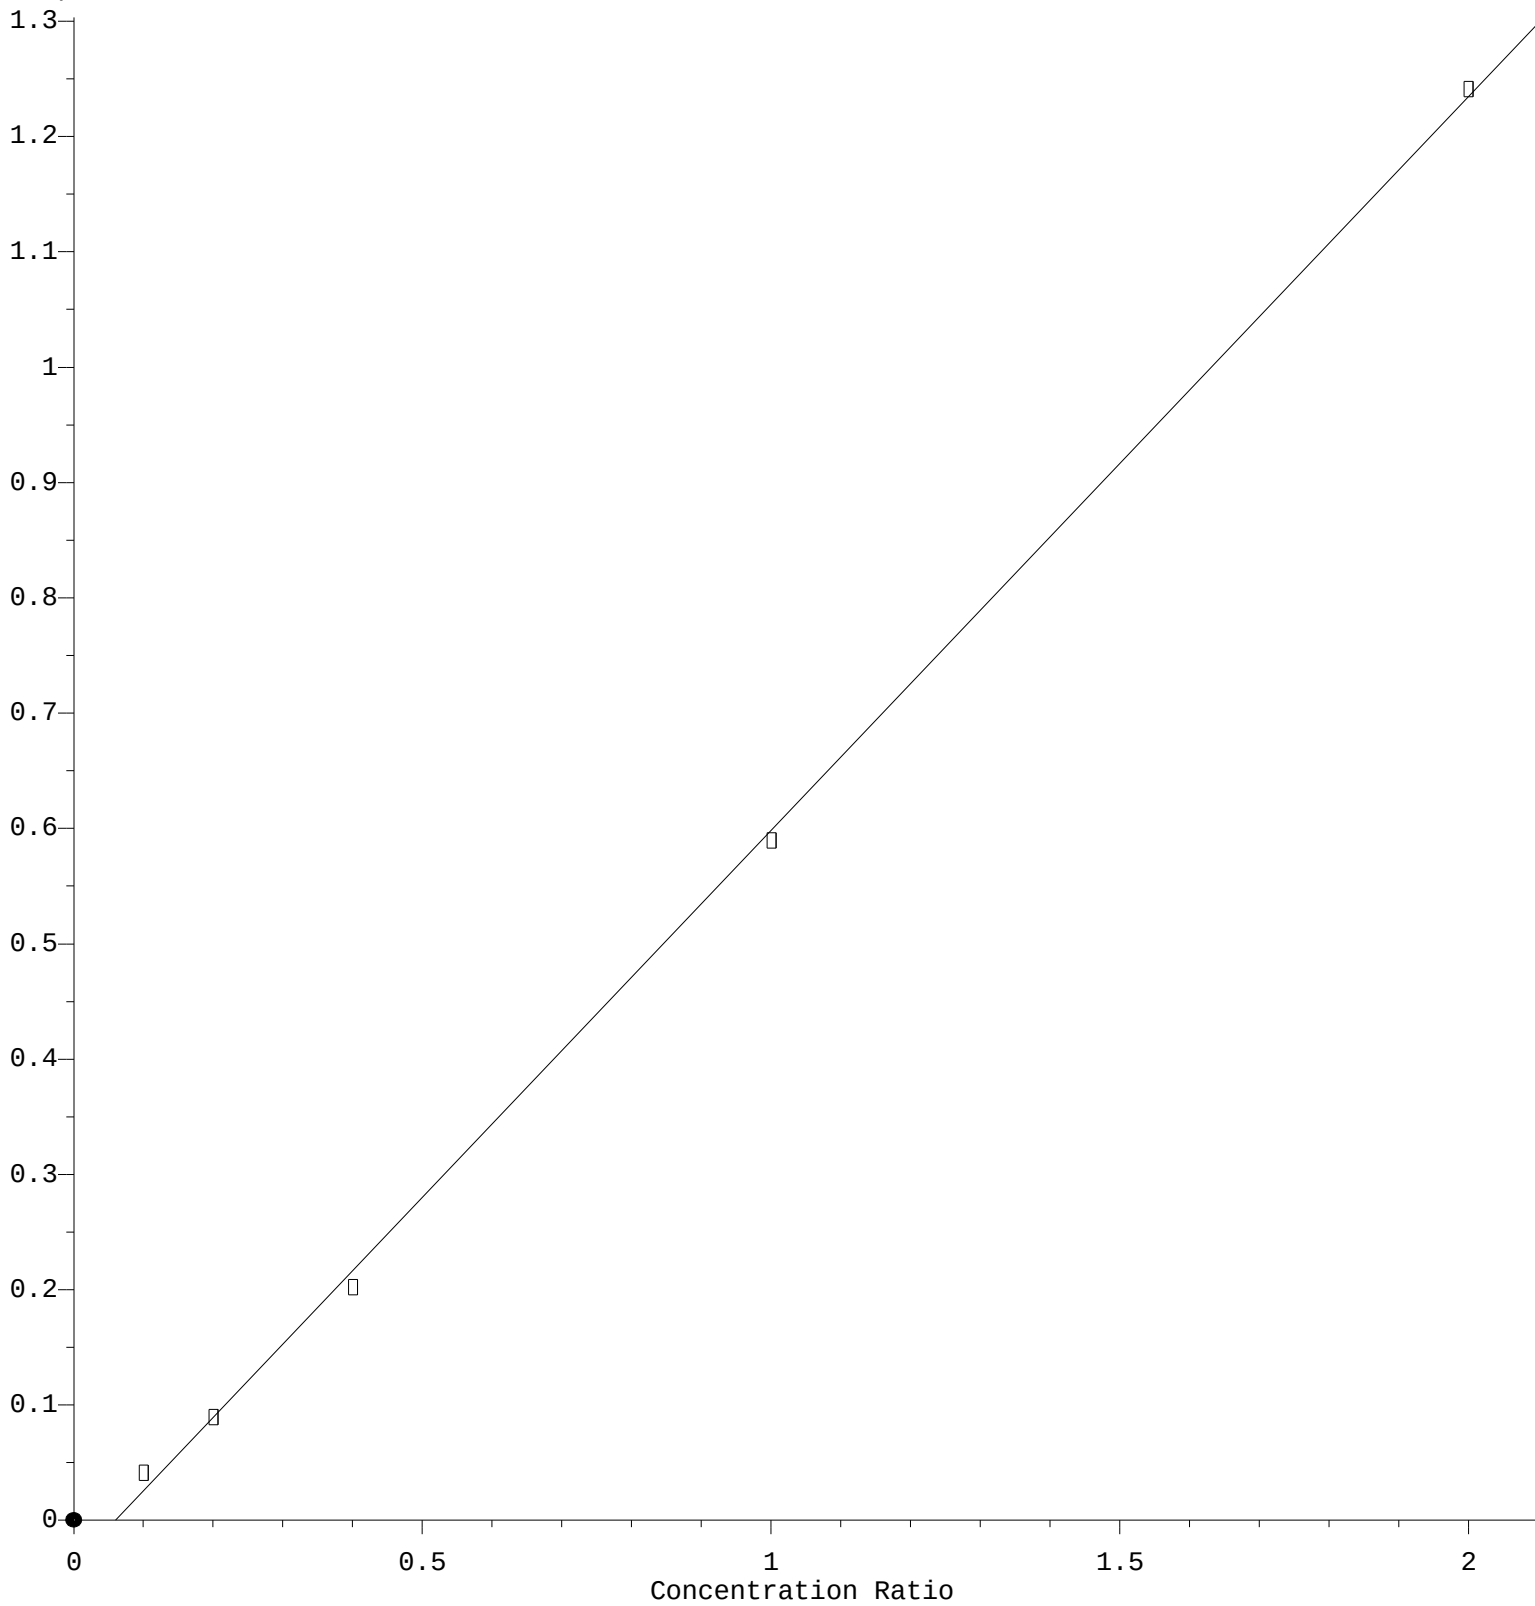

$$\text{Response} = 6.365\text{e-}001 * \text{Amt} - 3.841\text{e-}002$$


Coef of Det (r^2)= 0.999425 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Calibration Table Last Updated: Mon Jun 20 01:31:01 2022

Tert butylalcohol

Response Ratio

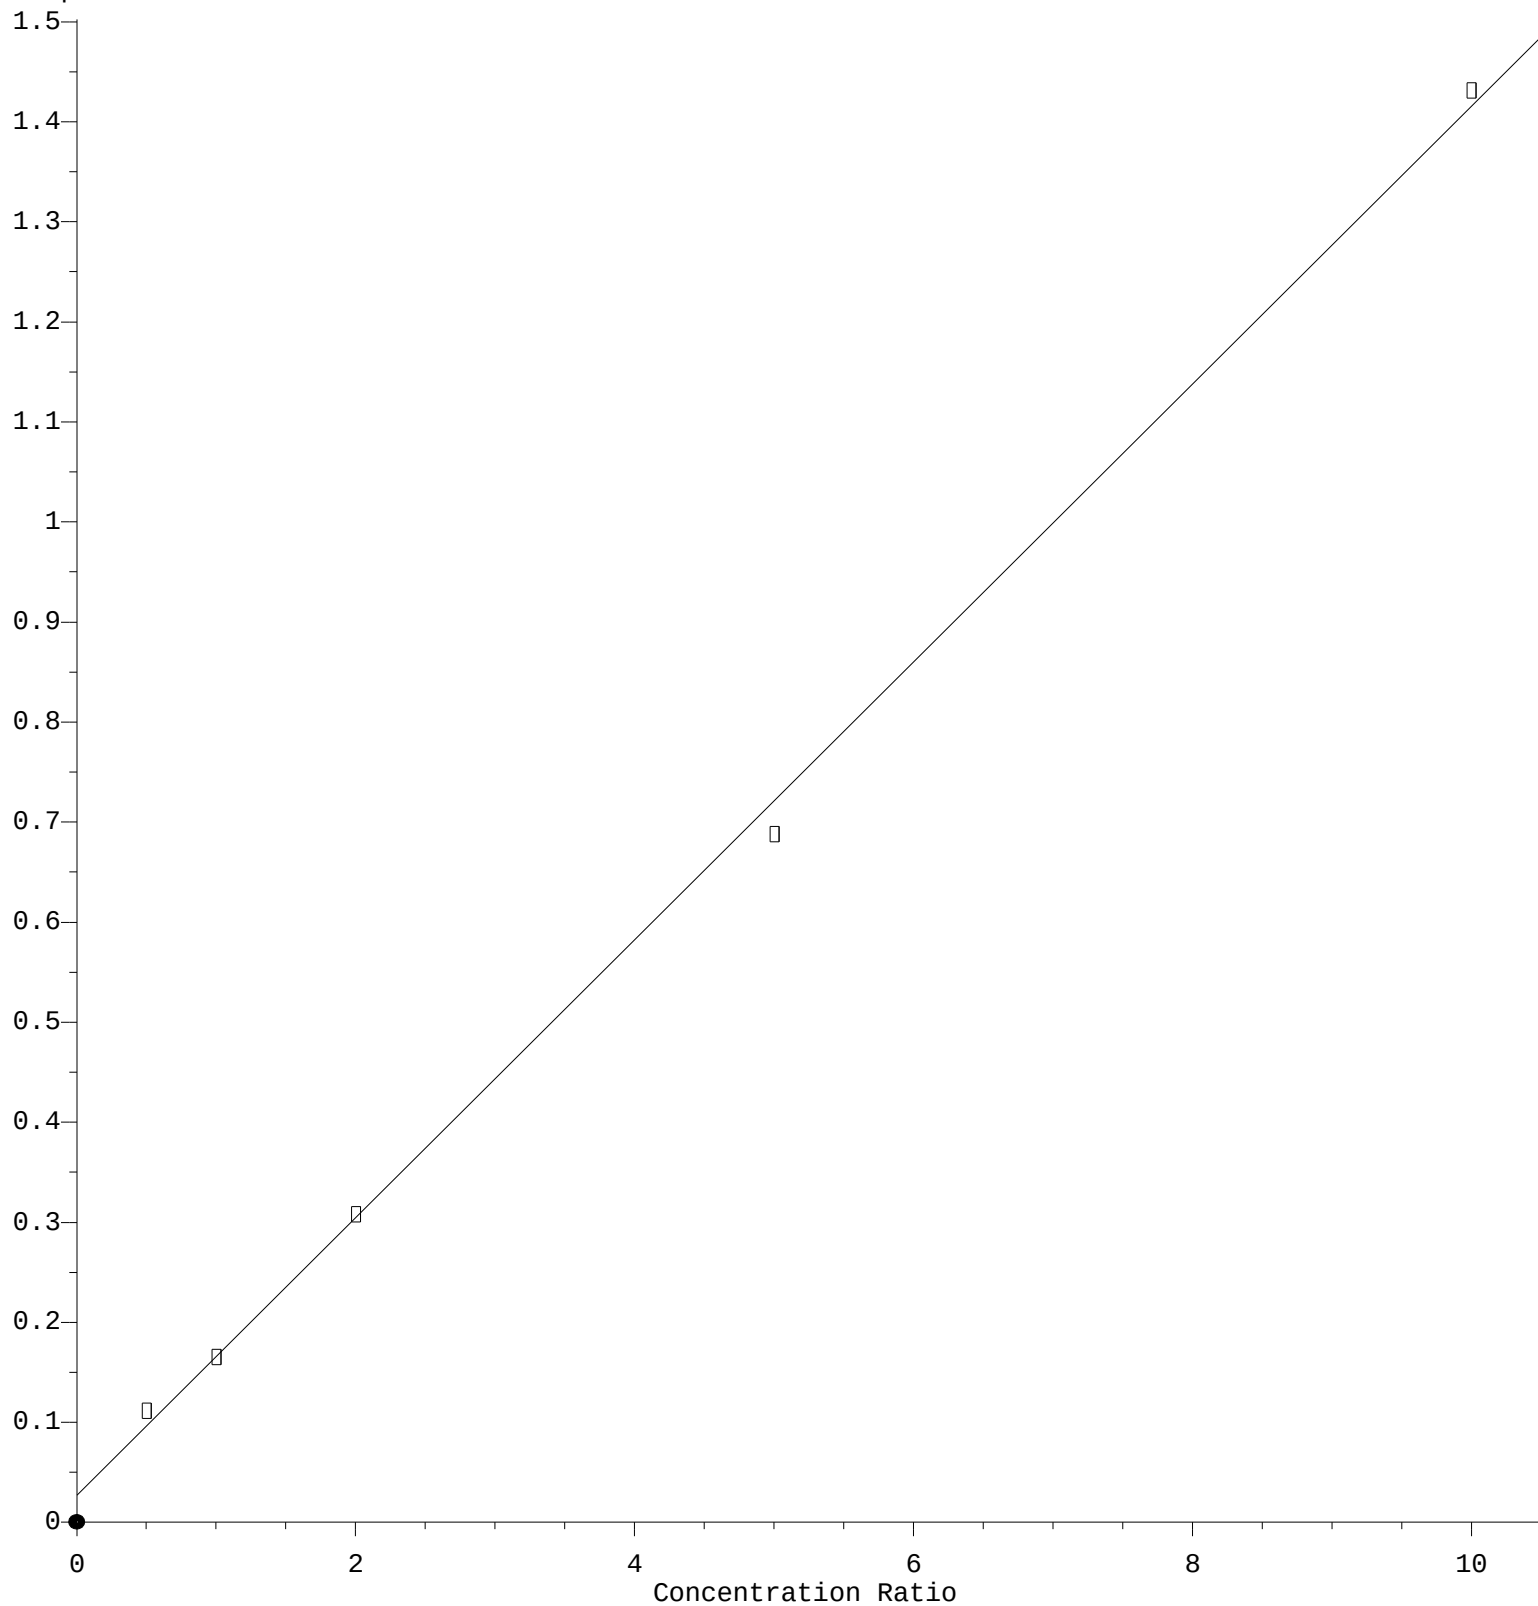


$$\text{Response} = 1.389\text{e-}001 * \text{Amt} + 2.669\text{e-}002$$

Coef of Det (r^2) = 0.998668 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Calibration Table Last Updated: Mon Jun 20 01:31:01 2022

Trichloroethene

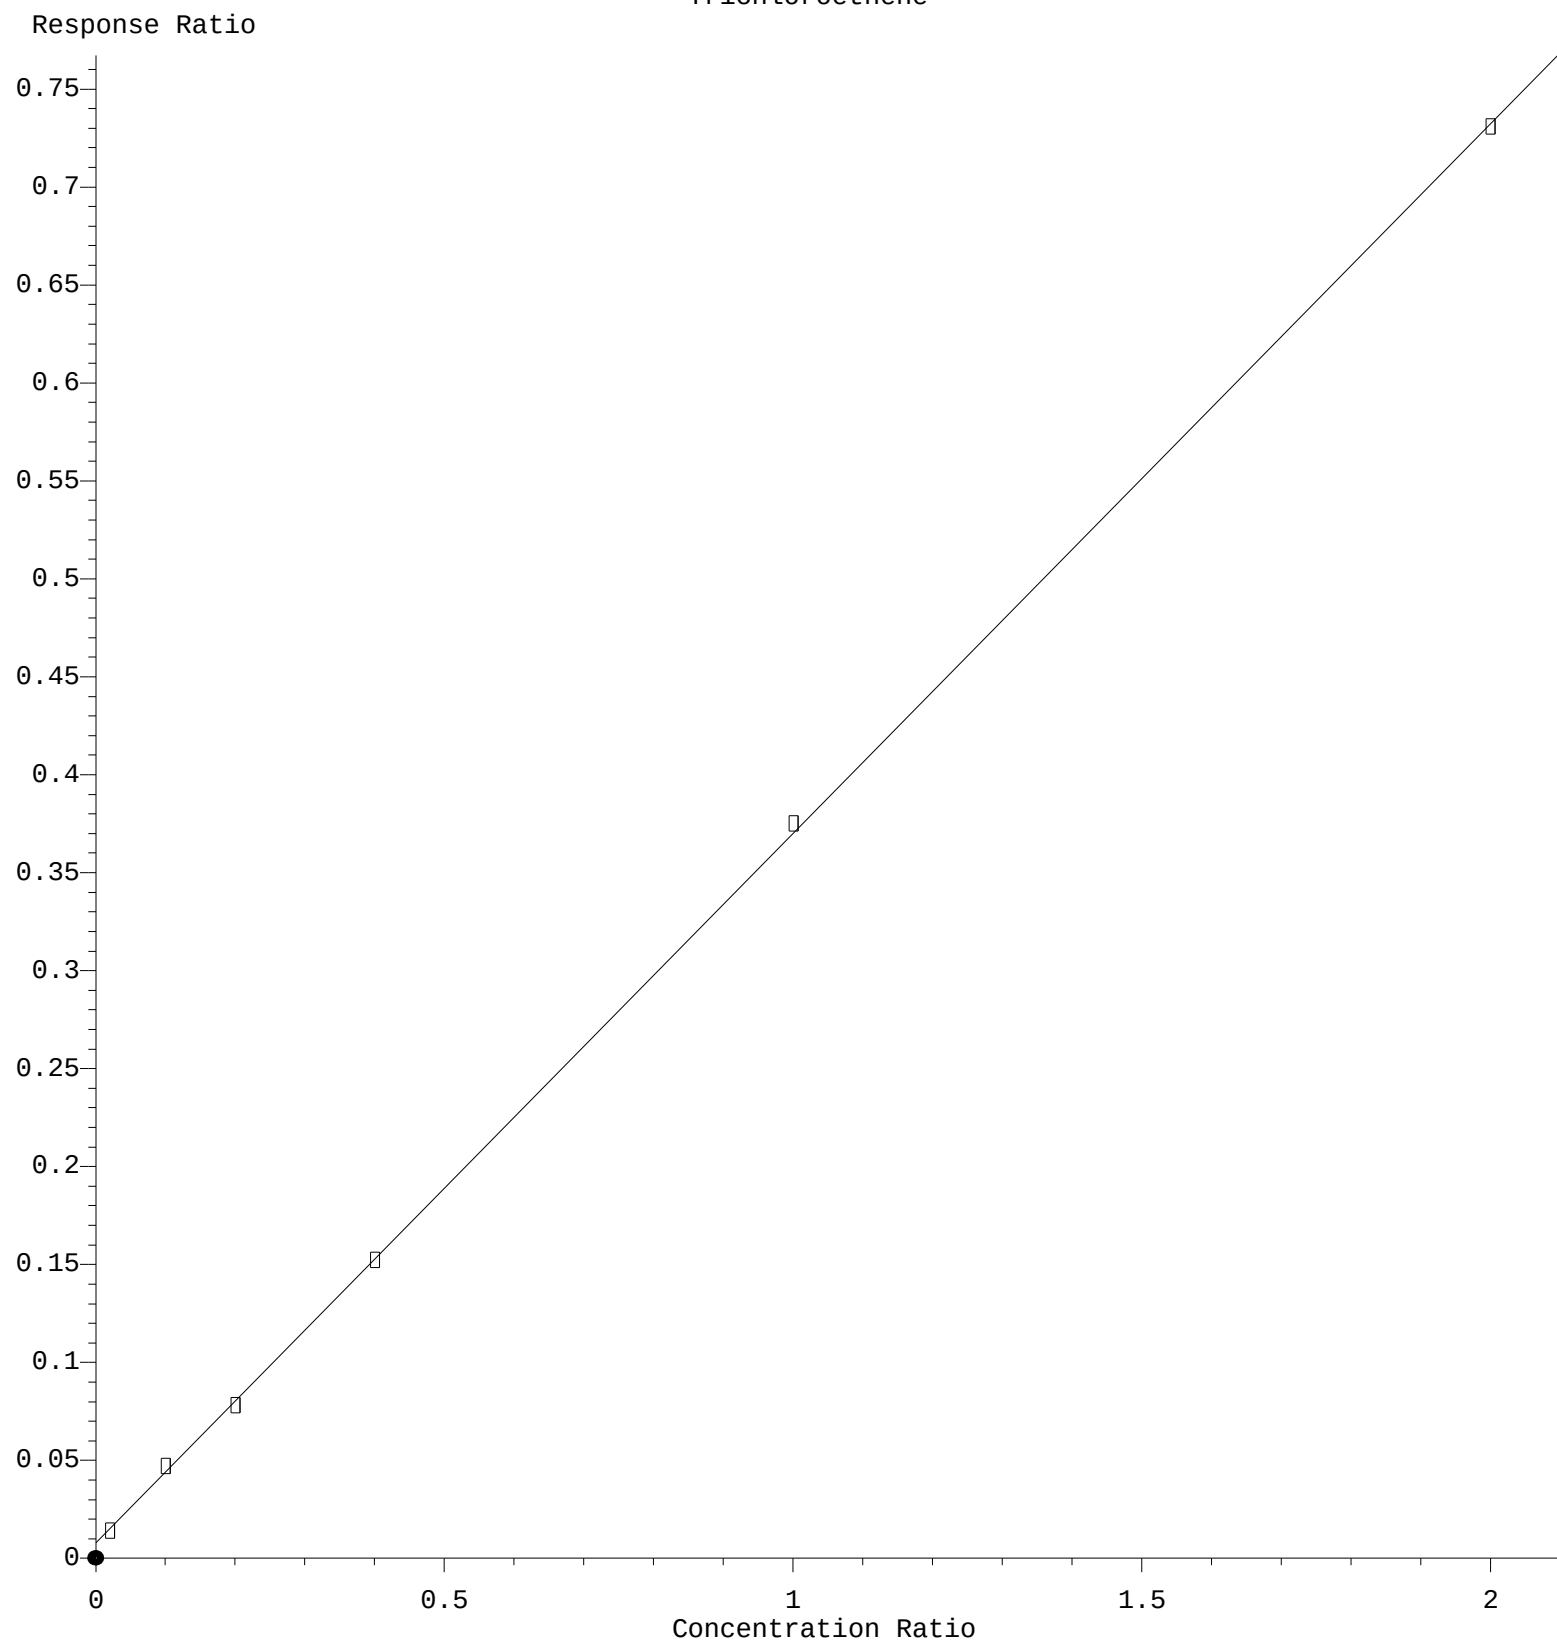

Response = $3.621 \times 10^{-1} \times \text{Amt} + 8.369 \times 10^{-3}$
Coef of Det (r^2) = 0.999894 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Calibration Table Last Updated: Mon Jun 20 01:31:01 2022