

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
Data File : VX029576.D
Acq On : 18 Jun 2022 17:46
Operator : JC/MD
Sample : N3325-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-25

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M

Title : SW846 8260

Signal : TIC: VX029576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	43	rBV	88818	208465	15.62%	2.845%
2	2.385	205	213	223	rBV	29673	51785	3.88%	0.707%
3	5.391	694	706	722	rBV	150573	440446	33.00%	6.012%
4	5.555	722	733	748	rVB	287388	807434	60.49%	11.021%
5	5.958	789	799	815	rBV	162322	434602	32.56%	5.932%
6	6.763	921	931	951	rBV	428256	1019734	76.40%	13.918%
7	8.652	1234	1241	1250	rBV	861967	1334768	100.00%	18.218%
8	10.055	1465	1471	1487	rBV	871708	1145407	85.81%	15.634%
9	11.085	1634	1640	1654	rBV	646454	839795	62.92%	11.462%
10	12.024	1789	1794	1802	rBV	844098	1028713	77.07%	14.041%
11	12.243	1823	1830	1837	rVB3	10022	15352	1.15%	0.210%




Sum of corrected areas: 7326501

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
Data File : VX029576.D
Acq On : 18 Jun 2022 17:46
Operator : JC/MD
Sample : N3325-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

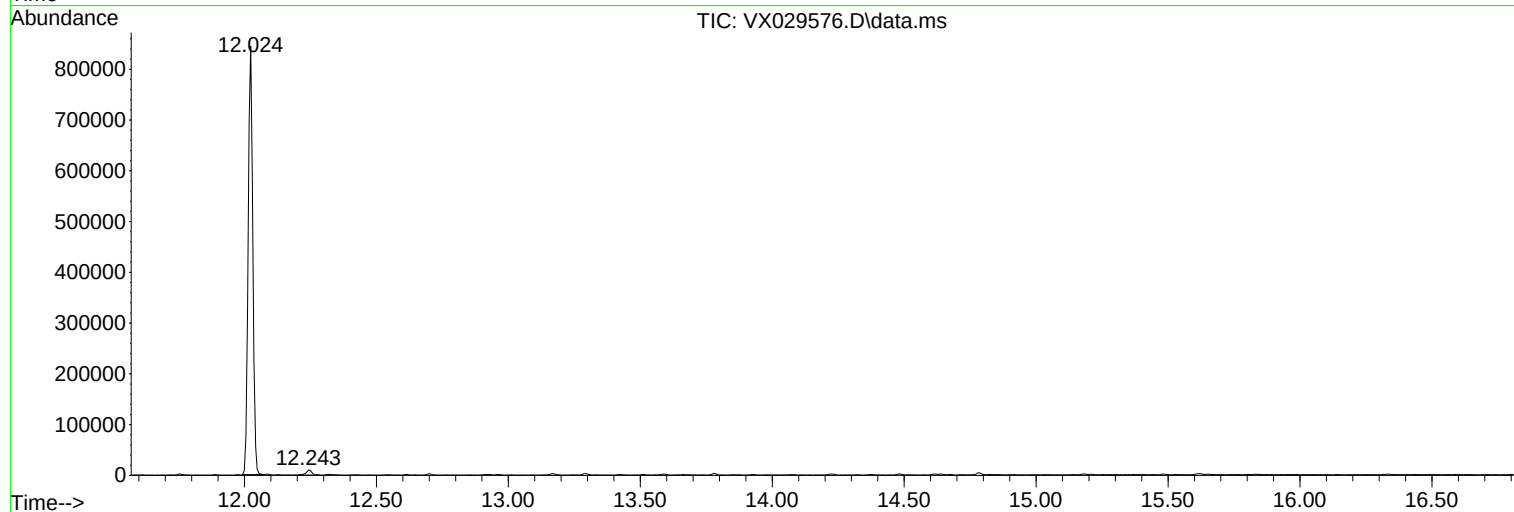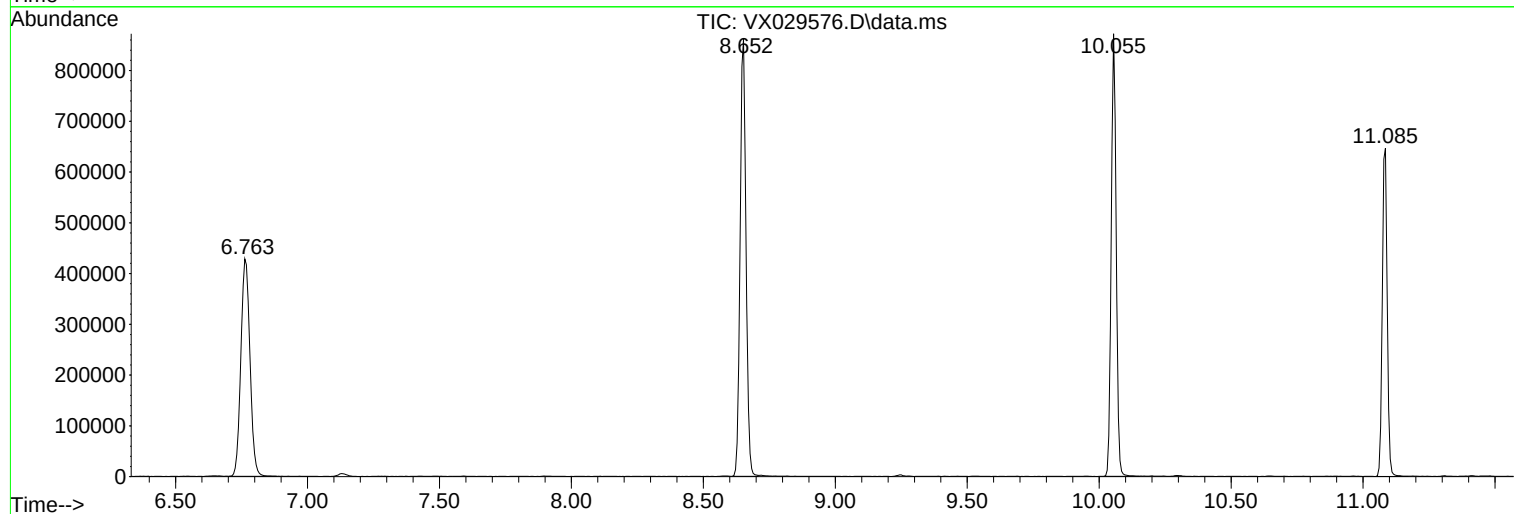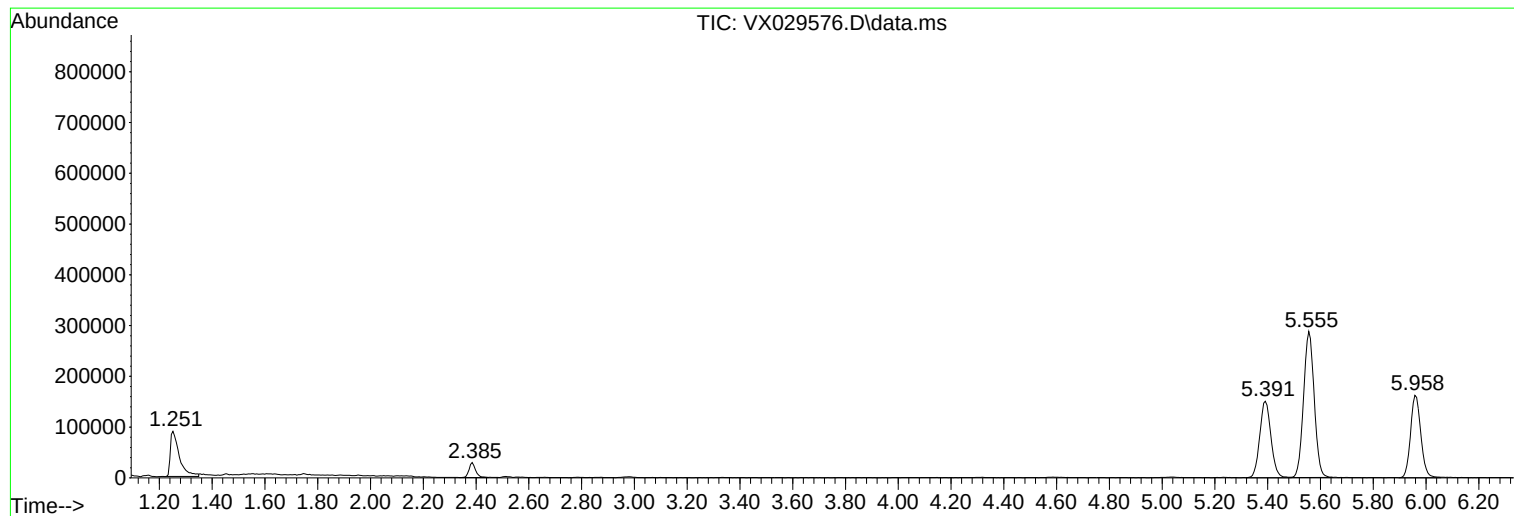

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
Data File : VX029576.D
Acq On : 18 Jun 2022 17:46
Operator : JC/MD
Sample : N3325-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
Data File : VX029576.D
Acq On : 18 Jun 2022 17:46
Operator : JC/MD
Sample : N3325-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
