

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
 Data File : VX029603.D
 Acq On : 19 Jun 2022 04:59
 Operator : JC/MD
 Sample : N3290-22 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-3

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260

Signal : TIC: VX029603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	23	34	39	rBV5	6143	16927	1.26%	0.235%
2	2.947	296	305	314	rBV	25276	58857	4.39%	0.819%
3	4.574	561	572	582	rBV2	7850	25025	1.86%	0.348%
4	5.391	695	706	721	rBV2	150172	439491	32.75%	6.112%
5	5.556	721	733	748	rVB2	281425	804963	59.99%	11.195%
6	5.958	789	799	819	rBV	166174	439169	32.73%	6.108%
7	6.763	920	931	950	rBV	432423	1026193	76.47%	14.272%
8	8.653	1233	1241	1249	rBV	853414	1341886	100.00%	18.663%
9	10.055	1465	1471	1486	rBV	883829	1155762	86.13%	16.074%
10	11.085	1634	1640	1651	rBV	637867	843117	62.83%	11.726%
11	12.024	1789	1794	1804	rBV	859918	1038760	77.41%	14.447%




Sum of corrected areas: 7190150

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
Data File : VX029603.D
Acq On : 19 Jun 2022 04:59
Operator : JC/MD
Sample : N3290-22 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

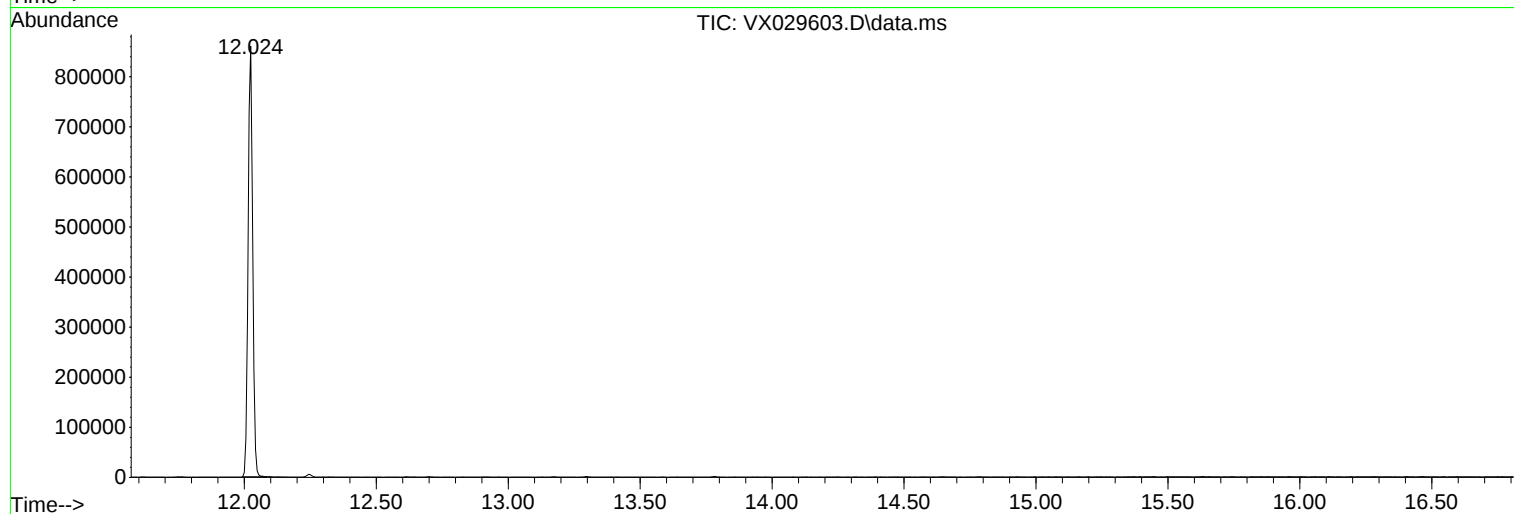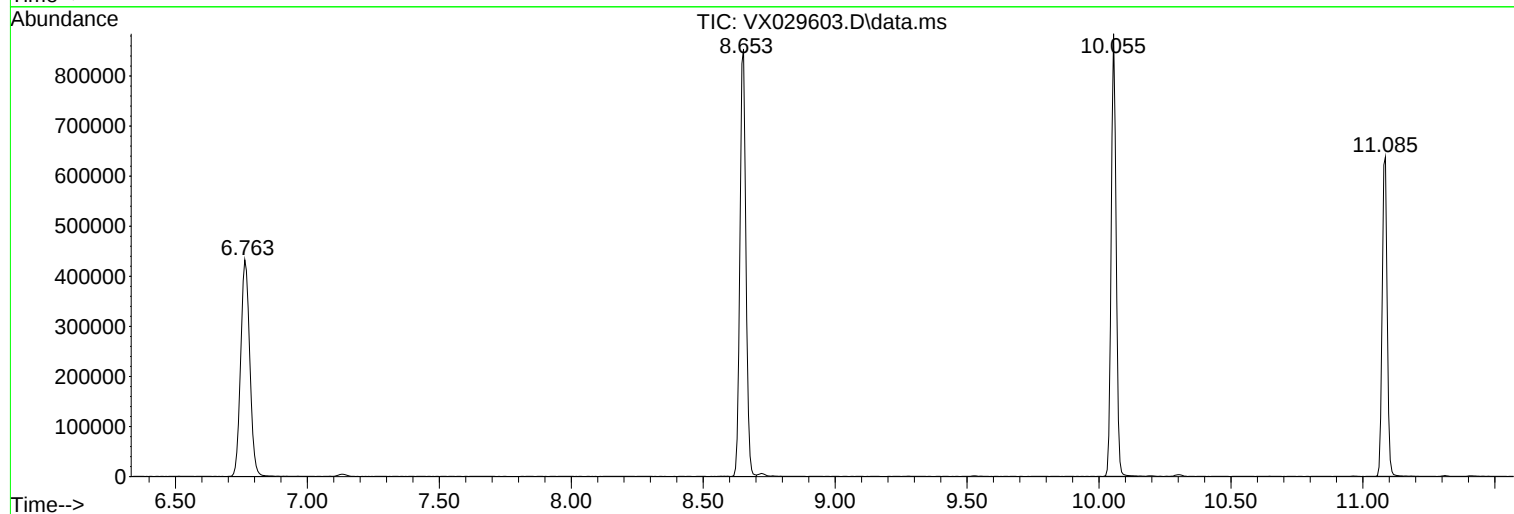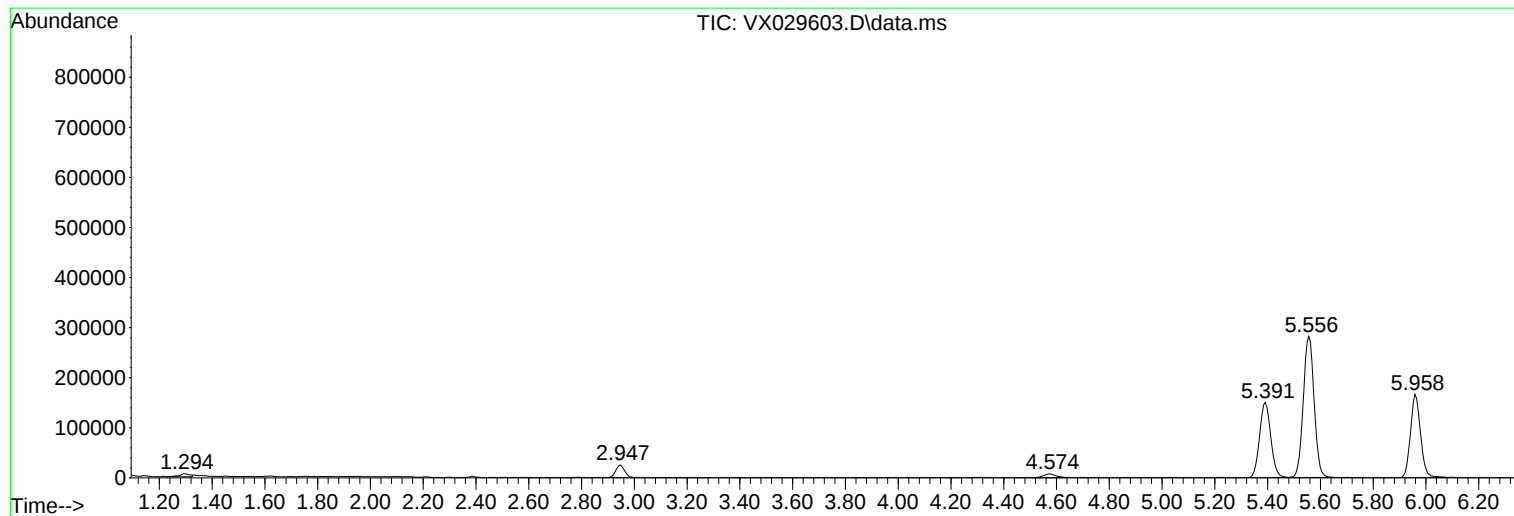

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
Data File : VX029603.D
Acq On : 19 Jun 2022 04:59
Operator : JC/MD
Sample : N3290-22 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
Data File : VX029603.D
Acq On : 19 Jun 2022 04:59
Operator : JC/MD
Sample : N3290-22 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------