


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
 Data File : VX029587.D
 Acq On : 18 Jun 2022 22:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Title : SW846 8260
 Last Update : Mon Jun 20 01:31:01 2022

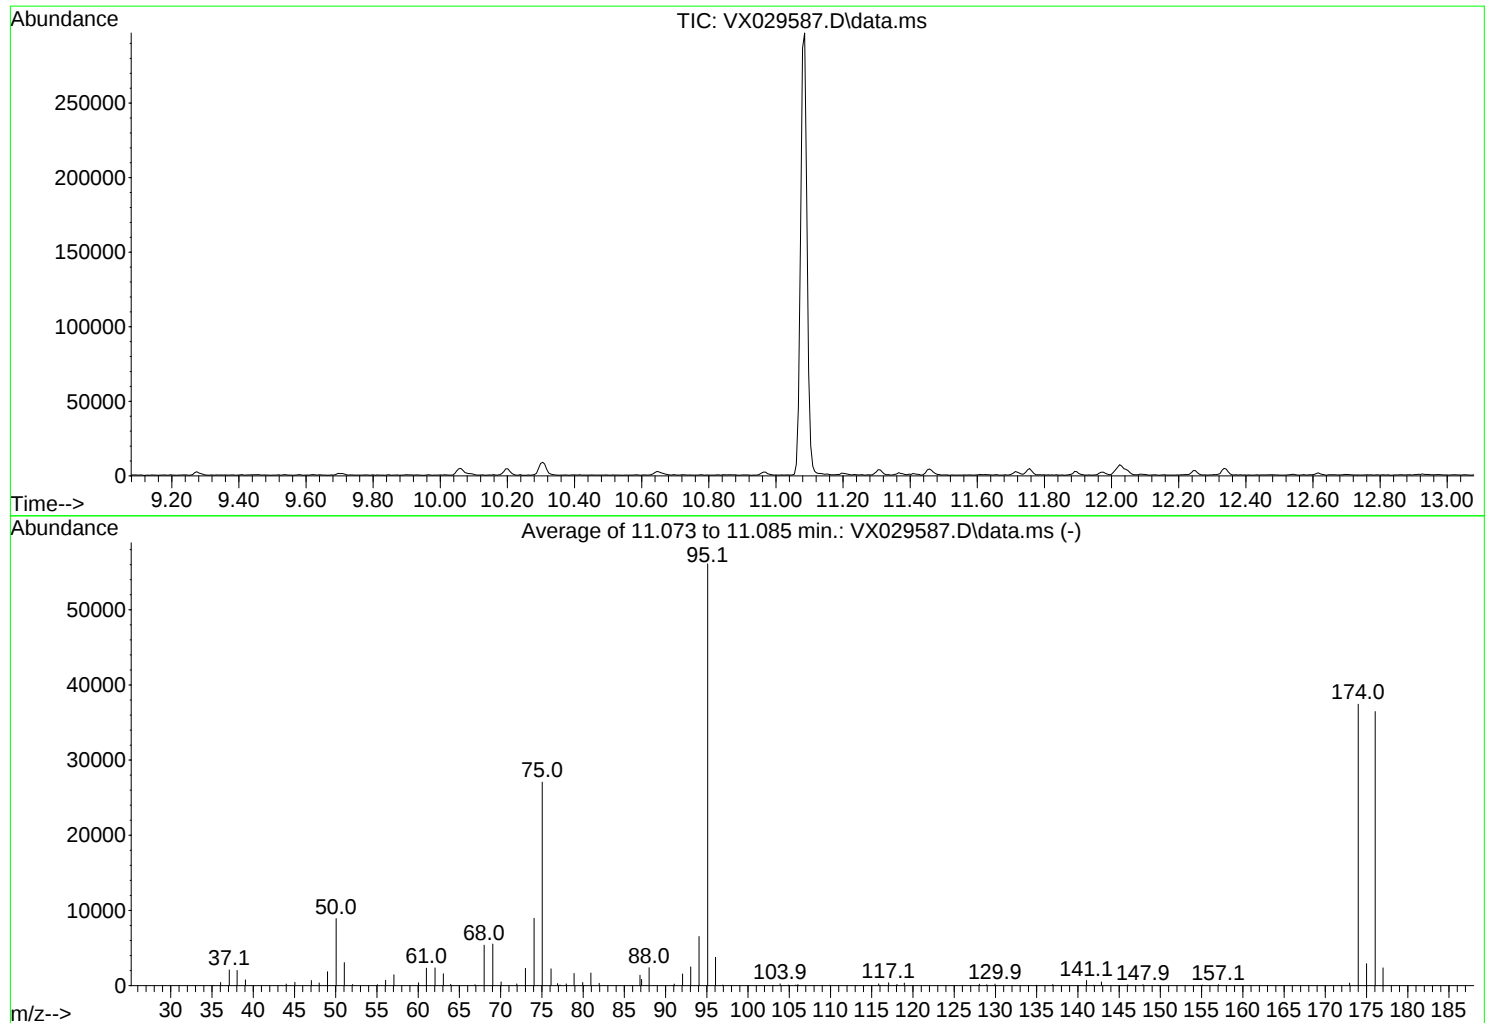

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	8926	PASS
75	95	30	60	48.2	27064	PASS
95	95	100	100	100.0	56107	PASS
96	95	5	9	6.7	3765	PASS
173	174	0.00	2	0.9	348	PASS
174	95	50	100	66.7	37437	PASS
175	174	5	9	7.8	2919	PASS
176	174	95	101	97.4	36459	PASS
177	176	5	9	6.5	2360	PASS