

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122623\
 Data File : VX039466.D
 Acq On : 26 Dec 2023 14:42
 Operator : JC/MD
 Sample : 06014-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 27 04:38:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	107539	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	223619	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	226554	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	102566	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	94819	48.131	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	96.260%		
35) Dibromofluoromethane	5.379	113	72934	47.211	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.420%		
50) Toluene-d8	8.647	98	286184	49.898	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	99.800%		
62) 4-Bromofluorobenzene	11.079	95	121165	51.202	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	102.400%		
Target Compounds					Qvalue	
3) Chloromethane	1.294	50	422	0.252	ug/l #	43
5) Bromomethane	1.611	94	321	0.358	ug/l #	3
6) Chloroethane	1.697	64	1224	1.304	ug/l #	53
8) Diethyl Ether	2.136	74	606	0.767	ug/l	95
11) Tert butyl alcohol	2.989	59	36685	74.155	ug/l #	92
14) Allyl chloride	2.654	41	1451	0.518	ug/l #	42
15) Acrylonitrile	2.977	53	249	0.251	ug/l #	33
16) Acetone	2.380	43	11219	Below Cal	#	89
17) Carbon Disulfide	2.508	76	2608	0.644	ug/l #	93
18) Methyl Acetate	2.709	43	1477	0.347	ug/l	96
19) Methyl tert-butyl Ether	3.117	73	2933	0.586	ug/l #	77
20) Methylene Chloride	2.794	84	1110	0.676	ug/l	92
25) 2-Butanone	4.586	43	1027	0.604	ug/l	92
36) 1,1-Dichloropropene	5.544	75	10361	4.250	ug/l #	50
38) Carbon Tetrachloride	5.544	117	12351	5.309	ug/l #	16
40) Benzene	6.037	78	185593	26.913	ug/l	99
49) 1,4-Dioxane	7.683	88	832	21.557	ug/l #	93
52) Toluene	8.720	92	5150	1.237	ug/l	96
67) Ethyl Benzene	10.195	91	3104	0.337	ug/l #	83
68) m/p-Xylenes	10.305	106	12511	3.791	ug/l	89
69) o-Xylene	10.640	106	2303	0.722	ug/l	95
73) Isopropylbenzene	10.963	105	3753	0.474	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.152	83	1212	0.412	ug/l #	34
76) 1,2,3-Trichloropropane	11.079	75	66620	25.106	ug/l #	39
78) n-propylbenzene	11.311	91	4813	0.494	ug/l	98
80) 1,3,5-Trimethylbenzene	11.451	105	7890	1.170	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.079	75	66620	70.824	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.756	105	17907	2.590	ug/l	99
85) sec-Butylbenzene	11.756	105	17907	2.193	ug/l #	57
90) Hexachloroethane	12.640	117	297	0.240	ug/l #	17
95) Naphthalene	13.774	128	27936	3.724	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122623\
Data File : VX039466.D
Acq On : 26 Dec 2023 14:42
Operator : JC/MD
Sample : 06014-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 27 04:38:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration

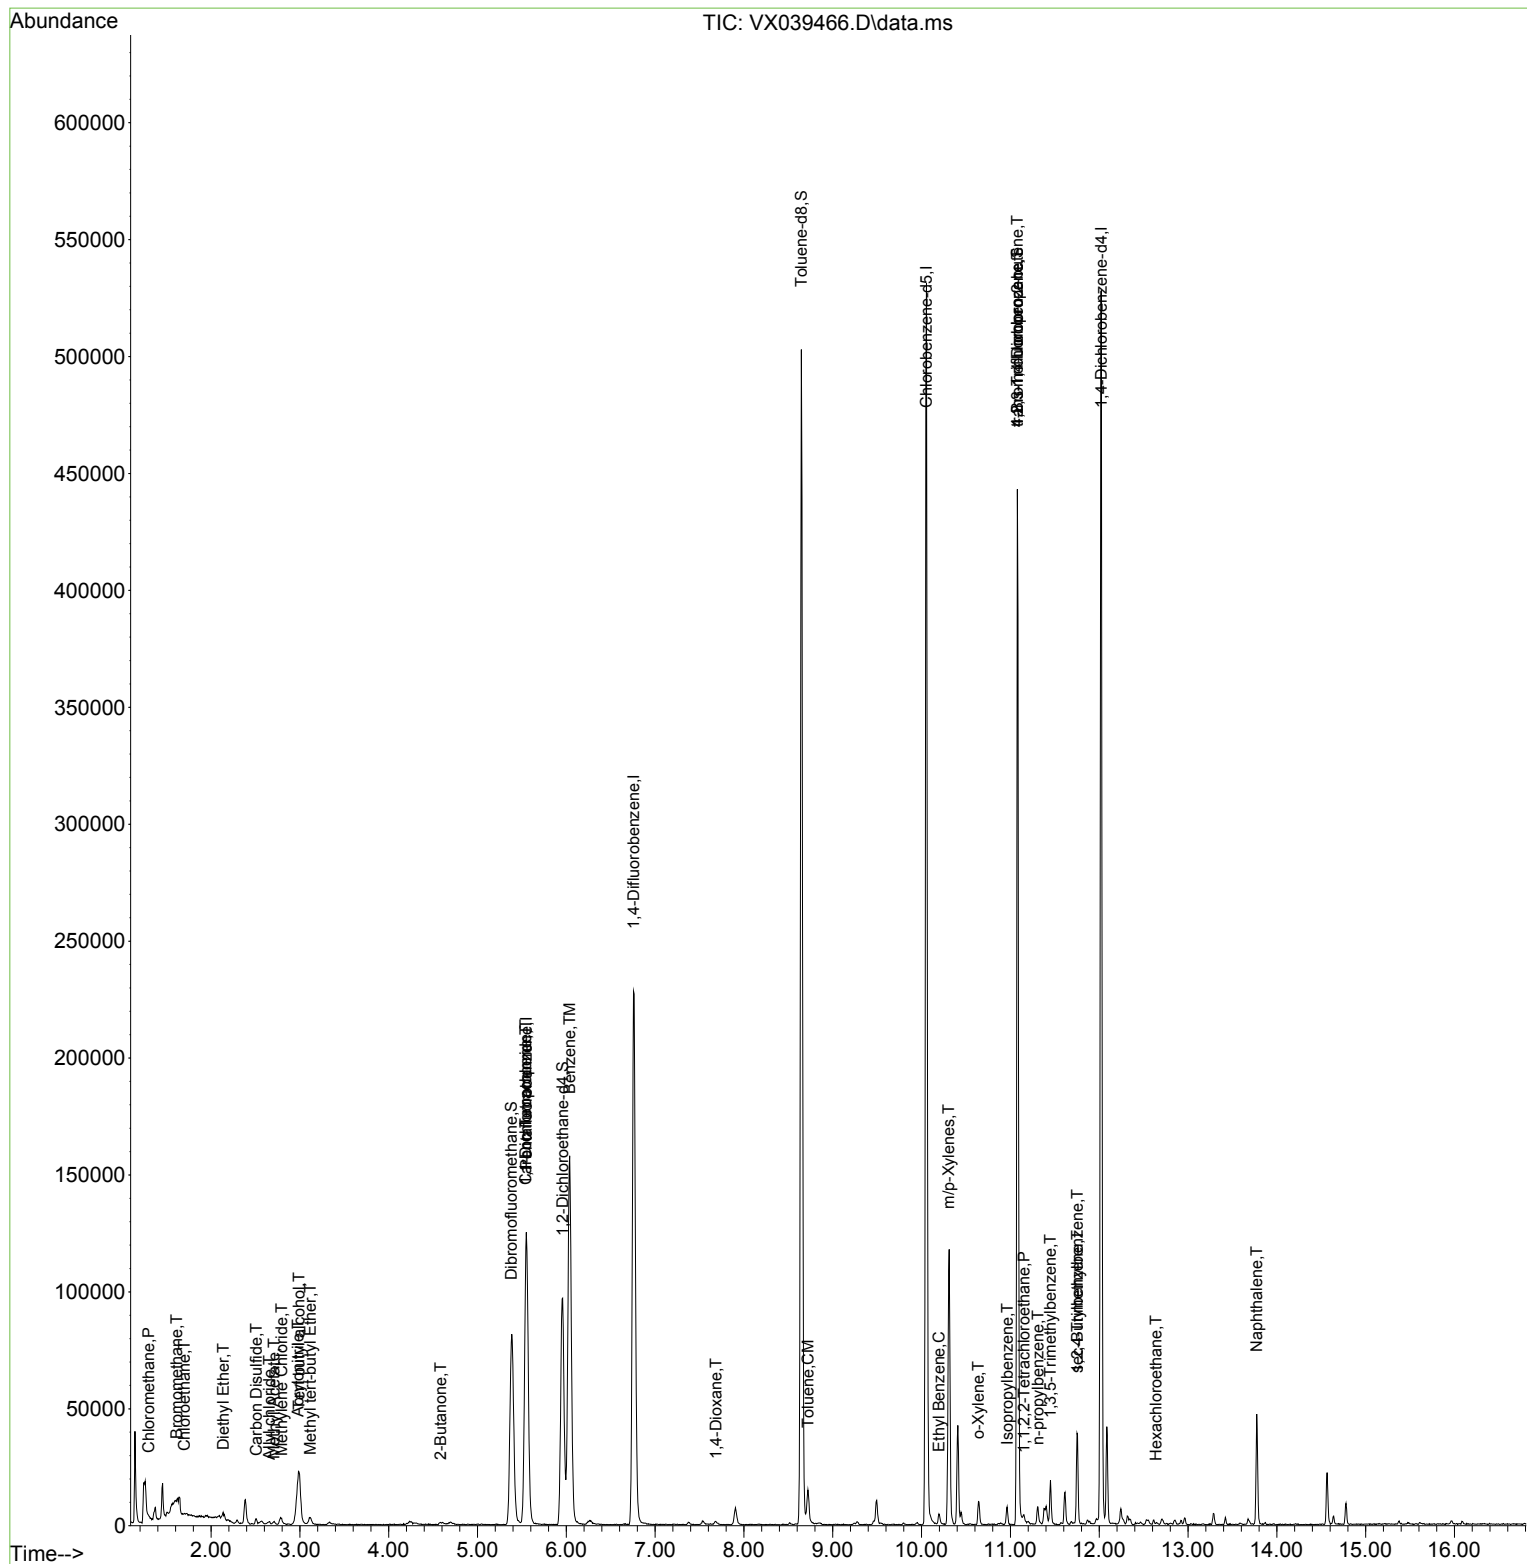






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 107539
Ion Ratio Lower Upper
168 100
99 66.7 56.6 85.0

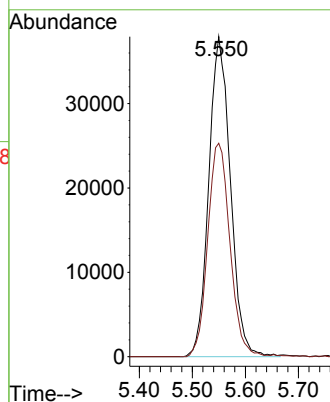

#3
Chloromethane
Concen: 0.252 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42


Tgt Ion: 50 Resp: 422
Ion Ratio Lower Upper
50 100
52 0.0 25.5 38.3#

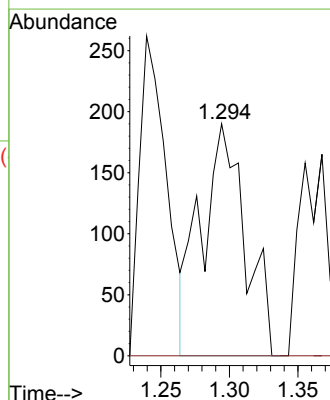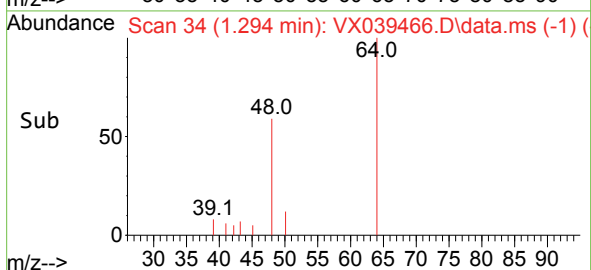



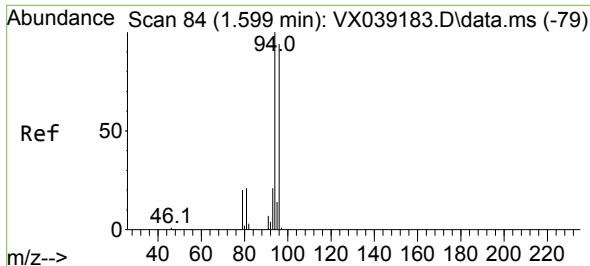


#5
Bromomethane
Concen: 0.358 ug/l
RT: 1.611 min Scan# 80
Delta R.T. 0.012 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Instrument :
MSVOA_X
ClientSampleId :


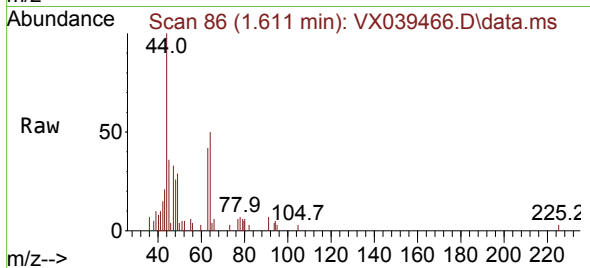



Tgt Ion: 94 Resp: 321
Ion Ratio Lower Upper
94 100
96 0.0 74.6 111.8#

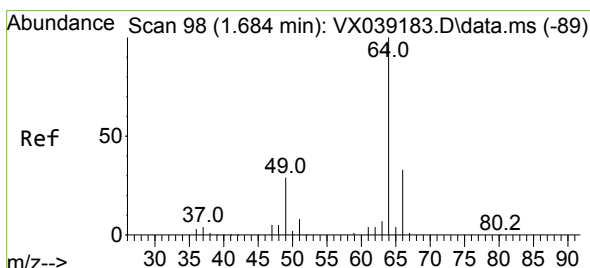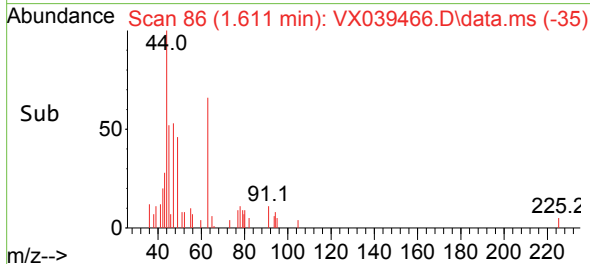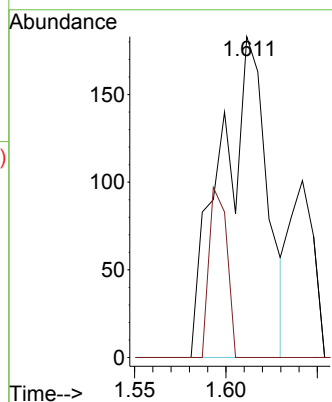

#6
Chloroethane
Concen: 1.304 ug/l
RT: 1.697 min Scan# 100
Delta R.T. 0.012 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42


Tgt Ion: 64 Resp: 1224
Ion Ratio Lower Upper
64 100
66 5.5 25.1 37.7#

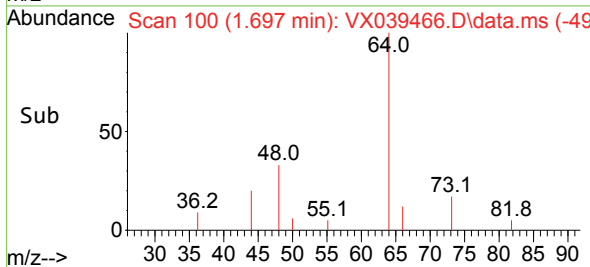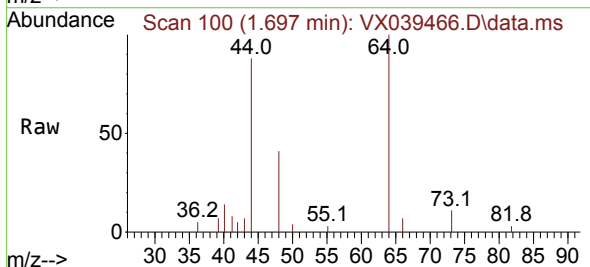



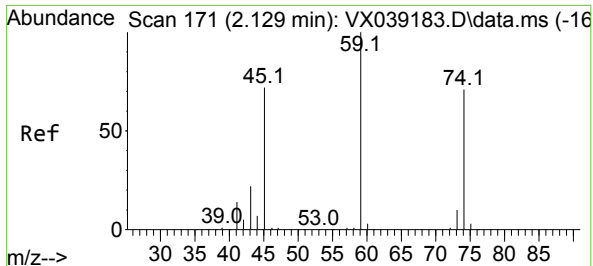


#8
Diethyl Ether
Concen: 0.767 ug/l
RT: 2.136 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Instrument :
MSVOA_X
ClientSampleId :



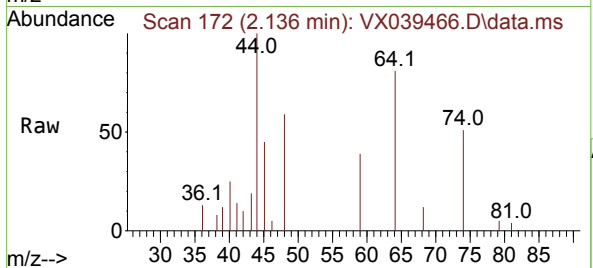



Tgt Ion: 74 Resp: 606
Ion Ratio Lower Upper
74 100
45 111.2 53.3 159.8

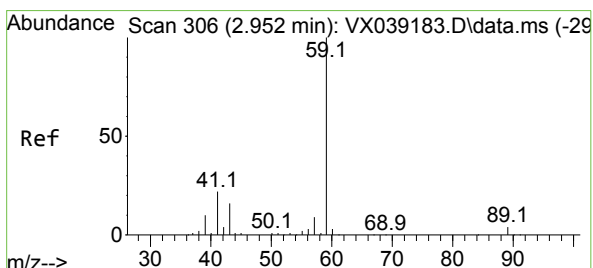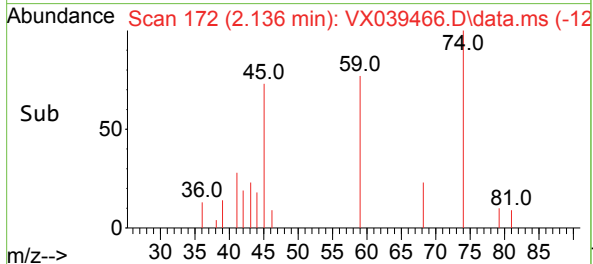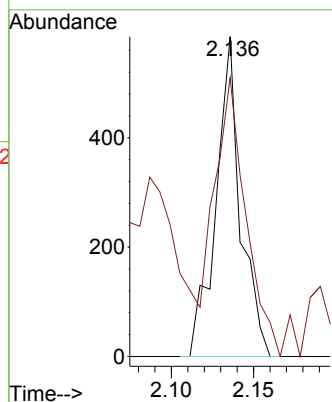

#11
Tert butyl alcohol
Concen: 74.155 ug/l
RT: 2.989 min Scan# 312
Delta R.T. 0.037 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42


Tgt Ion: 59 Resp: 36685
Ion Ratio Lower Upper
59 100
57 10.3 6.0 9.0#

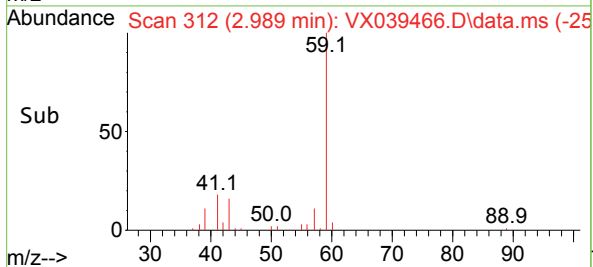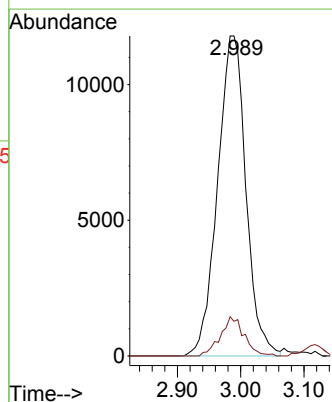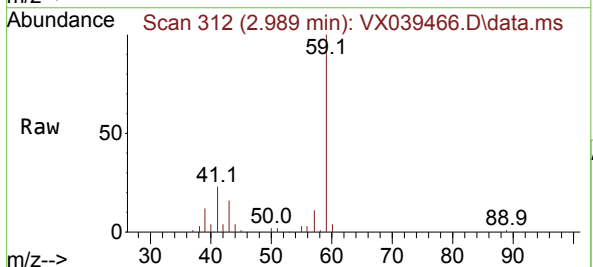






#14
 Allyl chloride
 Concen: 0.518 ug/l
 RT: 2.654 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: VX039466.D
 Acq: 26 Dec 2023 14:42

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion: 41 Resp: 1451
 Ion Ratio Lower Upper
 41 100
 39 21.0 55.8 83.6#
 76 0.0 24.3 36.5#

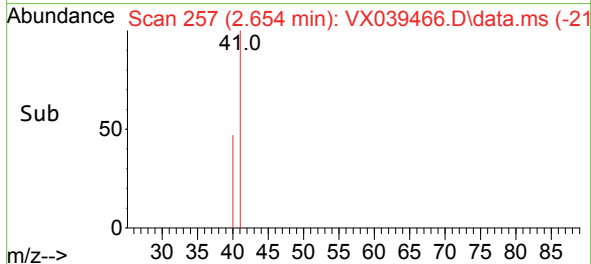

#15
 Acrylonitrile
 Concen: 0.251 ug/l
 RT: 2.977 min Scan# 310
 Delta R.T. -0.085 min
 Lab File: VX039466.D
 Acq: 26 Dec 2023 14:42

Tgt Ion: 53 Resp: 249
 Ion Ratio Lower Upper
 53 100
 52 0.0 66.0 99.0#
 51 29.7 29.8 44.6#

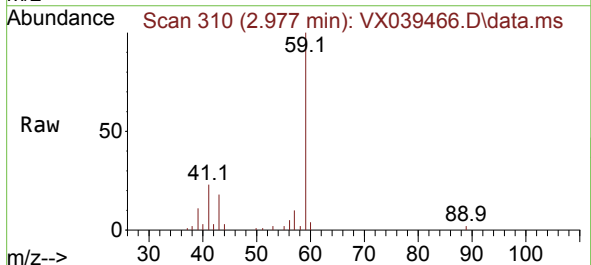

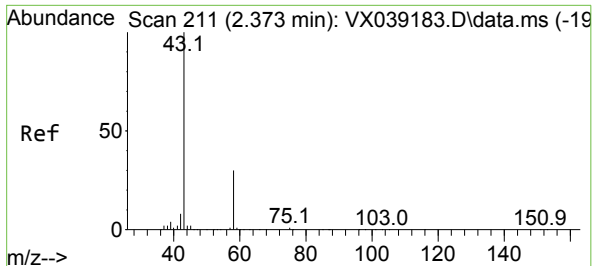

#16

Acetone

Concen: Below Cal

RT: 2.380 min Scan# 211

Delta R.T. 0.007 min

Lab File: VX039466.D

Acq: 26 Dec 2023 14:42

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 11219

Ion Ratio Lower Upper

43 100

58 33.3 21.9 32.9#

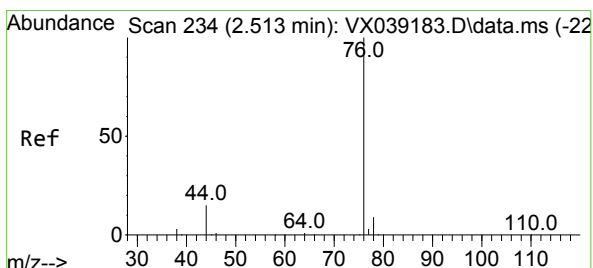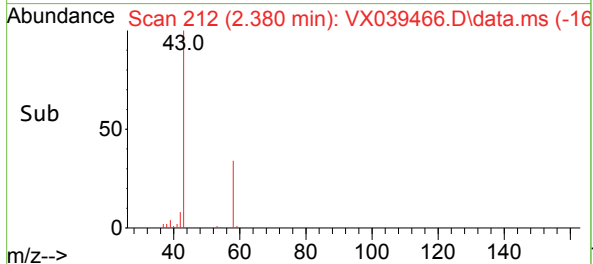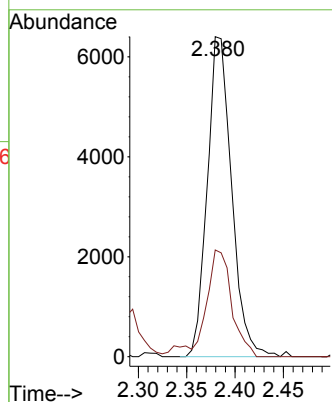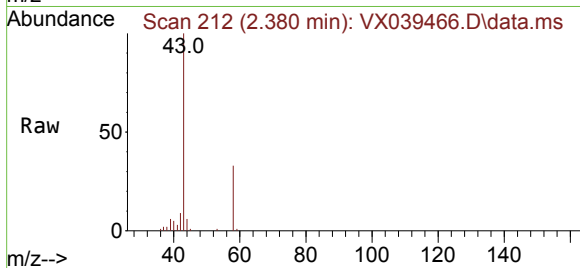

#17

Carbon Disulfide

Concen: 0.644 ug/l

RT: 2.508 min Scan# 233

Delta R.T. -0.006 min

Lab File: VX039466.D




Acq: 26 Dec 2023 14:42


Tgt Ion: 76 Resp: 2608

Ion Ratio Lower Upper

76 100

78 11.5 7.0 10.6#

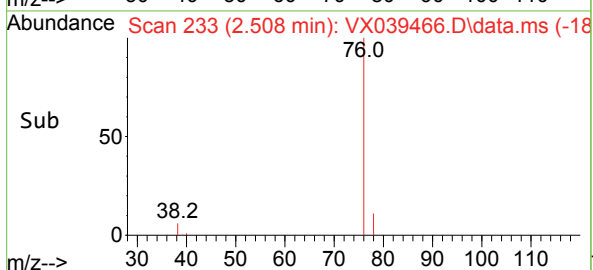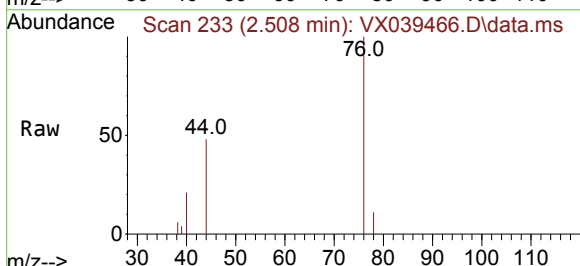



#18

Methyl Acetate

Concen: 0.347 ug/l

RT: 2.709 min Scan# 2

Delta R.T. 0.012 min

Lab File: VX039466.D

Acq: 26 Dec 2023 14:42

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 1477

Ion Ratio Lower Upper

43 100

74 20.6 17.8 26.8

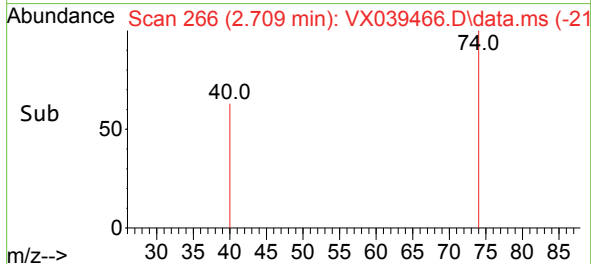

#19

Methyl tert-butyl Ether

Concen: 0.586 ug/l

RT: 3.117 min Scan# 333

Delta R.T. 0.006 min

Lab File: VX039466.D




Acq: 26 Dec 2023 14:42


Tgt Ion: 73 Resp: 2933

Ion Ratio Lower Upper

73 100


57 32.3 17.3 25.9#








#20
Methylene Chloride
Concen: 0.676 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion: 84 Resp: 1110




Ion	Ratio	Lower	Upper
84	100		
49	119.2	103.6	155.4
51	37.7	33.8	50.6
86	67.1	49.4	74.0

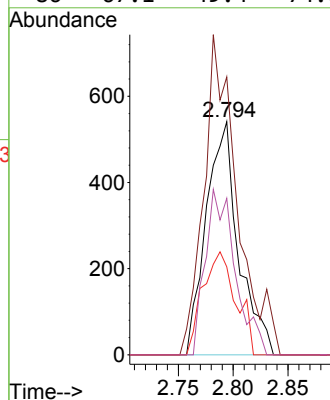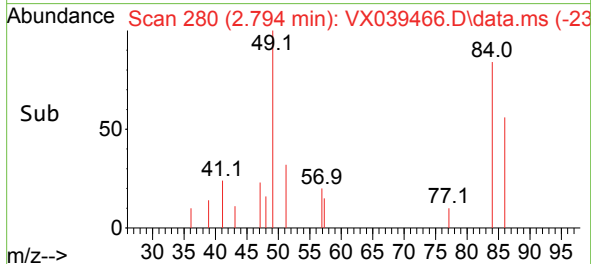


#25
2-Butanone
Concen: 0.604 ug/l
RT: 4.586 min Scan# 574
Delta R.T. 0.037 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Tgt Ion: 43 Resp: 1027

Ion	Ratio	Lower	Upper
43	100		
72	20.5	19.4	29.2


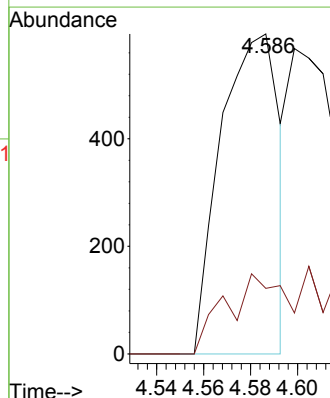
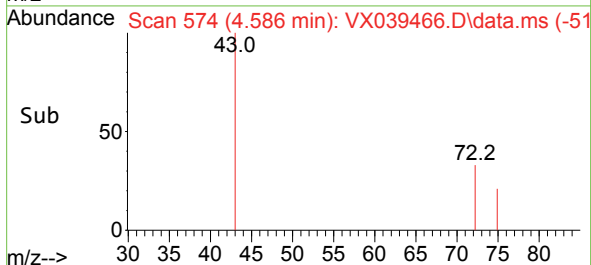





#33
1,2-Dichloroethane-d4
Concen: 48.131 ug/l
RT: 5.958 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 65 Resp: 94819
Ion Ratio Lower Upper
65 100
67 53.2 0.0 100.2

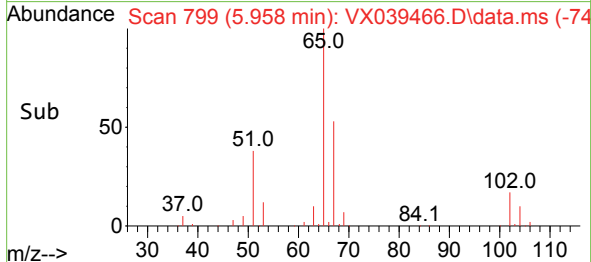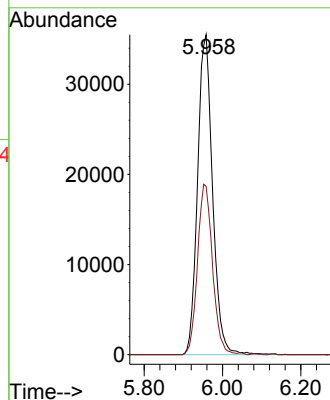

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.006 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Tgt Ion: 114 Resp: 223619
Ion Ratio Lower Upper
114 100
63 22.8 0.0 45.0
88 17.1 0.0 36.6

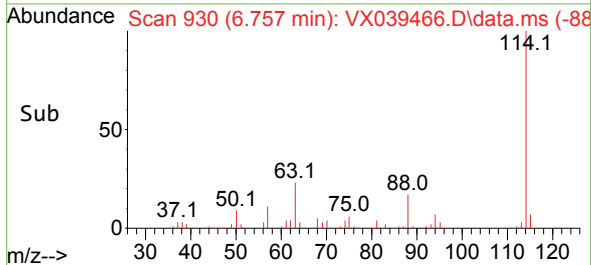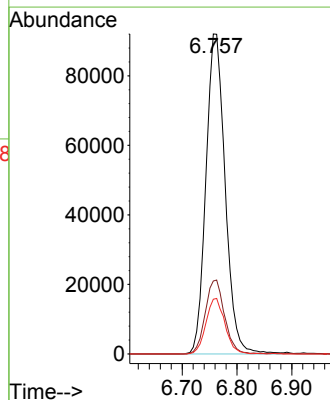

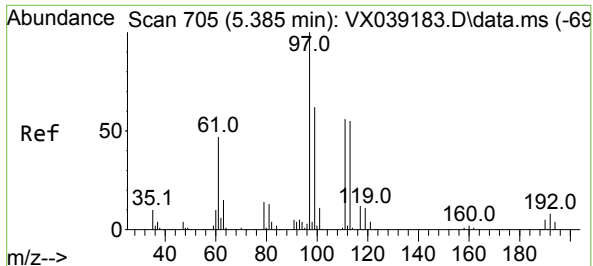

#35

Dibromofluoromethane

Concen: 47.211 ug/l

RT: 5.379 min Scan# 705

Delta R.T. -0.006 min


Lab File: VX039466.D

Acq: 26 Dec 2023 14:42

Instrument :

MSVOA_X

ClientSampleId :

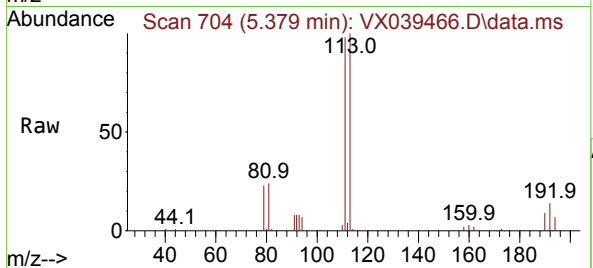




Tgt Ion:113 Resp: 72934

Ion Ratio Lower Upper

113 100

111 102.9 82.9 124.3

192 15.3 13.3 19.9

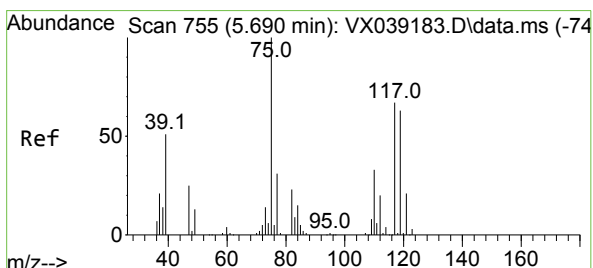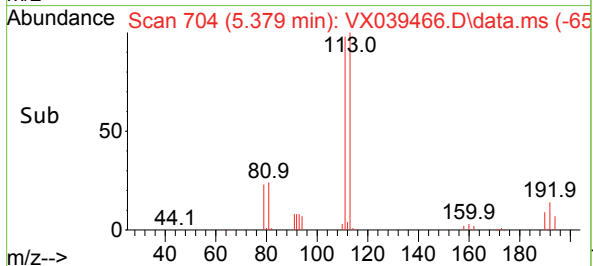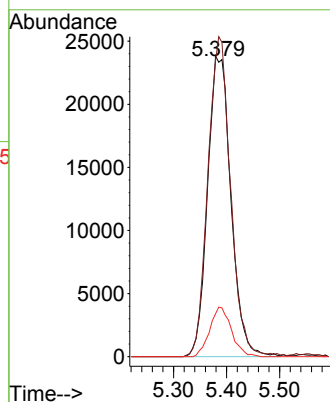

#36

1,1-Dichloropropene

Concen: 4.250 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.146 min

Lab File: VX039466.D

Acq: 26 Dec 2023 14:42




Tgt Ion: 75 Resp: 10361


Ion Ratio Lower Upper

75 100

110 8.9 17.0 50.9#


77 0.0 24.7 37.1#

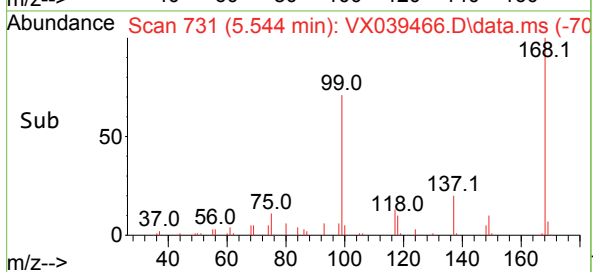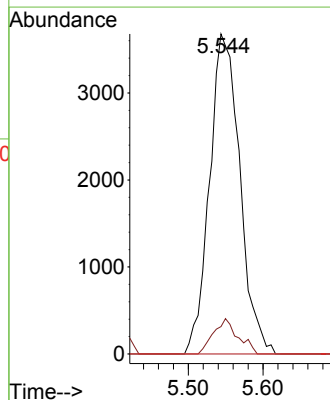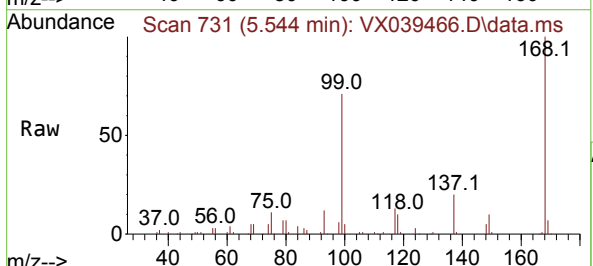






#38
Carbon Tetrachloride
Concen: 5.309 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Instrument :
MSVOA_X
ClientSampleId :



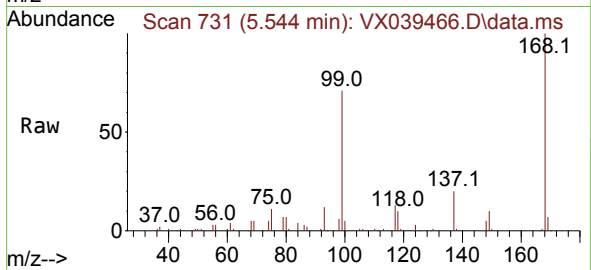



Tgt Ion:117 Resp: 12351
Ion Ratio Lower Upper
117 100
119 6.4 78.2 117.2#
121 0.0 24.4 36.6#



#40
Benzene
Concen: 26.913 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Tgt Ion: 78 Resp: 185593
Ion Ratio Lower Upper
78 100
77 23.5 19.3 28.9

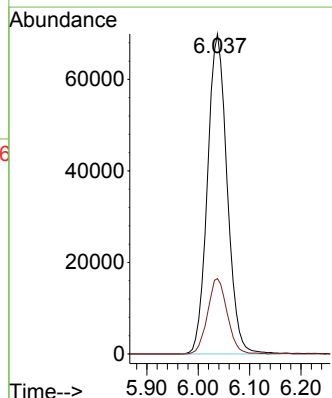



#49

1,4-Dioxane

Concen: 21.557 ug/l

RT: 7.683 min Scan# 1082

Delta R.T. 0.031 min

Lab File: VX039466.D

Acq: 26 Dec 2023 14:42

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 88 Resp: 832

Ion Ratio Lower Upper

88 100

43 0.0 0.0 0.0

58 80.6 60.1 90.1

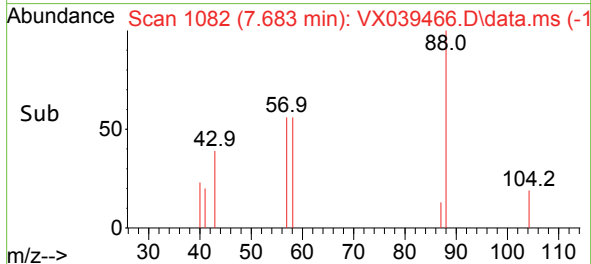

#50

Toluene-d8

Concen: 49.898 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX039466.D




Acq: 26 Dec 2023 14:42


Tgt Ion: 98 Resp: 286184

Ion Ratio Lower Upper

98 100

100 64.2 53.1 79.7


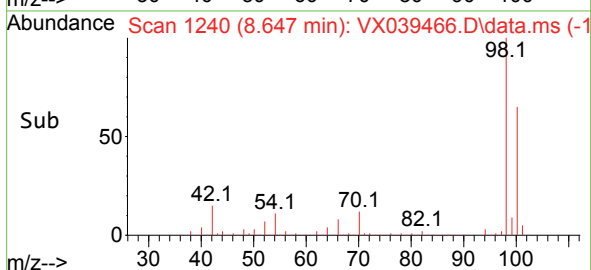






#52
Toluene
Concen: 1.237 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 5150
Ion Ratio Lower Upper
92 100
91 173.1 134.2 201.2

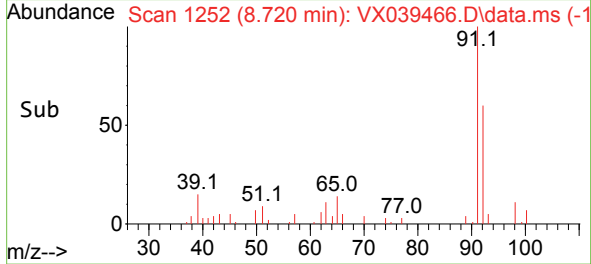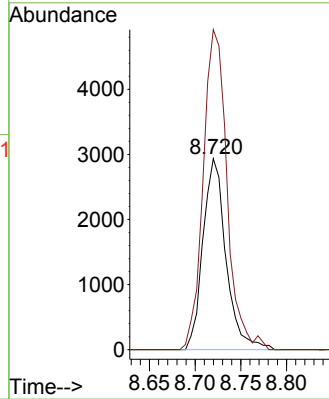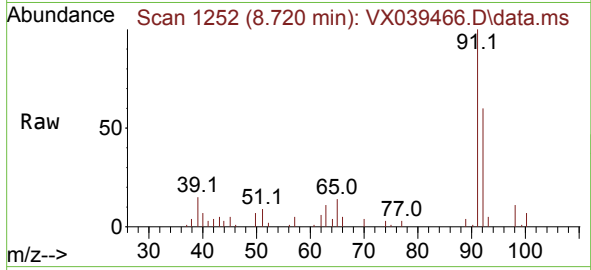

#62
4-Bromofluorobenzene
Concen: 51.202 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42


Tgt Ion: 95 Resp: 121165
Ion Ratio Lower Upper
95 100
174 64.3 0.0 135.6
176 61.1 0.0 131.0

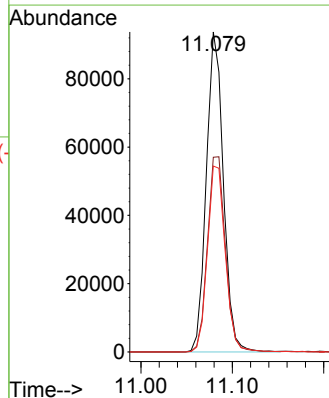






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Instrument :
MSVOA_X
ClientSampleId :



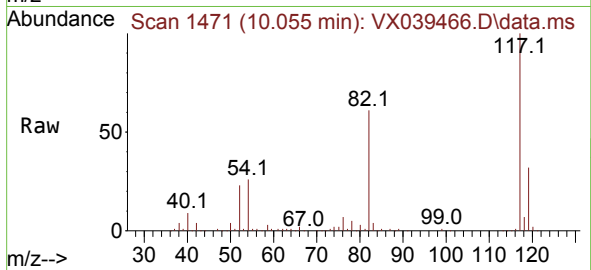



Tgt Ion:117 Resp: 226554
Ion Ratio Lower Upper
117 100
82 60.7 46.2 69.4
119 32.3 25.5 38.3

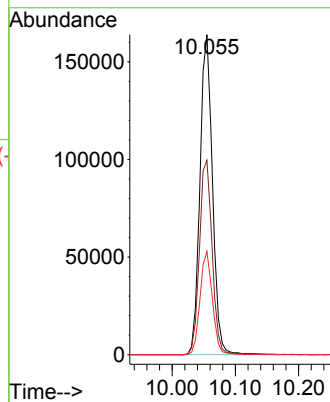

#67
Ethyl Benzene
Concen: 0.337 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Tgt Ion: 91 Resp: 3104
Ion Ratio Lower Upper
91 100
106 21.8 24.9 37.3#


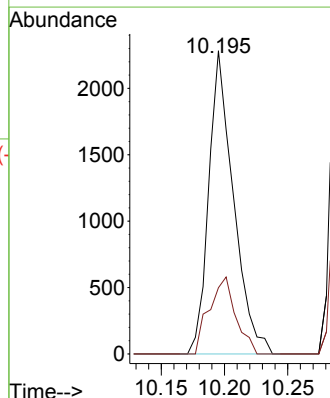




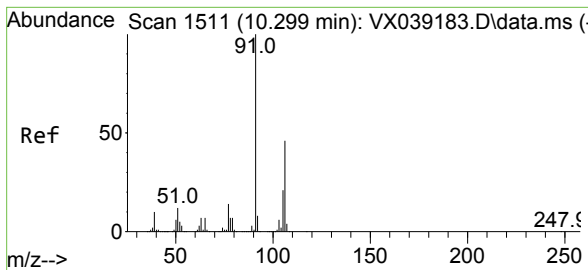

#68
m/p-Xylenes
Concen: 3.791 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 12511
Ion Ratio Lower Upper
106 100
91 223.2 165.5 248.3

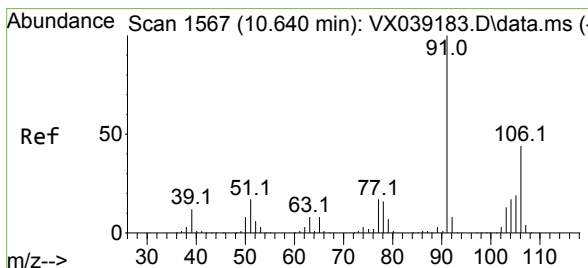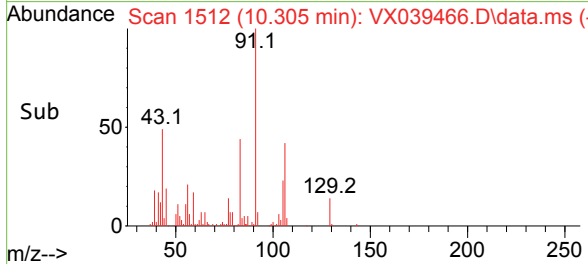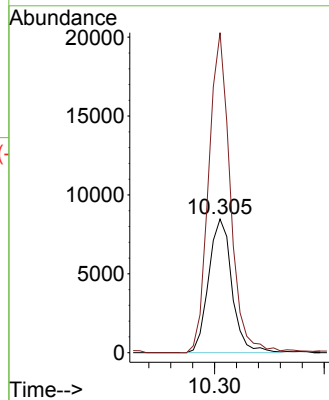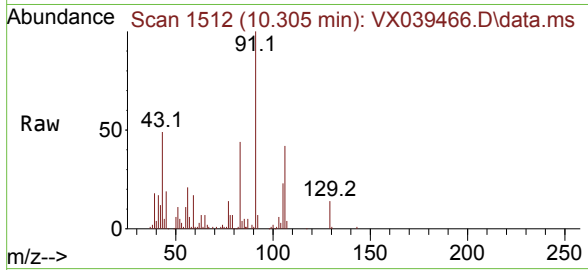

#69
o-Xylene
Concen: 0.722 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Tgt Ion:106 Resp: 2303
Ion Ratio Lower Upper
106 100
91 226.7 108.9 326.8


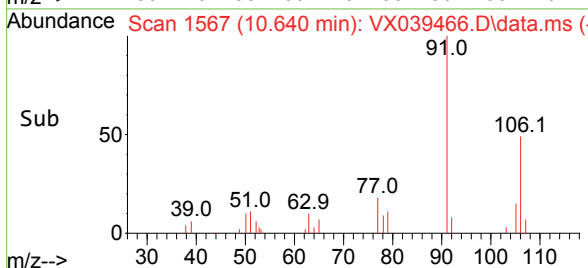
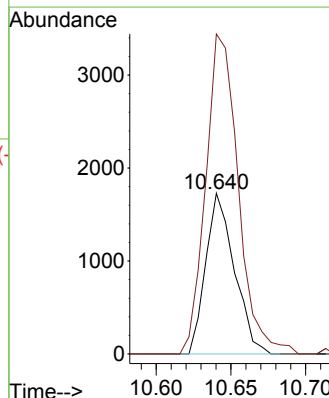
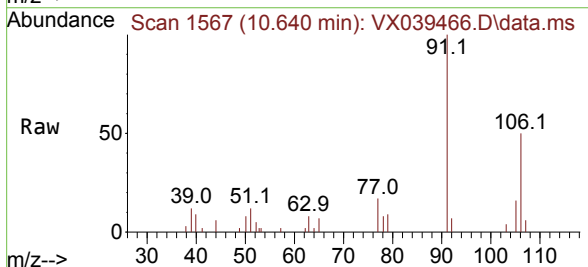




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX039466.D
 Acq: 26 Dec 2023 14:42




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:152 Resp: 102566
 Ion Ratio Lower Upper
 152 100
 115 66.8 43.3 129.9
 150 159.2 0.0 345.0

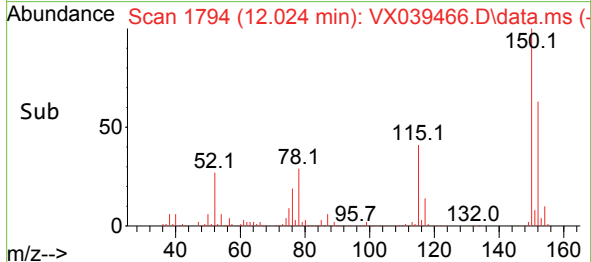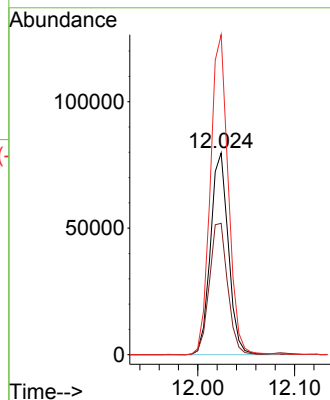

#73
 Isopropylbenzene
 Concen: 0.474 ug/l
 RT: 10.963 min Scan# 1620
 Delta R.T. 0.000 min
 Lab File: VX039466.D
 Acq: 26 Dec 2023 14:42

Tgt Ion:105 Resp: 3753
 Ion Ratio Lower Upper
 105 100
 120 26.8 12.9 38.6

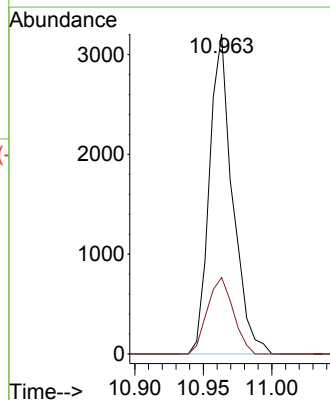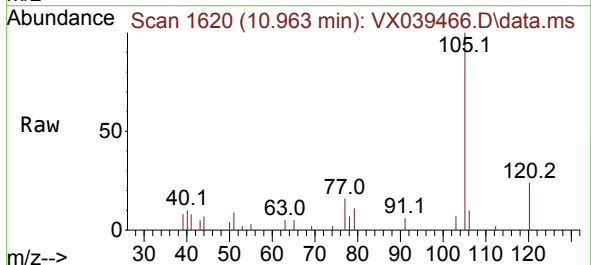



#75

1,1,2,2-Tetrachloroethane

Concen: 0.412 ug/l

RT: 11.152 min Scan# 1651

Delta R.T. -0.061 min

Lab File: VX039466.D

Acq: 26 Dec 2023 14:42

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 1212

Ion Ratio Lower Upper

83 100

131 0.0 5.3 15.8#

85 7.4 32.0 96.2#

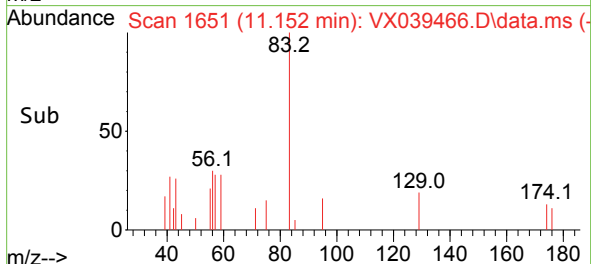

#76

1,2,3-Trichloropropane

Concen: 25.106 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX039466.D




Acq: 26 Dec 2023 14:42


Tgt Ion: 75 Resp: 66620

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#

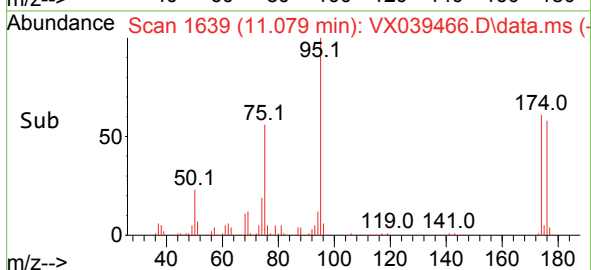



#78

n-propylbenzene

Concen: 0.494 ug/l

RT: 11.311 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX039466.D

Acq: 26 Dec 2023 14:42

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 4813

Ion Ratio Lower Upper

91 100

120 21.8 11.5 34.4

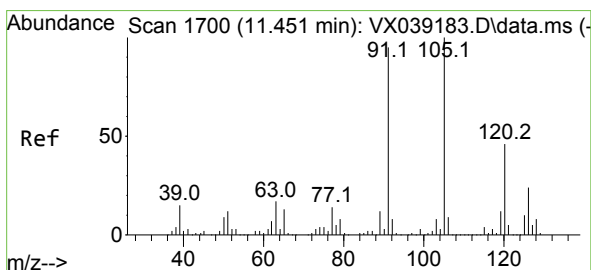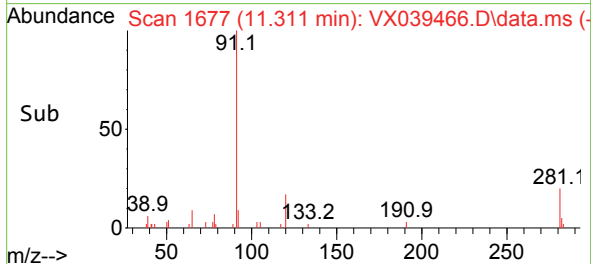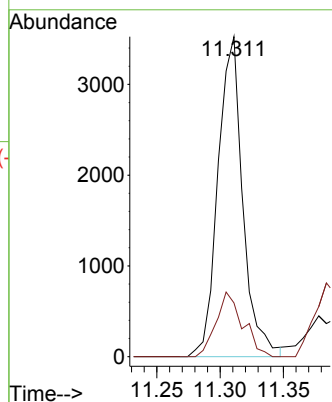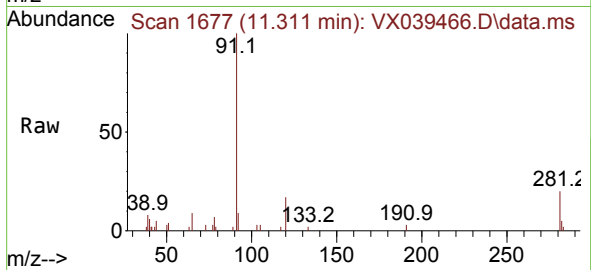

#80

1,3,5-Trimethylbenzene

Concen: 1.170 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX039466.D




Acq: 26 Dec 2023 14:42


Tgt Ion:105 Resp: 7890

Ion Ratio Lower Upper

105 100

120 44.3 24.1 72.3









#81
trans-1,4-Dichloro-2-butene
Concen: 70.824 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 66620
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

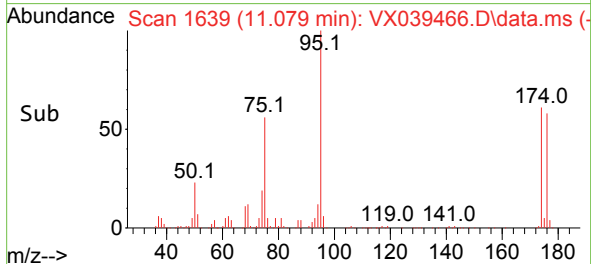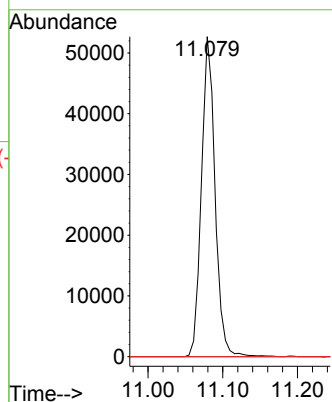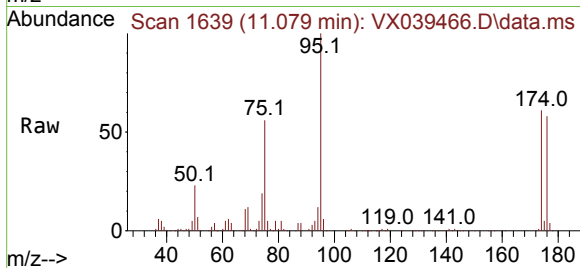

#84
1,2,4-Trimethylbenzene
Concen: 2.590 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX039466.D
Acq: 26 Dec 2023 14:42

Tgt Ion:105 Resp: 17907
Ion Ratio Lower Upper
105 100
120 41.9 21.2 63.6


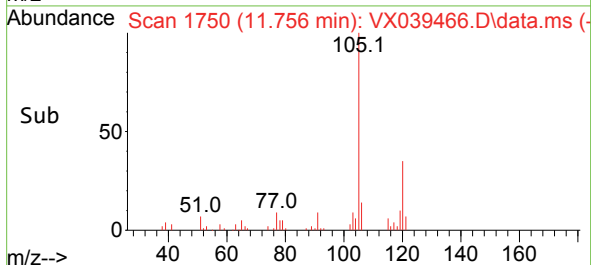

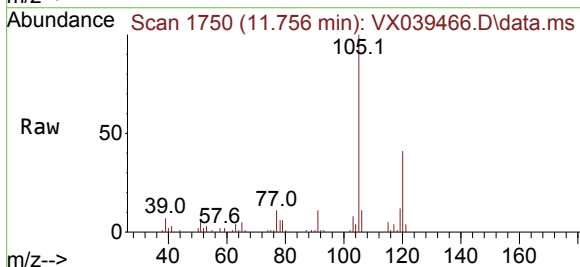




#85
 sec-Butylbenzene
 Concen: 2.193 ug/l
 RT: 11.756 min Scan# 11
 Delta R.T. -0.134 min
 Lab File: VX039466.D
 Acq: 26 Dec 2023 14:42




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 17907
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.4#

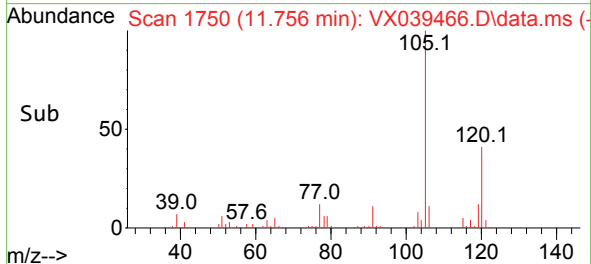

#90
 Hexachloroethane
 Concen: 0.240 ug/l
 RT: 12.640 min Scan# 1895
 Delta R.T. 0.104 min
 Lab File: VX039466.D
 Acq: 26 Dec 2023 14:42

Tgt Ion:117 Resp: 297
 Ion Ratio Lower Upper
 117 100
 201 0.0 32.9 98.6#





#95

Naphthalene

Concen: 3.724 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. 0.000 min


Lab File: VX039466.D

Acq: 26 Dec 2023 14:42

Instrument :

MSVOA_X

ClientSampleId :

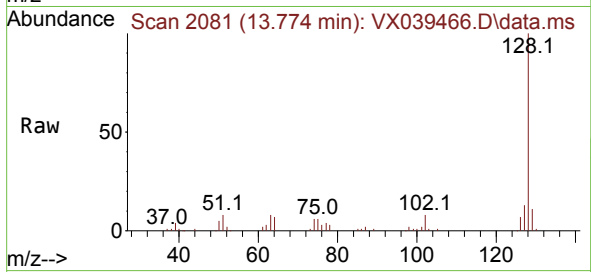

Tgt Ion:128 Resp: 27936

Ion Ratio Lower Upper

128 100

127 12.2 10.3 15.5

129 10.8 8.8 13.2

