
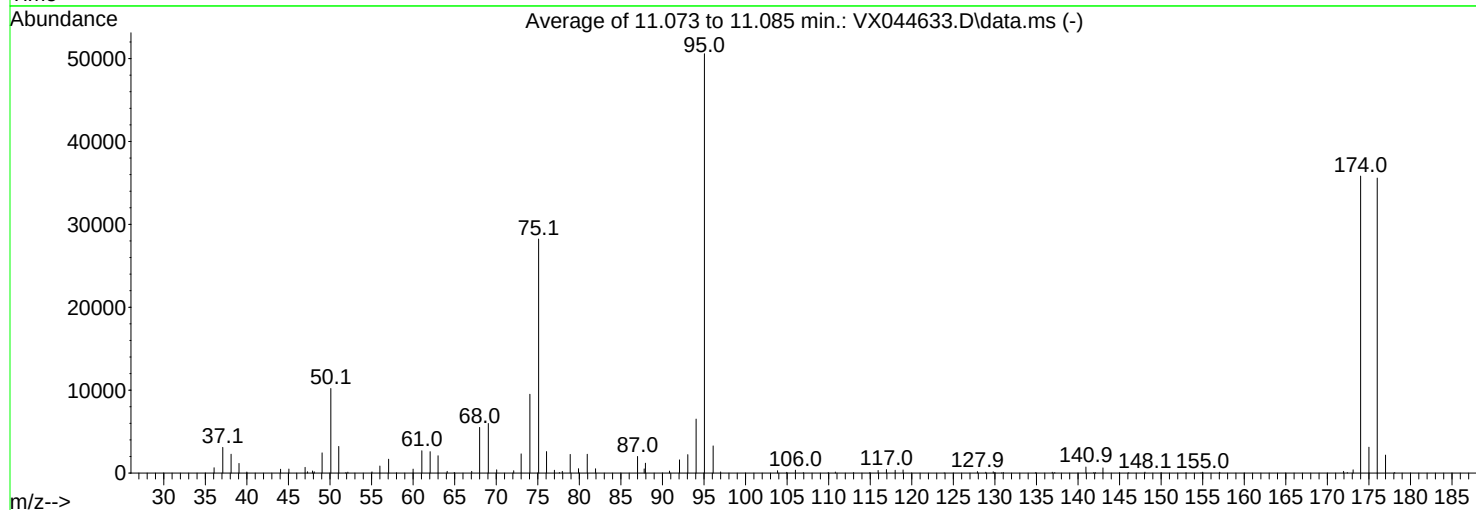


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010825\
Data File : VX044633.D
Acq On : 08 Jan 2025 23:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X010825W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Jan 09 02:10:37 2025

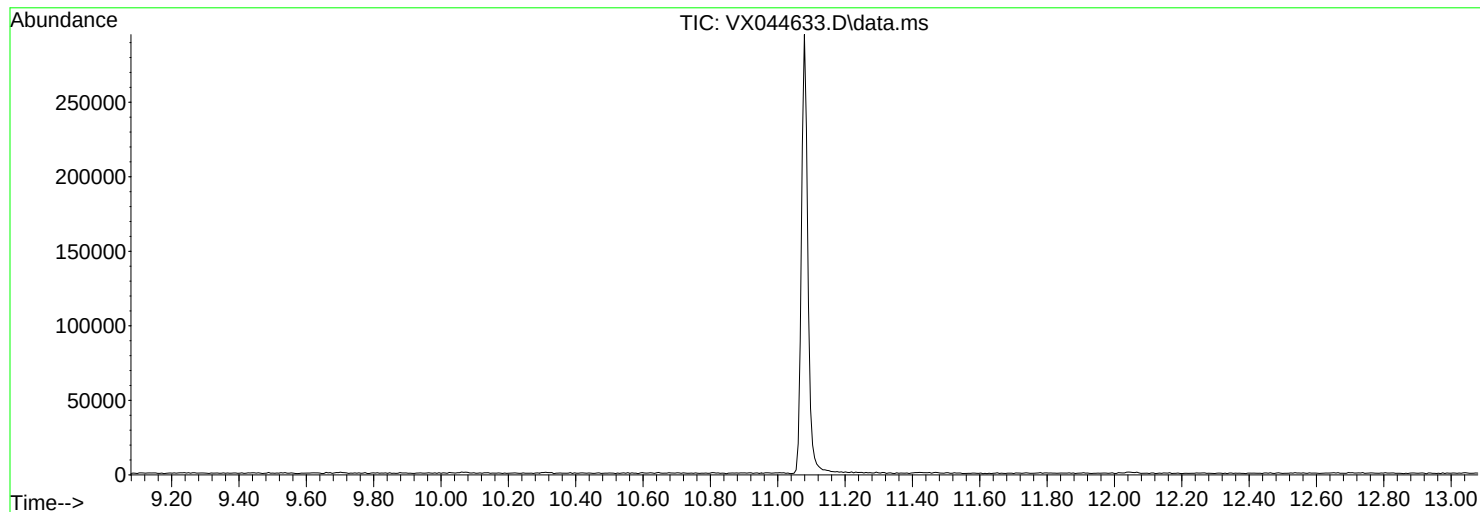

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	10204	PASS
75	95	30	60	55.8	28232	PASS
95	95	100	100	100.0	50584	PASS
96	95	5	9	6.5	3280	PASS
173	174	0.00	2	1.1	395	PASS
174	95	50	100	70.8	35824	PASS
175	174	5	9	8.7	3121	PASS
176	174	95	101	99.3	35584	PASS
177	176	5	9	6.1	2170	PASS