


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX010919\
 Data File : VX006955.D
 Acq On : 09 Jan 2019 09:47
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Title : SW846 8260
 Last Update : Tue Jan 08 14:06:59 2019

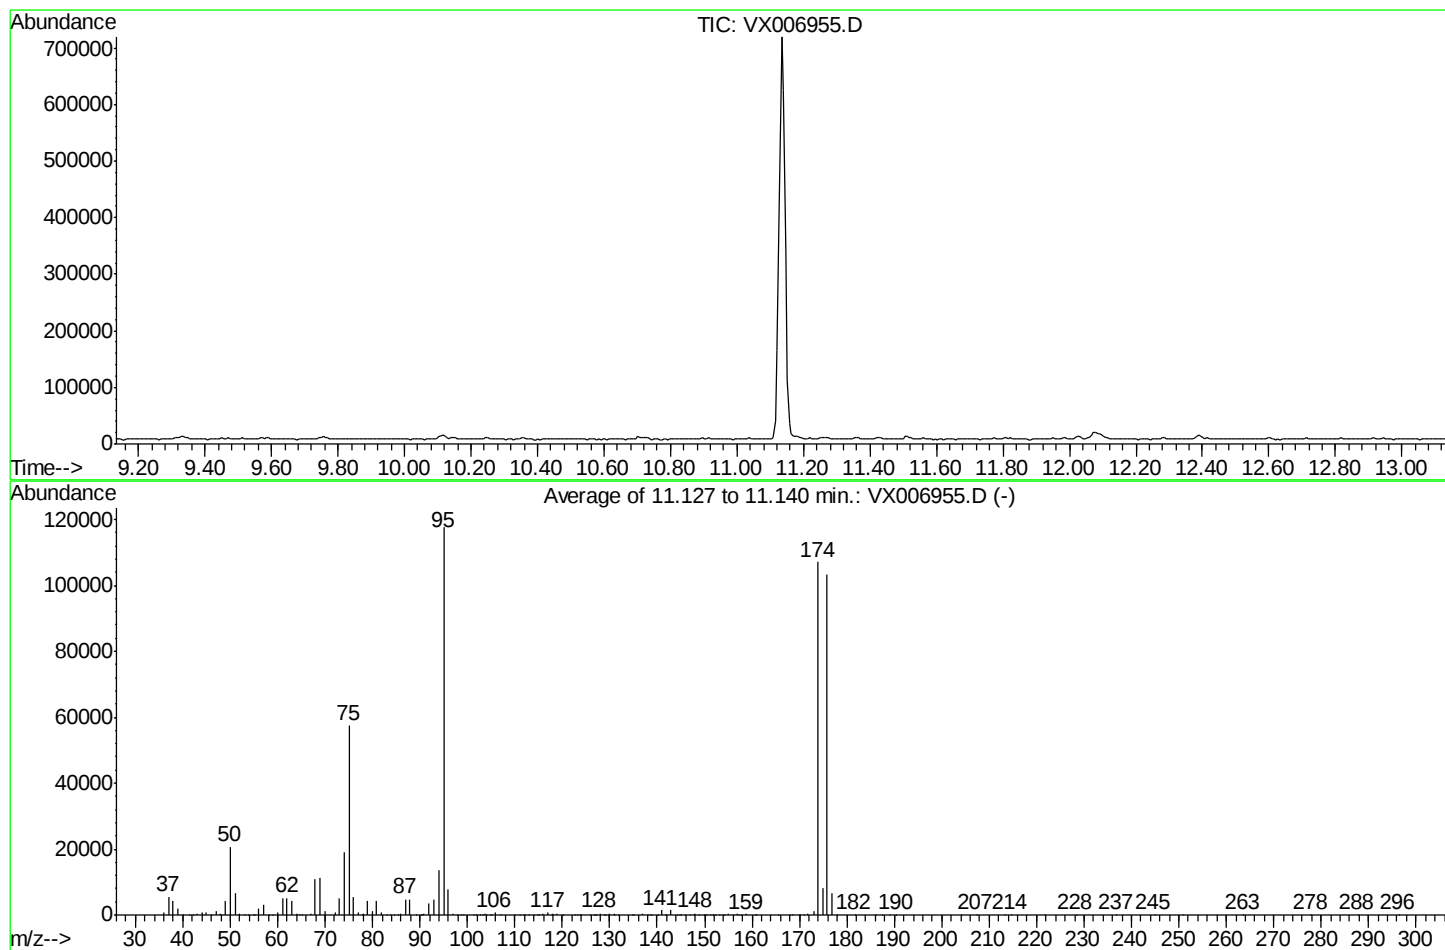

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	20741	PASS
75	95	30	60	48.8	57363	PASS
95	95	100	100	100.0	117621	PASS
96	95	5	9	6.8	7958	PASS
173	174	0.00	2	1.2	1307	PASS
174	95	50	100	91.0	107018	PASS
175	174	5	9	7.7	8265	PASS
176	174	95	101	96.5	103317	PASS
177	176	5	9	6.6	6805	PASS