

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
 Data File : VX033714.D
 Acq On : 13 Jan 2023 10:12
 Operator : JC/MD
 Sample : VX0113WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 13 13:49:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 28 01:59:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	269047	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	213702	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	82771	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	69589	52.830	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.660%
7) Chloroethane-d5	1.672	69	54647	44.047	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.100%
11) 1,1-Dichloroethene-d2	2.306	63	110541	39.858	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.720%
21) 2-Butanone-d5	4.459	46	107119	108.996	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	109.000%
24) Chloroform-d	5.050	84	146604	41.849	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.700%
26) 1,2-Dichloroethane-d4	5.952	65	95774	43.474	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.940%
32) Benzene-d6	5.970	84	302674	51.886	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.780%
36) 1,2-Dichloropropane-d6	7.306	67	92861	53.928	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.860%
41) Toluene-d8	8.647	98	278869	48.404	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.800%
43) trans-1,3-Dichloroprop...	8.945	79	39138	46.383	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.760%
47) 2-Hexanone-d5	9.384	63	76632	116.768	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.770%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	86259	36.204	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	72.400%
66) 1,2-Dichlorobenzene-d4	12.317	152	77703	47.314	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.620%
Target Compounds						
					Qvalue	
13) Acetone	2.398	43	1905	2.682	ug/L	72
37) 1,2-Dichloropropane	7.306	63	10743	7.487	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
Data File : VX033714.D
Acq On : 13 Jan 2023 10:12
Operator : JC/MD
Sample : VX0113WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 13 13:49:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 28 01:59:02 2022
Response via : Initial Calibration

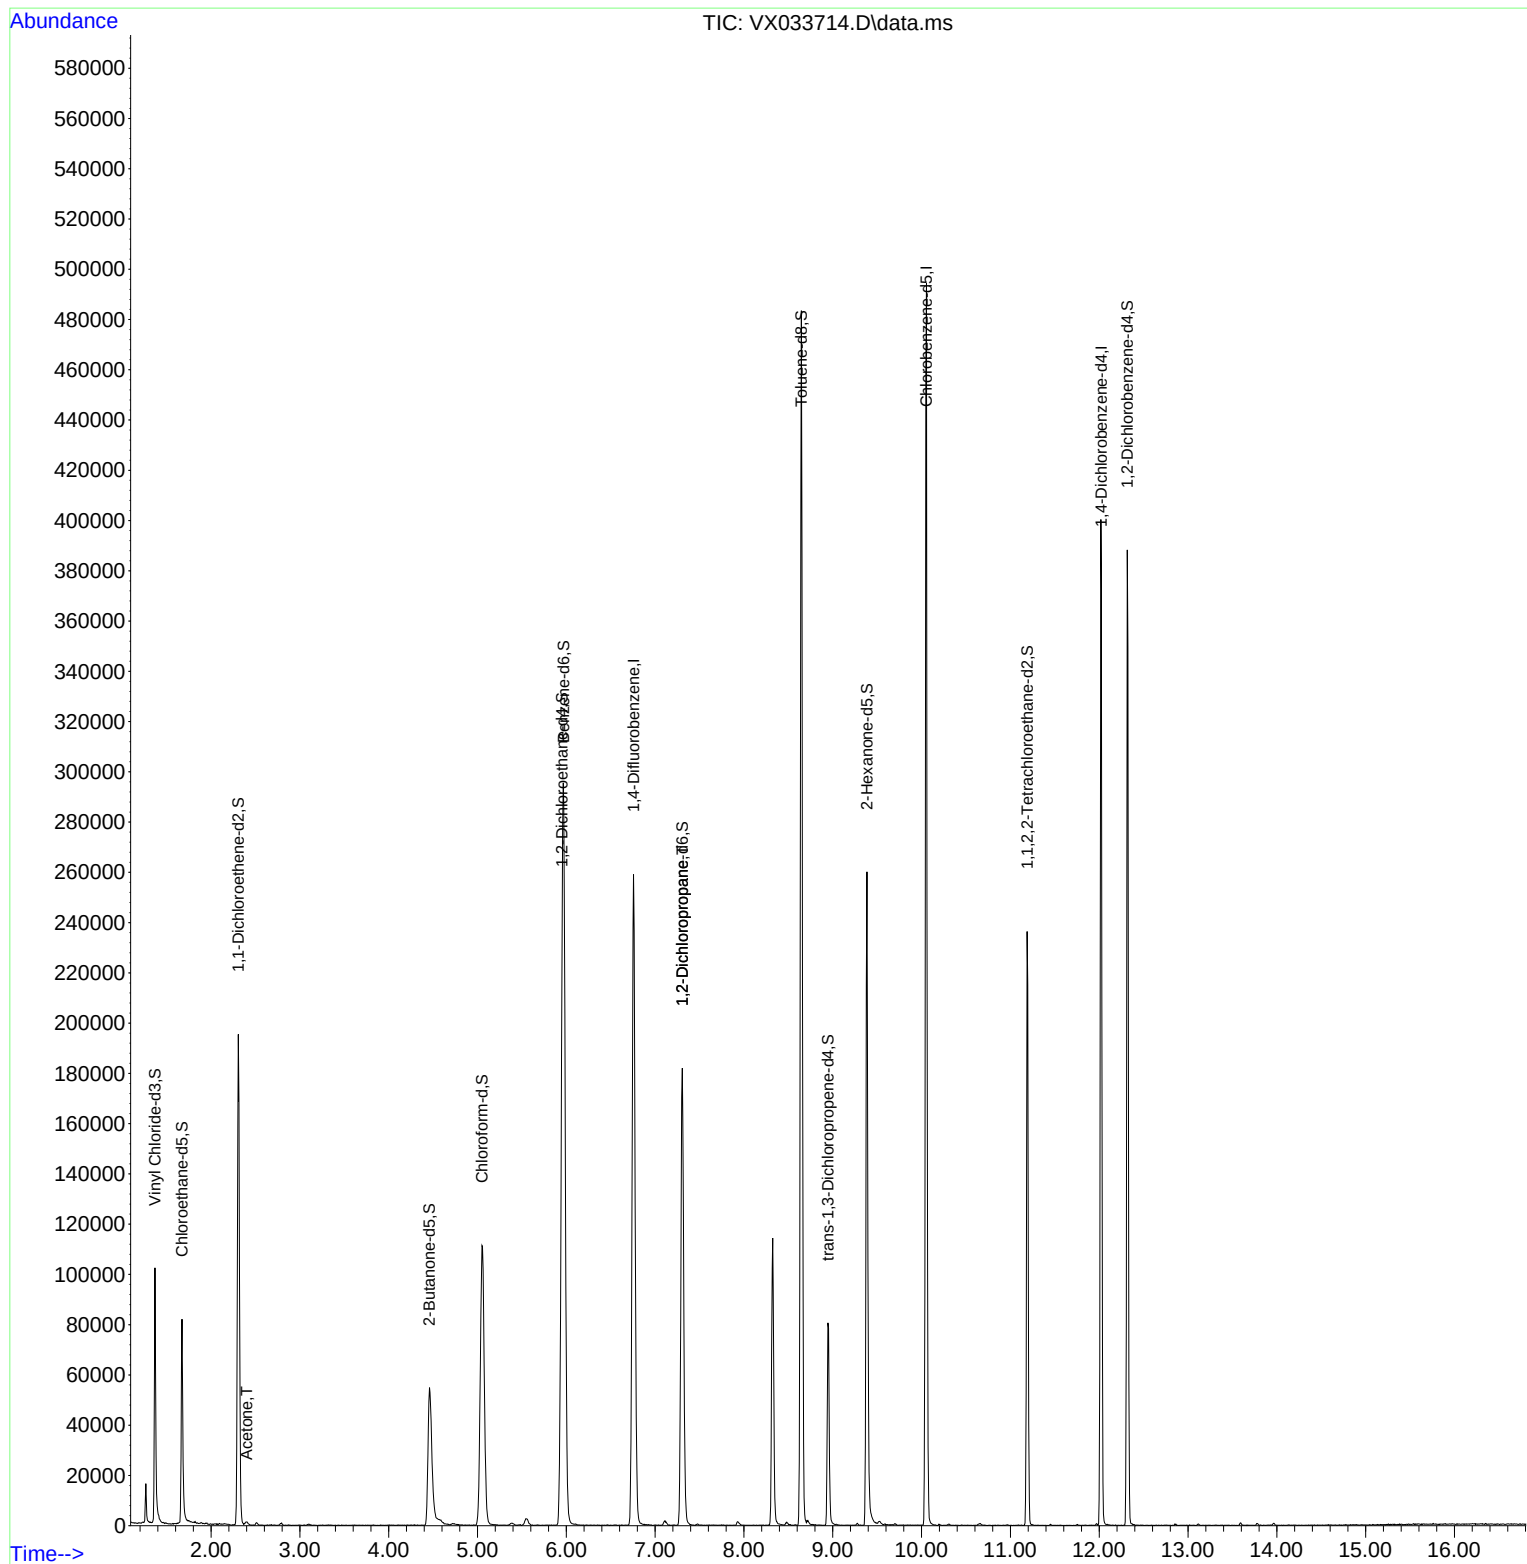



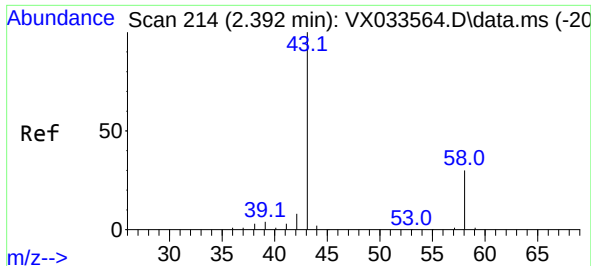


#13
Acetone
Concen: 2.682 ug/L
RT: 2.398 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX033714.D
Acq: 13 Jan 2023 10:12

Instrument :
MSVOA_X
ClientSampleId :

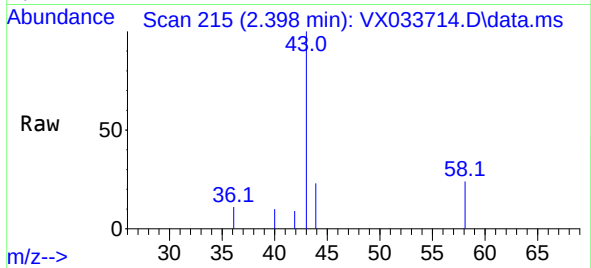

Tgt Ion: 43 Resp: 1905
Ion Ratio Lower Upper
43 100
58 16.0 0.0 62.4

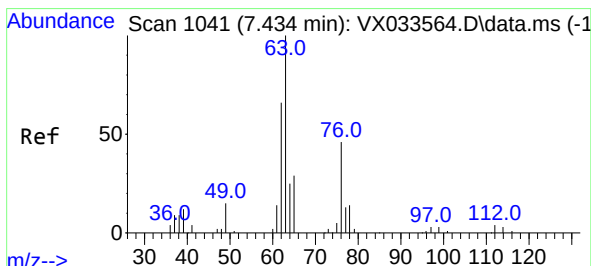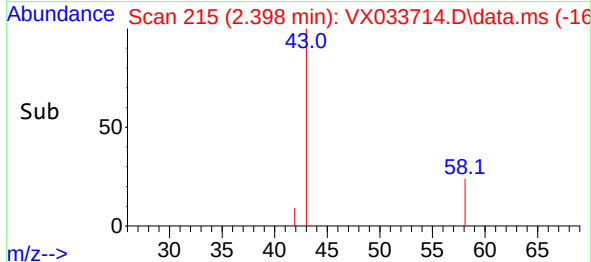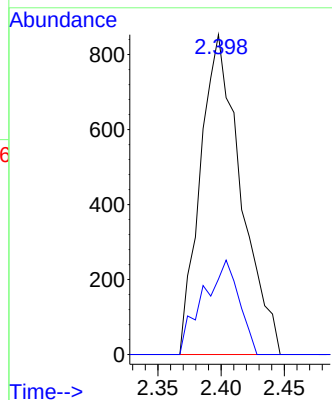

#37
1,2-Dichloropropane
Concen: 7.487 ug/L
RT: 7.306 min Scan# 1020
Delta R.T. -0.128 min
Lab File: VX033714.D
Acq: 13 Jan 2023 10:12

Tgt Ion: 63 Resp: 10743
Ion Ratio Lower Upper
63 100
112 0.0 3.6 5.4#

