

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
 Data File : VX033715.D
 Acq On : 13 Jan 2023 10:43
 Operator : JC/MD
 Sample : 01120-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C1144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
 Title : VOC Analysis

Signal : TIC: VX033715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rBV	98746	107159	12.65%	1.648%
2	1.673	91	96	109	rVB	78779	101880	12.03%	1.566%
3	2.154	174	175	180	rBV2	229	304	0.04%	0.005%
4	2.307	194	200	209	rBV	188782	290091	34.24%	4.460%
5	2.465	224	226	227	rBV2	147	87	0.01%	0.001%
6	2.514	230	234	239	rVB	999	1434	0.17%	0.022%
7	2.587	245	246	248	rBV	143	79	0.01%	0.001%
8	2.788	274	279	282	rBV	517	807	0.10%	0.012%
9	2.916	297	300	303	rVB2	154	135	0.02%	0.002%
10	3.099	327	330	333	rBV2	166	188	0.02%	0.003%
11	3.672	422	424	426	rBV	131	107	0.01%	0.002%
12	3.776	439	441	442	rVB	151	82	0.01%	0.001%
13	3.910	462	463	465	rVB	141	88	0.01%	0.001%
14	4.129	497	499	502	rBV2	170	169	0.02%	0.003%
15	4.300	526	527	528	rBV	160	96	0.01%	0.001%
16	4.459	544	553	568	rBV	53980	163318	19.28%	2.511%
17	4.727	596	597	599	rVB	228	107	0.01%	0.002%
18	4.763	601	603	608	rVV	227	297	0.04%	0.005%
19	4.837	612	615	618	rBV2	120	184	0.02%	0.003%
20	4.940	631	632	635	rBV	140	85	0.01%	0.001%
21	5.056	638	651	666	rVV	110184	342810	40.46%	5.271%
22	5.215	675	677	680	rVB2	213	213	0.03%	0.003%
23	5.245	680	682	684	rBV2	126	109	0.01%	0.002%
24	5.379	700	704	707	rBV4	350	559	0.07%	0.009%
25	5.544	724	731	740	rBV5	1130	3345	0.39%	0.051%
26	5.672	751	752	757	rBV2	129	193	0.02%	0.003%
27	5.964	788	800	816	rVV2	285100	847179	100.00%	13.026%
28	6.227	841	843	844	rBV	97	84	0.01%	0.001%
29	6.324	855	859	860	rBV2	139	144	0.02%	0.002%
30	6.635	908	910	911	rBV	152	100	0.01%	0.002%
31	6.757	921	930	945	rBV	237266	558489	65.92%	8.587%
32	6.989	966	968	969	rBV	205	86	0.01%	0.001%
33	7.111	983	988	994	rVB5	1343	2768	0.33%	0.043%
34	7.306	1011	1020	1036	rBV	177019	384769	45.42%	5.916%
35	7.482	1045	1049	1052	rBV2	370	553	0.07%	0.009%
36	7.781	1096	1098	1100	rBV	150	140	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
 Data File : VX033715.D
 Acq On : 13 Jan 2023 10:43
 Operator : JC/MD
 Sample : 01120-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C1144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
 Title : VOC Analysis

37	7.897	1111	1117	1119	rBV2	638	1045	0.12%	0.016%
38	8.324	1181	1187	1198	rBV	110329	183394	21.65%	2.820%
39	8.482	1208	1213	1220	rVB4	1381	2447	0.29%	0.038%
40	8.586	1226	1230	1233	rBV2	301	411	0.05%	0.006%
41	8.647	1233	1240	1252	rBV	460268	706097	83.35%	10.856%
42	8.903	1280	1282	1283	rVB	193	107	0.01%	0.002%
43	8.946	1284	1289	1301	rVV	74644	116171	13.71%	1.786%
44	9.092	1311	1313	1314	rVB	208	117	0.01%	0.002%
45	9.116	1314	1317	1320	rBV2	182	196	0.02%	0.003%
46	9.214	1332	1333	1336	rBV	149	102	0.01%	0.002%
47	9.275	1339	1343	1347	rVB3	583	860	0.10%	0.013%
48	9.385	1355	1361	1377	rBV	245800	366928	43.31%	5.642%
49	9.519	1381	1383	1393	rVB4	1734	3470	0.41%	0.053%
50	9.665	1405	1407	1410	rBV2	135	125	0.01%	0.002%
51	9.689	1410	1411	1413	rVB2	144	91	0.01%	0.001%
52	9.714	1413	1415	1416	rBV2	176	136	0.02%	0.002%
53	9.787	1425	1427	1430	rBV2	187	193	0.02%	0.003%
54	10.055	1465	1471	1485	rBV	459935	641429	75.71%	9.862%
55	10.201	1491	1495	1499	rVB3	433	577	0.07%	0.009%
56	10.305	1508	1512	1518	rVB3	691	898	0.11%	0.014%
57	10.378	1522	1524	1527	rBV2	110	121	0.01%	0.002%
58	10.409	1527	1529	1530	rBV	138	110	0.01%	0.002%
59	10.512	1542	1546	1548	rBV2	150	216	0.03%	0.003%
60	10.640	1565	1567	1568	rBV	328	269	0.03%	0.004%
61	10.781	1588	1590	1593	rBV3	272	200	0.02%	0.003%
62	10.860	1601	1603	1606	rBV2	191	168	0.02%	0.003%
63	10.964	1618	1620	1623	rVB2	382	342	0.04%	0.005%
64	11.085	1638	1640	1644	rVB	382	323	0.04%	0.005%
65	11.189	1652	1657	1673	rVB	300468	388068	45.81%	5.967%
66	11.299	1673	1675	1676	rBV2	220	164	0.02%	0.003%
67	11.354	1682	1684	1687	rBV2	129	130	0.02%	0.002%
68	11.500	1706	1708	1709	rBV	109	89	0.01%	0.001%
69	11.604	1722	1725	1726	rBV2	175	177	0.02%	0.003%
70	11.756	1745	1750	1752	rBV3	494	572	0.07%	0.009%
71	11.848	1762	1765	1766	rBV	236	161	0.02%	0.002%
72	11.872	1767	1769	1772	rVB2	266	221	0.03%	0.003%
73	11.933	1776	1779	1781	rBV3	252	322	0.04%	0.005%
74	11.969	1783	1785	1788	rVB3	646	660	0.08%	0.010%
75	12.018	1788	1793	1804	rBV	480773	632275	74.63%	9.721%
76	12.219	1822	1826	1837	rBV2	9147	15034	1.77%	0.231%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
 Data File : VX033715.D
 Acq On : 13 Jan 2023 10:43
 Operator : JC/MD
 Sample : 01120-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C1144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1851	rVV	501057	622917	73.53%	9.577%
78	12.543	1878	1879	1883	rBV2	156	172	0.02%	0.003%
79	12.585	1883	1886	1887	rVB2	383	345	0.04%	0.005%
80	12.853	1927	1930	1937	rBV2	2120	2647	0.31%	0.041%
81	12.969	1948	1949	1952	rBV	153	121	0.01%	0.002%
82	13.116	1970	1973	1977	rBV3	386	431	0.05%	0.007%
83	13.250	1994	1995	2000	rBV2	197	200	0.02%	0.003%
84	13.286	2000	2001	2004	rBV2	100	96	0.01%	0.001%
85	13.408	2018	2021	2023	rBV2	198	248	0.03%	0.004%
86	13.542	2041	2043	2045	rBV	191	205	0.02%	0.003%
87	13.591	2048	2051	2055	rBV3	579	729	0.09%	0.011%
88	13.719	2070	2072	2076	rBV2	117	132	0.02%	0.002%
89	13.780	2079	2082	2087	rBV2	626	858	0.10%	0.013%
90	13.896	2099	2101	2102	rVB	160	94	0.01%	0.001%
91	13.963	2110	2112	2115	rBV3	471	525	0.06%	0.008%
92	14.134	2136	2140	2143	rBV2	252	390	0.05%	0.006%
93	14.243	2157	2158	2159	rBV	180	90	0.01%	0.001%
94	14.280	2163	2164	2166	rBV	223	115	0.01%	0.002%
95	14.439	2187	2190	2191	rBV2	176	137	0.02%	0.002%
96	14.463	2191	2194	2195	rVV	161	132	0.02%	0.002%
97	14.634	2221	2222	2223	rBV	242	131	0.02%	0.002%
98	14.853	2256	2258	2259	rBV	271	186	0.02%	0.003%
99	15.755	2404	2406	2407	rBV2	262	196	0.02%	0.003%
100	15.932	2434	2435	2438	rBV3	396	218	0.03%	0.003%




Sum of corrected areas: 6503969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
Data File : VX033715.D
Acq On : 13 Jan 2023 10:43
Operator : JC/MD
Sample : 01120-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C1144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

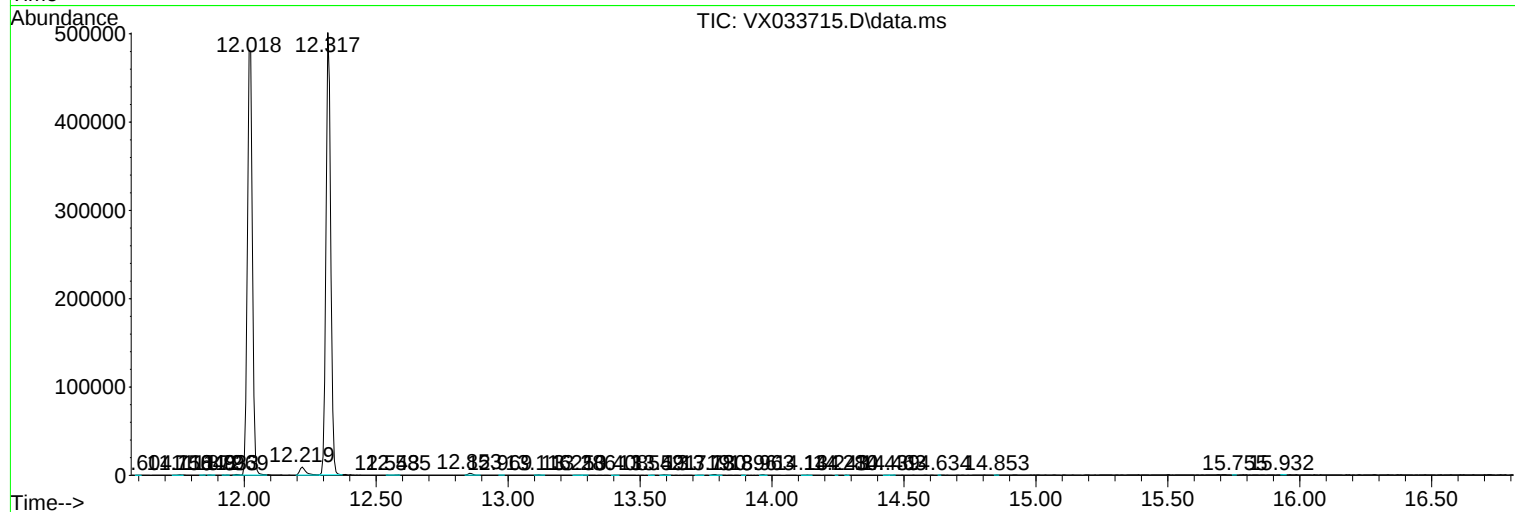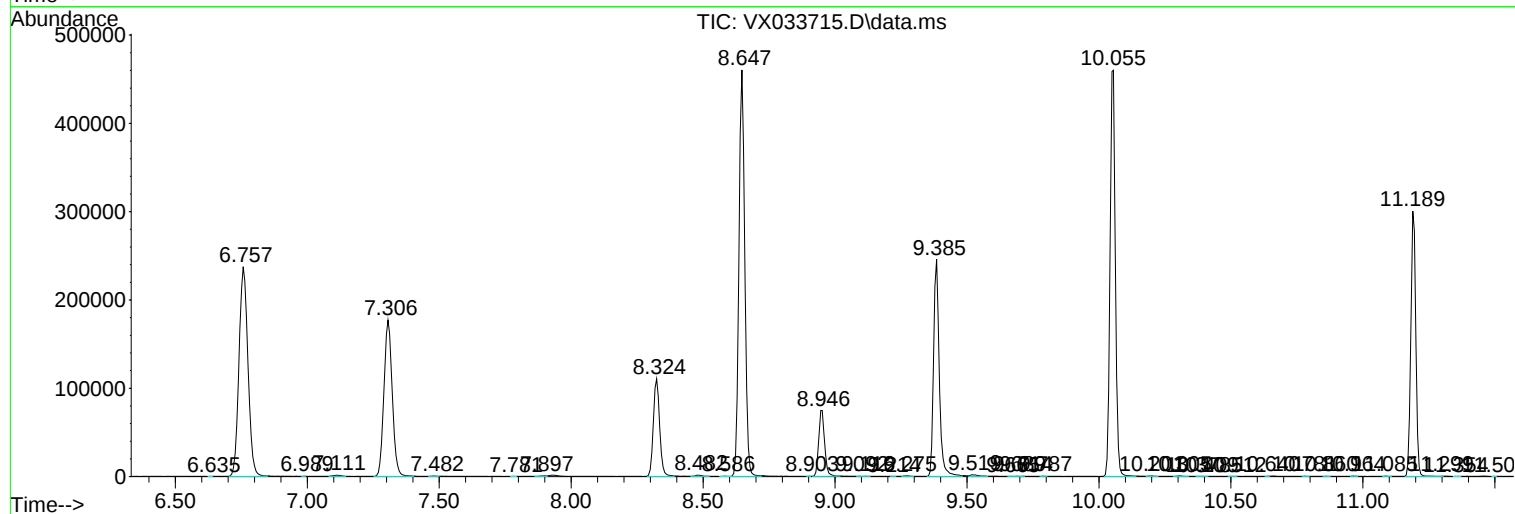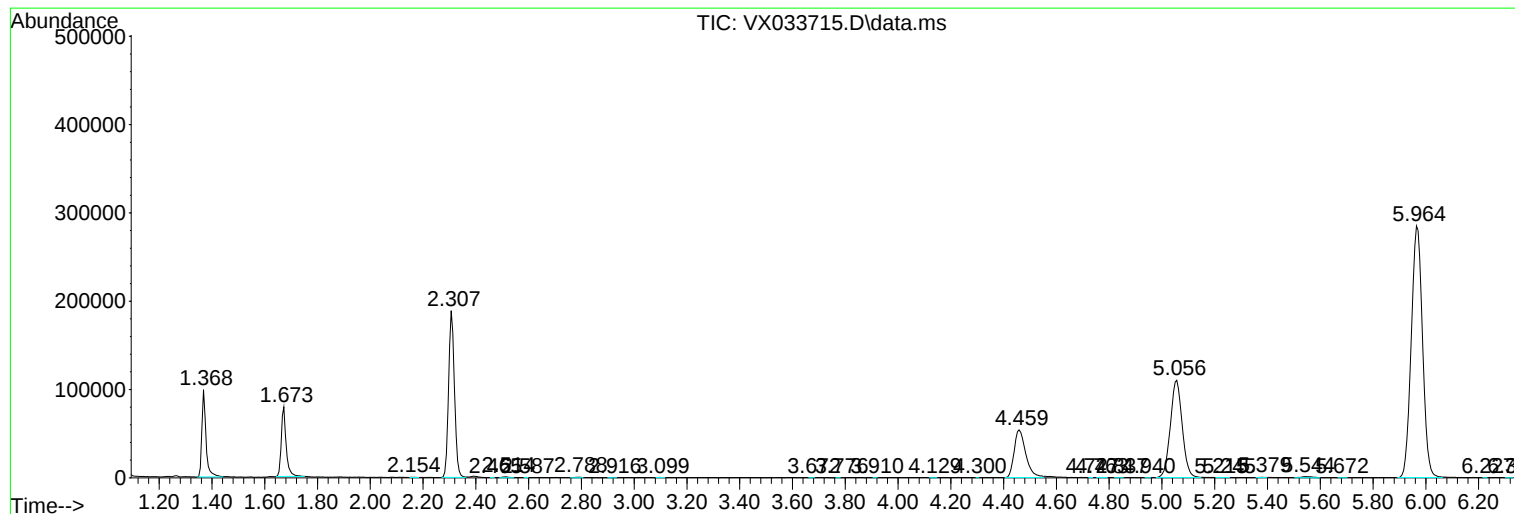

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
Data File : VX033715.D
Acq On : 13 Jan 2023 10:43
Operator : JC/MD
Sample : 01120-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C1144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
Data File : VX033715.D
Acq On : 13 Jan 2023 10:43
Operator : JC/MD
Sample : 01120-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C1144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc