

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
 Data File : VX033716.D
 Acq On : 13 Jan 2023 11:49
 Operator : JC/MD
 Sample : 01120-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
 Title : VOC Analysis

Signal : TIC: VX033716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	36	rVB	11830	10171	1.28%	0.165%
2	1.368	42	46	58	rVB	64820	71048	8.96%	1.155%
3	1.544	74	75	77	rBV2	320	197	0.02%	0.003%
4	1.672	91	96	114	rBV	66548	91077	11.49%	1.481%
5	2.221	185	186	187	rBV	144	65	0.01%	0.001%
6	2.306	194	200	211	rBV	175737	270261	34.09%	4.394%
7	2.465	224	226	228	rBV	159	108	0.01%	0.002%
8	2.514	229	234	240	rVB3	532	873	0.11%	0.014%
9	2.684	260	262	263	rBV2	178	150	0.02%	0.002%
10	2.788	274	279	285	rVB3	1384	2779	0.35%	0.045%
11	2.886	293	295	299	rVB2	104	98	0.01%	0.002%
12	2.928	300	302	304	rBV2	101	90	0.01%	0.001%
13	3.068	323	325	326	rBV	109	83	0.01%	0.001%
14	3.093	326	329	332	rBV3	226	366	0.05%	0.006%
15	3.257	354	356	357	rVV2	103	80	0.01%	0.001%
16	3.300	361	363	364	rBV	103	80	0.01%	0.001%
17	3.318	364	366	371	rVB	228	228	0.03%	0.004%
18	3.428	383	384	385	rBV	154	79	0.01%	0.001%
19	3.446	385	387	389	rVV2	106	109	0.01%	0.002%
20	3.605	412	413	415	rBV	113	83	0.01%	0.001%
21	3.757	436	438	441	rBV	102	127	0.02%	0.002%
22	3.812	446	447	448	rBV	142	89	0.01%	0.001%
23	3.922	463	465	467	rBV2	89	76	0.01%	0.001%
24	3.971	472	473	474	rBV	118	63	0.01%	0.001%
25	4.233	514	516	518	rVB	134	75	0.01%	0.001%
26	4.306	525	528	529	rBV2	132	135	0.02%	0.002%
27	4.465	545	554	568	rBV	47198	153811	19.40%	2.500%
28	4.928	629	630	631	rBV	180	71	0.01%	0.001%
29	5.050	638	650	668	rBV	89014	277469	35.00%	4.511%
30	5.391	704	706	710	rVB	301	260	0.03%	0.004%
31	5.458	715	717	720	rVB2	155	148	0.02%	0.002%
32	5.556	726	733	739	rVB4	957	2275	0.29%	0.037%
33	5.672	751	752	755	rBV2	150	124	0.02%	0.002%
34	5.812	774	775	778	rVB	111	64	0.01%	0.001%
35	5.964	787	800	816	rBV2	264393	792742	100.00%	12.887%
36	6.190	836	837	840	rBV	162	146	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
 Data File : VX033716.D
 Acq On : 13 Jan 2023 11:49
 Operator : JC/MD
 Sample : 01120-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
 Title : VOC Analysis

37	6.458	880	881	885	rVV	139	126	0.02%	0.002%
38	6.604	902	905	906	rBV2	84	97	0.01%	0.002%
39	6.757	920	930	945	rBV	234423	546543	68.94%	8.885%
40	6.976	965	966	974	rVB2	216	246	0.03%	0.004%
41	7.068	979	981	982	rBV	219	98	0.01%	0.002%
42	7.104	982	987	988	rBV2	1041	1337	0.17%	0.022%
43	7.305	1011	1020	1031	rBV	161437	357370	45.08%	5.810%
44	7.604	1068	1069	1072	rBV	137	103	0.01%	0.002%
45	7.872	1111	1113	1115	rBV	83	78	0.01%	0.001%
46	7.897	1115	1117	1118	rVB	143	75	0.01%	0.001%
47	7.927	1118	1122	1130	rBV4	1376	3047	0.38%	0.050%
48	8.202	1166	1167	1169	rBV2	100	96	0.01%	0.002%
49	8.250	1172	1175	1180	rVB2	1060	1290	0.16%	0.021%
50	8.324	1180	1187	1201	rBV	101970	168208	21.22%	2.735%
51	8.452	1206	1208	1209	rVV2	178	131	0.02%	0.002%
52	8.476	1210	1212	1226	rVB4	752	1765	0.22%	0.029%
53	8.647	1233	1240	1250	rBV	434149	662613	83.58%	10.772%
54	8.945	1284	1289	1300	rBV	69089	106642	13.45%	1.734%
55	9.122	1317	1318	1319	rBV	152	79	0.01%	0.001%
56	9.195	1328	1330	1333	rVB	134	94	0.01%	0.002%
57	9.244	1337	1338	1340	rBV	155	91	0.01%	0.001%
58	9.275	1340	1343	1345	rVB2	555	445	0.06%	0.007%
59	9.384	1355	1361	1376	rBV	227650	338499	42.70%	5.503%
60	9.525	1381	1384	1391	rVV3	1313	2546	0.32%	0.041%
61	9.604	1395	1397	1398	rBV2	122	58	0.01%	0.001%
62	9.701	1409	1413	1414	rBV2	471	432	0.05%	0.007%
63	9.762	1422	1423	1425	rBV	114	69	0.01%	0.001%
64	9.787	1425	1427	1431	rVV	157	187	0.02%	0.003%
65	9.890	1442	1444	1446	rBV	131	99	0.01%	0.002%
66	10.055	1465	1471	1483	rVV	461235	643857	81.22%	10.467%
67	10.195	1490	1494	1498	rVB2	565	767	0.10%	0.012%
68	10.262	1503	1505	1506	rVV2	180	129	0.02%	0.002%
69	10.305	1508	1512	1518	rVB2	564	920	0.12%	0.015%
70	10.476	1536	1540	1541	rBV	145	179	0.02%	0.003%
71	10.652	1565	1569	1577	rVB3	689	1376	0.17%	0.022%
72	10.866	1602	1604	1609	rVB	240	215	0.03%	0.003%
73	10.939	1614	1616	1617	rBV	135	97	0.01%	0.002%
74	10.957	1617	1619	1620	rBV2	349	227	0.03%	0.004%
75	11.085	1638	1640	1643	rVB3	320	328	0.04%	0.005%
76	11.189	1652	1657	1671	rBV	272346	357389	45.08%	5.810%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
 Data File : VX033716.D
 Acq On : 13 Jan 2023 11:49
 Operator : JC/MD
 Sample : 01120-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
 Title : VOC Analysis

77	11.457	1695	1701	1703	rBV2	303	479	0.06%	0.008%
78	11.707	1741	1742	1744	rBV	177	138	0.02%	0.002%
79	11.927	1776	1778	1780	rBV	136	91	0.01%	0.001%
80	11.951	1780	1782	1783	rBV	164	95	0.01%	0.002%
81	11.969	1783	1785	1788	rVB2	451	497	0.06%	0.008%
82	12.018	1788	1793	1803	rBV	537125	693615	87.50%	11.276%
83	12.170	1816	1818	1820	rBV2	134	80	0.01%	0.001%
84	12.317	1837	1842	1851	rBV	453766	578919	73.03%	9.411%
85	12.701	1903	1905	1906	rBV2	111	96	0.01%	0.002%
86	12.737	1910	1911	1914	rBV	132	84	0.01%	0.001%
87	12.859	1927	1931	1934	rBV	535	425	0.05%	0.007%
88	12.987	1949	1952	1954	rBV	151	168	0.02%	0.003%
89	13.109	1971	1972	1975	rVV2	191	176	0.02%	0.003%
90	13.170	1981	1982	1987	rBV	171	166	0.02%	0.003%
91	13.493	2033	2035	2037	rVB2	162	92	0.01%	0.001%
92	13.597	2048	2052	2057	rVB3	412	600	0.08%	0.010%
93	13.816	2086	2088	2091	rVB	165	140	0.02%	0.002%
94	13.884	2097	2099	2102	rVB	261	206	0.03%	0.003%
95	13.969	2110	2113	2115	rBV2	341	345	0.04%	0.006%
96	14.042	2123	2125	2128	rBV	237	156	0.02%	0.003%
97	14.127	2137	2139	2143	rVB3	441	554	0.07%	0.009%
98	14.524	2202	2204	2208	rBV3	200	167	0.02%	0.003%
99	14.804	2249	2250	2252	rBV	233	129	0.02%	0.002%
100	15.024	2284	2286	2287	rBV2	295	202	0.03%	0.003%




Sum of corrected areas: 6151268

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
Data File : VX033716.D
Acq On : 13 Jan 2023 11:49
Operator : JC/MD
Sample : 01120-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

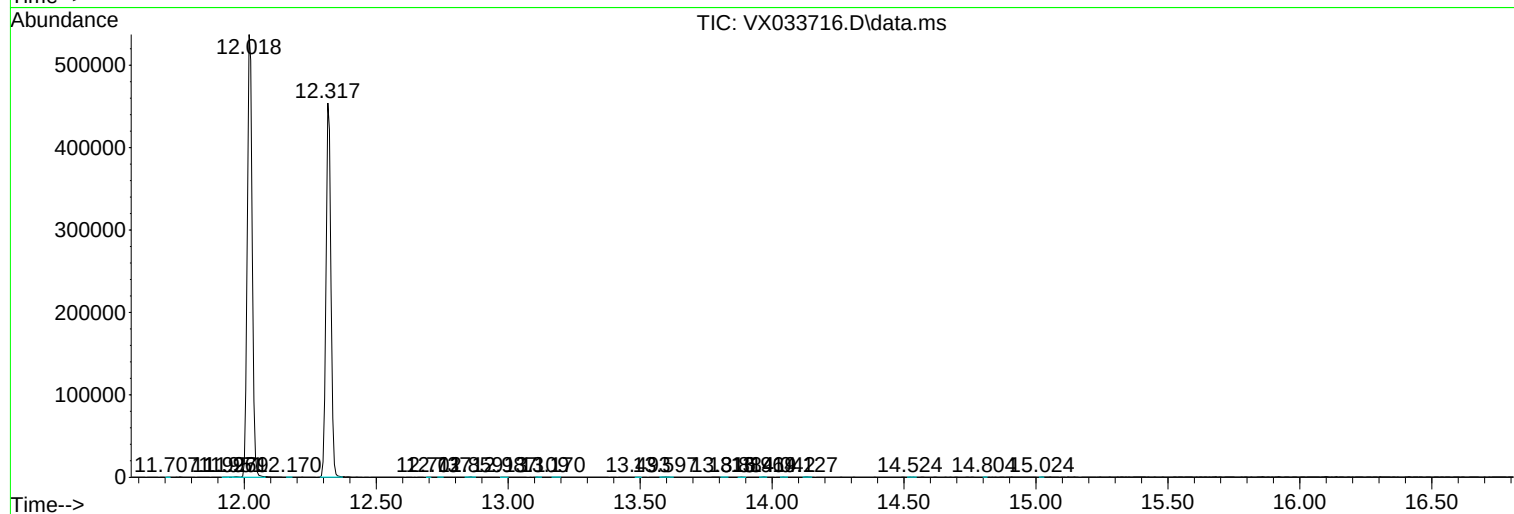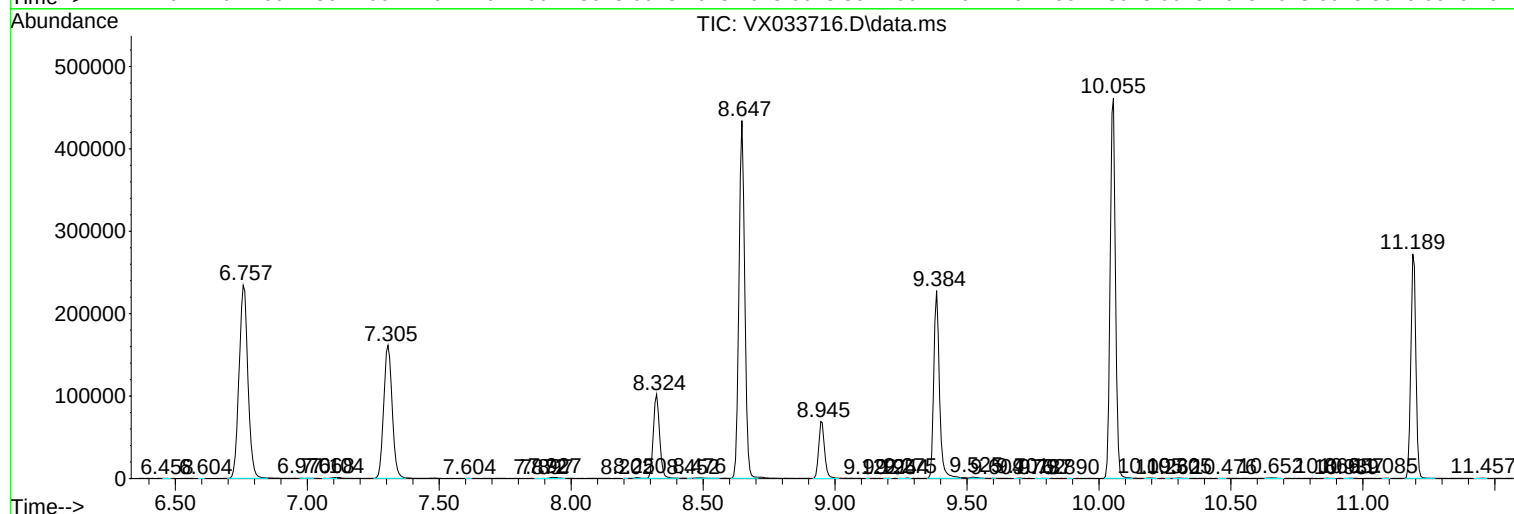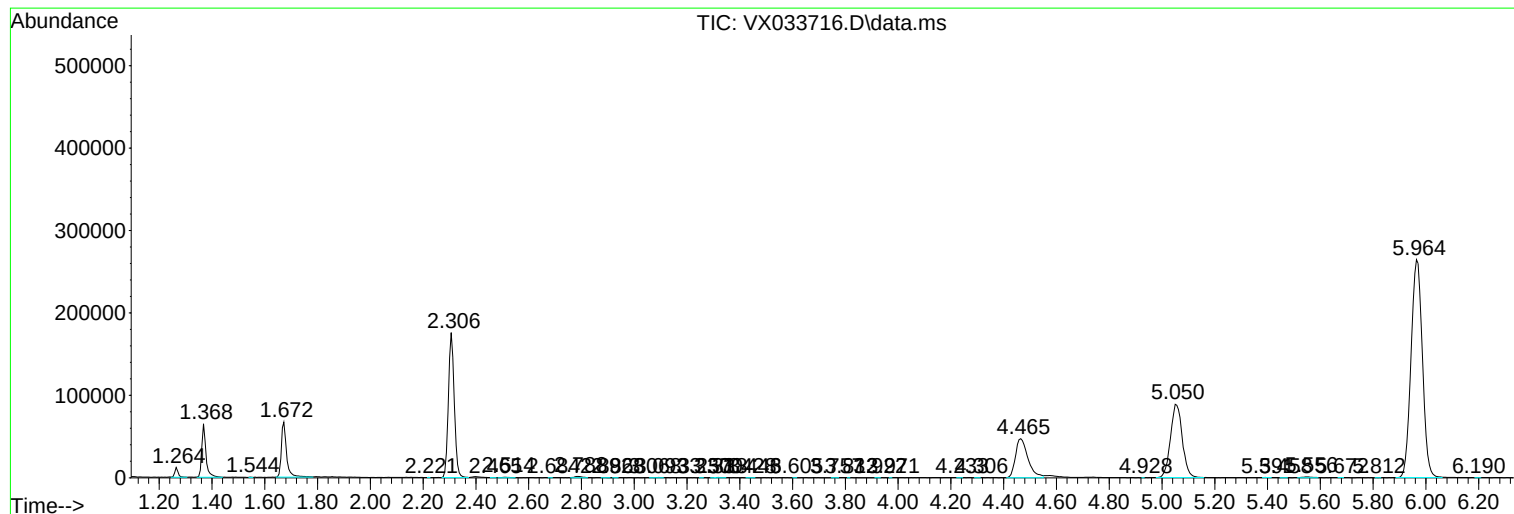

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
Data File : VX033716.D
Acq On : 13 Jan 2023 11:49
Operator : JC/MD
Sample : 01120-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
Data File : VX033716.D
Acq On : 13 Jan 2023 11:49
Operator : JC/MD
Sample : 01120-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc