
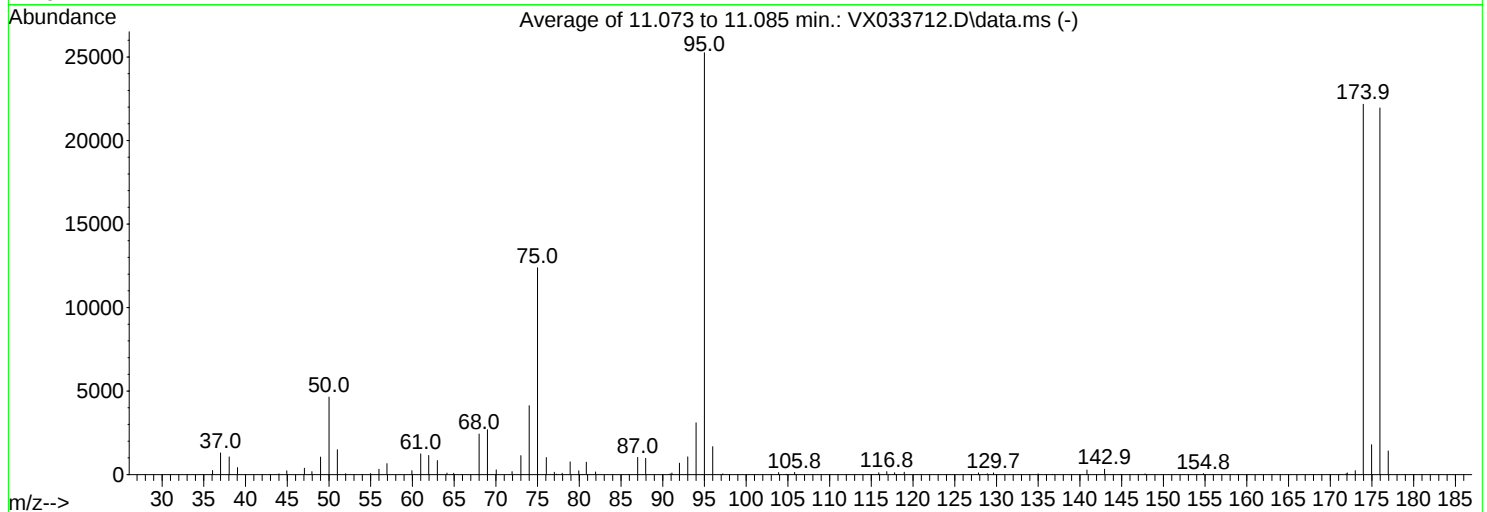


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011323\
 Data File : VX033712.D
 Acq On : 13 Jan 2023 08:23
 Operator : JC/MD
 Sample : BFB604
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB604

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122722WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 28 01:59:02 2022

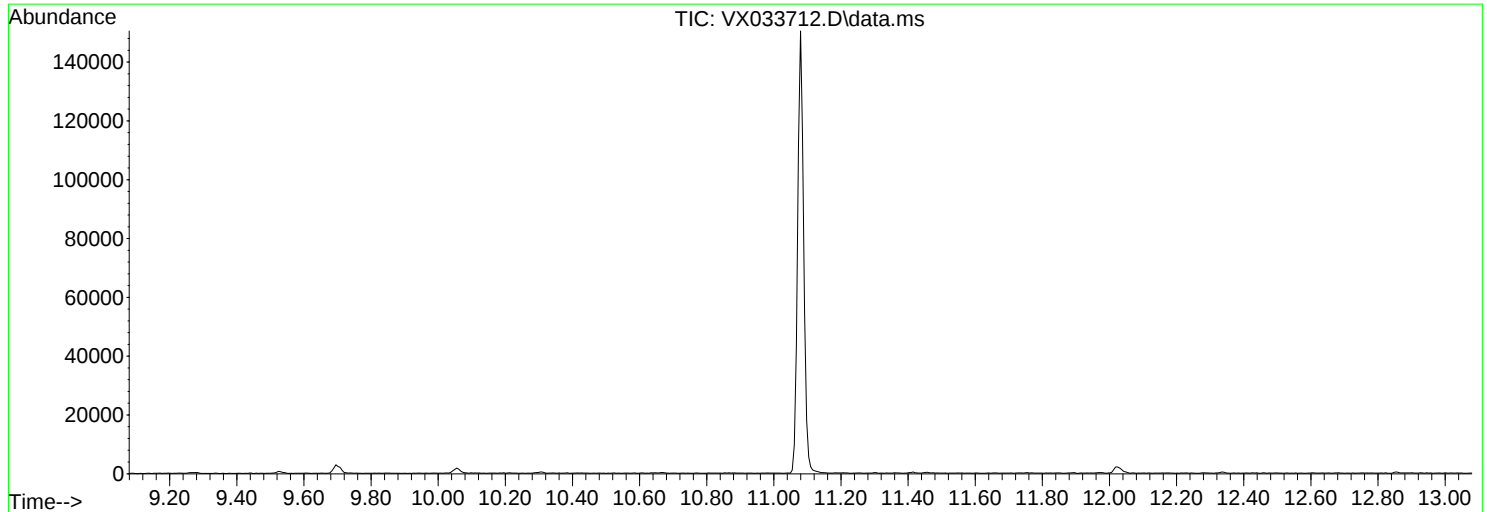

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	4641	PASS
75	95	30	80	49.0	12380	PASS
95	95	100	100	100.0	25253	PASS
96	95	5	9	6.6	1668	PASS
173	174	0.00	2	1.1	239	PASS
174	95	50	120	87.8	22176	PASS
175	174	5	9	8.1	1789	PASS
176	174	95	101	99.0	21947	PASS
177	176	5	9	6.4	1411	PASS

m/z	Abundance
40.00	116.0
44.00	172.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
36.00	322.0
37.00	1458.0
38.10	1054.0
39.10	420.0
40.00	109.0
44.00	184.0
44.90	258.0
47.10	443.0
47.90	167.0
49.00	999.0
50.00	4544.0
51.00	1567.0
52.00	56.0
55.00	57.0
55.90	320.0
57.00	703.0
59.90	227.0
61.00	1178.0
61.90	1084.0
63.00	919.0
64.10	99.0
65.00	64.0
68.00	2381.0
69.00	2730.0
70.00	325.0
72.00	163.0
73.00	1187.0
74.00	4020.0
75.00	11726.0
76.00	980.0
77.00	184.0
77.80	58.0
78.90	840.0
79.90	279.0
80.90	746.0
82.10	124.0
87.00	791.0
88.00	893.0
90.90	117.0
92.00	573.0
93.00	975.0
94.00	2588.0
95.00	23192.0
96.00	1707.0
97.20	56.0
103.90	113.0
105.80	114.0
115.90	98.0
117.00	170.0
117.90	97.0
118.90	95.0
127.90	85.0
129.70	116.0
140.90	210.0
143.00	270.0
171.90	148.0
173.00	220.0
173.90	17200.0
175.00	1513.0
176.00	17240.0
176.90	1016.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
36.10	298.0
37.00	1475.0
38.00	1349.0
39.10	448.0
40.00	108.0
43.90	241.0
45.00	261.0
47.00	482.0
47.90	223.0
49.00	1286.0
50.00	5425.0
51.00	1777.0
52.00	97.0
55.00	117.0
56.00	395.0
57.00	772.0
60.00	260.0
61.00	1394.0
62.00	1456.0
63.00	941.0
64.20	136.0
65.00	113.0
68.00	2800.0
69.00	3113.0
70.00	296.0
72.00	223.0
73.00	1449.0
74.00	4811.0
75.00	15048.0
76.00	1323.0
77.00	234.0
77.90	59.0
78.90	765.0
80.00	229.0
80.90	901.0
81.90	180.0
87.00	1374.0
87.90	1081.0
91.10	124.0
92.00	915.0
93.00	1173.0
94.00	3983.0
95.00	29736.0
96.00	2060.0
97.20	60.0
104.00	116.0
104.80	73.0
105.80	148.0
115.90	119.0
116.80	165.0
117.80	122.0
118.90	159.0
127.80	136.0
128.90	97.0
129.70	114.0
135.00	61.0
140.80	323.0
142.90	371.0
147.80	77.0
154.80	111.0
172.10	136.0
173.00	319.0
174.00	26928.0
175.00	1982.0
175.90	26176.0
176.90	1866.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604

m/z	Abundance
36.10	109.0
37.10	948.0
38.10	785.0
39.00	379.0
40.00	151.0
44.10	236.0
44.90	155.0
47.00	224.0
48.00	138.0
49.00	861.0
50.00	3953.0
51.00	1139.0
56.10	257.0
56.90	500.0
60.00	213.0
61.00	1138.0
62.00	884.0
63.00	652.0
64.20	51.0
64.90	72.0
68.00	2104.0
69.00	2212.0
70.10	232.0
71.90	144.0
72.90	776.0
74.00	3546.0
75.00	10366.0
76.10	768.0
77.30	75.0
78.00	121.0
78.90	694.0
79.90	174.0
80.80	584.0
81.90	183.0
87.00	927.0
87.90	936.0
91.10	157.0
92.00	565.0
93.00	1037.0
94.00	2731.0
95.00	22832.0
96.00	1238.0
103.80	120.0
105.80	135.0
115.90	105.0
116.80	186.0
117.70	110.0
119.00	150.0
127.80	76.0
128.90	57.0
129.60	86.0
135.00	61.0
136.70	58.0
140.90	291.0
142.90	336.0
144.90	54.0
147.80	59.0
154.80	86.0
172.00	154.0
172.90	179.0
174.00	22400.0
174.90	1871.0
176.00	22424.0
177.00	1350.0

Instrument :
MSVOA_X
ClientSampleId :
BFB604