


Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX020918\
Data File : VX000042.D
Acq On : 09 Feb 2018 14:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X020918W.M
Title : SW846 8260
Last Update : Fri Feb 09 23:01:05 2018

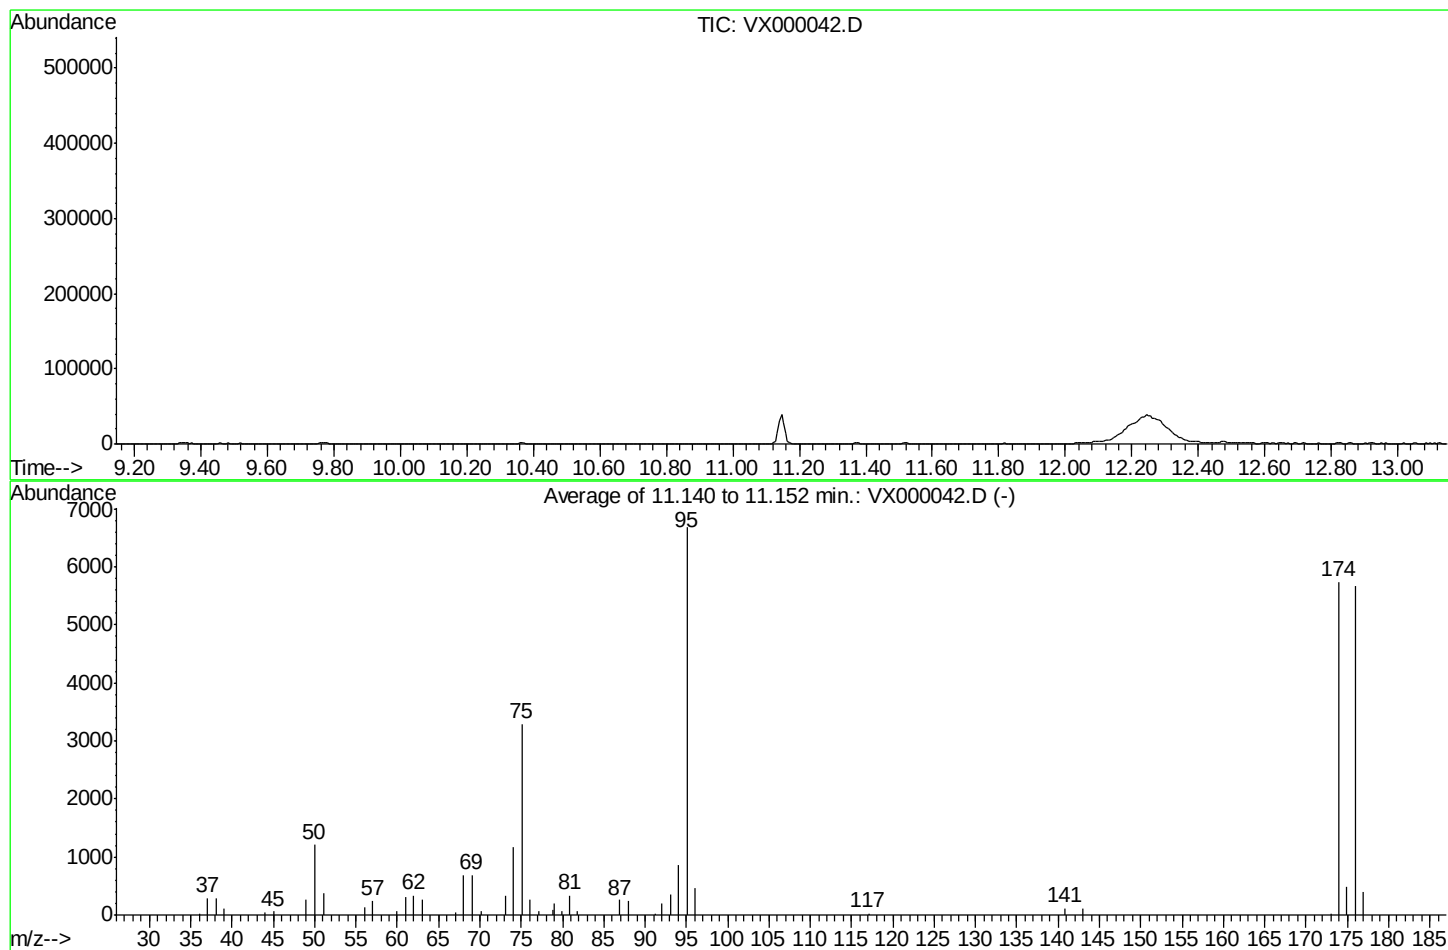

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	1203	PASS
75	95	30	60	49.4	3297	PASS
95	95	100	100	100.0	6679	PASS
96	95	5	9	7.0	470	PASS
173	174	0.00	2	0.3	20	PASS
174	95	50	100	85.9	5736	PASS
175	174	5	9	8.4	481	PASS
176	174	95	101	98.9	5675	PASS
177	176	5	9	7.1	402	PASS