


Data Path : W:\HPCHEM1\MSVOA X\Data\VX021218\
Data File : VX000057.D
Acq On : 12 Feb 2018 09:04
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X020918W.M
Title : SW846 8260
Last Update : Fri Feb 09 23:01:05 2018

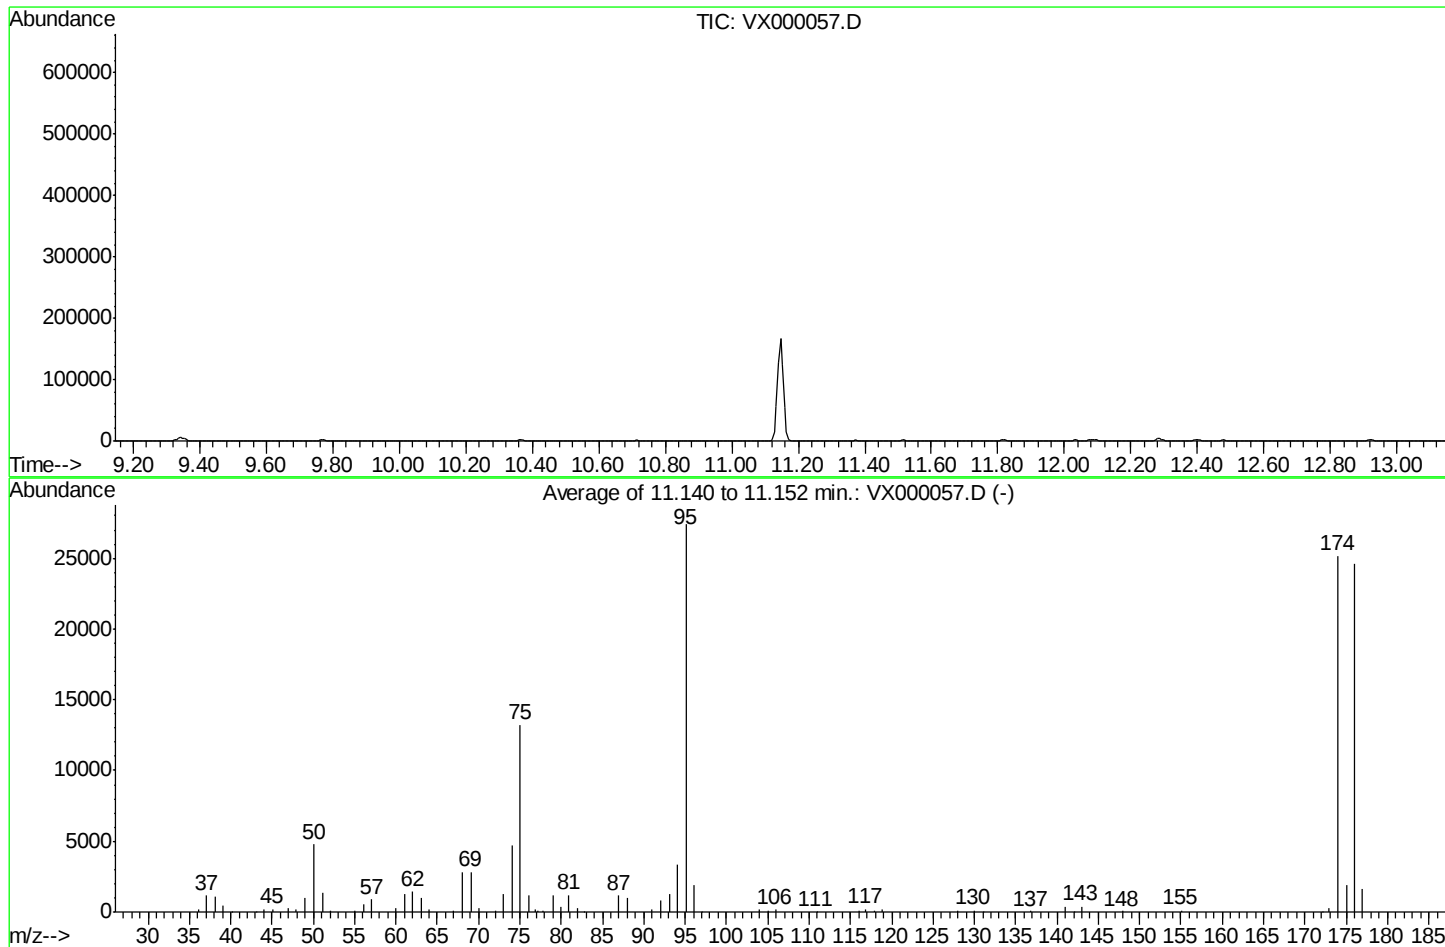

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4787	PASS
75	95	30	60	48.4	13252	PASS
95	95	100	100	100.0	27394	PASS
96	95	5	9	6.9	1900	PASS
173	174	0.00	2	1.0	257	PASS
174	95	50	100	91.9	25186	PASS
175	174	5	9	7.4	1872	PASS
176	174	95	101	97.6	24576	PASS
177	176	5	9	6.6	1628	PASS