


Data Path : W:\HPCHEM1\MSVOA X\Data\VX021418\
Data File : VX000085.D
Acq On : 14 Feb 2018 12:32
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X021418W.M
Title : SW846 8260
Last Update : Thu Feb 15 12:46:41 2018

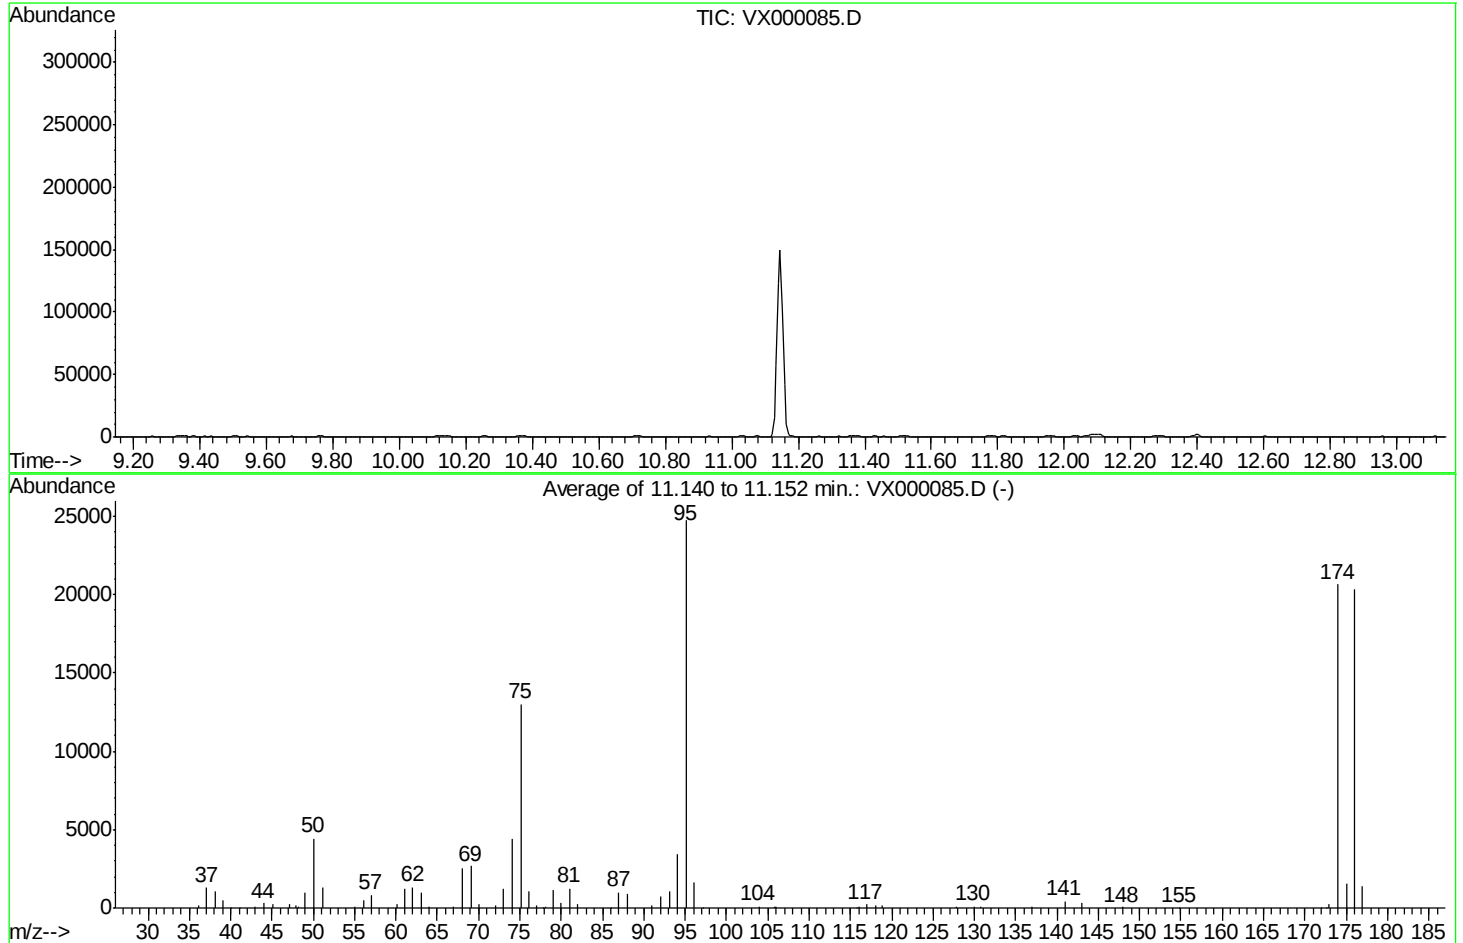

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	4428	PASS
75	95	30	60	52.6	13017	PASS
95	95	100	100	100.0	24725	PASS
96	95	5	9	6.7	1663	PASS
173	174	0.00	2	1.1	222	PASS
174	95	50	100	83.4	20629	PASS
175	174	5	9	7.6	1570	PASS
176	174	95	101	98.5	20322	PASS
177	176	5	9	7.0	1422	PASS