


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX021518\  
Data File : VX000095.D  
Acq On : 15 Feb 2018 09:13  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA\_X\METHOD\82X021418W.M  
Title : SW846 8260  
Last Update : Thu Feb 15 12:46:41 2018

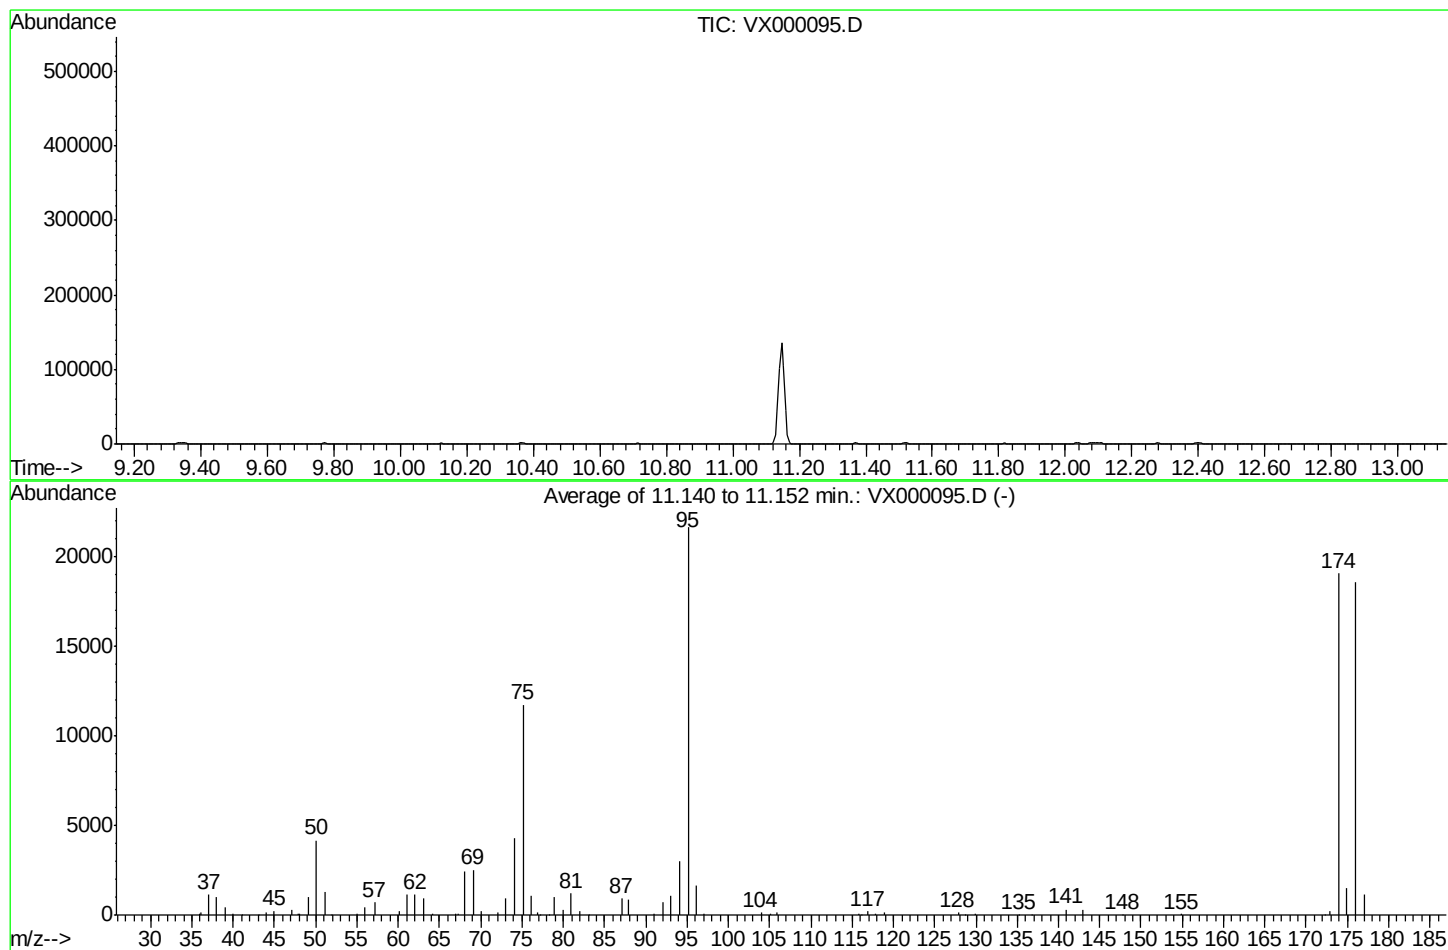

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1725

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.2      | 4149    | PASS             |
| 75          | 95           | 30           | 60           | 54.3      | 11754   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 21664   | PASS             |
| 96          | 95           | 5            | 9            | 7.5       | 1623    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.0       | 200     | PASS             |
| 174         | 95           | 50           | 100          | 88.1      | 19084   | PASS             |
| 175         | 174          | 5            | 9            | 7.9       | 1499    | PASS             |
| 176         | 174          | 95           | 101          | 97.3      | 18568   | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 1164    | PASS             |