


Data Path : W:\HPCHEM1\MSVOA X\Data\VX022018\
Data File : VX000103.D
Acq On : 20 Feb 2018 11:55
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X022018W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Feb 21 06:17:26 2018

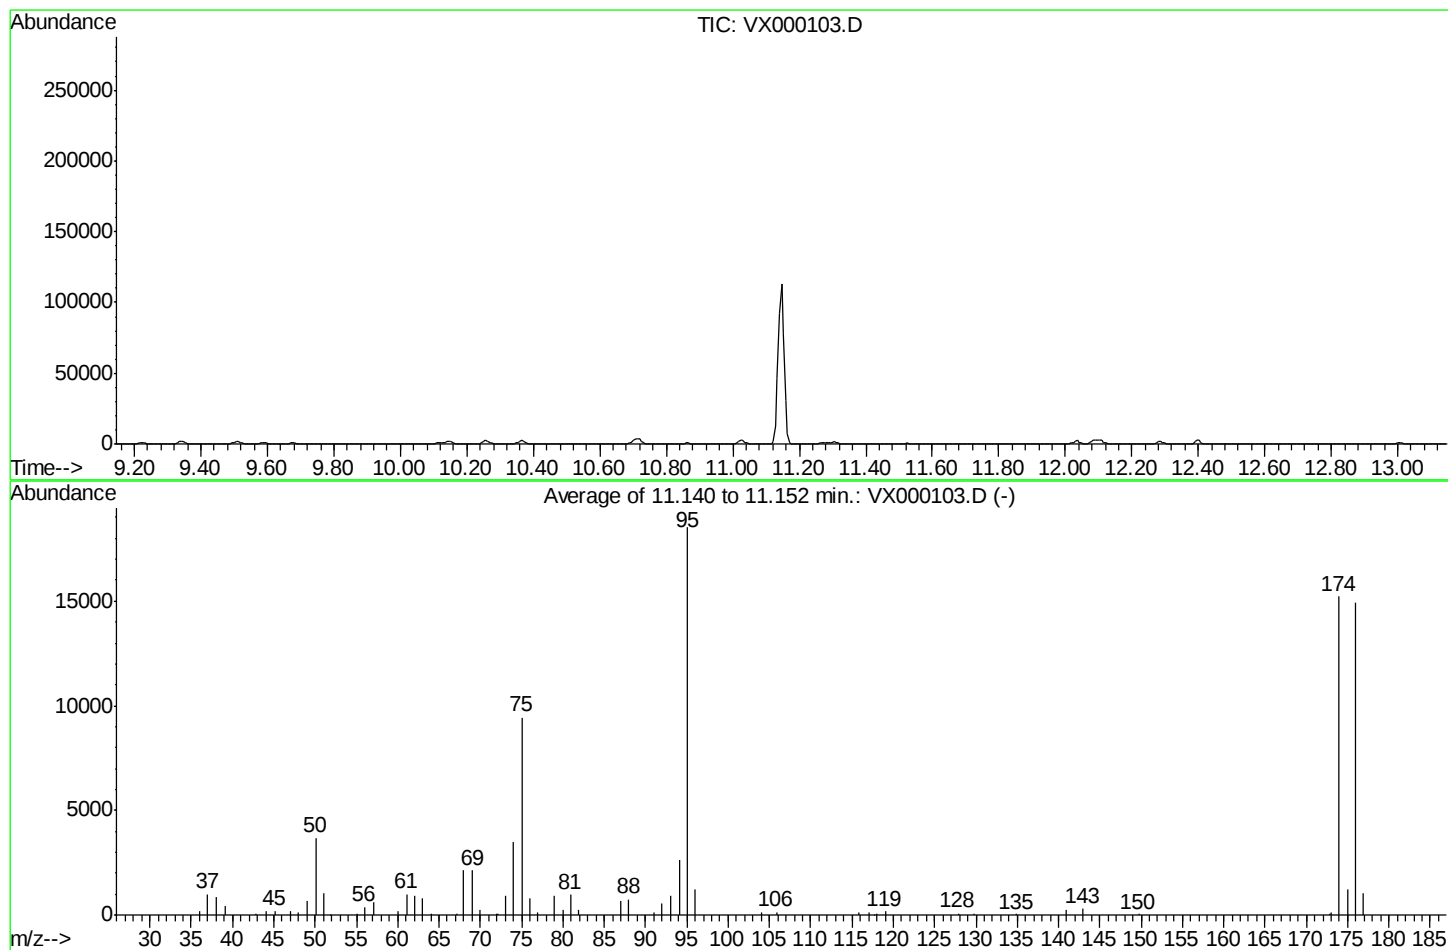

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1726

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	3676	PASS
75	95	30	60	50.9	9438	PASS
95	95	100	100	100.0	18528	PASS
96	95	5	9	6.5	1202	PASS
173	174	0.00	2	0.6	94	PASS
174	95	50	100	82.1	15220	PASS
175	174	5	9	7.9	1202	PASS
176	174	95	101	98.2	14952	PASS
177	176	5	9	6.8	1014	PASS