


Data Path : W:\HPCHEM1\MSVOA_X\Data\VX022318\
Data File : VX000135.D
Acq On : 23 Feb 2018 11:08
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\624X022018W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Feb 21 06:17:26 2018

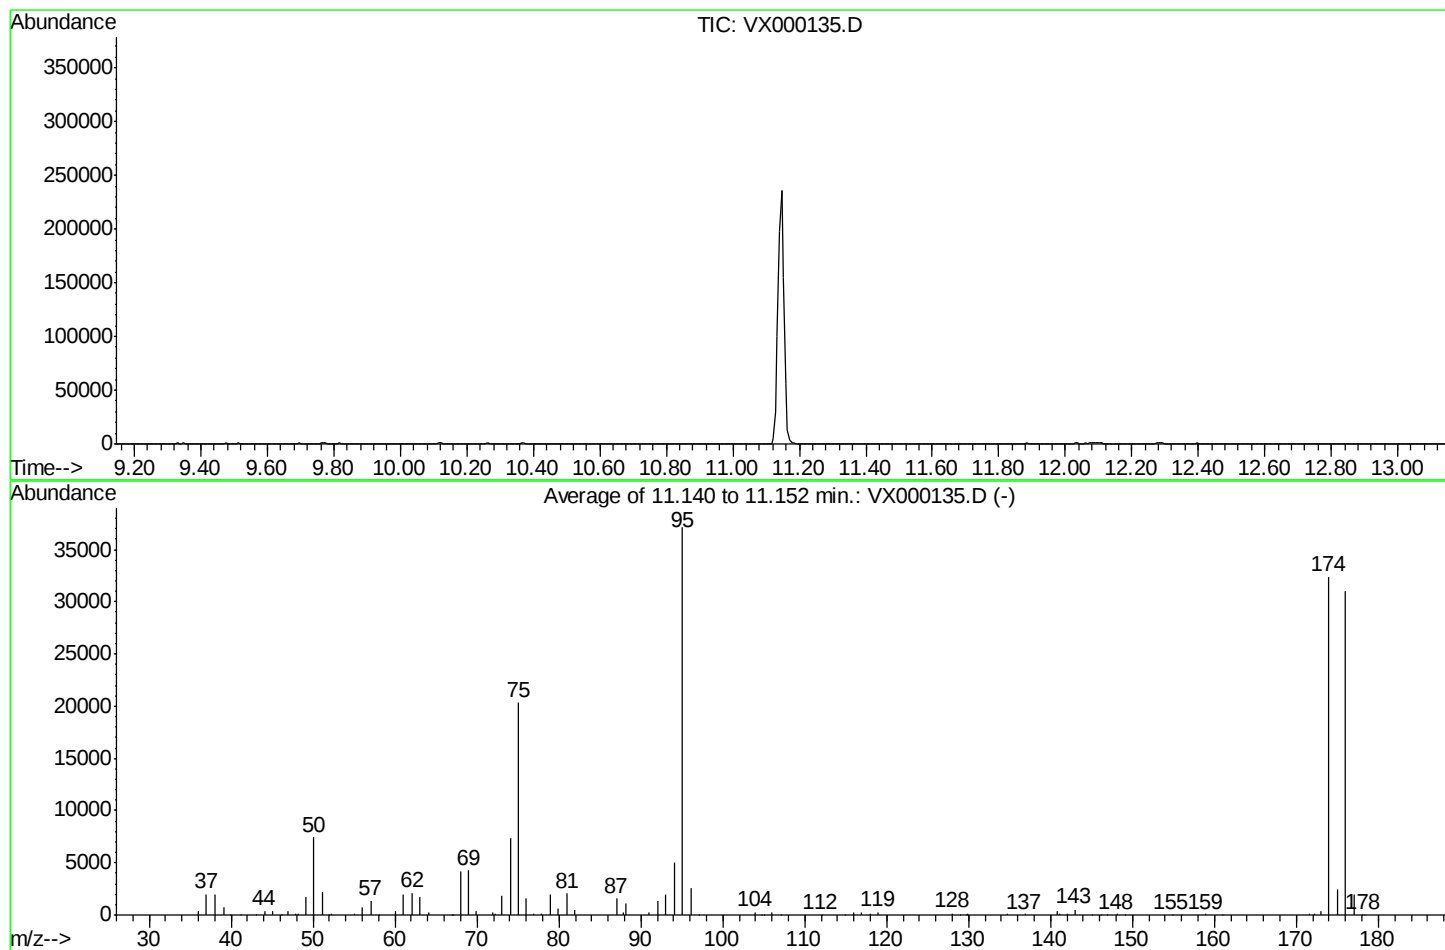

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	7437	PASS
75	95	30	60	54.8	20337	PASS
95	95	100	100	100.0	37130	PASS
96	95	5	9	6.8	2528	PASS
173	174	0.00	2	1.2	400	PASS
174	95	50	100	87.2	32378	PASS
175	174	5	9	7.6	2471	PASS
176	174	95	101	95.7	30997	PASS
177	176	5	9	6.2	1930	PASS