


Data Path : W:\HPCHEM1\MSVOA X\Data\VX022718\
 Data File : VX000141.D
 Acq On : 27 Feb 2018 09:32
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X021418W.M
 Title : SW846 8260
 Last Update : Thu Feb 15 12:46:41 2018

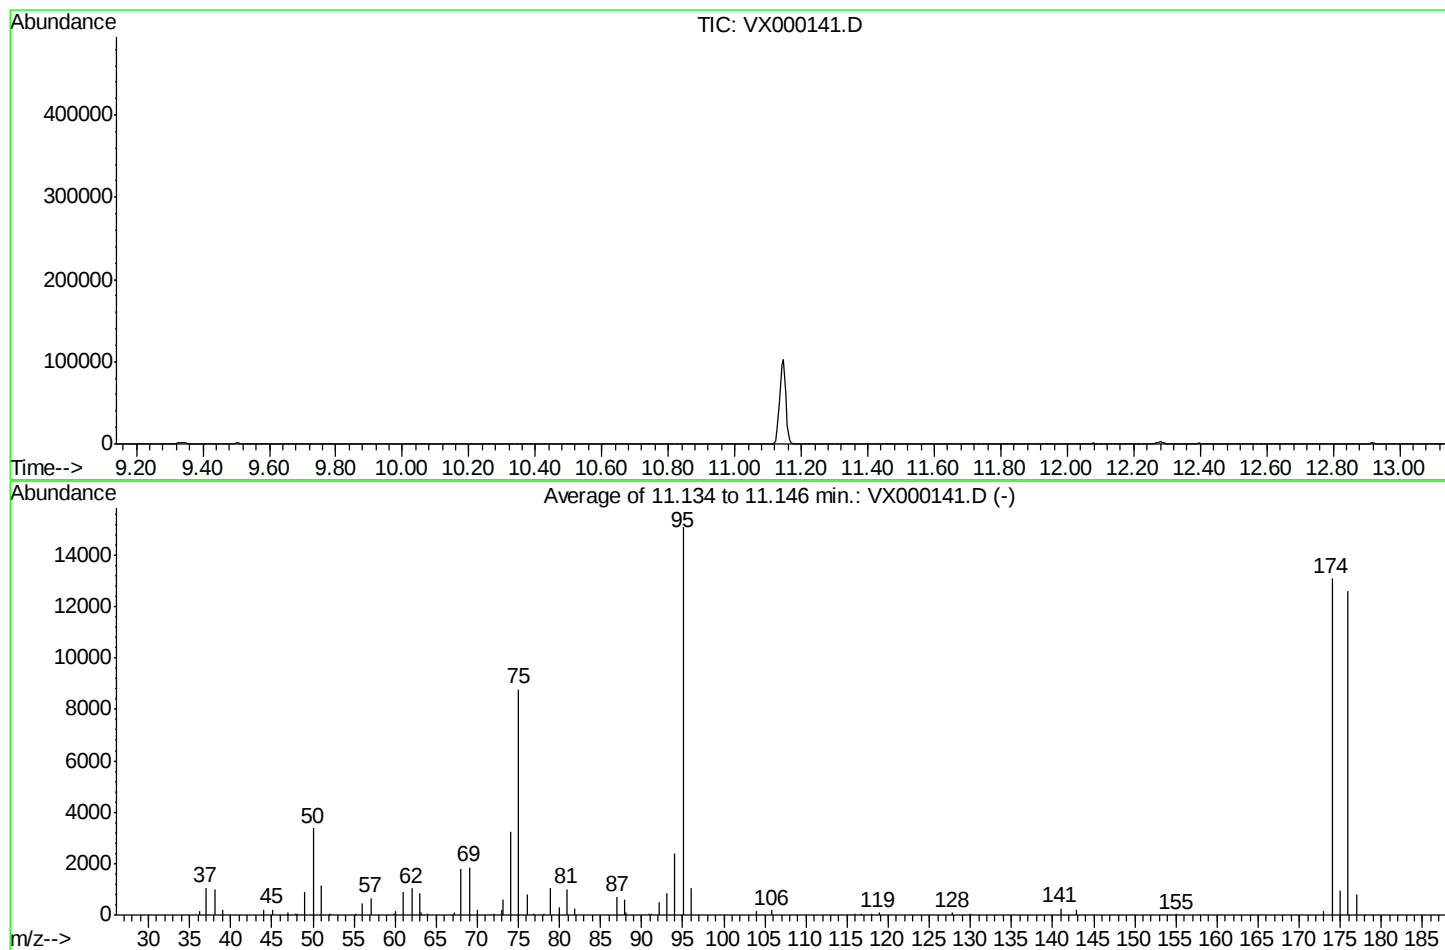

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	3383	PASS
75	95	30	60	58.2	8776	PASS
95	95	100	100	100.0	15084	PASS
96	95	5	9	6.9	1044	PASS
173	174	0.00	2	1.0	136	PASS
174	95	50	100	86.7	13076	PASS
175	174	5	9	7.2	937	PASS
176	174	95	101	96.3	12596	PASS
177	176	5	9	6.2	778	PASS