


Data Path : W:\HPCHEM1\MSVOA X\Data\VX022818\
Data File : VX000159.D
Acq On : 28 Feb 2018 10:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X021418W.M
Title : SW846 8260
Last Update : Thu Feb 15 12:46:41 2018

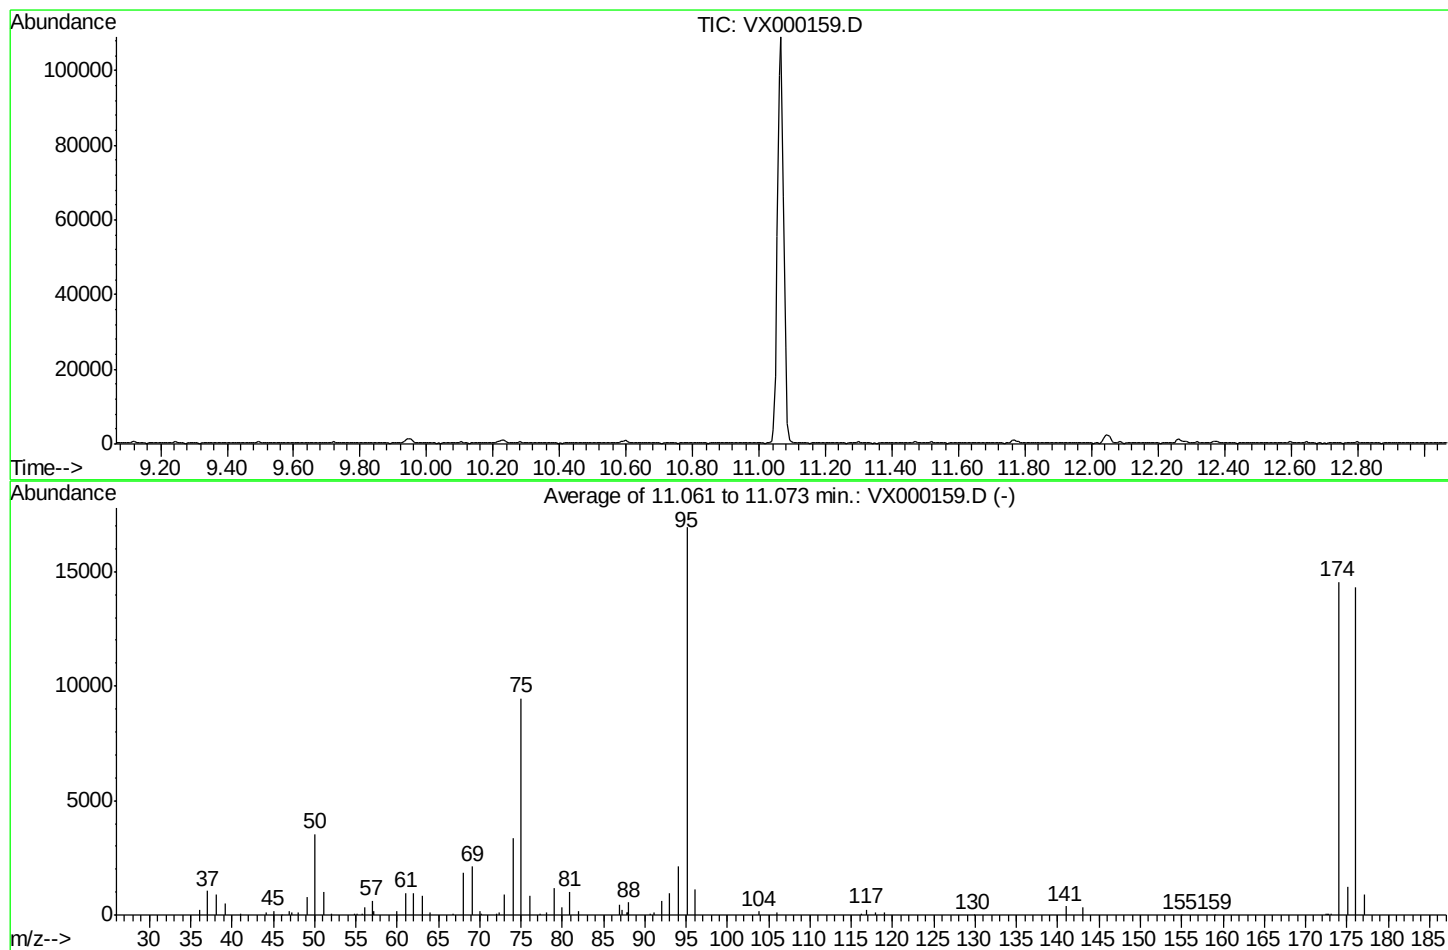

AutoFind: Scans 1718, 1719, 1720; Background Corrected with Scan 1711

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	3552	PASS
75	95	30	60	55.9	9473	PASS
95	95	100	100	100.0	16940	PASS
96	95	5	9	6.7	1137	PASS
173	174	0.00	2	0.4	65	PASS
174	95	50	100	85.9	14558	PASS
175	174	5	9	8.4	1228	PASS
176	174	95	101	98.4	14326	PASS
177	176	5	9	6.4	921	PASS