


Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX030218\
Data File : VX000188.D
Acq On : 02 Mar 2018 09:11
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X021418W.M
Title : SW846 8260
Last Update : Thu Feb 15 12:46:41 2018

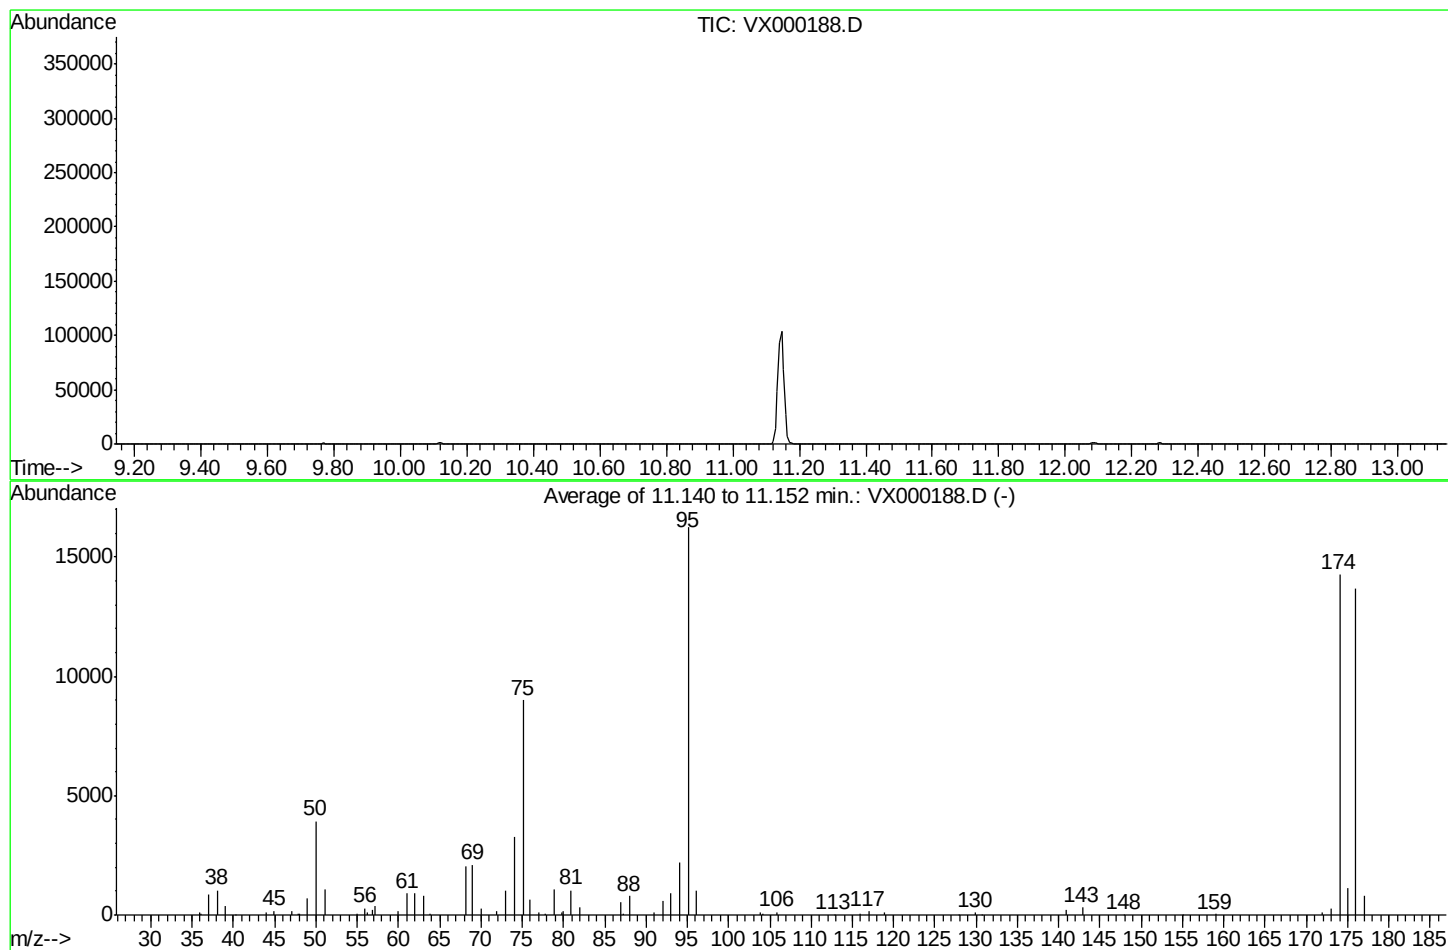

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	3930	PASS
75	95	30	60	55.5	9013	PASS
95	95	100	100	100.0	16250	PASS
96	95	5	9	6.2	1015	PASS
173	174	0.00	2	1.8	251	PASS
174	95	50	100	87.7	14255	PASS
175	174	5	9	7.8	1113	PASS
176	174	95	101	96.0	13684	PASS
177	176	5	9	5.9	807	PASS