


Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX030918\
 Data File : VX000248.D
 Acq On : 09 Mar 2018 08:42
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X030718W.M
 Title : SW846 8260
 Last Update : Thu Mar 08 02:15:47 2018

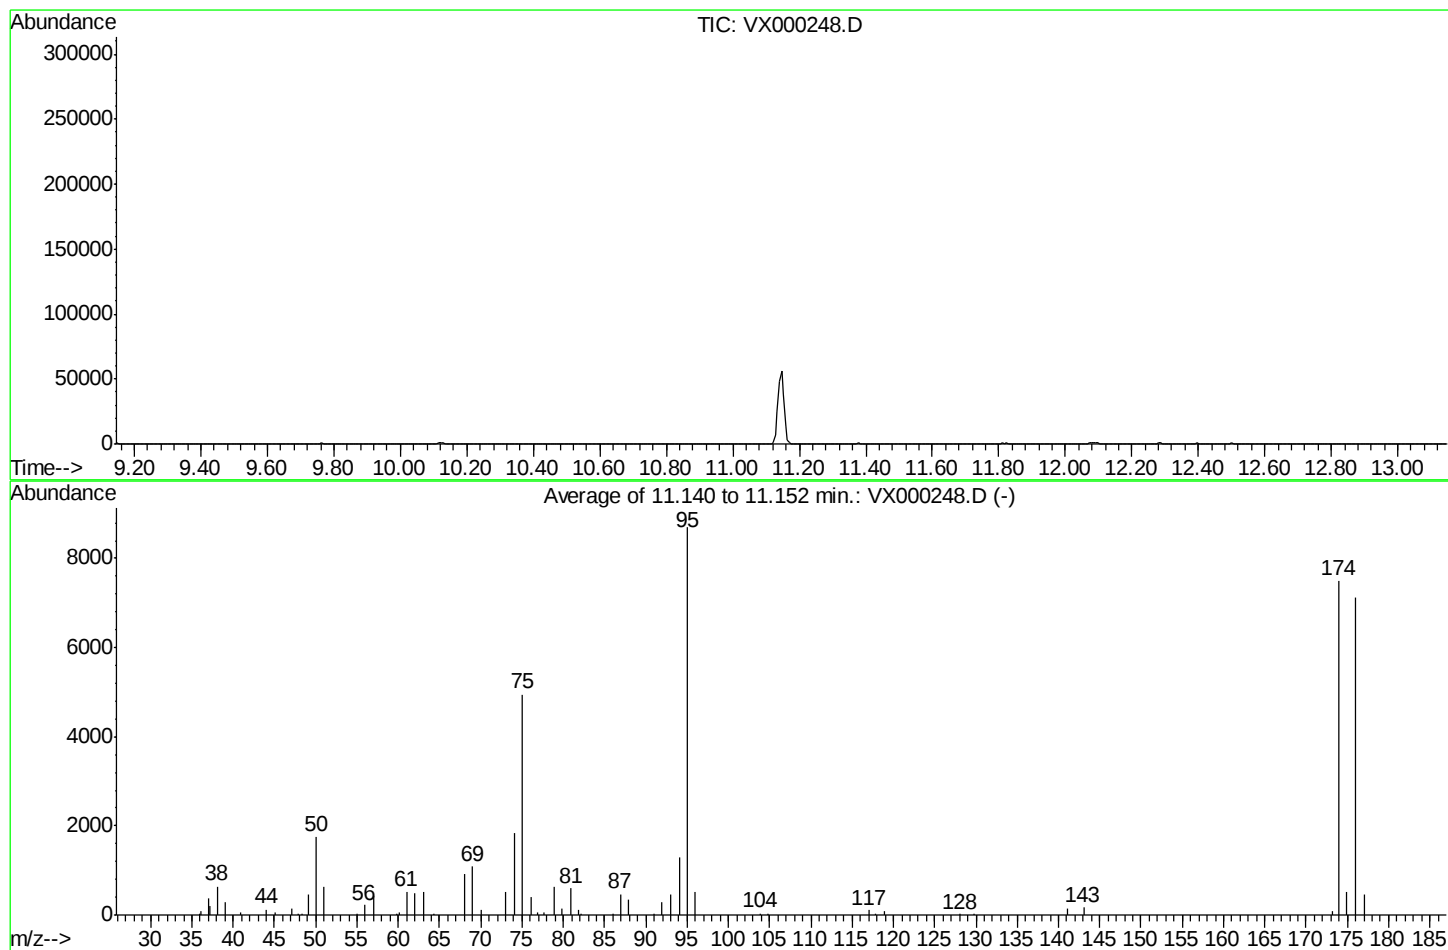

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	1752	PASS
75	95	30	60	56.9	4949	PASS
95	95	100	100	100.0	8697	PASS
96	95	5	9	6.1	529	PASS
173	174	0.00	2	1.0	73	PASS
174	95	50	100	86.3	7506	PASS
175	174	5	9	6.7	506	PASS
176	174	95	101	95.1	7136	PASS
177	176	5	9	6.4	454	PASS