


Data Path : W:\HPCHEM1\MSVOA X\Data\VX031418\
Data File : VX000314.D
Acq On : 14 Mar 2018 15:04
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X031418W.M
Title : SW846 8260
Last Update : Thu Mar 15 03:39:21 2018

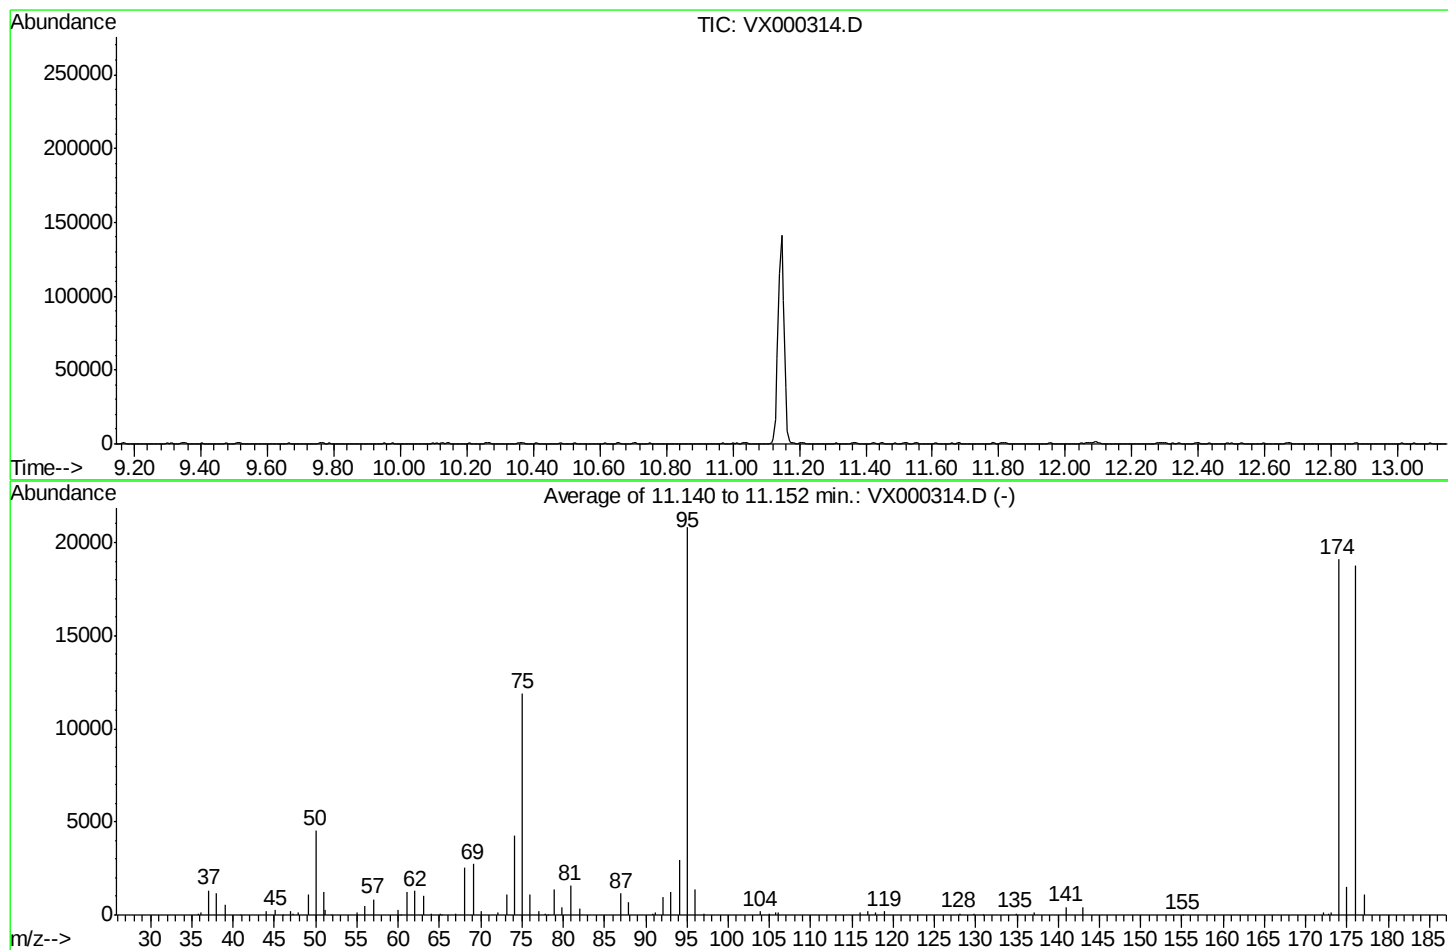

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	4533	PASS
75	95	30	60	57.1	11885	PASS
95	95	100	100	100.0	20813	PASS
96	95	5	9	6.7	1402	PASS
173	174	0.00	2	0.8	157	PASS
174	95	50	100	91.8	19104	PASS
175	174	5	9	7.9	1504	PASS
176	174	95	101	98.1	18738	PASS
177	176	5	9	5.8	1089	PASS