


Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX031618\
Data File : VX000342.D
Acq On : 16 Mar 2018 11:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X031418W.M
Title : SW846 8260
Last Update : Thu Mar 15 03:39:21 2018

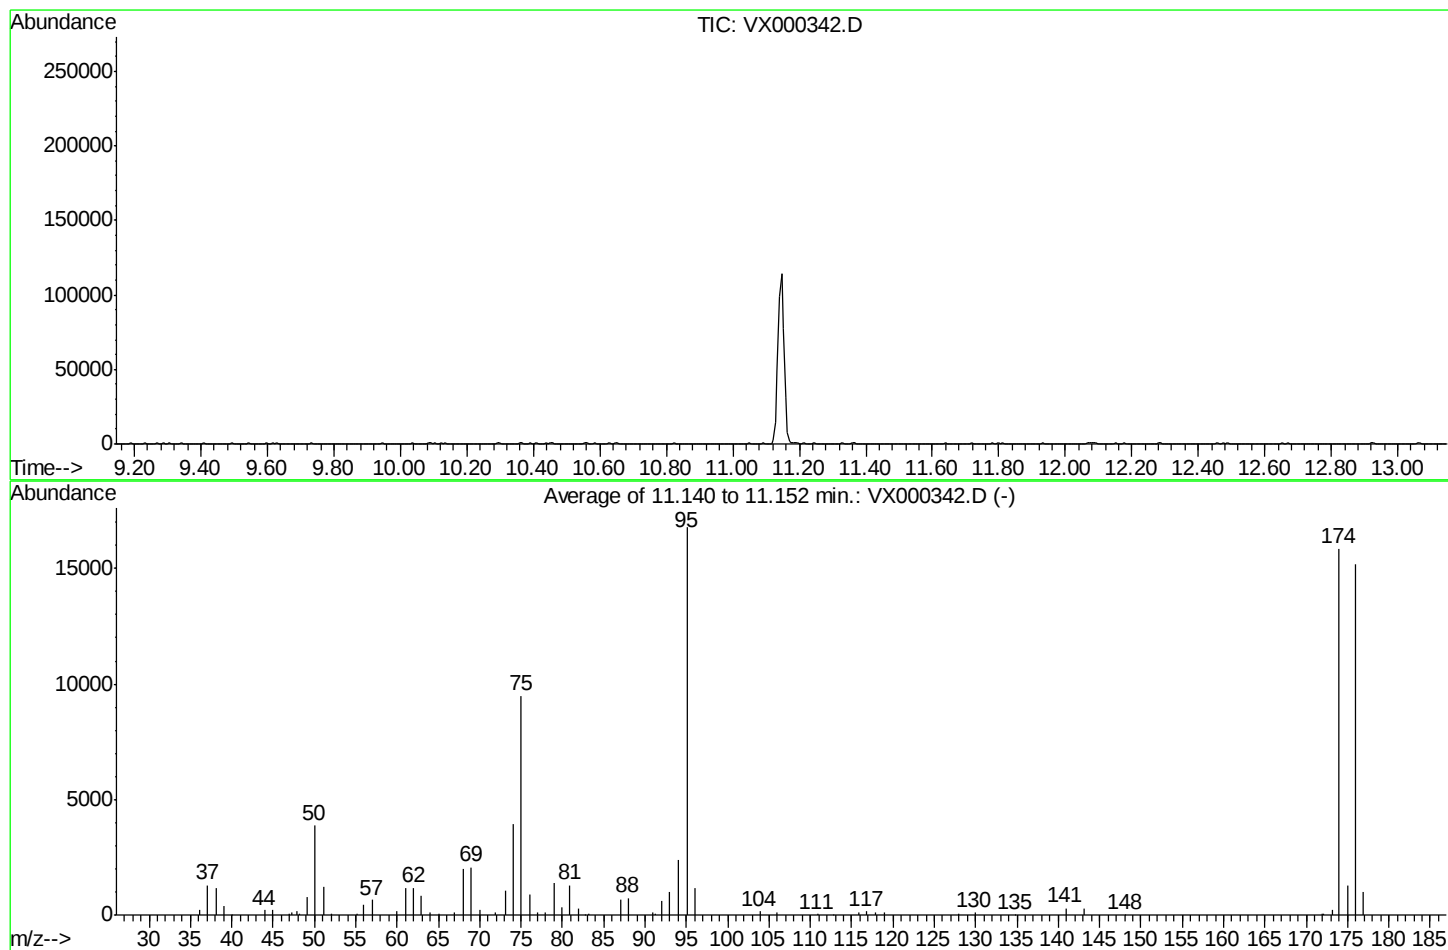

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	3854	PASS
75	95	30	60	56.5	9490	PASS
95	95	100	100	100.0	16783	PASS
96	95	5	9	7.0	1170	PASS
173	174	0.00	2	1.4	215	PASS
174	95	50	100	94.5	15854	PASS
175	174	5	9	8.1	1282	PASS
176	174	95	101	95.9	15203	PASS
177	176	5	9	6.4	974	PASS