




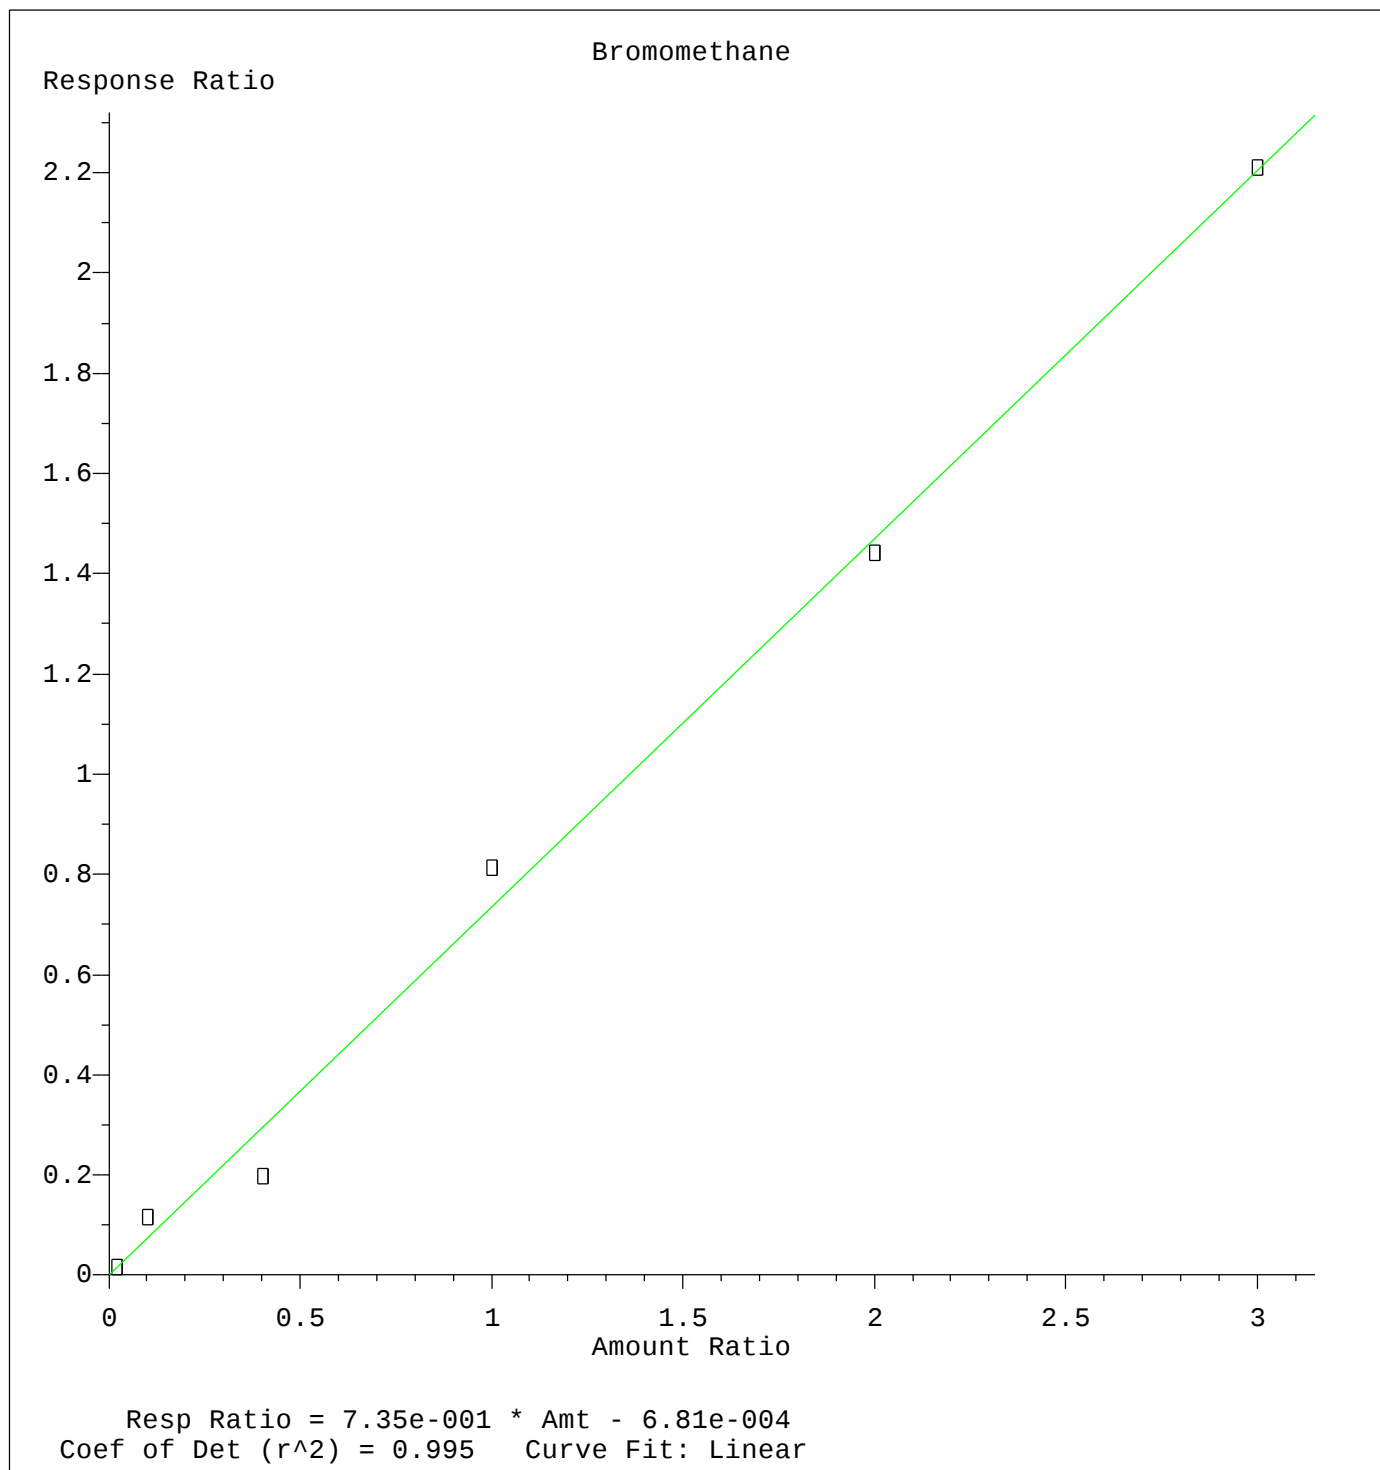

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018

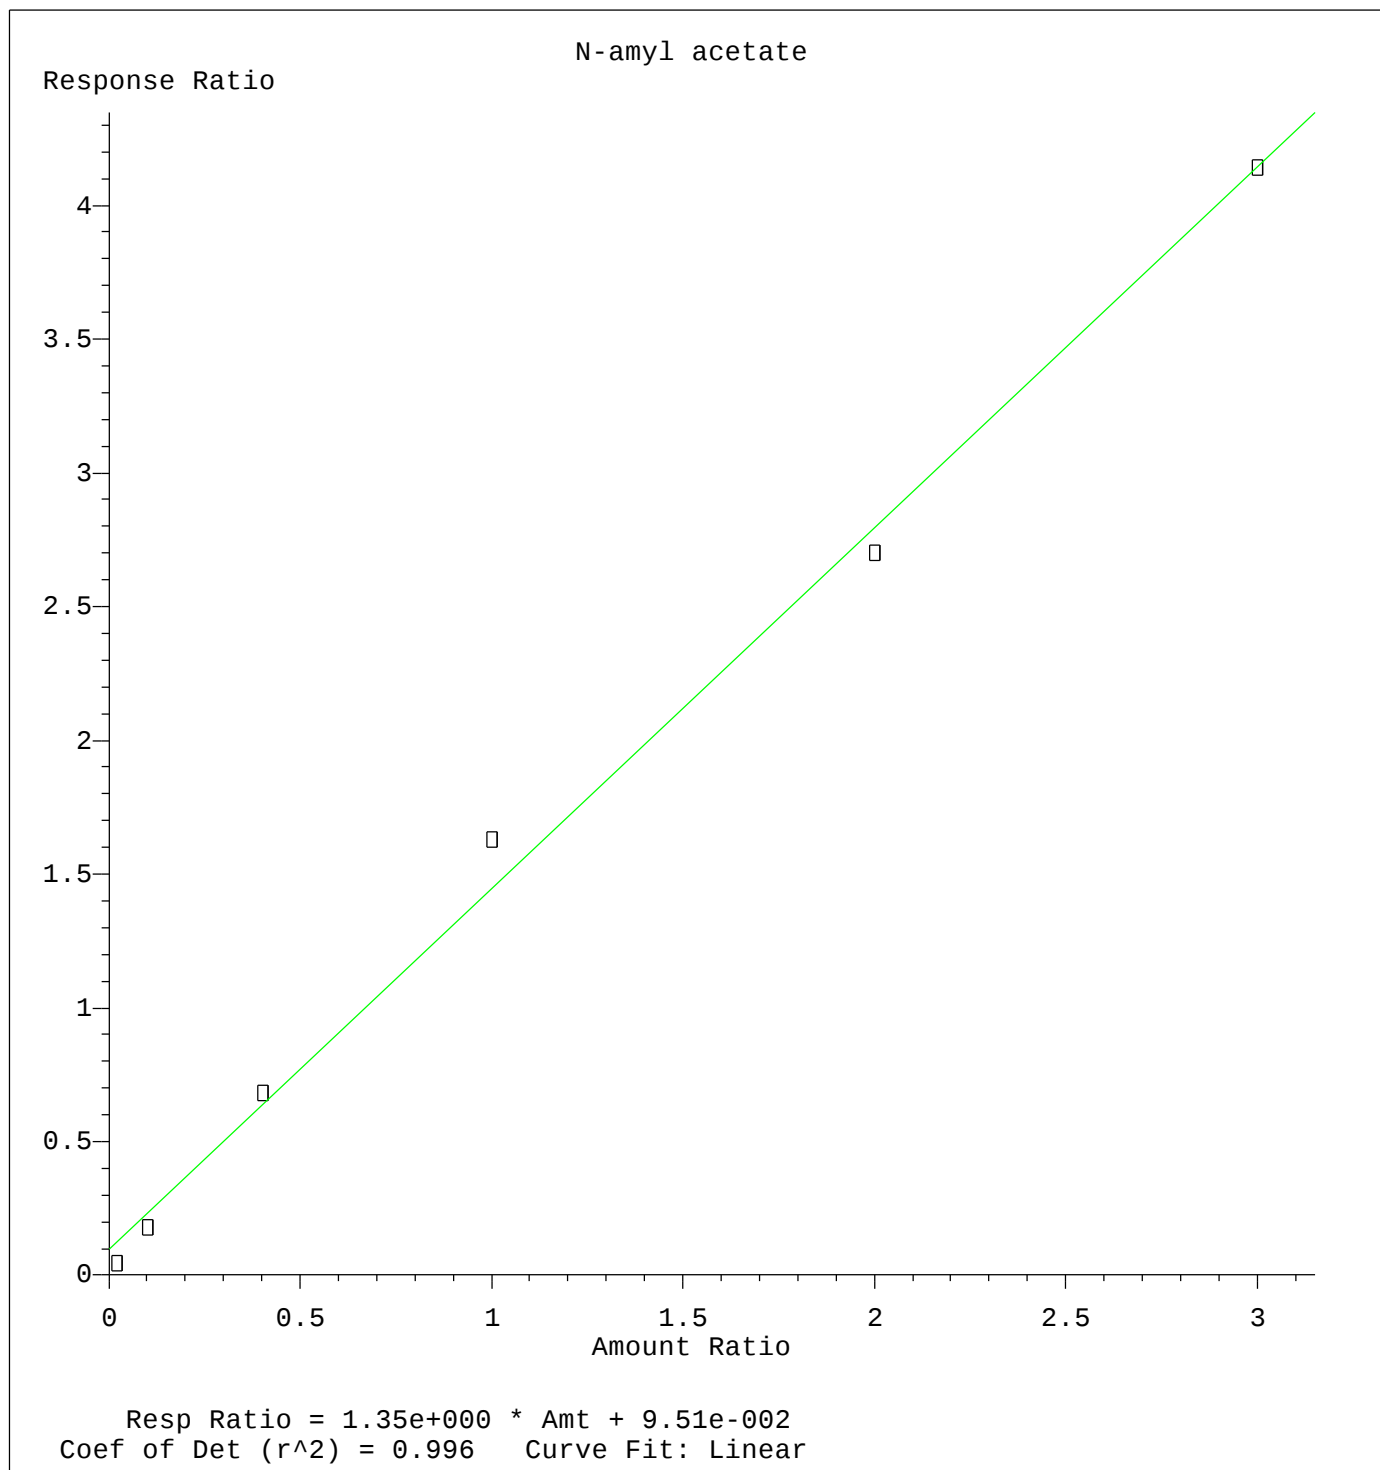


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018

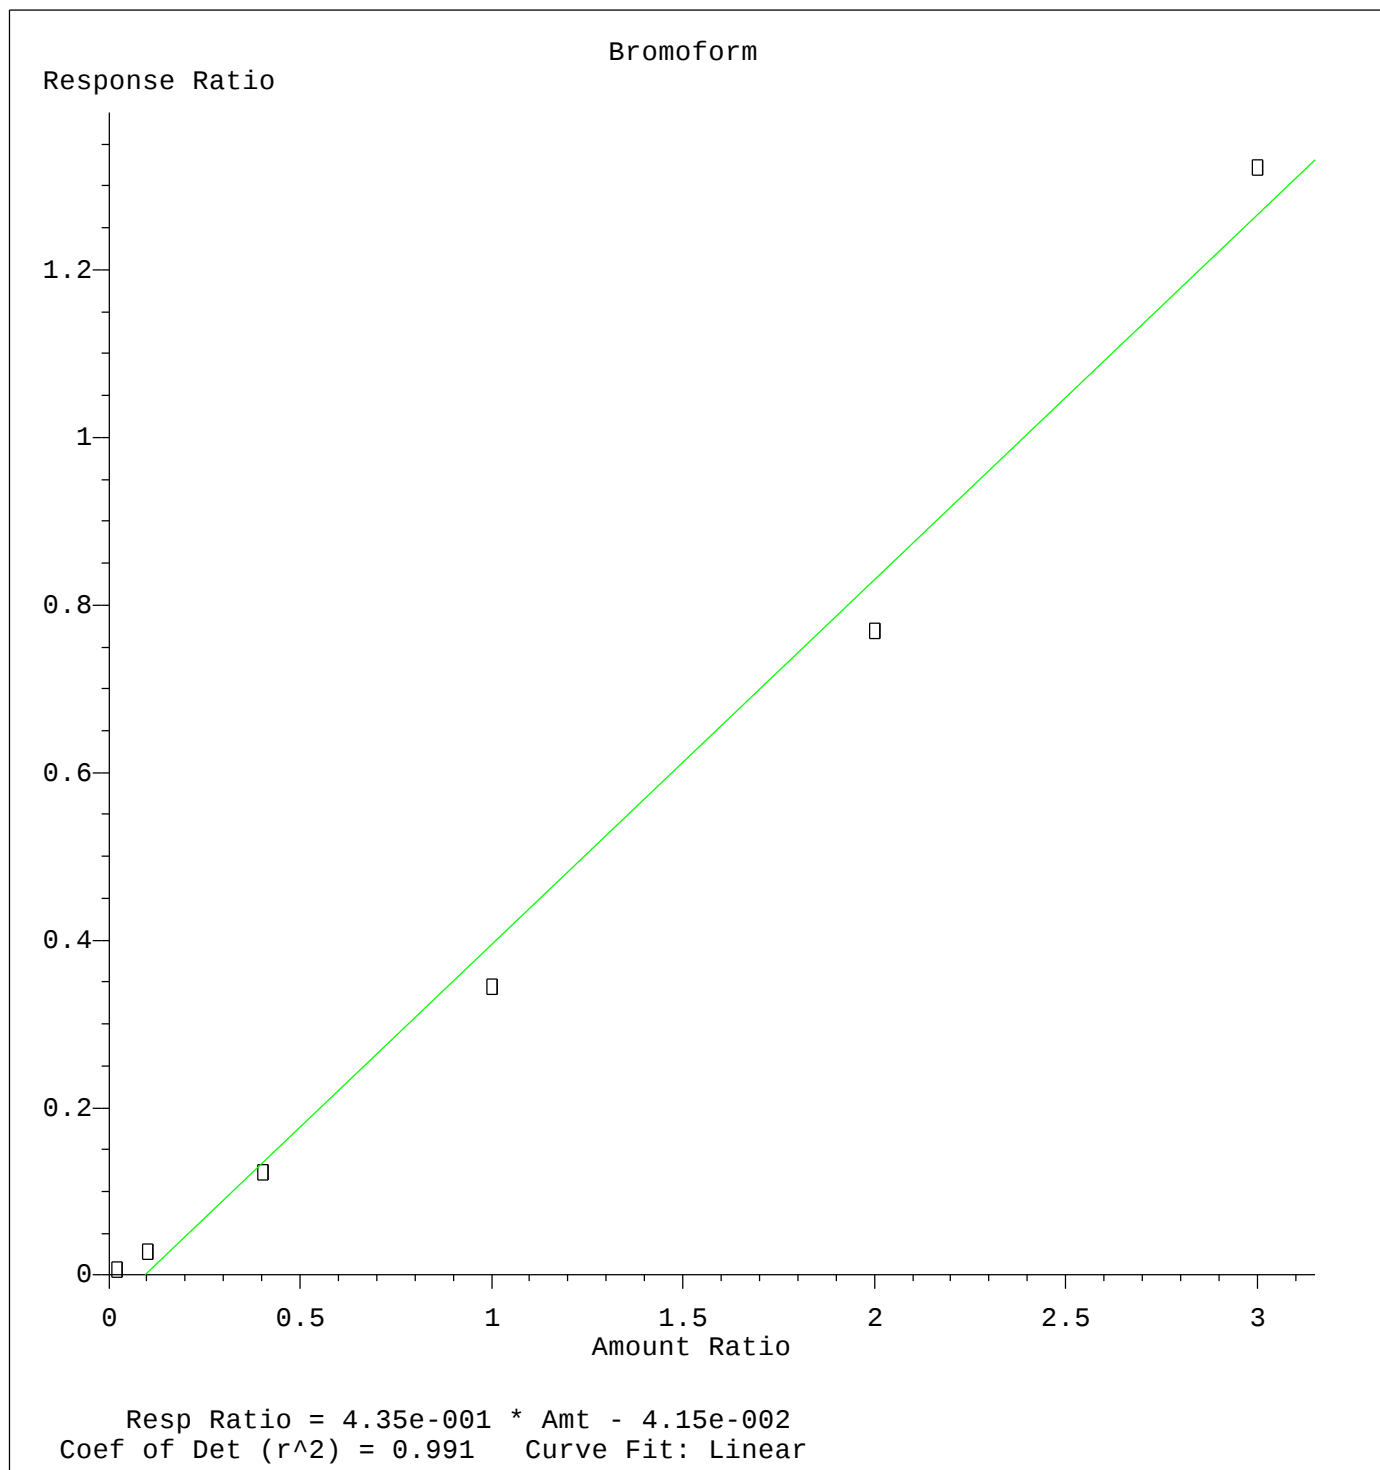

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018


4-Bromofluorobenzene

Response Ratio

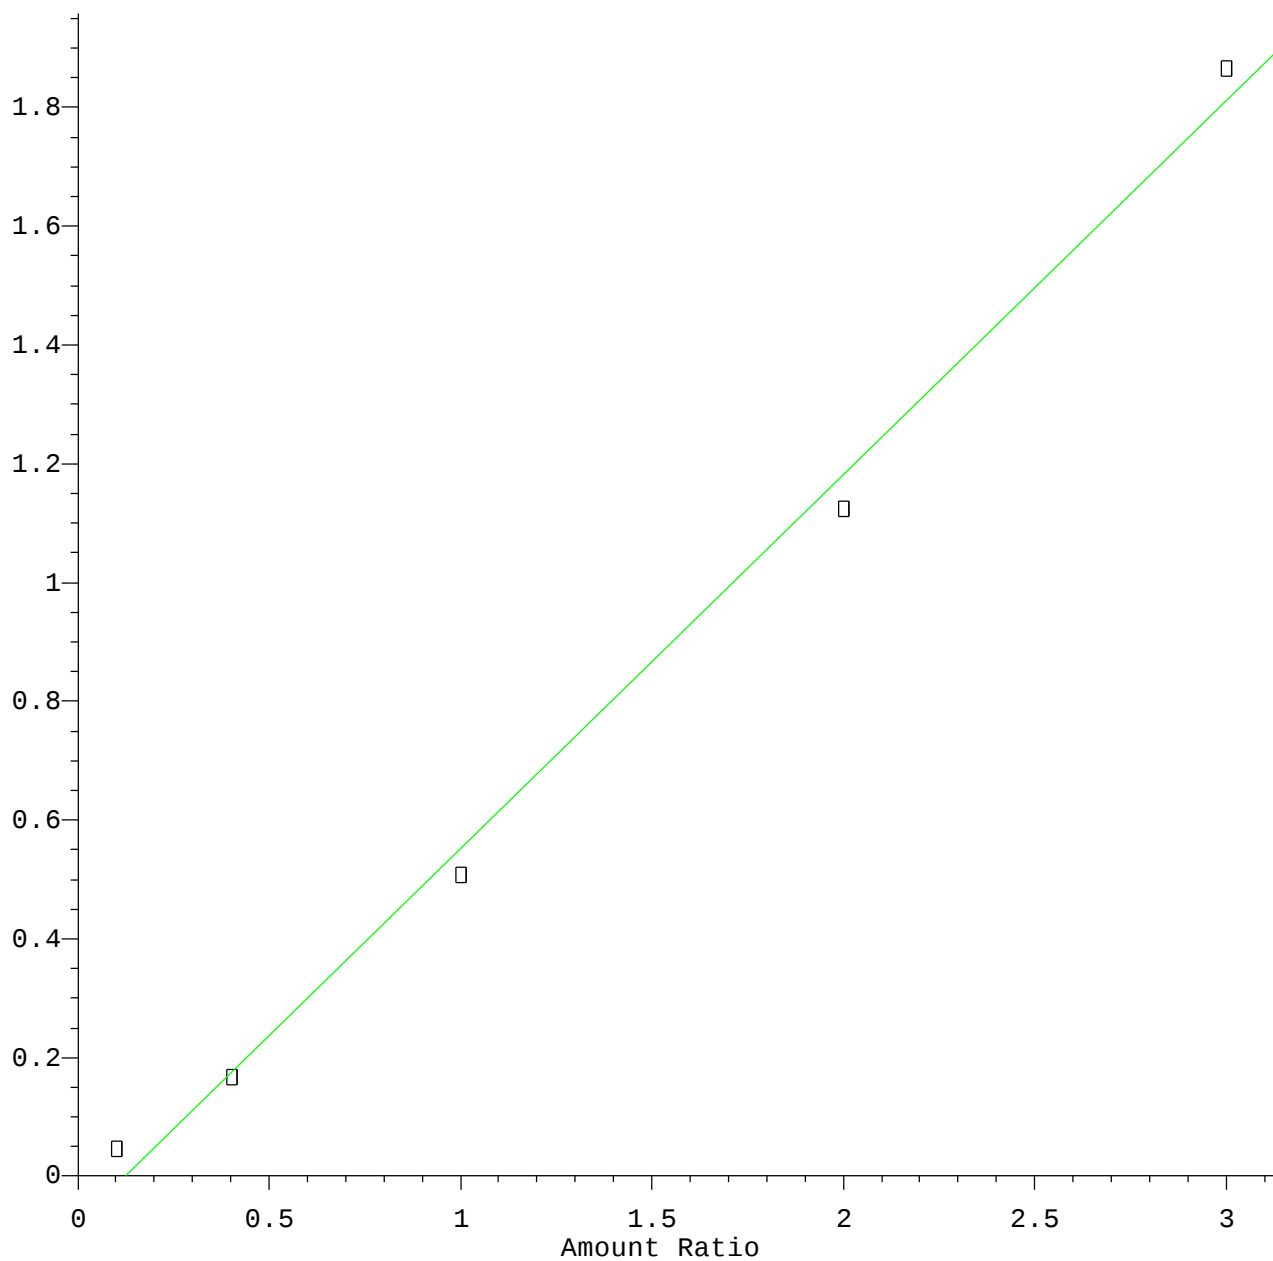


Resp Ratio = $6.30 \times 10^{-1} \times \text{Amt} - 7.81 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018

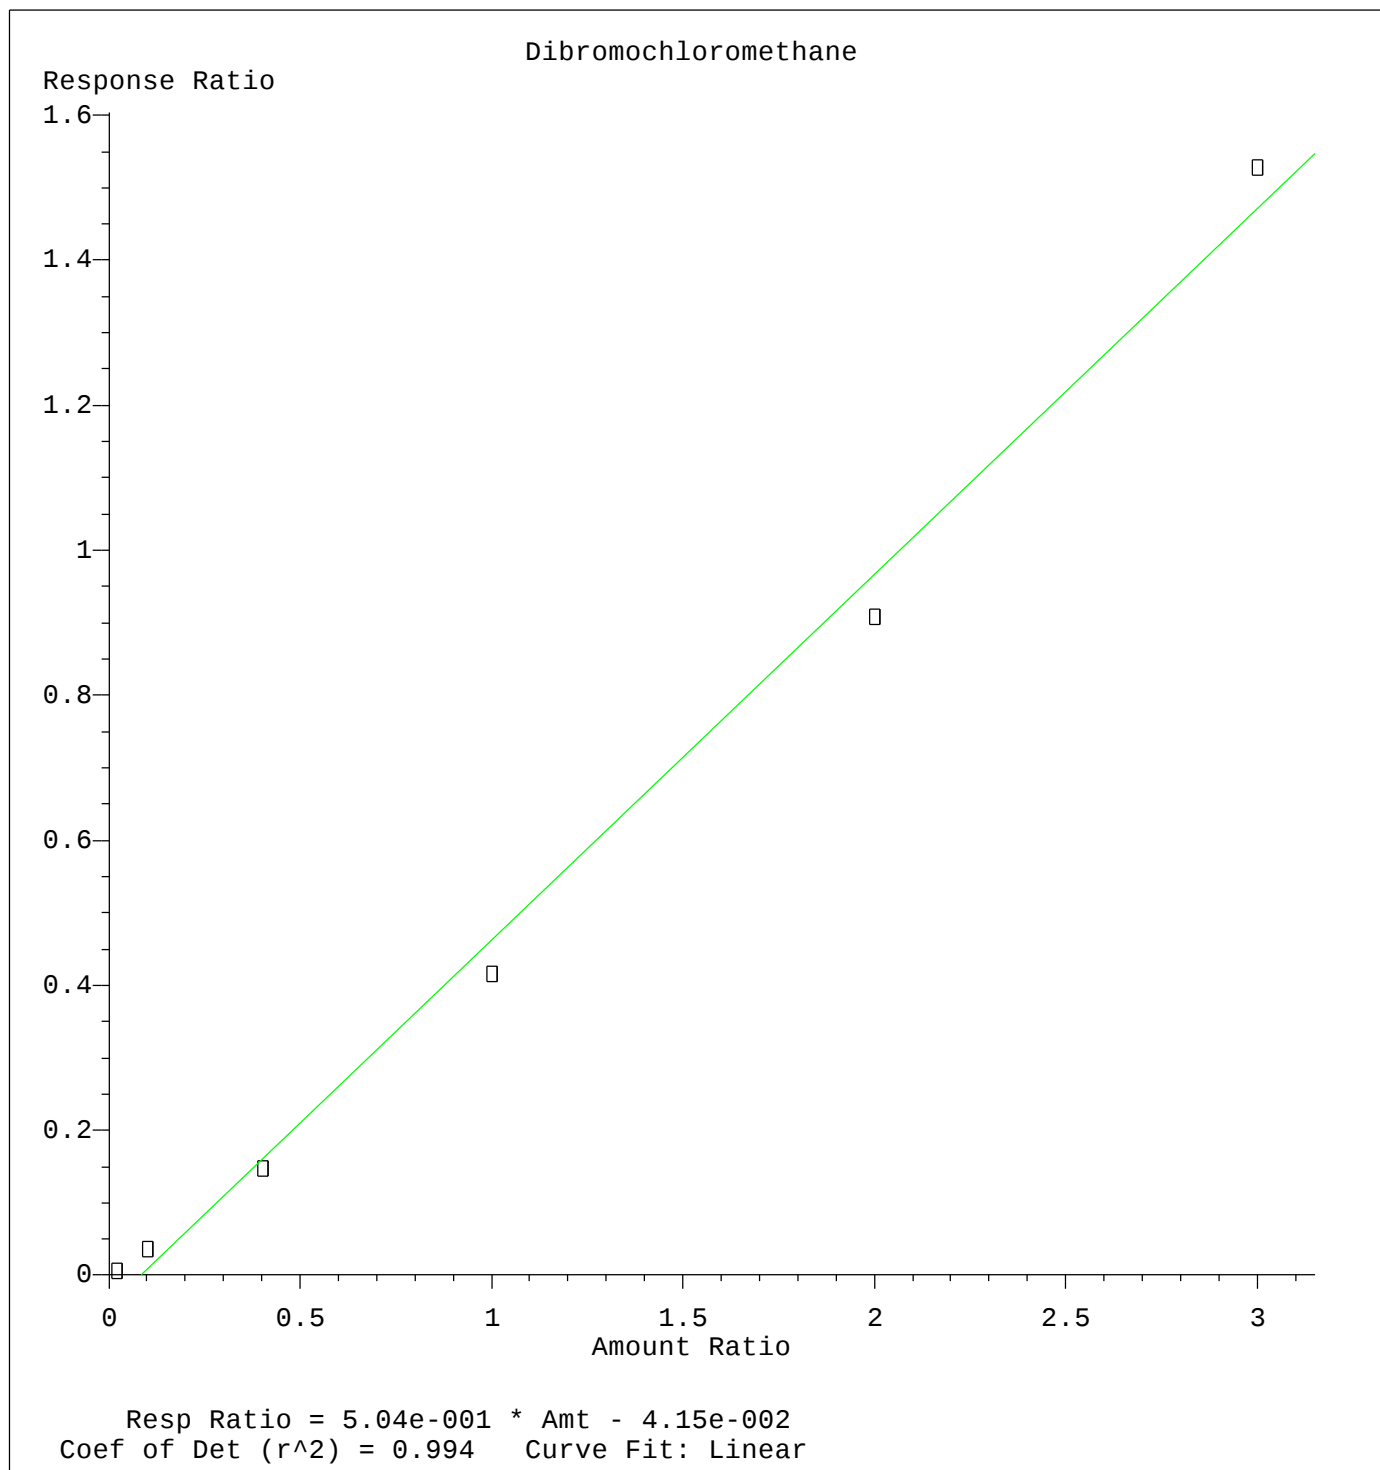


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018

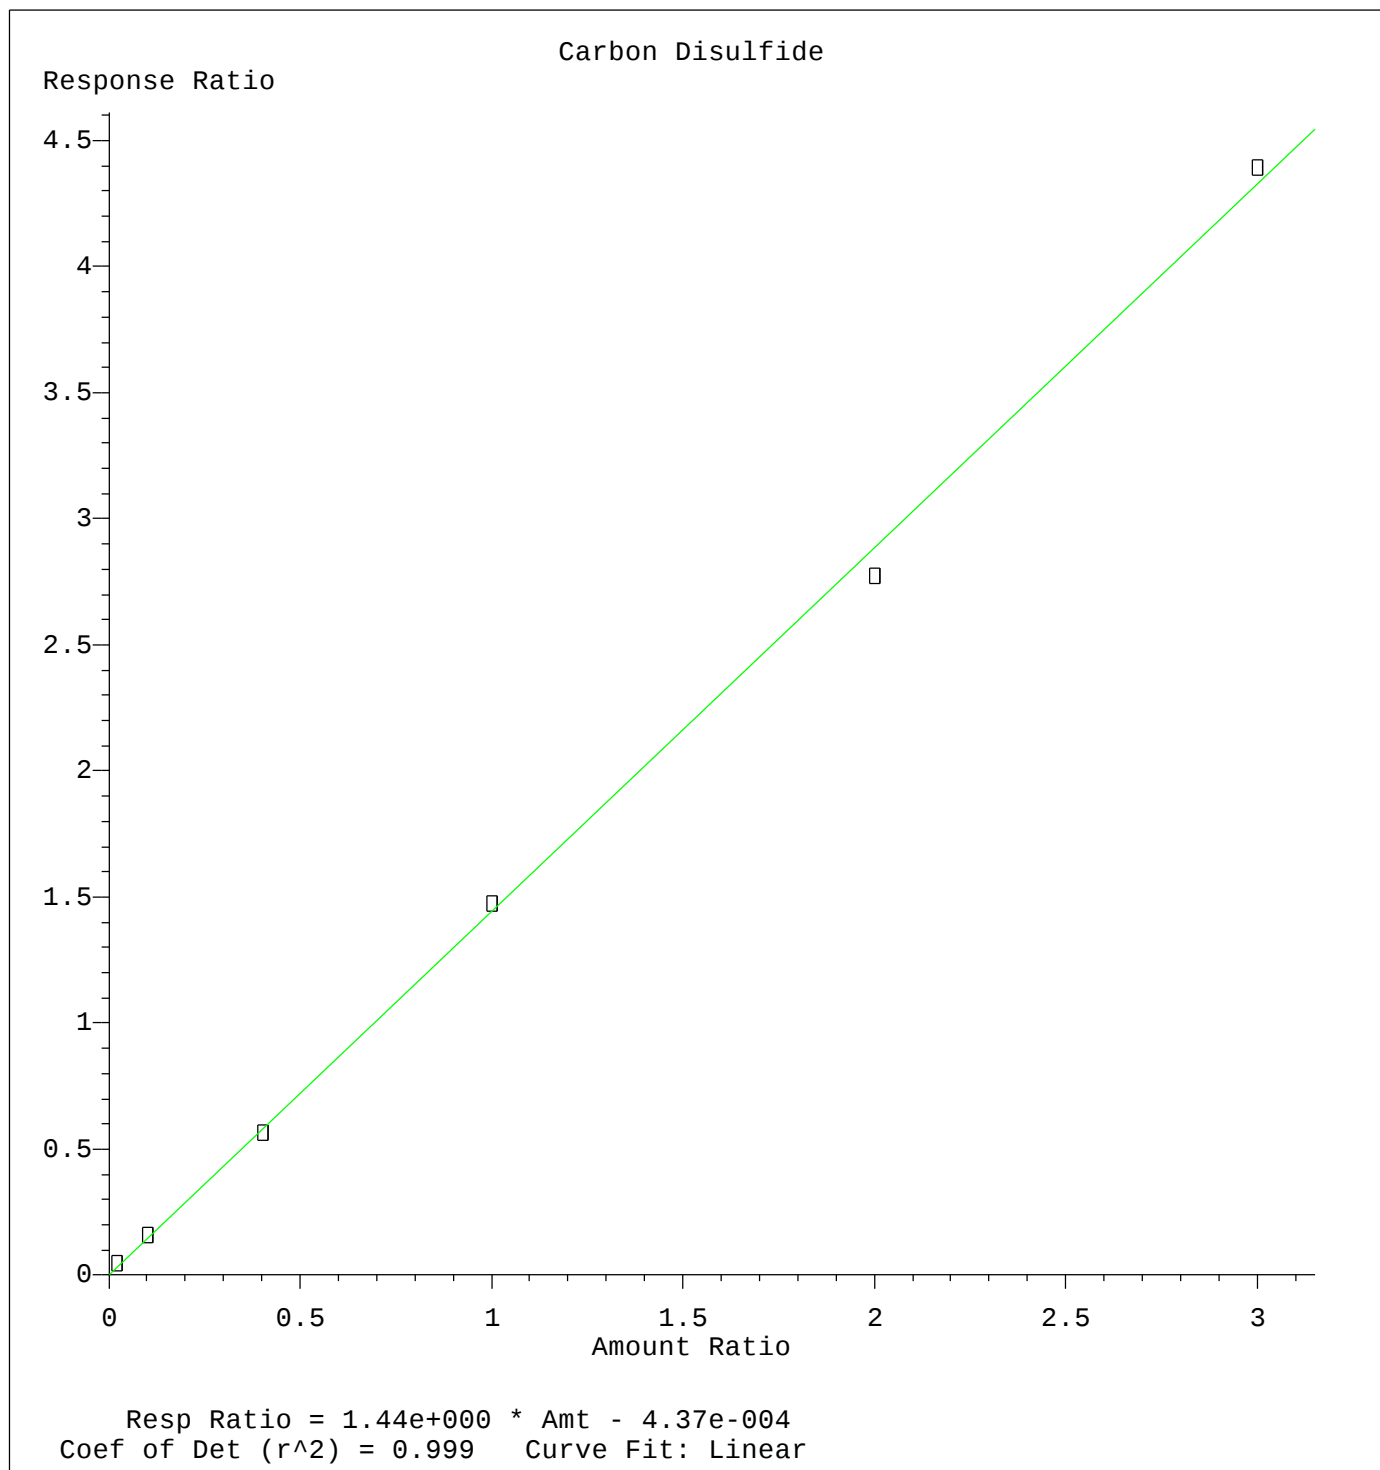

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018

Allyl chloride

Response Ratio

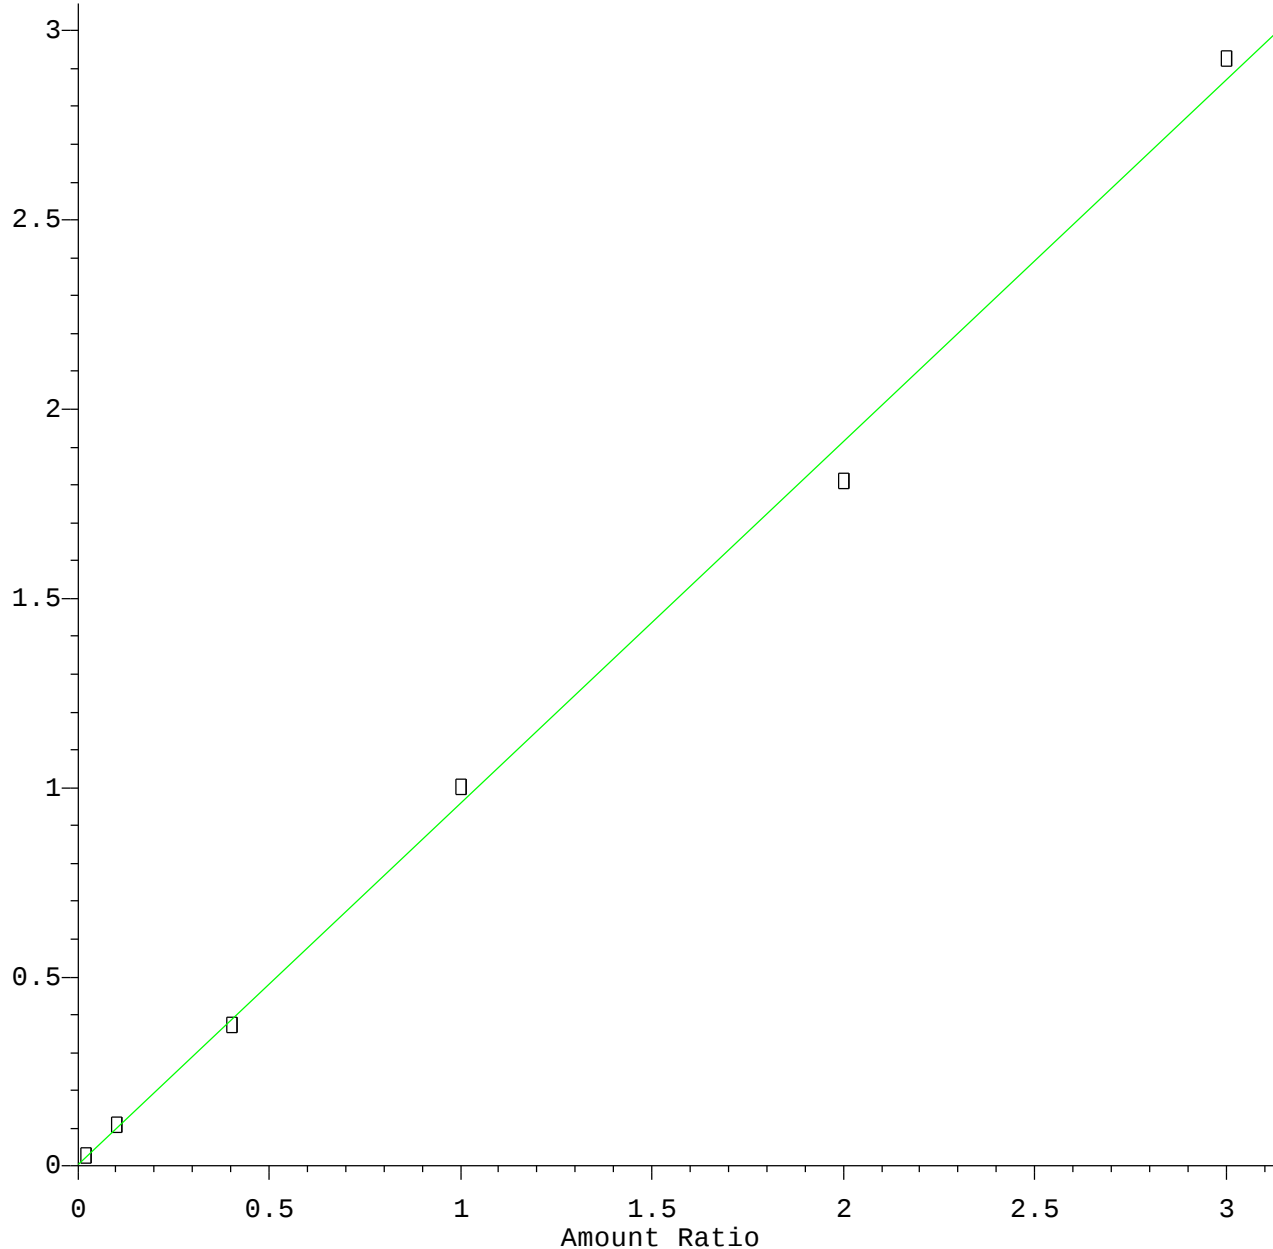


Resp Ratio = $9.55 \times 10^{-1} \times \text{Amt} + 1.95 \times 10^{-3}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018


Acrolein

Response Ratio

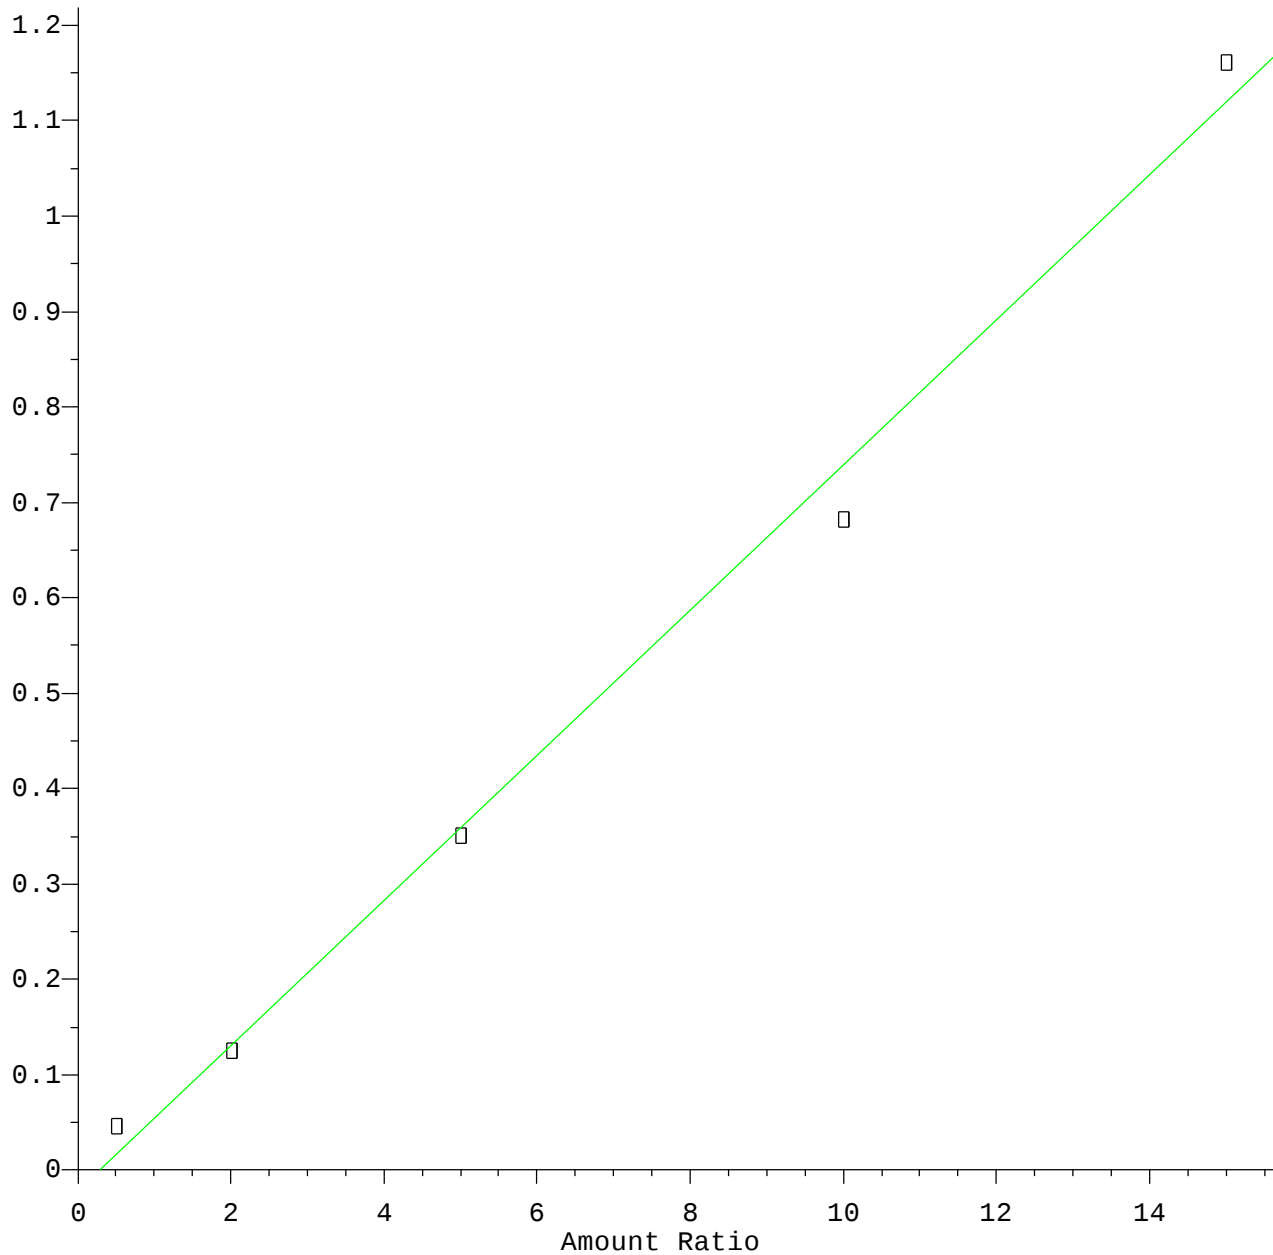

Resp Ratio = $7.61 \times 10^{-2} \times \text{Amt} - 2.22 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018

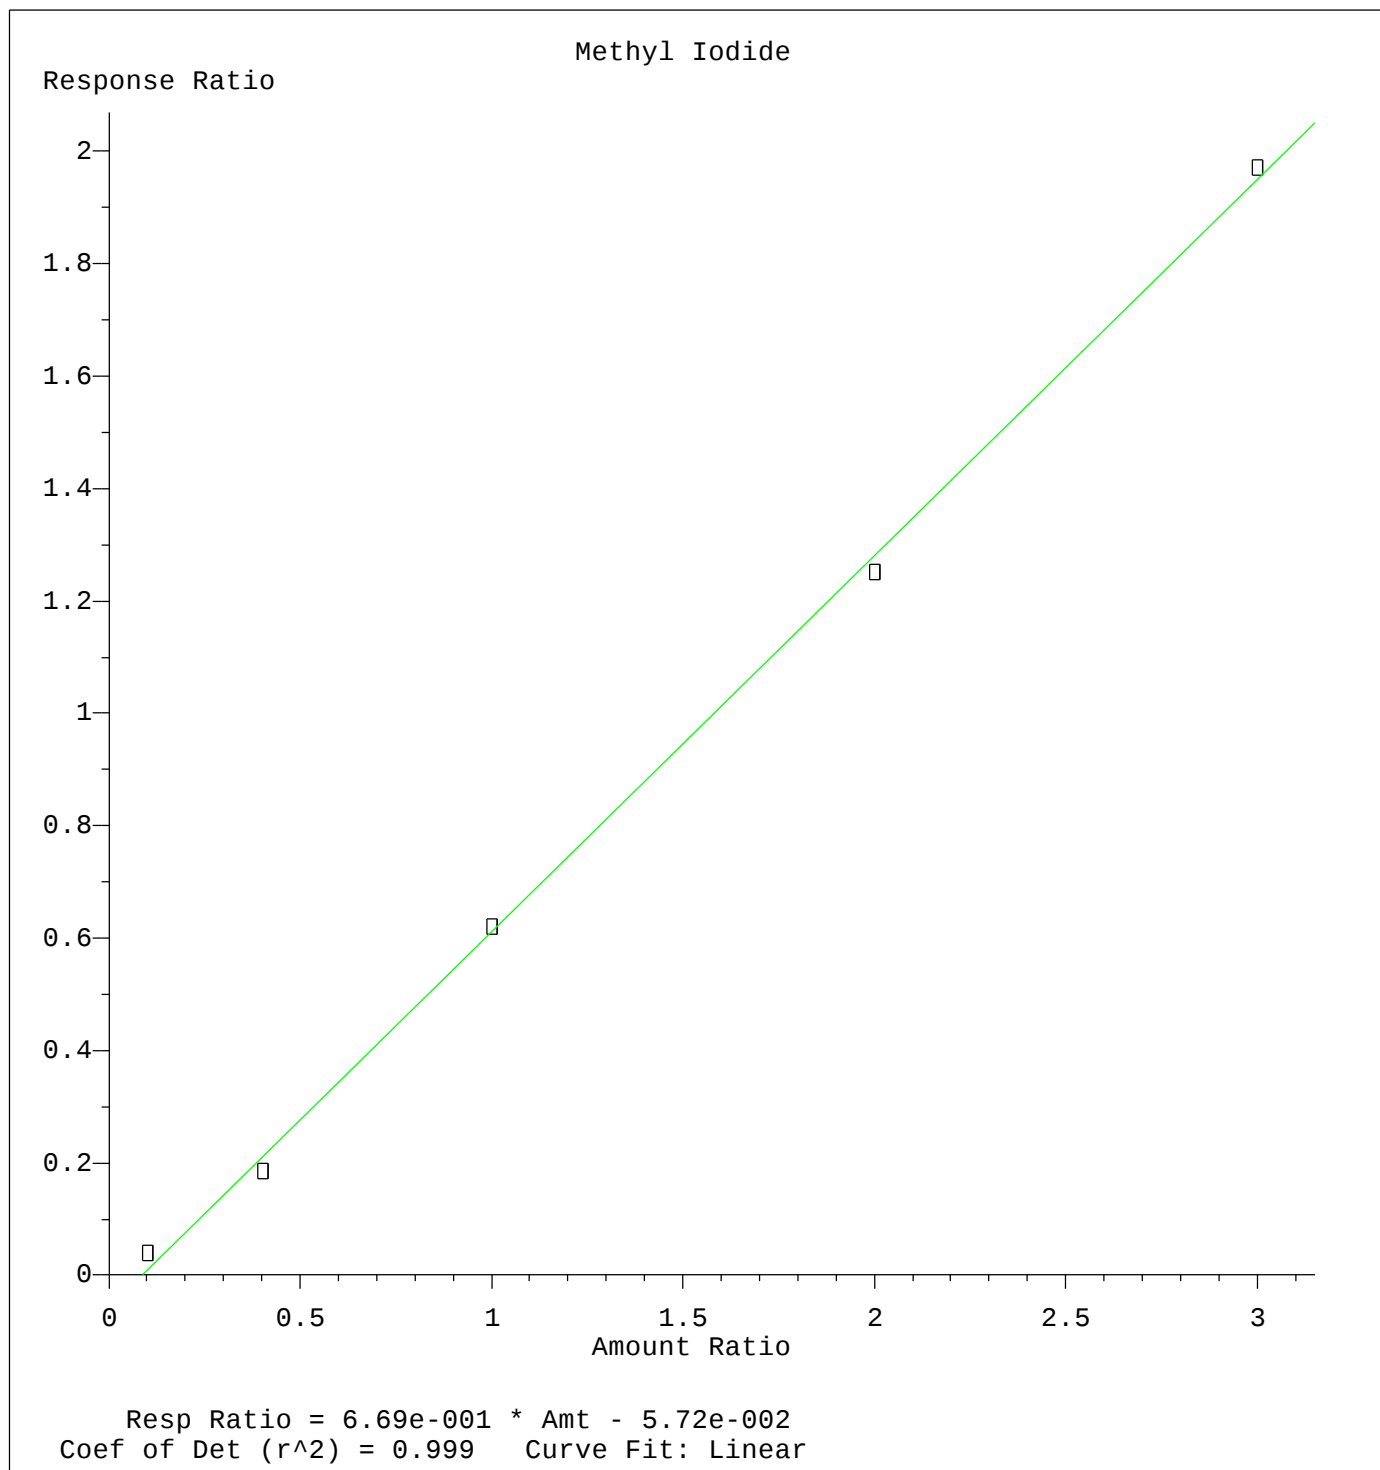

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018

Chloroethane

Response Ratio

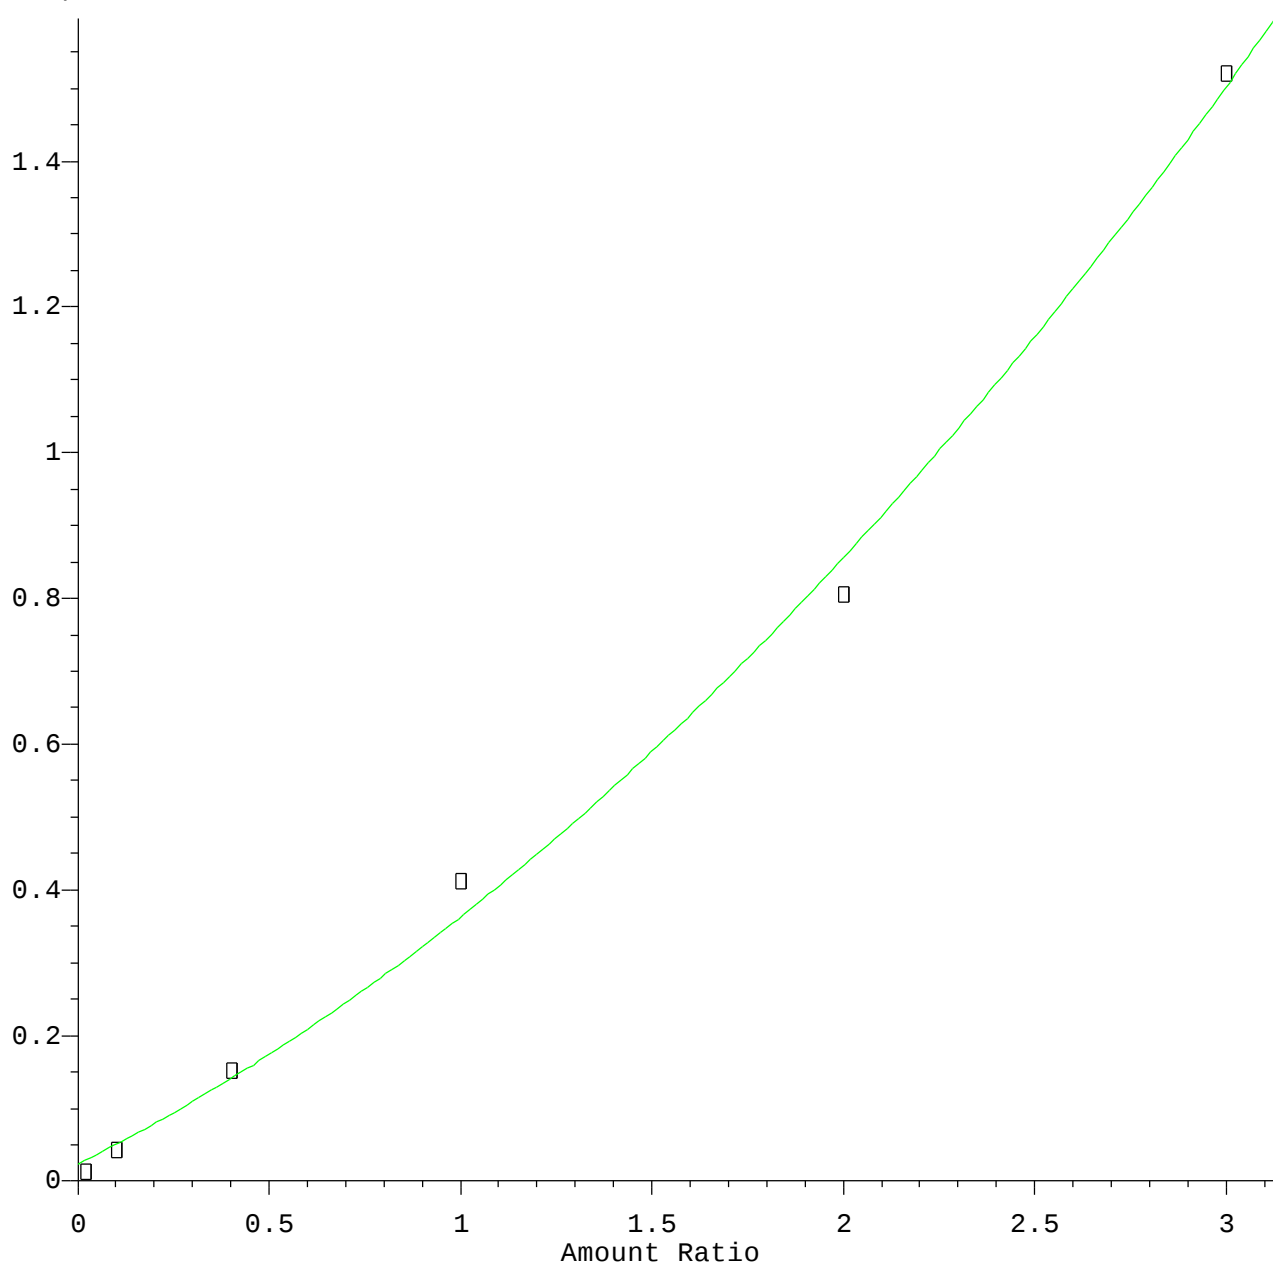

$R = 7.68e-002 A^2 + 2.62e-001 A + 2.34e-002$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Calibration Table Last Updated: Wed Mar 21 11:09:22 2018