


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX032018\
Data File : VX000353.D
Acq On : 20 Mar 2018 09:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Title : SW846 8260
Last Update : Wed Mar 21 04:52:42 2018

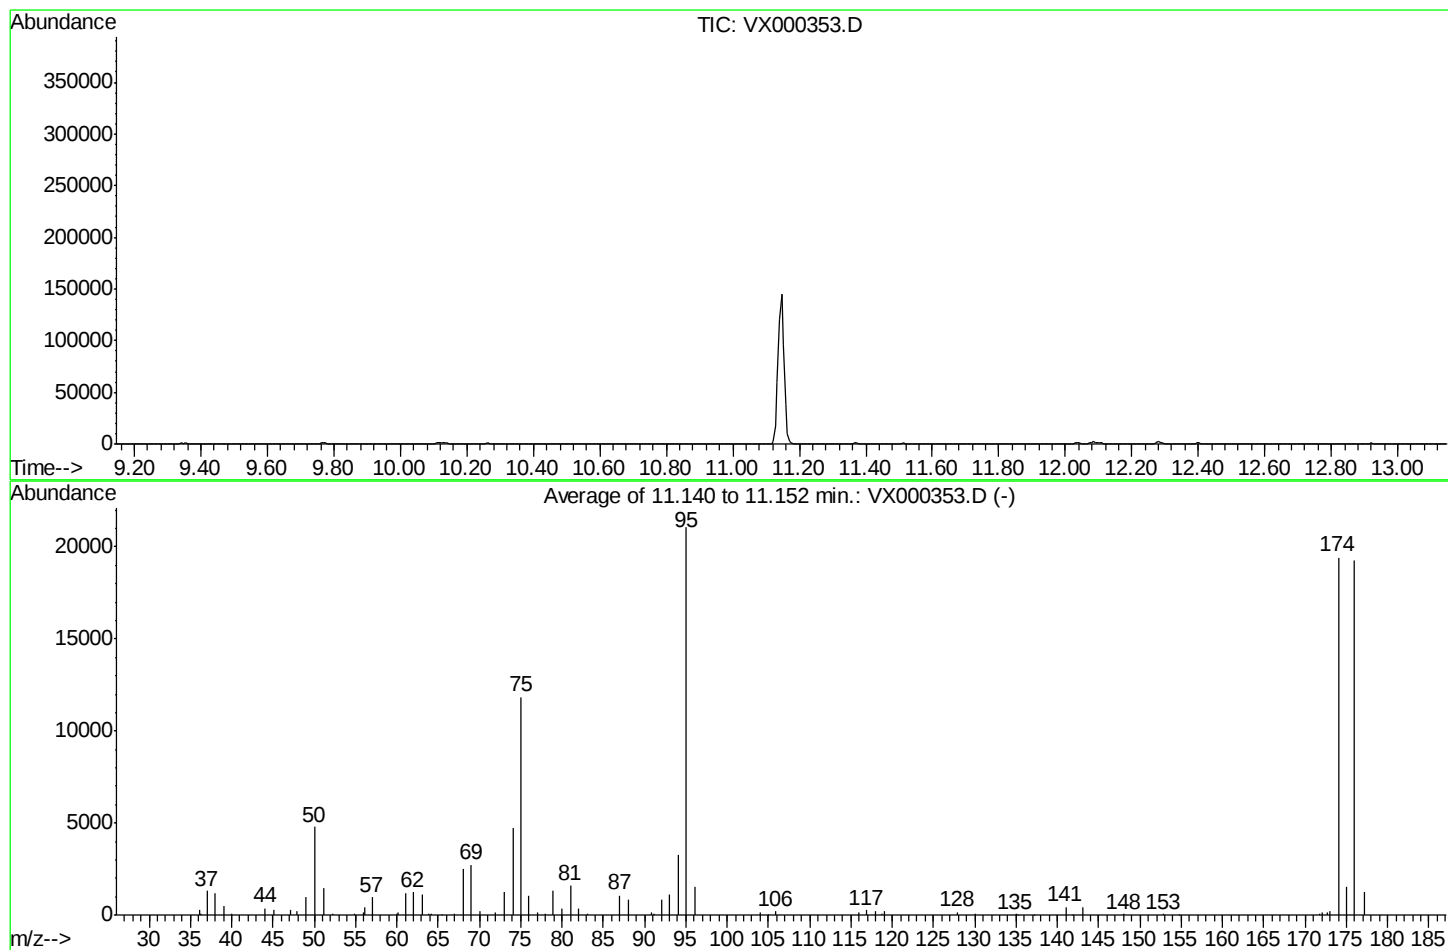

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	4792	PASS
75	95	30	60	56.2	11831	PASS
95	95	100	100	100.0	21066	PASS
96	95	5	9	7.3	1535	PASS
173	174	0.00	2	1.1	207	PASS
174	95	50	100	92.2	19418	PASS
175	174	5	9	8.0	1560	PASS
176	174	95	101	99.3	19274	PASS
177	176	5	9	6.4	1230	PASS