
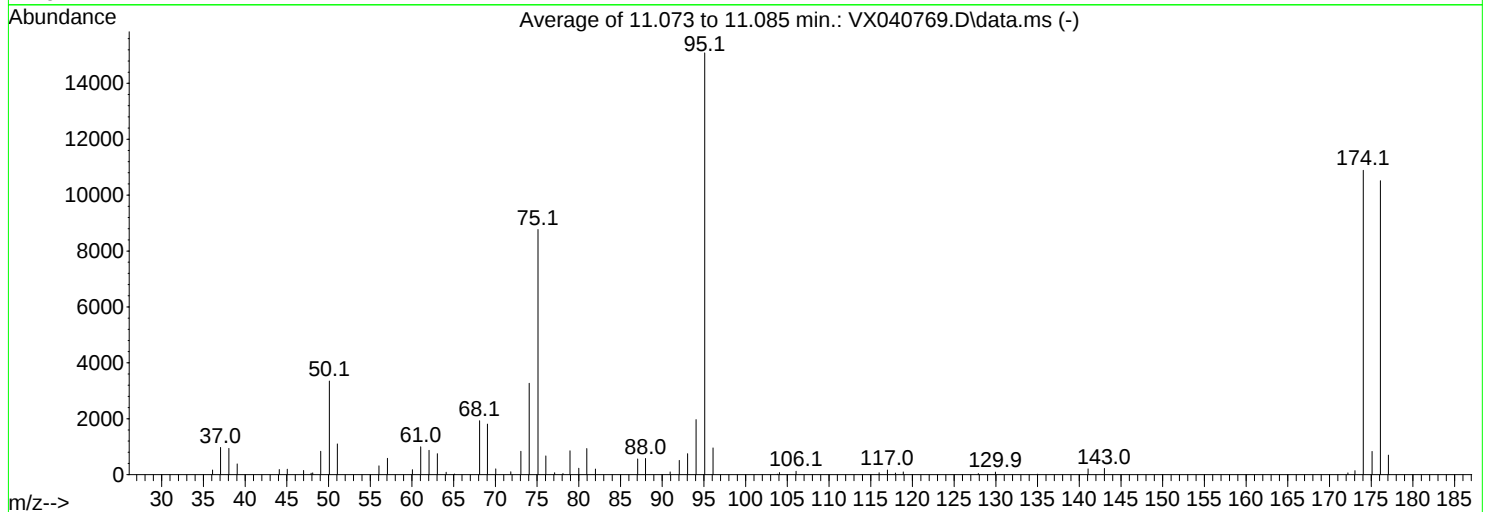


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032224\
Data File : VX040769.D
Acq On : 22 Mar 2024 09:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X030524W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Mar 05 13:21:29 2024

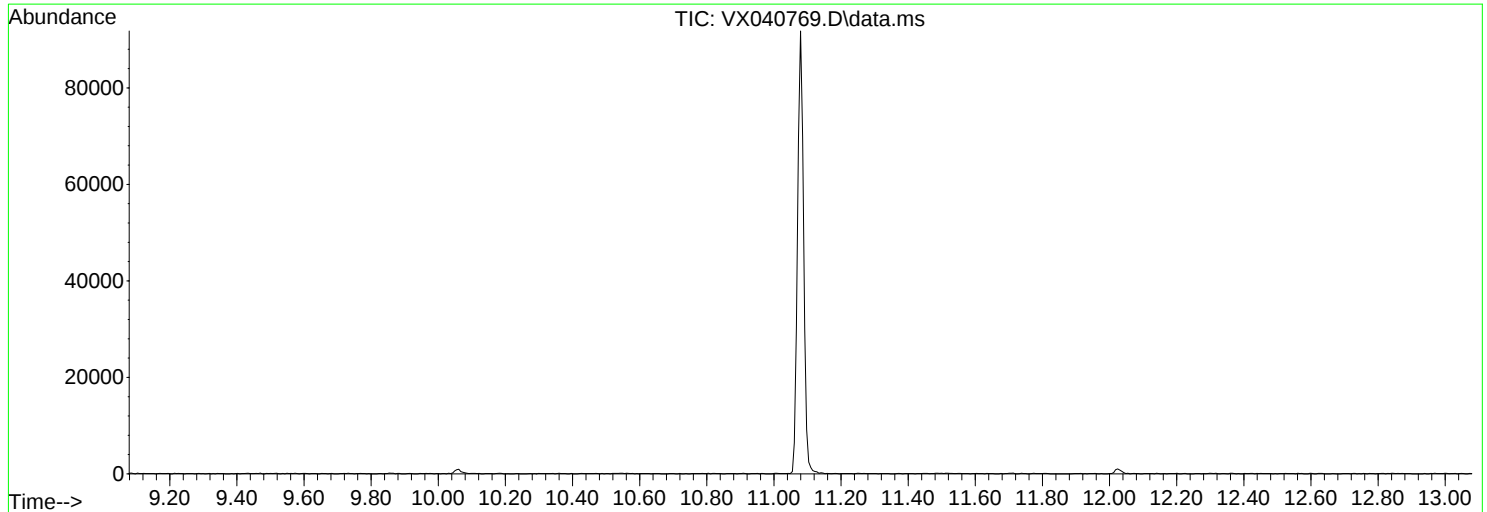

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	3351	PASS
75	95	30	60	58.1	8773	PASS
95	95	100	100	100.0	15091	PASS
96	95	5	9	6.4	959	PASS
173	174	0.00	2	1.3	144	PASS
174	95	50	100	72.2	10889	PASS
175	174	5	9	7.6	829	PASS
176	174	95	101	96.6	10519	PASS
177	176	5	9	6.7	701	PASS