


Data Path : W:\HPCHEM1\MSVOA X\Data\VX032318\
Data File : VX000421.D
Acq On : 23 Mar 2018 09:49
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Title : SW846 8260
Last Update : Wed Mar 21 04:52:42 2018

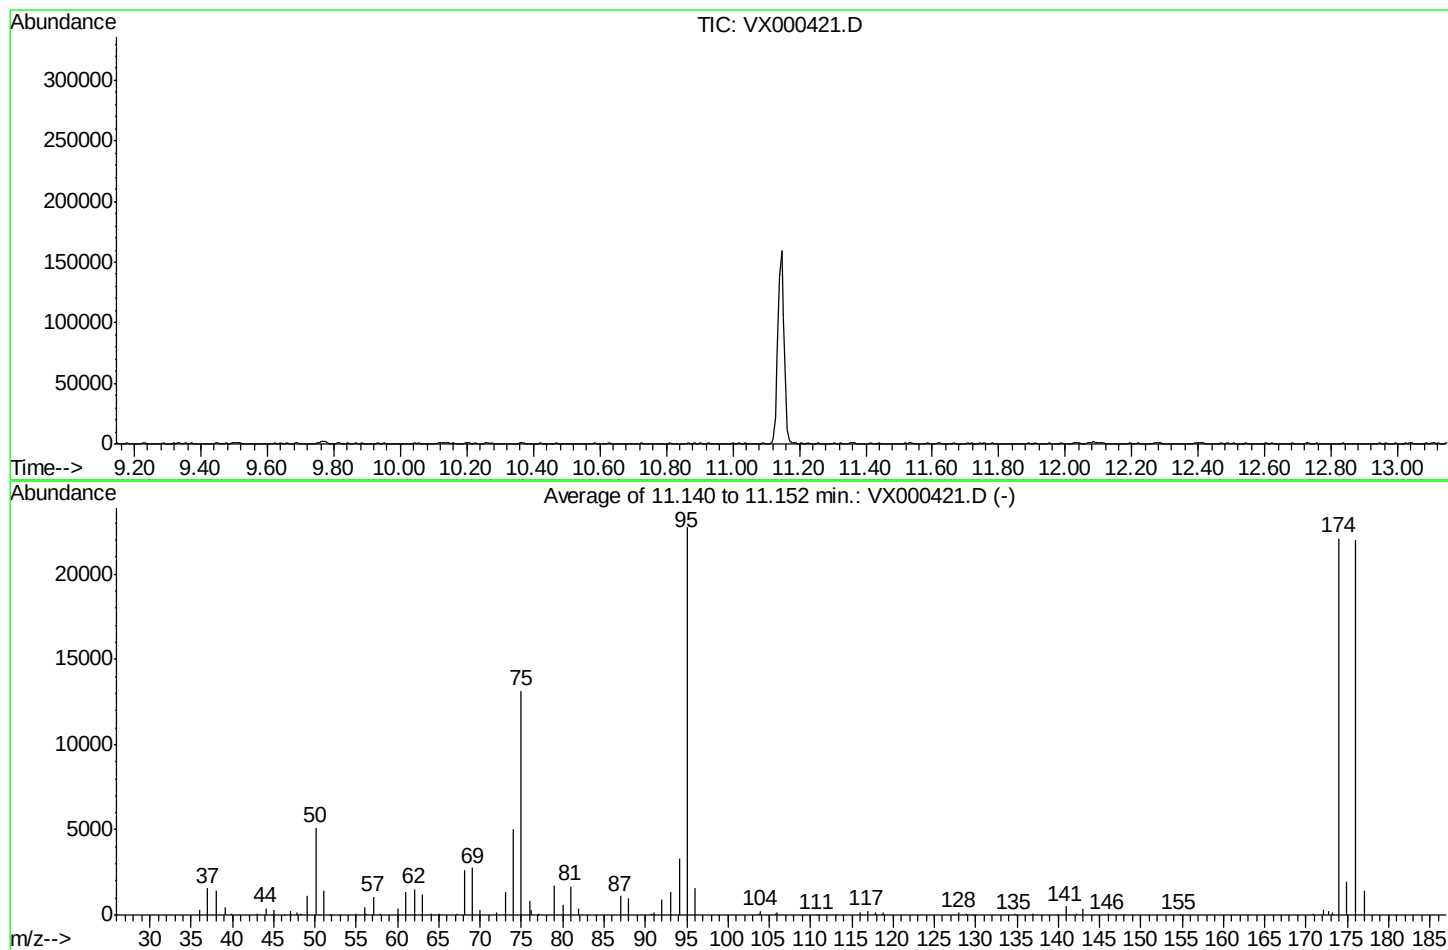

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	5125	PASS
75	95	30	60	57.9	13177	PASS
95	95	100	100	100.0	22749	PASS
96	95	5	9	6.8	1553	PASS
173	174	0.00	2	1.0	230	PASS
174	95	50	100	97.1	22085	PASS
175	174	5	9	8.8	1936	PASS
176	174	95	101	99.8	22037	PASS
177	176	5	9	6.5	1432	PASS