

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032323\
 Data File : VX034703.D
 Acq On : 23 Mar 2023 17:02
 Operator : JC/MD
 Sample : 02045-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC1-5-20230322

Quant Time: Mar 24 05:47:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Mar 13 10:29:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	310474	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	523922	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	468126	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	212756	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	223998	49.593	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	99.180%		
35) Dibromofluoromethane	5.385	113	165241	47.769	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.540%		
50) Toluene-d8	8.647	98	625755	48.458	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.920%		
62) 4-Bromofluorobenzene	11.079	95	241976	46.391	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	92.780%		
Target Compounds						Qvalue
3) Chloromethane	1.294	50	467	Below Cal	#	67
11) Tert butyl alcohol	2.953	59	276	0.293	ug/l #	73
16) Acetone	2.380	43	28005	13.163	ug/l	99
17) Carbon Disulfide	2.514	76	4389	0.459	ug/l #	95
18) Methyl Acetate	2.697	43	3019	0.434	ug/l	93
20) Methylene Chloride	2.788	84	13806	3.343	ug/l	87
25) 2-Butanone	4.593	43	2505	0.823	ug/l	96
29) Tetrahydrofuran	5.050	42	751	0.400	ug/l #	36
31) Cyclohexane	5.556	56	6589	1.040	ug/l #	1
36) 1,1-Dichloropropene	5.544	75	25978	4.889	ug/l #	50
37) Ethyl Acetate	4.715	43	59827	10.307	ug/l	97
38) Carbon Tetrachloride	5.550	117	33065	6.256	ug/l #	15
40) Benzene	6.037	78	19788	1.273	ug/l	100
43) Isopropyl Acetate	6.336	43	254556	25.888	ug/l	99
48) Methyl methacrylate	7.799	41	202997	42.924	ug/l #	46
49) 1,4-Dioxane	7.799	88	372	3.745	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	192863	33.811	ug/l #	50
52) Toluene	8.720	92	10164	1.056	ug/l	99
53) t-1,3-Dichloropropene	8.958	75	1305	0.217	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	84208	12.938	ug/l #	57
57) 1,3-Dichloropropane	9.482	76	10207	1.504	ug/l #	42
59) 2-Hexanone	9.482	43	146778	33.287	ug/l #	52
60) Dibromochloromethane	9.275	129	4271	1.066	ug/l #	10
64) Tetrachloroethene	9.275	164	4101	1.304	ug/l	91
67) Ethyl Benzene	10.195	91	5237	0.285	ug/l	92
68) m/p-Xylenes	10.299	106	2722	0.385	ug/l	84
69) o-Xylene	10.646	106	1600	0.226	ug/l	83
74) N-amyl acetate	10.640	43	54899	6.971	ug/l #	53
76) 1,2,3-Trichloropropane	11.079	75	127076	26.013	ug/l #	35
81) trans-1,4-Dichloro-2-b...	11.079	75	127076	70.373	ug/l #	8
95) Naphthalene	13.780	128	7942	0.507	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032323\
Data File : VX034703.D
Acq On : 23 Mar 2023 17:02
Operator : JC/MD
Sample : 02045-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322

Quant Time: Mar 24 05:47:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260
QLast Update : Mon Mar 13 10:29:32 2023
Response via : Initial Calibration




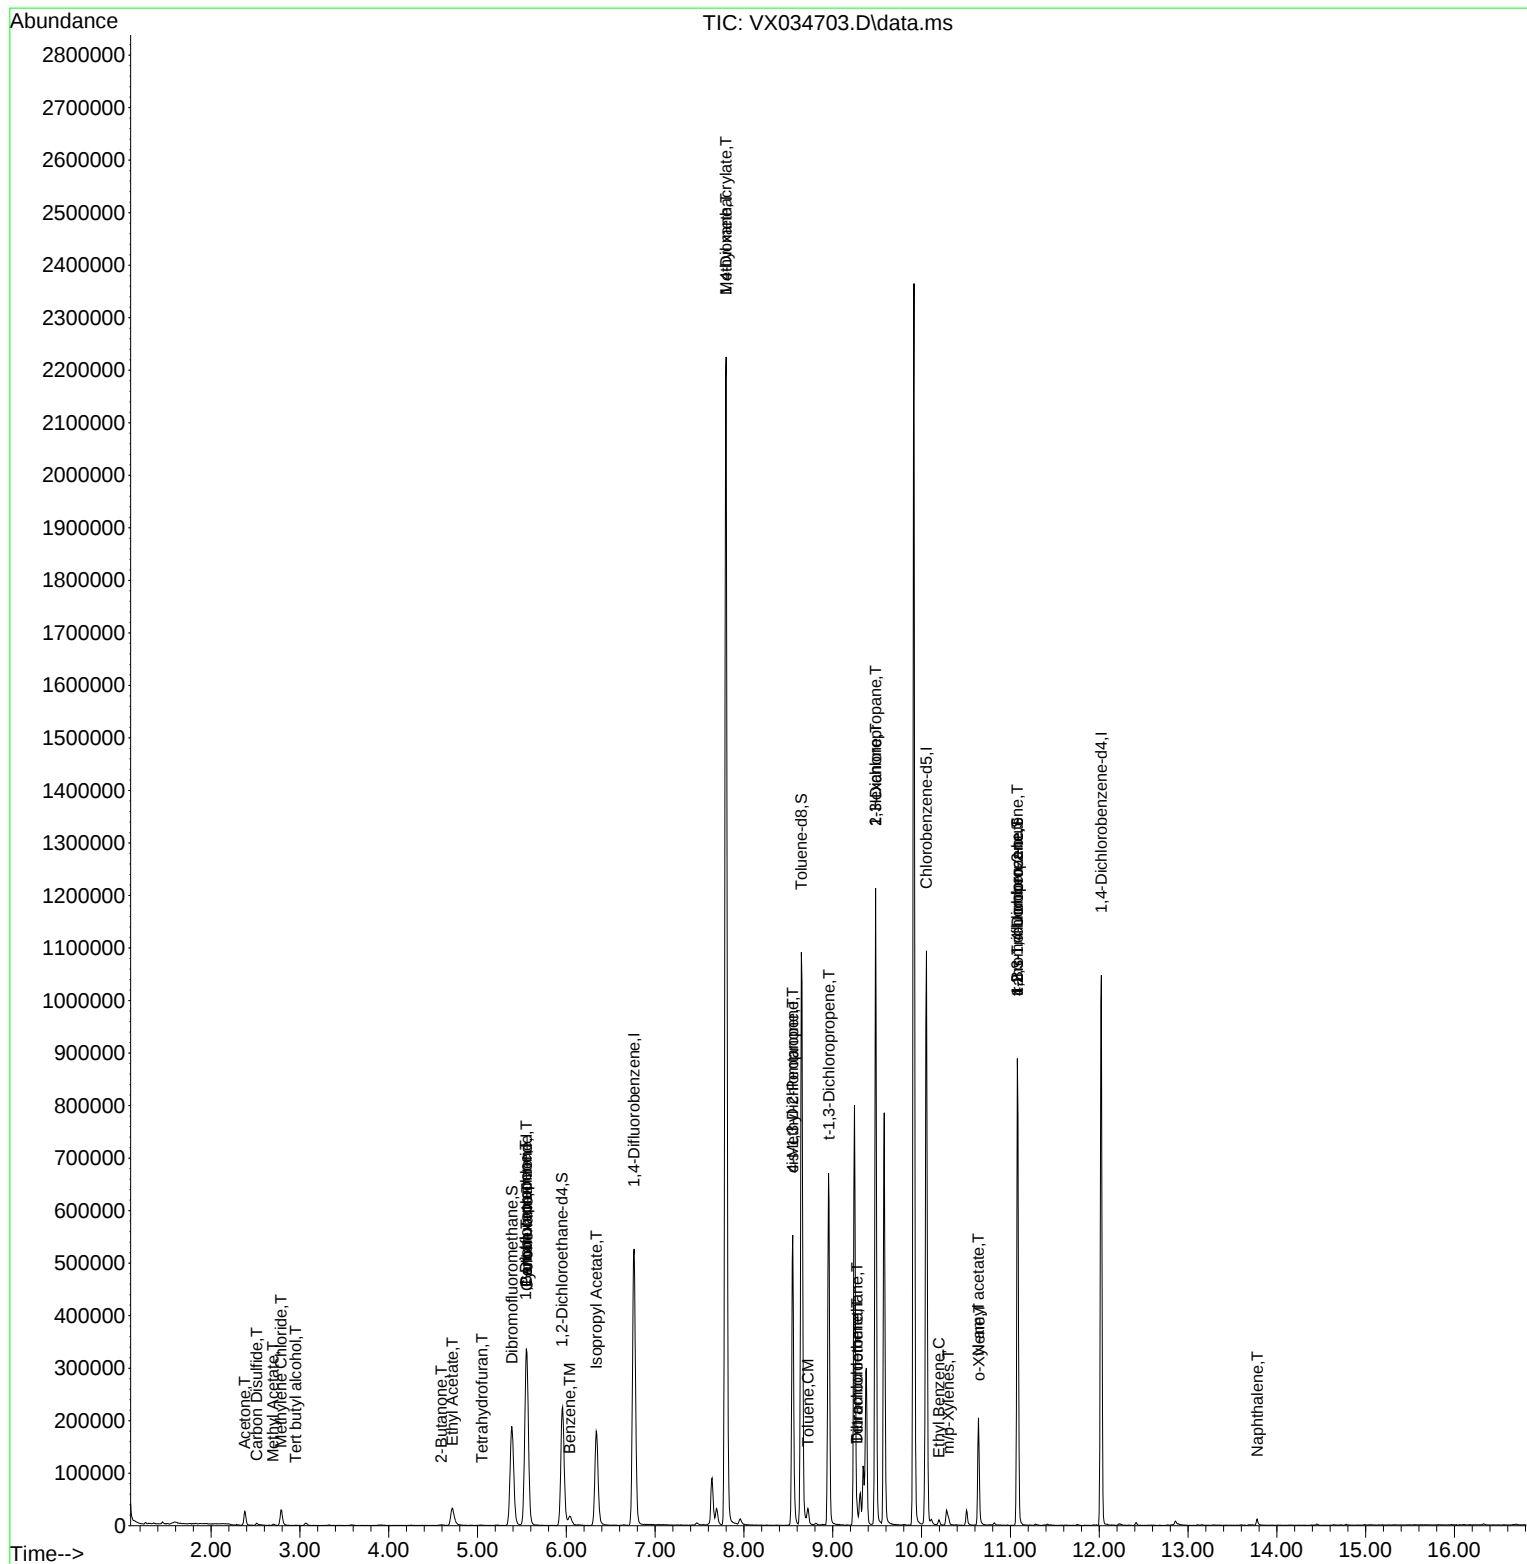




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion:168 Resp: 310474
Ion Ratio Lower Upper
168 100
99 64.0 45.7 68.5



#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. -0.007 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion: 50 Resp: 467
Ion Ratio Lower Upper
50 100
52 14.0 25.9 38.9#


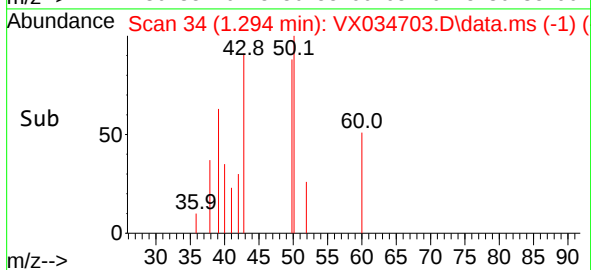

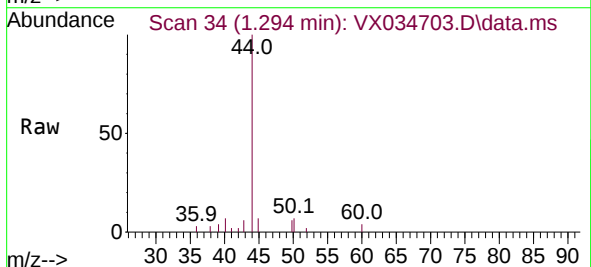


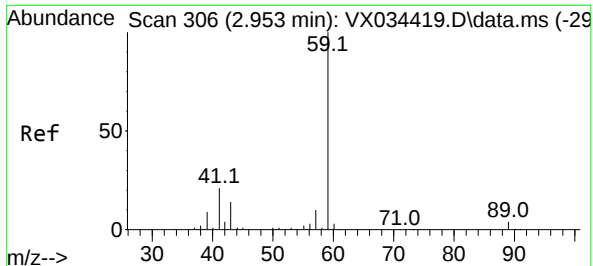

#11
Tert butyl alcohol
Concen: 0.293 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.000 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion: 59 Resp: 276
Ion Ratio Lower Upper
59 100
57 0.0 8.1 12.1#

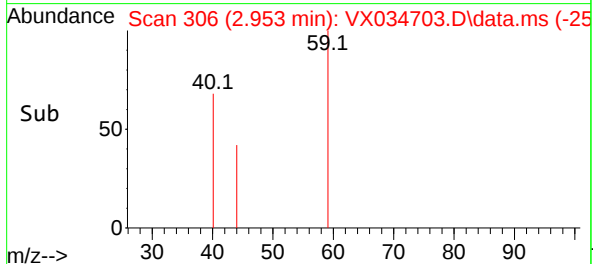

#16
Acetone
Concen: 13.163 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.006 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion: 43 Resp: 28005
Ion Ratio Lower Upper
43 100
58 30.4 24.7 37.1

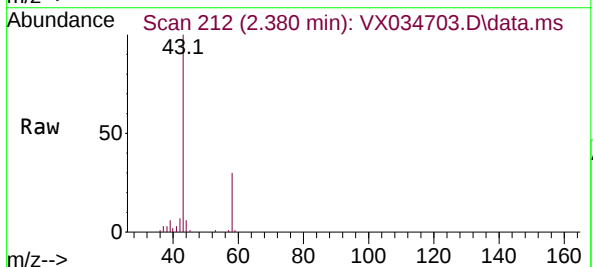



#17

Carbon Disulfide

Concen: 0.459 ug/l

RT: 2.514 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02

Instrument :

MSVOA_X

ClientSampleId :





WC1-5-20230322

Tgt Ion: 76 Resp: 4389

Ion Ratio Lower Upper

76 100

78 10.9 7.2 10.8#

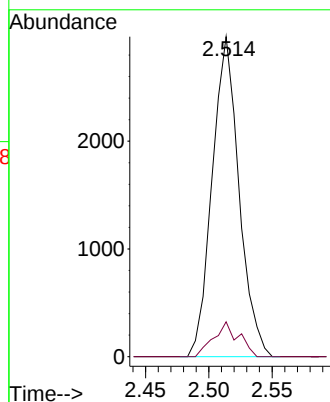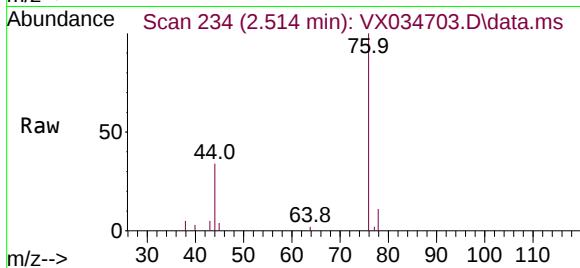

#18

Methyl Acetate

Concen: 0.434 ug/l

RT: 2.697 min Scan# 264

Delta R.T. -0.000 min

Lab File: VX034703.D




Acq: 23 Mar 2023 17:02


Tgt Ion: 43 Resp: 3019

Ion Ratio Lower Upper

43 100

74 19.3 18.3 27.5


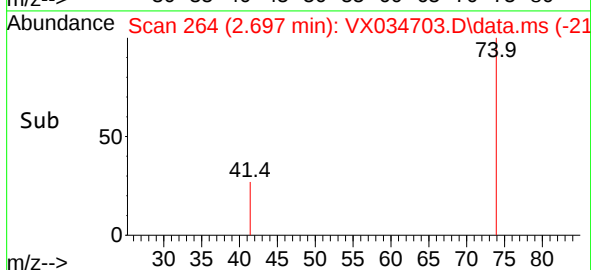
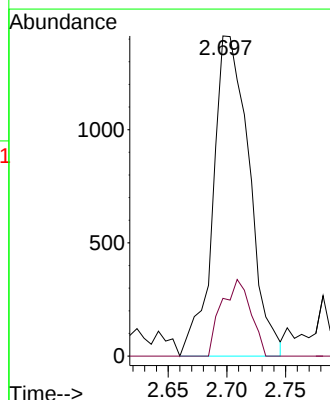
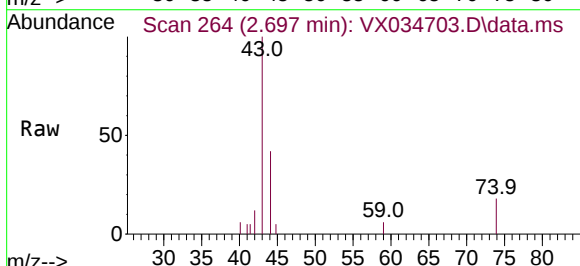




#20
Methylene Chloride
Concen: 3.343 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion:	84	Resp:	13806
Ion	Ratio	Lower	Upper
84	100		
49	108.9	103.8	155.8
51	35.3	31.8	47.8
86	58.9	51.4	77.2

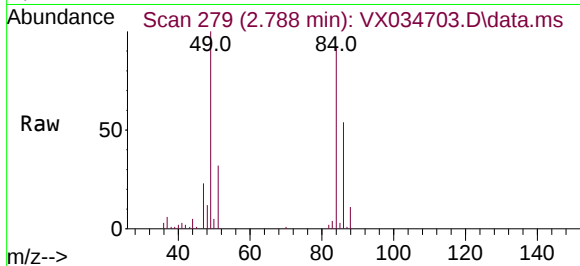

#25
2-Butanone
Concen: 0.823 ug/l
RT: 4.593 min Scan# 575
Delta R.T. 0.049 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion:	43	Resp:	2505
Ion	Ratio	Lower	Upper
43	100		
72	22.3	19.3	28.9

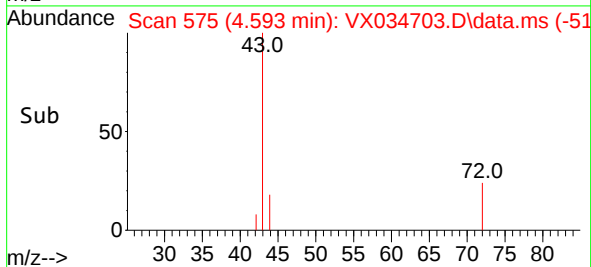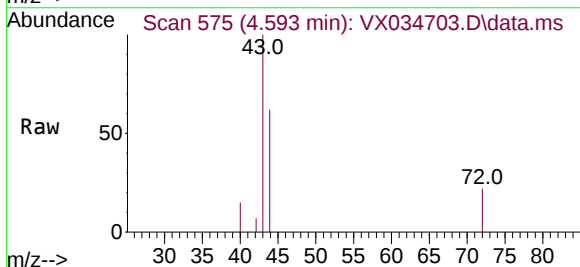



#29

Tetrahydrofuran

Concen: 0.400 ug/l

RT: 5.050 min Scan# 61

Delta R.T. 0.055 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02

Instrument :

MSVOA_X

ClientSampleId :

WC1-5-20230322





Tgt Ion: 42 Resp: 751

Ion Ratio Lower Upper

42 100

72 0.0 34.5 51.7#

71 2.5 32.1 48.1#

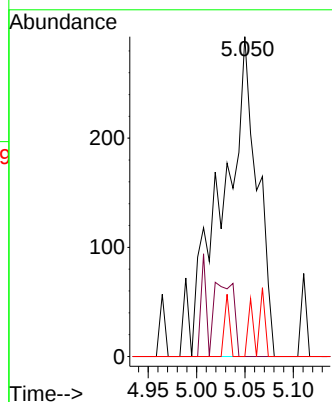

#31

Cyclohexane

Concen: 1.040 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.091 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02




Tgt Ion: 56 Resp: 6589


Ion Ratio Lower Upper

56 100

69 162.3 23.7 35.5#

84 129.1 68.5 102.7#


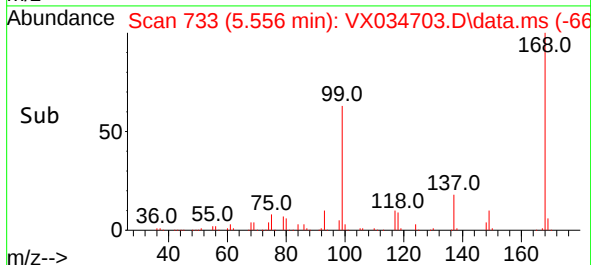

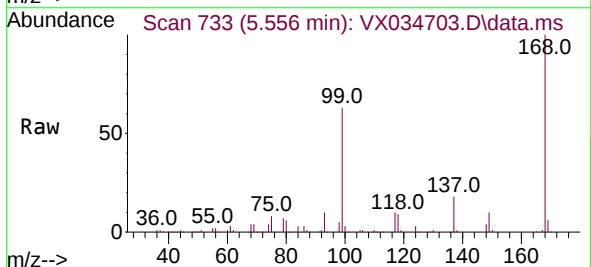




#33
 1,2-Dichloroethane-d4
 Concen: 49.593 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. 0.006 min
 Lab File: VX034703.D
 Acq: 23 Mar 2023 17:02




Instrument :
 MSVOA_X
 ClientSampleId :
 WC1-5-20230322


Tgt Ion: 65 Resp: 223998
 Ion Ratio Lower Upper
 65 100
 67 50.3 0.0 104.0



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. 0.006 min
 Lab File: VX034703.D
 Acq: 23 Mar 2023 17:02

Tgt Ion: 114 Resp: 523922
 Ion Ratio Lower Upper
 114 100
 63 22.4 0.0 42.2
 88 17.2 0.0 33.2

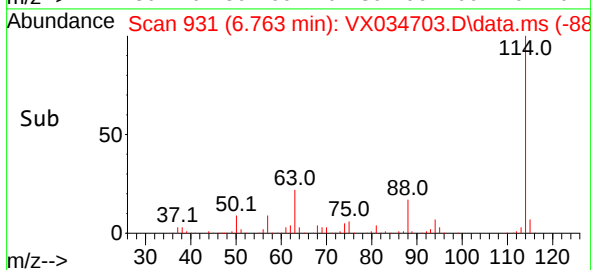

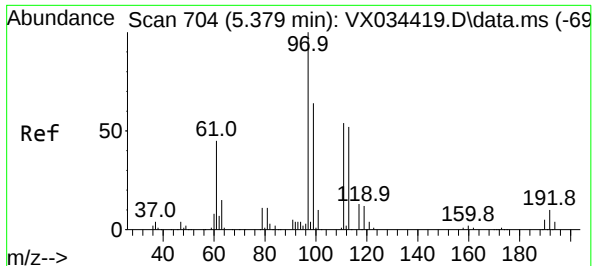

#35

Dibromofluoromethane

Concen: 47.769 ug/l

RT: 5.385 min Scan# 704

Delta R.T. 0.006 min

Lab File: VX034703.D


Acq: 23 Mar 2023 17:02

Instrument :

MSVOA_X

ClientSampleId :

WC1-5-20230322

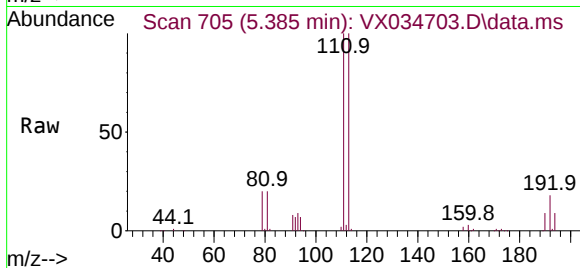




Tgt Ion:113 Resp: 165241

Ion Ratio Lower Upper

113 100

111 102.2 83.7 125.5

192 18.4 15.4 23.2

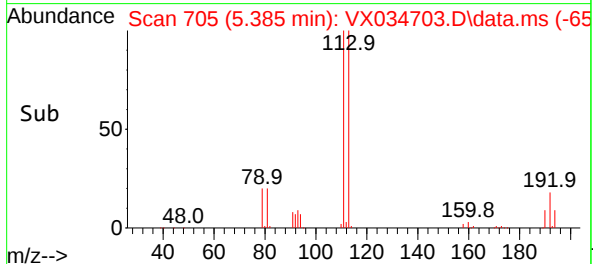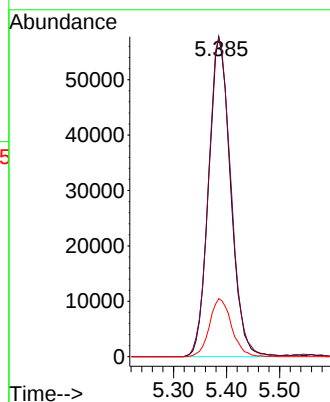

#36

1,1-Dichloropropene

Concen: 4.889 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.140 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02




Tgt Ion: 75 Resp: 25978


Ion Ratio Lower Upper

75 100

110 9.1 17.5 52.5#

77 0.0 24.3 36.5#

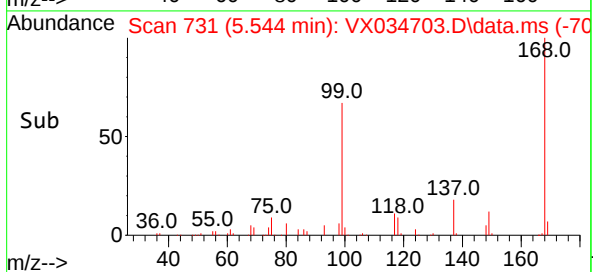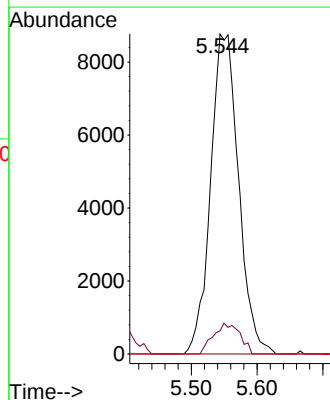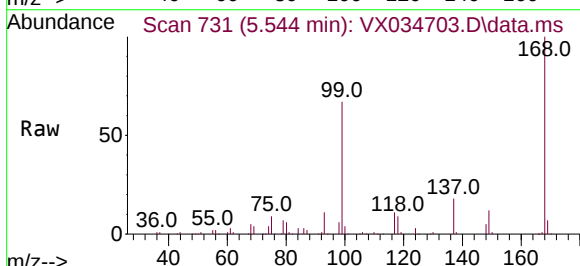



#37

Ethyl Acetate

Concen: 10.307 ug/l

RT: 4.715 min Scan# 593

Delta R.T. 0.012 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02





Instrument :

MSVOA_X

ClientSampleId :

WC1-5-20230322

Tgt Ion: 43	Resp: 59827
Ion Ratio	Lower Upper
43 100	
61 14.0	10.2 15.4
70 11.1	8.2 12.4



#38

Carbon Tetrachloride

Concen: 6.256 ug/l




RT: 5.550 min Scan# 732


Delta R.T. -0.122 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02

Tgt Ion: 117	Resp: 33065
Ion Ratio	Lower Upper
117 100	
119 4.3	76.6 114.8#
121 0.0	23.8 35.6#

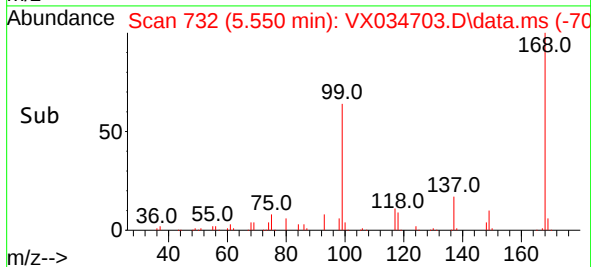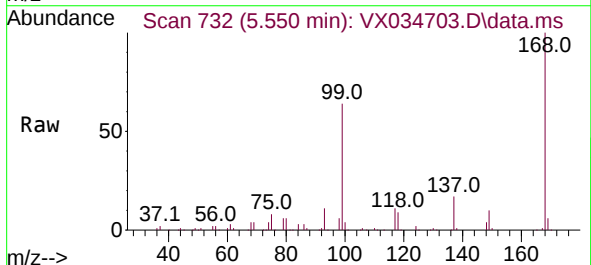

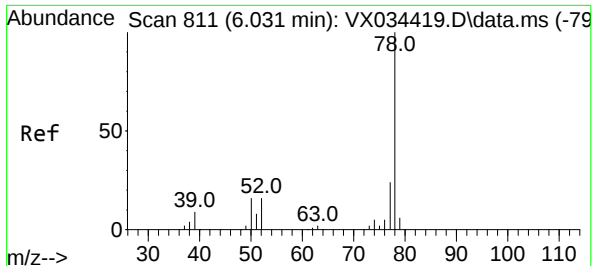

#40

Benzene

Concen: 1.273 ug/l

RT: 6.037 min Scan# 811

Delta R.T. 0.006 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02

Instrument :

MSVOA_X

ClientSampleId :





WC1-5-20230322

Tgt Ion: 78 Resp: 19788

Ion Ratio Lower Upper

78 100

77 23.8 19.0 28.4

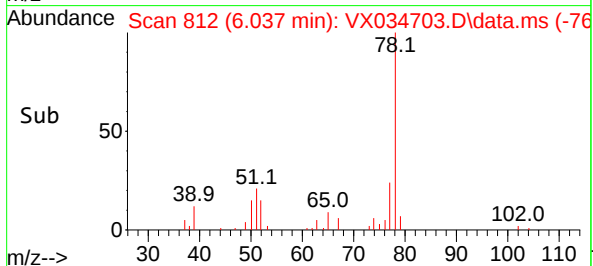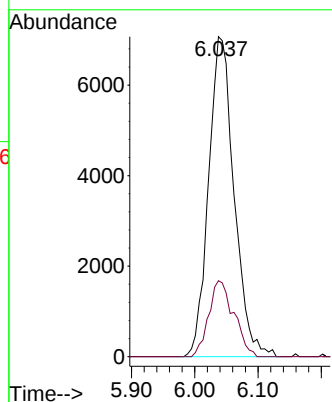

#43

Isopropyl Acetate

Concen: 25.888 ug/l

RT: 6.336 min Scan# 861

Delta R.T. 0.006 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02




Tgt Ion: 43 Resp: 254556


Ion Ratio Lower Upper

43 100

61 18.4 15.2 22.8

87 12.2 9.8 14.8

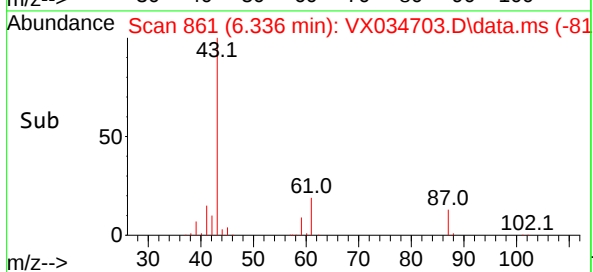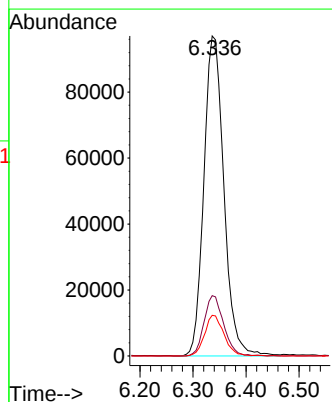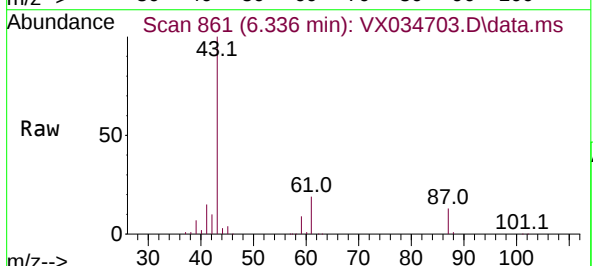

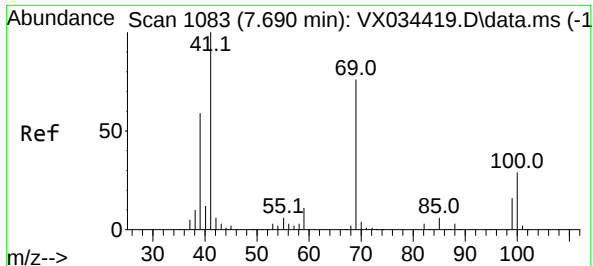

#48

Methyl methacrylate

Concen: 42.924 ug/l

RT: 7.799 min Scan# 1101

Delta R.T. 0.110 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02

Instrument :

MSVOA_X

ClientSampleId :

WC1-5-20230322





Tgt Ion: 41 Resp: 202997

Ion Ratio Lower Upper

41 100

69 0.1 62.2 93.4#

39 53.0 47.7 71.5

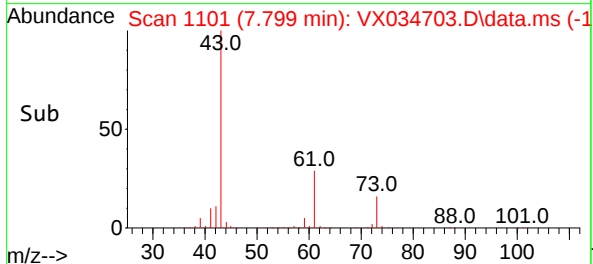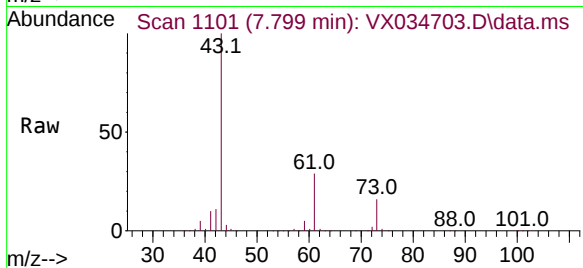

#49

1,4-Dioxane

Concen: 3.745 ug/l

RT: 7.799 min Scan# 1101

Delta R.T. 0.146 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02




Tgt Ion: 88 Resp: 372


Ion Ratio Lower Upper

88 100

43 567587.4 27.7 41.5#

58 2284.7 56.8 85.2#

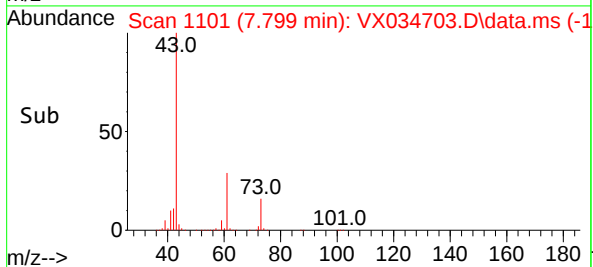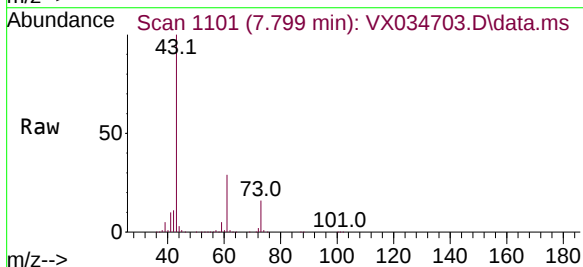

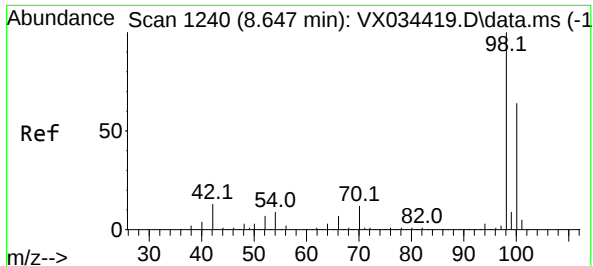

#50

Toluene-d8

Concen: 48.458 ug/l

RT: 8.647 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX034703.D

Acq: 23 Mar 2023 17:02

Instrument :

MSVOA_X

ClientSampleId :





WC1-5-20230322

Tgt Ion: 98 Resp: 625755

Ion Ratio Lower Upper

98 100

100 67.0 52.5 78.7

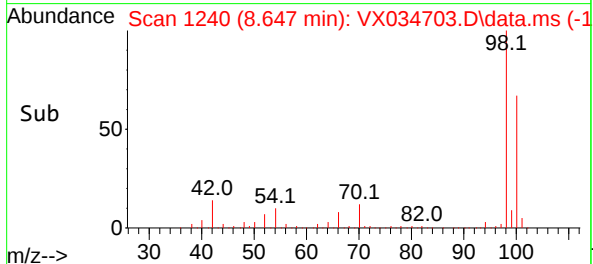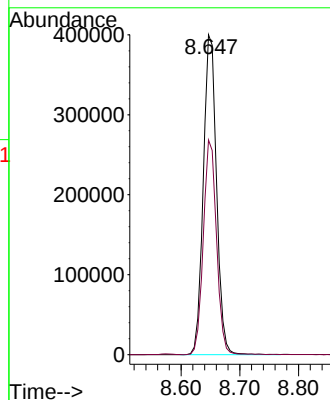

#51

4-Methyl-2-Pentanone

Concen: 33.811 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. -0.018 min

Lab File: VX034703.D




Acq: 23 Mar 2023 17:02


Tgt Ion: 43 Resp: 192863

Ion Ratio Lower Upper

43 100

58 7.9 30.6 46.0#


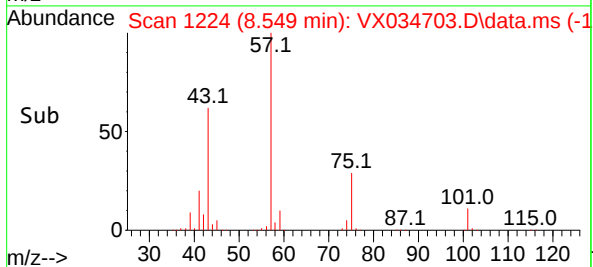
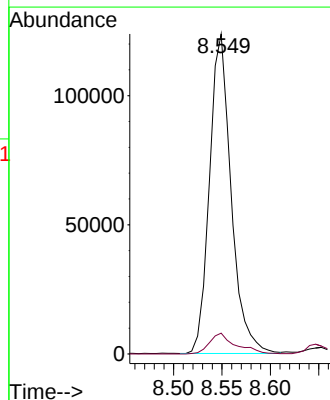
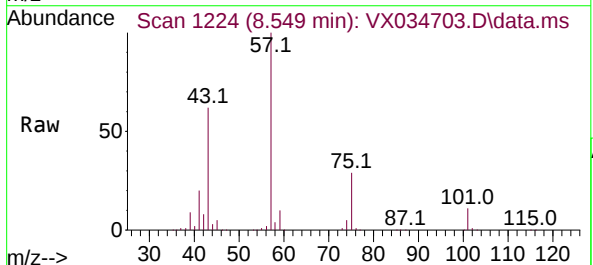




#52
Toluene
Concen: 1.056 ug/l
RT: 8.720 min Scan# 1251
Delta R.T. 0.006 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion: 92 Resp: 10164
Ion Ratio Lower Upper
92 100
91 171.8 136.8 205.2

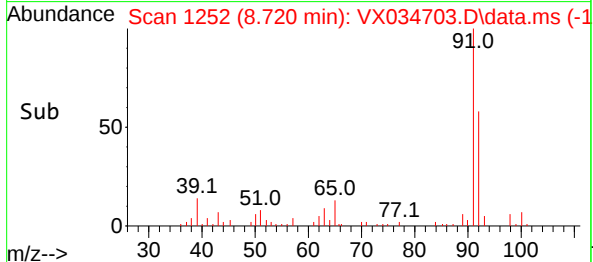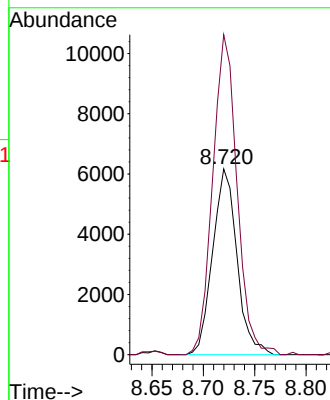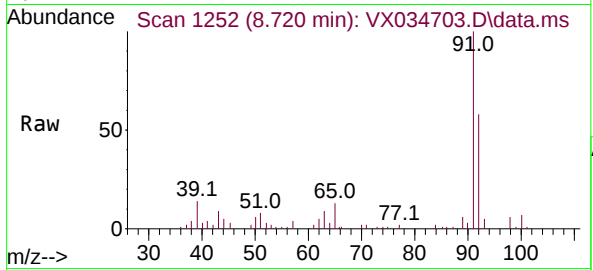

#53
t-1,3-Dichloropropene
Concen: 0.217 ug/l
RT: 8.958 min Scan# 1291
Delta R.T. -0.018 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion: 75 Resp: 1305
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.2#


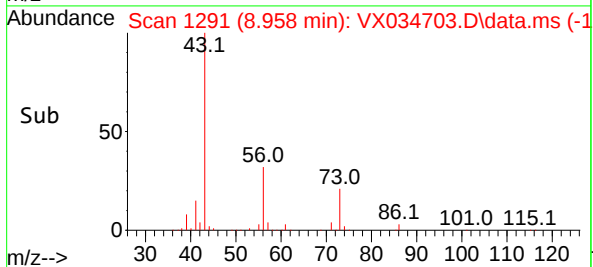
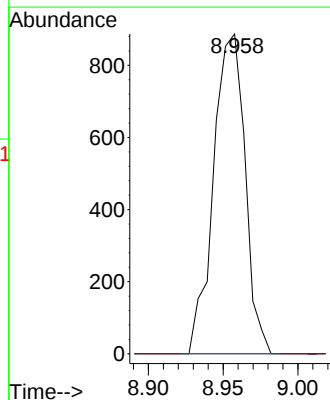
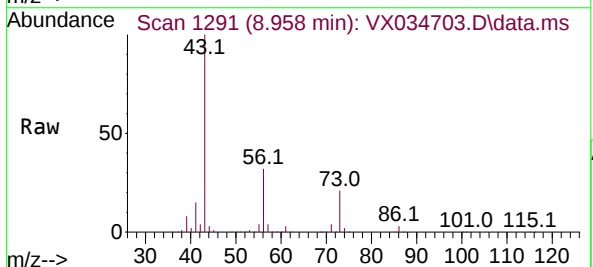


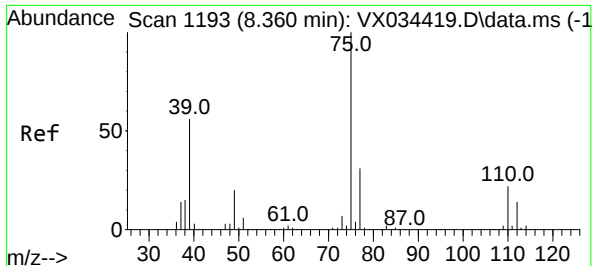

#54
cis-1,3-Dichloropropene
Concen: 12.938 ug/l
RT: 8.549 min Scan# 1193
Delta R.T. 0.189 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion: 75 Resp: 84208
Ion Ratio Lower Upper
75 100
77 0.6 25.0 37.4#
39 29.5 44.6 66.8#

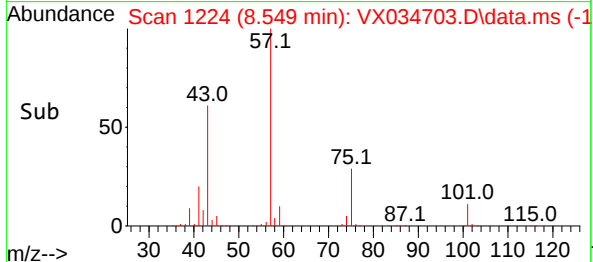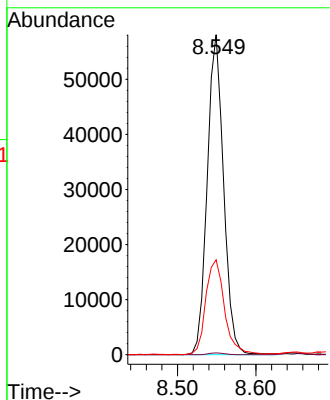

#57
1,3-Dichloropropane
Concen: 1.504 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.177 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion: 76 Resp: 10207
Ion Ratio Lower Upper
76 100
78 0.0 25.8 38.8#


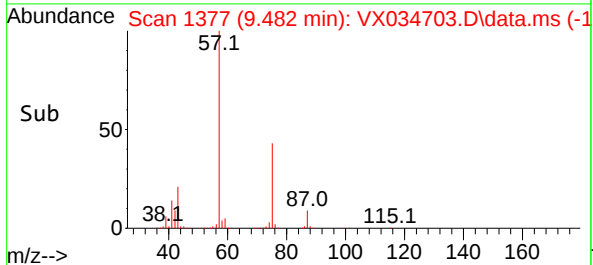
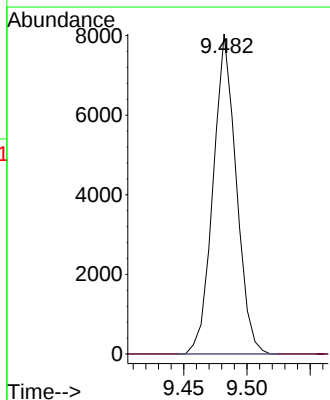
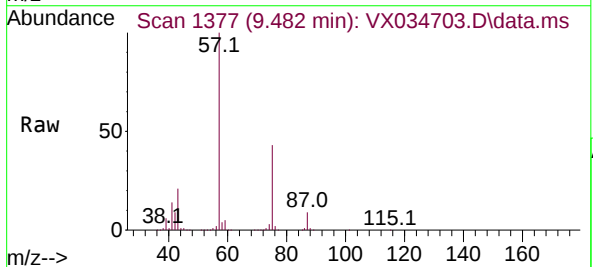


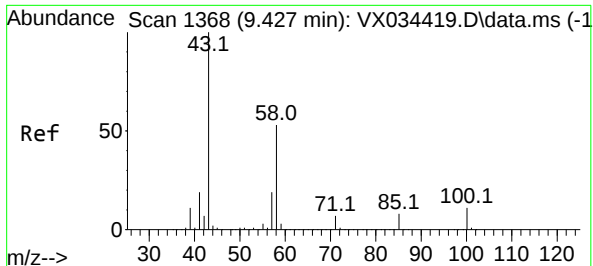

#59
2-Hexanone
Concen: 33.287 ug/l
RT: 9.482 min Scan# 11
Delta R.T. 0.055 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion: 43 Resp: 146778
Ion Ratio Lower Upper
43 100
58 18.4 26.3 78.9#

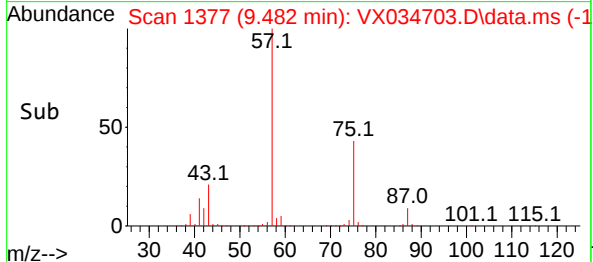

#60
Dibromochloromethane
Concen: 1.066 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.244 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion: 129 Resp: 4271
Ion Ratio Lower Upper
129 100
127 0.0 39.0 117.0#


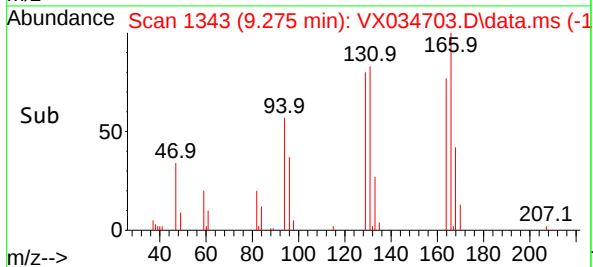

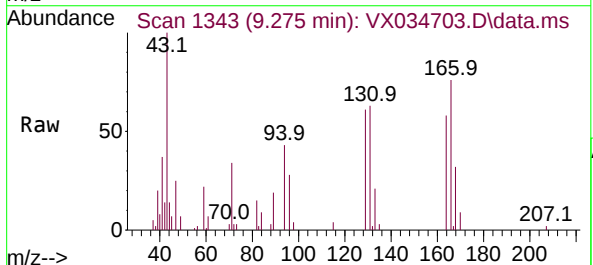




#62
4-Bromofluorobenzene
Concen: 46.391 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion: 95 Resp: 241976
Ion Ratio Lower Upper
95 100
174 70.6 0.0 147.4
176 68.8 0.0 140.6

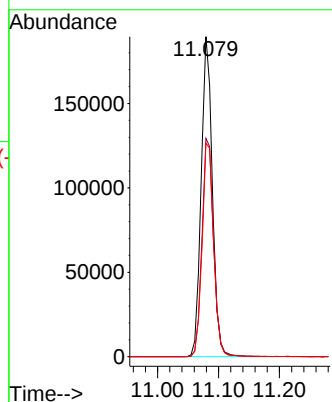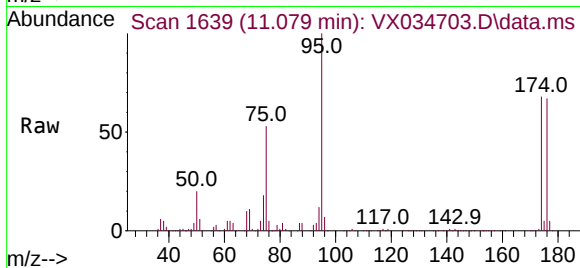

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion: 117 Resp: 468126
Ion Ratio Lower Upper
117 100
82 57.3 45.0 67.4
119 31.9 26.0 39.0


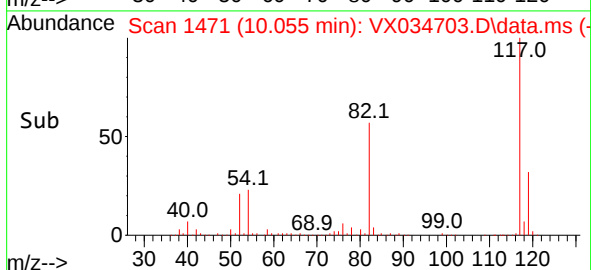

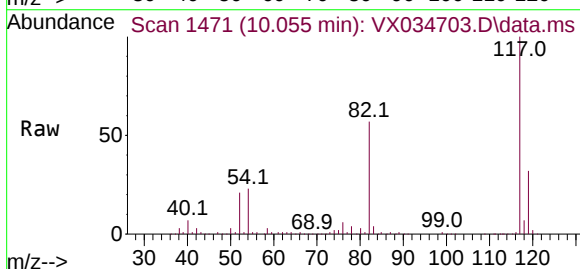




#64
Tetrachloroethene
Concen: 1.304 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion:164	Resp:	4101
Ion	Ratio	Lower Upper
164	100	
166	130.3	102.7 154.1
129	104.7	75.6 113.4
131	108.0	73.7 110.5

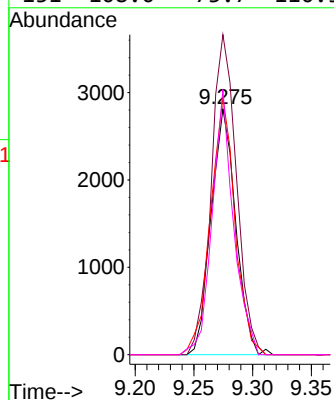

#67
Ethyl Benzene
Concen: 0.285 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion: 91	Resp:	5237
Ion	Ratio	Lower Upper
91	100	
106	36.5	25.6 38.4


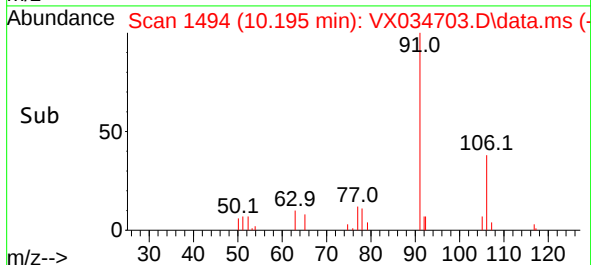
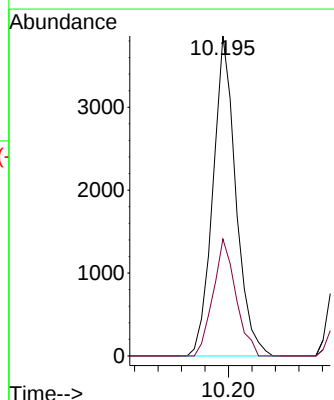
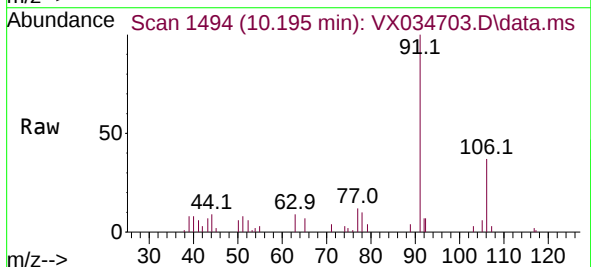




#68
m/p-Xylenes
Concen: 0.385 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion:106 Resp: 2722
Ion Ratio Lower Upper
106 100
91 229.8 164.0 246.0

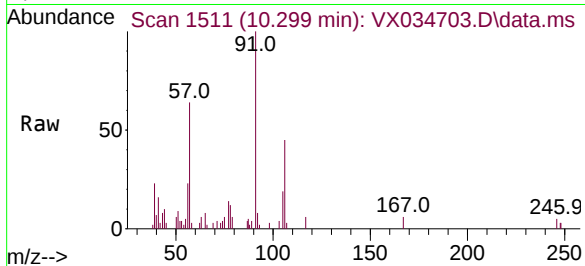

#69
o-Xylene
Concen: 0.226 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion:106 Resp: 1600
Ion Ratio Lower Upper
106 100
91 243.3 108.5 325.3


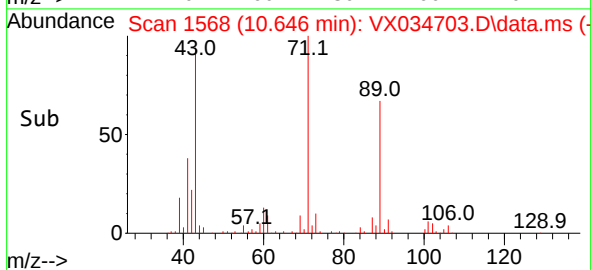

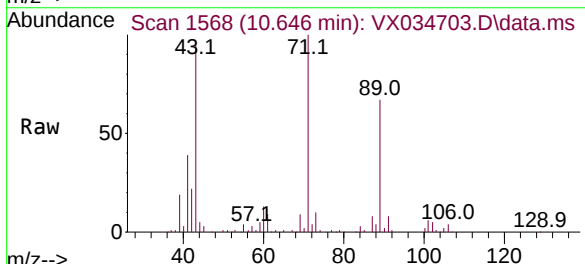




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX034703.D
 Acq: 23 Mar 2023 17:02




Instrument :
 MSVOA_X
 ClientSampleId :
 WC1-5-20230322


Tgt Ion:152 Resp: 212756
 Ion Ratio Lower Upper
 152 100
 115 62.9 45.0 135.0
 150 156.3 0.0 352.4

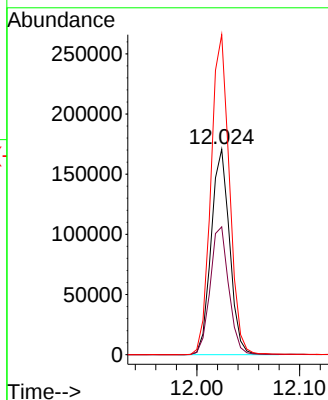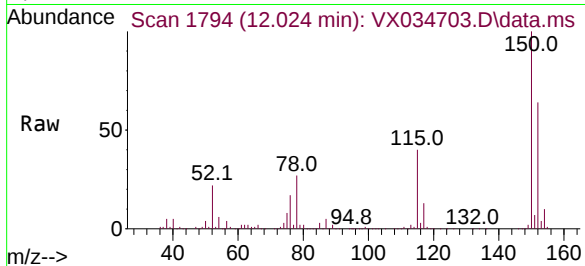

#74
 N-ethyl acetate
 Concen: 6.971 ug/l
 RT: 10.640 min Scan# 1567
 Delta R.T. -0.201 min
 Lab File: VX034703.D
 Acq: 23 Mar 2023 17:02

Tgt Ion: 43 Resp: 54899
 Ion Ratio Lower Upper
 43 100
 70 1.8 32.1 48.1#
 55 4.2 18.3 27.5#
 61 9.2 18.8 28.2#


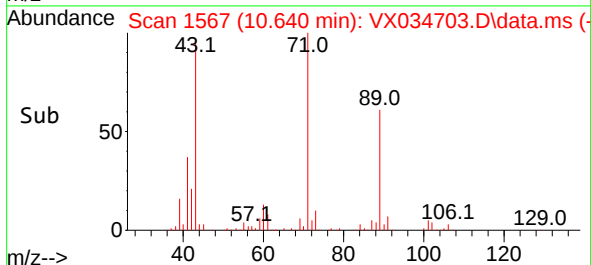
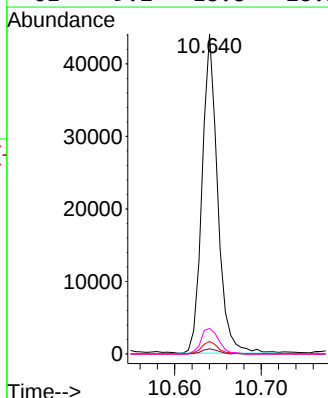
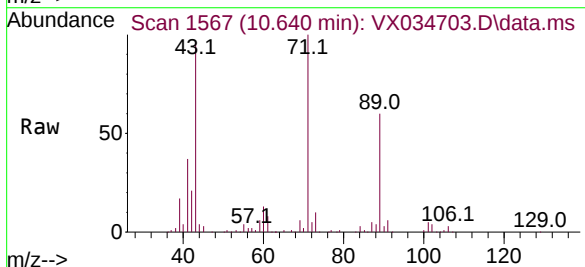




#76
1,2,3-Trichloropropane
Concen: 26.013 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02




Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322


Tgt Ion: 75 Resp: 127076
Ion Ratio Lower Upper
75 100
77 1.3 21.6 64.8#

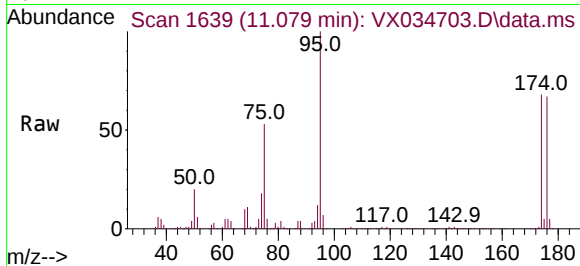

#81
trans-1,4-Dichloro-2-butene
Concen: 70.373 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Tgt Ion: 75 Resp: 127076
Ion Ratio Lower Upper
75 100
53 0.0 82.6 124.0#
89 0.0 36.9 55.3#

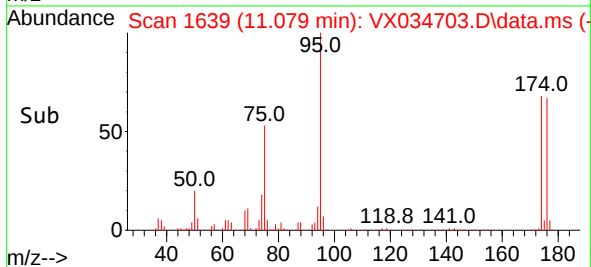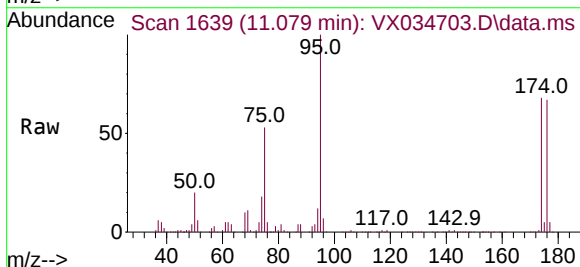



#95
Naphthalene
Concen: 0.507 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX034703.D
Acq: 23 Mar 2023 17:02

Instrument :
MSVOA_X
ClientSampleId :
WC1-5-20230322

Tgt Ion	Ratio	Lower	Upper
128	100		
127	12.5	10.2	15.4
129	12.0	8.6	13.0

