

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032323\
 Data File : VX034705.D
 Acq On : 23 Mar 2023 17:49
 Operator : JC/MD
 Sample : 02055-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-2A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
 Title : SW846 8260

Signal : TIC: VX034705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.751	104	109	116	rBV2	13108	19046	1.19%	0.214%
2	2.788	270	279	289	rBV3	12038	29610	1.84%	0.332%
3	3.105	323	331	342	rVB3	9459	22406	1.40%	0.252%
4	5.385	693	705	718	rBV2	178468	523611	32.62%	5.879%
5	5.549	722	732	755	rVB	319513	938521	58.47%	10.537%
6	5.958	788	799	815	rBV	212436	579769	36.12%	6.509%
7	6.263	840	849	858	rVB5	5609	16262	1.01%	0.183%
8	6.763	921	931	946	rBV	497574	1207761	75.25%	13.560%
9	8.646	1234	1240	1252	rVB	1018366	1605045	100.00%	18.021%
10	10.055	1465	1471	1485	rBV	1026260	1383677	86.21%	15.535%
11	11.079	1634	1639	1650	rBV	819667	1060891	66.10%	11.911%
12	11.890	1770	1772	1780	rVB	13561	16321	1.02%	0.183%
13	12.024	1788	1794	1804	rBV	971580	1243592	77.48%	13.963%
14	12.243	1824	1830	1836	rBV2	56415	74502	4.64%	0.836%
15	12.335	1843	1845	1852	rVB2	12546	16242	1.01%	0.182%
16	12.646	1893	1896	1901	rVV3	15633	20339	1.27%	0.228%
17	12.701	1901	1905	1912	rVB	52916	67942	4.23%	0.763%
18	13.170	1979	1982	1985	rBV	17623	19546	1.22%	0.219%
19	13.639	2052	2059	2060	rVV2	19222	31574	1.97%	0.354%
20	13.664	2060	2063	2068	rVB	22521	29980	1.87%	0.337%




Sum of corrected areas: 8906637

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032323\
Data File : VX034705.D
Acq On : 23 Mar 2023 17:49
Operator : JC/MD
Sample : 02055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

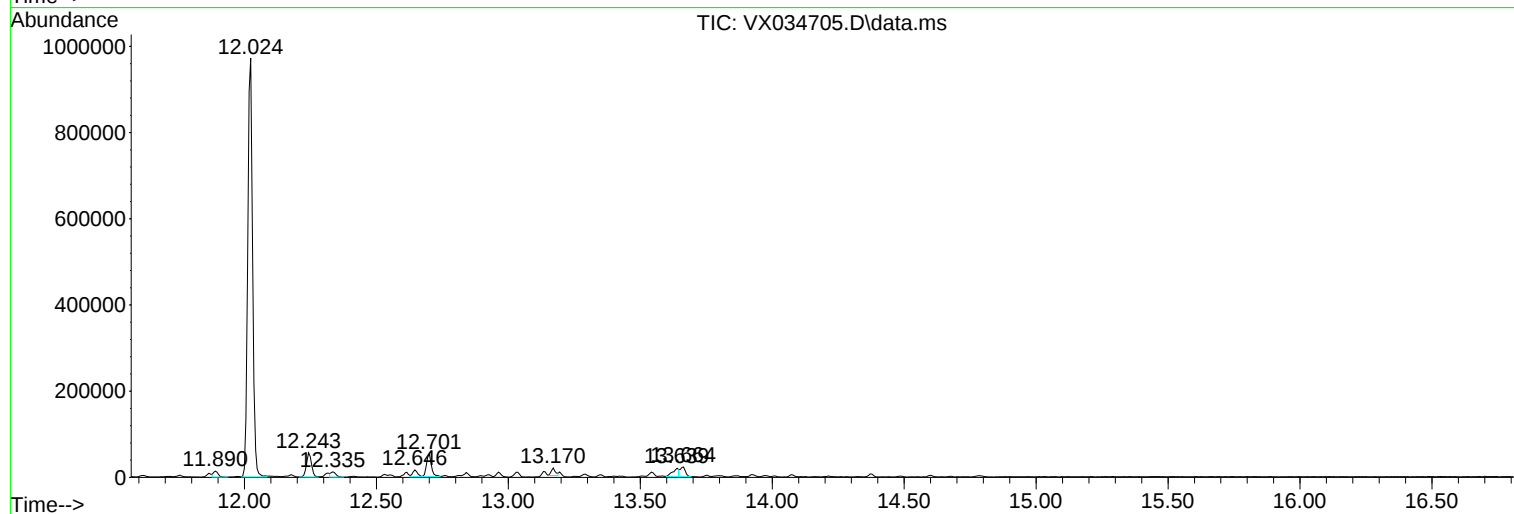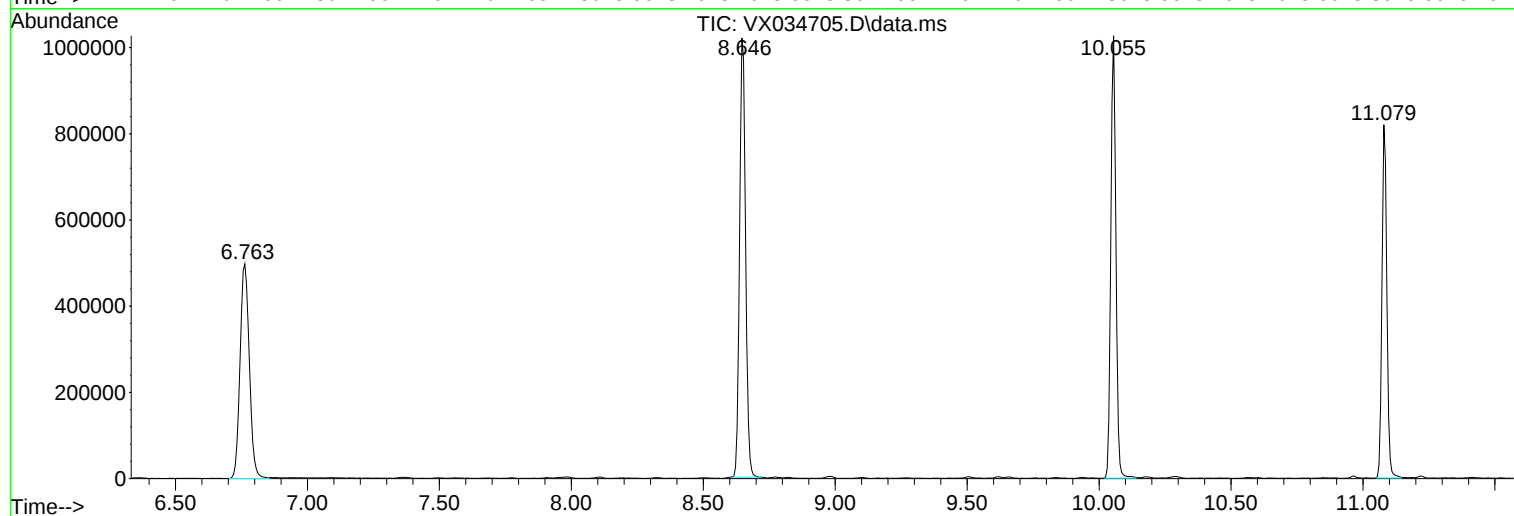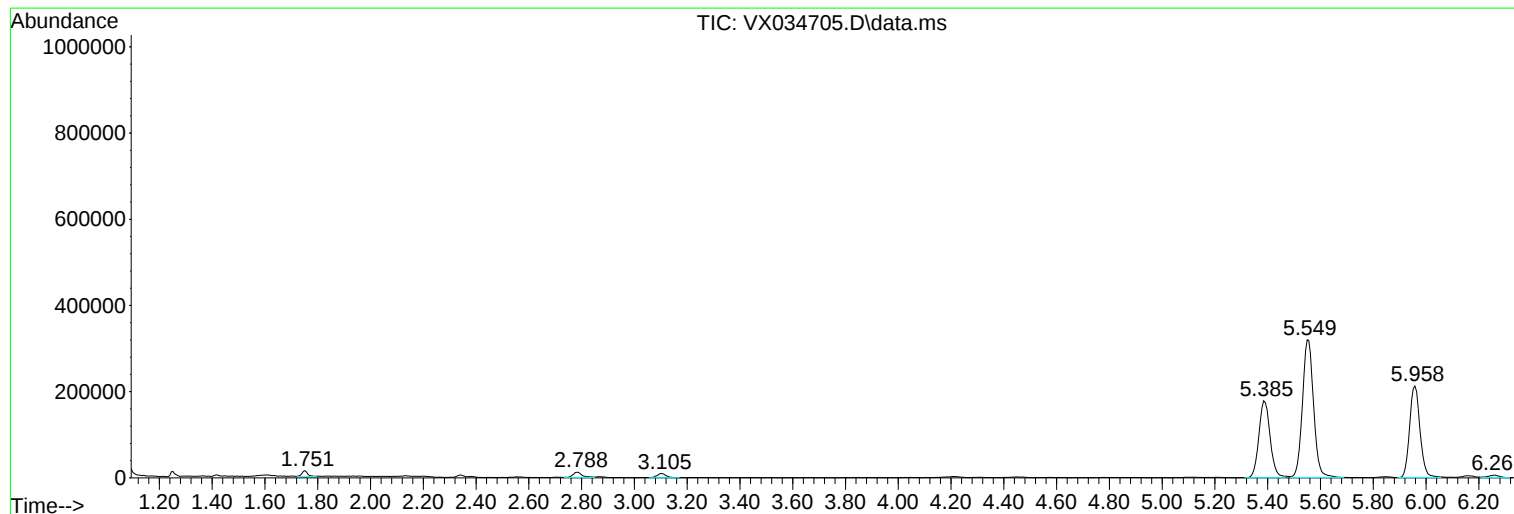

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032323\
Data File : VX034705.D
Acq On : 23 Mar 2023 17:49
Operator : JC/MD
Sample : 02055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032323\
Data File : VX034705.D
Acq On : 23 Mar 2023 17:49
Operator : JC/MD
Sample : 02055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X031023W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------