

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032323\  
Data File : VX034707.D  
Acq On : 23 Mar 2023 18:35  
Operator : JC/MD  
Sample : 02055-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M

Title : SW846 8260

Signal : TIC: VX034707.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 693           | 705         | 722          | rBV      | 183253         | 537054        | 32.66%          | 6.203%        |
| 2         | 5.550       | 722           | 732         | 752          | rVB      | 328966         | 938751        | 57.09%          | 10.842%       |
| 3         | 5.958       | 788           | 799         | 820          | rBV      | 217634         | 593319        | 36.08%          | 6.853%        |
| 4         | 6.763       | 919           | 931         | 947          | rBV      | 511374         | 1223177       | 74.39%          | 14.127%       |
| 5         | 8.647       | 1234          | 1240        | 1259         | rBV      | 1049737        | 1644346       | 100.00%         | 18.992%       |
| 6         | 10.055      | 1465          | 1471        | 1492         | rBV      | 1047610        | 1411889       | 85.86%          | 16.307%       |
| 7         | 11.079      | 1634          | 1639        | 1651         | rBV      | 825017         | 1070336       | 65.09%          | 12.362%       |
| 8         | 12.024      | 1788          | 1794        | 1809         | rBV      | 987178         | 1239292       | 75.37%          | 14.314%       |




Sum of corrected areas: 8658164

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032323\  
Data File : VX034707.D  
Acq On : 23 Mar 2023 18:35  
Operator : JC/MD  
Sample : 02055-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

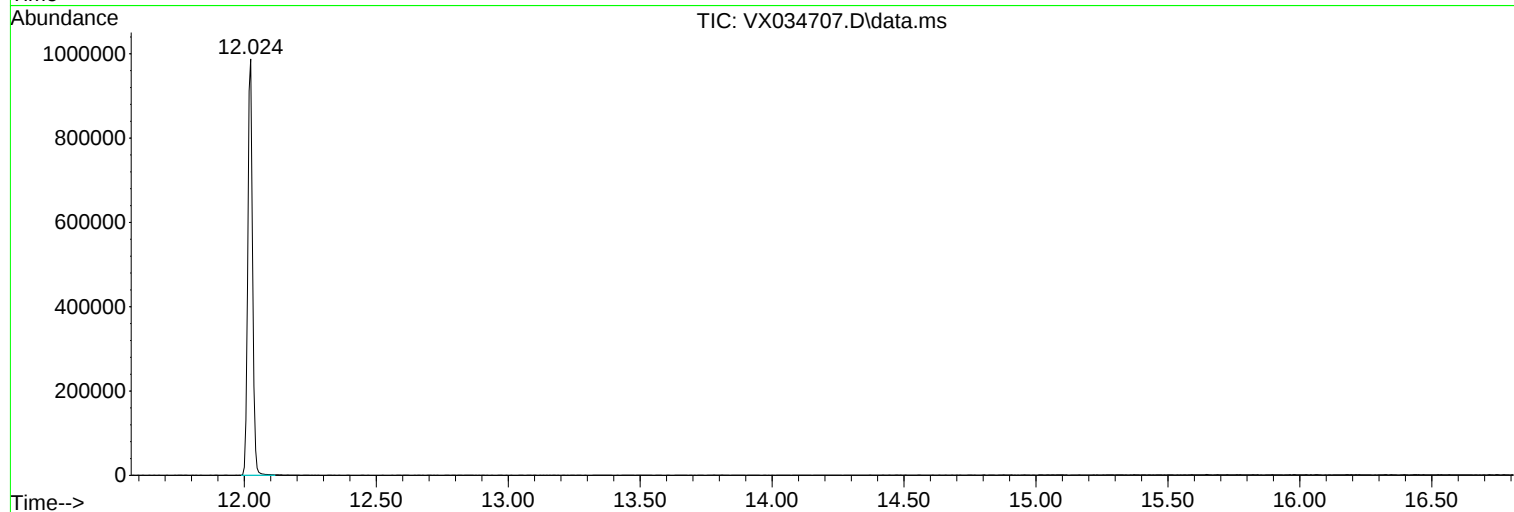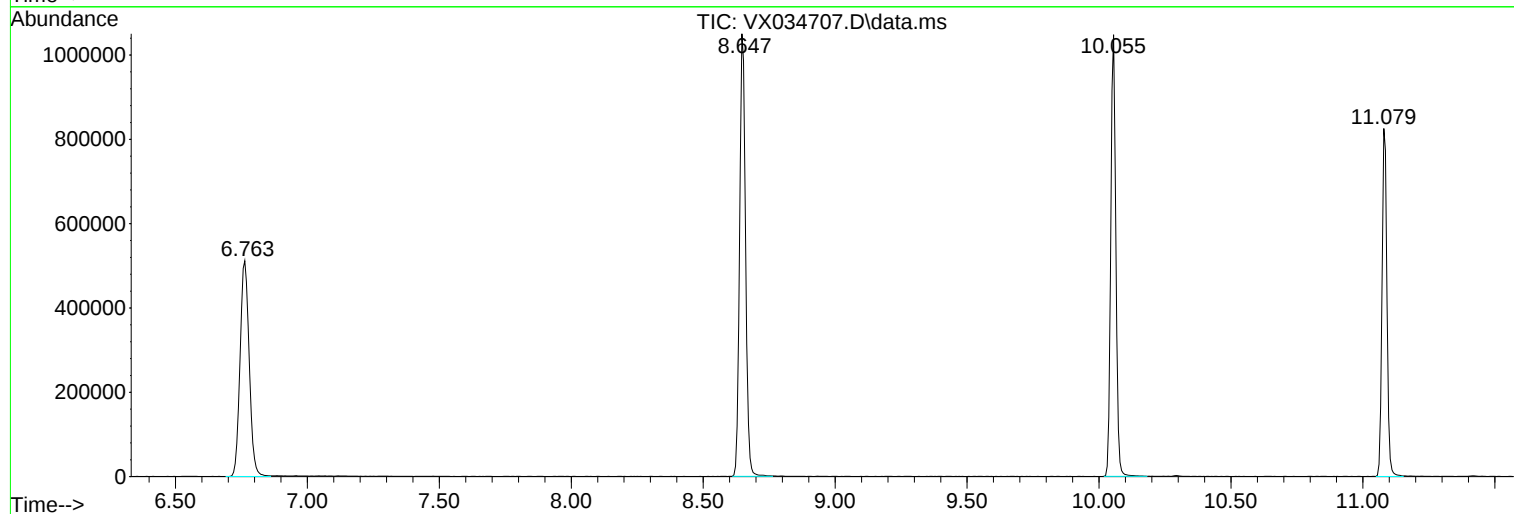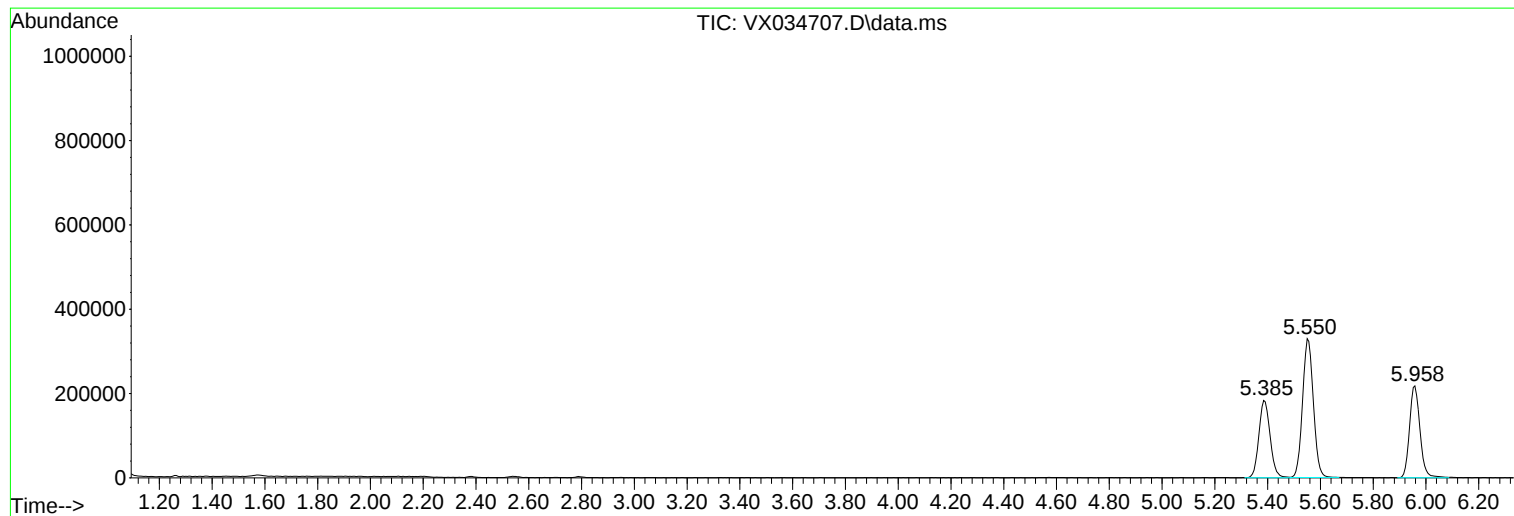

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032323\  
Data File : VX034707.D  
Acq On : 23 Mar 2023 18:35  
Operator : JC/MD  
Sample : 02055-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032323\  
Data File : VX034707.D  
Acq On : 23 Mar 2023 18:35  
Operator : JC/MD  
Sample : 02055-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X031023W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|