


Data Path : W:\HPCHEM1\MSVOA X\Data\VX032718\
Data File : VX000456.D
Acq On : 27 Mar 2018 12:05
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Title : SW846 8260
Last Update : Wed Mar 21 04:52:42 2018

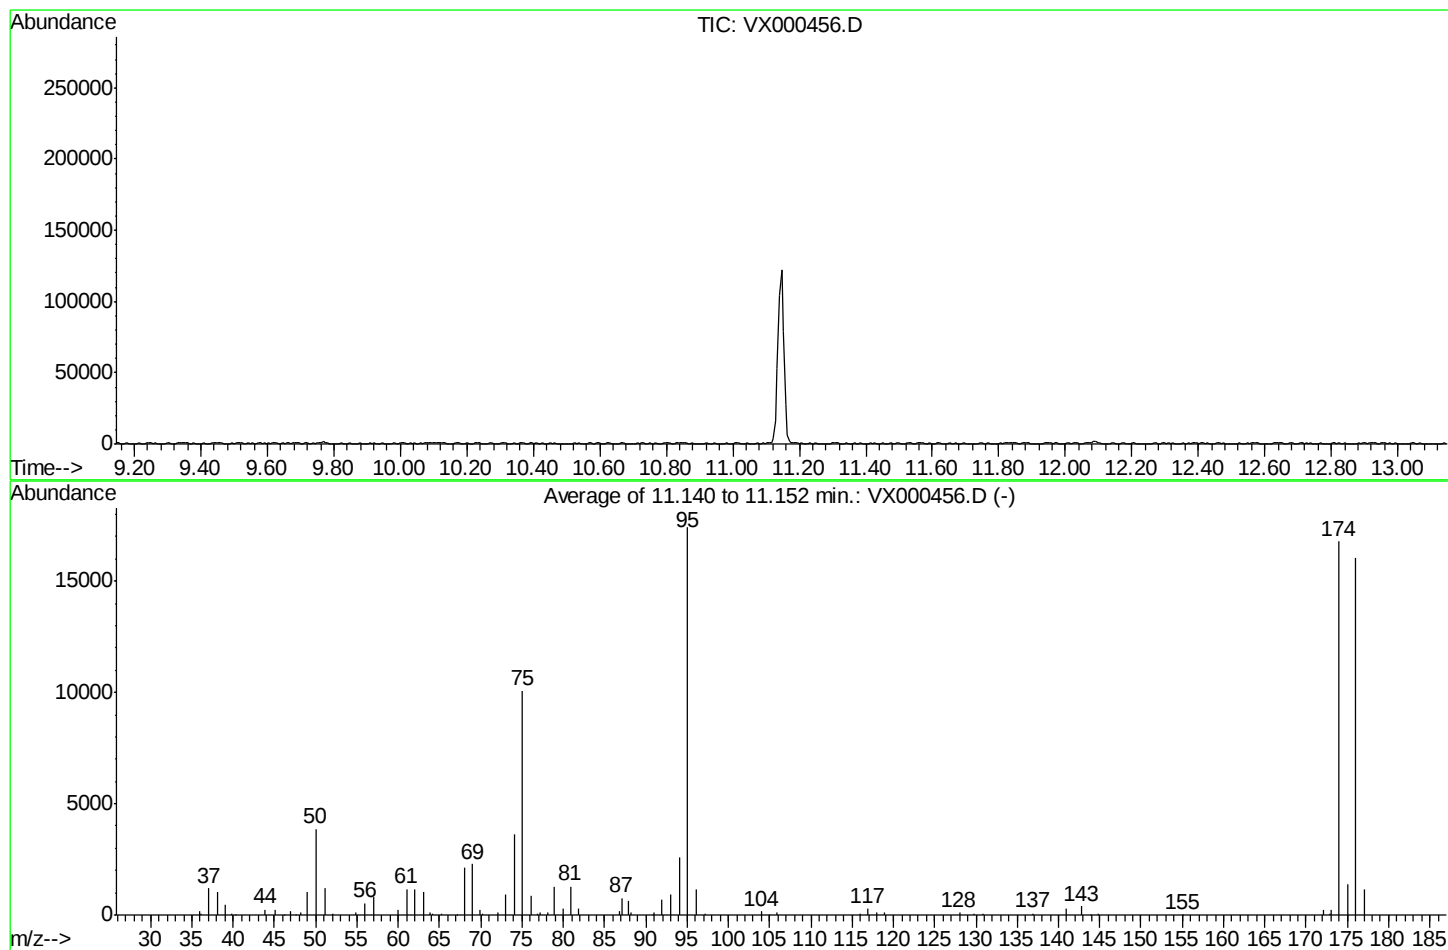

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	3860	PASS
75	95	30	60	57.8	10070	PASS
95	95	100	100	100.0	17420	PASS
96	95	5	9	6.8	1176	PASS
173	174	0.00	2	1.3	224	PASS
174	95	50	100	96.3	16771	PASS
175	174	5	9	8.2	1376	PASS
176	174	95	101	95.8	16066	PASS
177	176	5	9	7.0	1131	PASS