

Data File : VX000523.D

Acq On : 29 Mar 2018 19:48

Operator : JC/MD

Sample : J2098-01

Misc : 5.0mL/MSVOA_X/WATER

ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-5

Quant Time: Mar 30 06:56:09 2018

Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M

Quant Title : SW846 8260

QLast Update : Wed Mar 21 04:52:42 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.68	168	107881	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	198588	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	201314	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	107255	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.08	65	79375	56.37	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.74%	
35) Dibromofluoromethane	5.52	113	61227	48.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.86%	
50) Toluene-d8	8.73	98	253971	49.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.02%	
62) 4-Bromofluorobenzene	11.15	95	91368	42.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	85.48%	

Target Compounds

						Qvalue
3) Chloromethane	1.32	50	333	0.27	ug/l #	34
4) Vinyl Chloride	1.28	62	1625	1.23	ug/l #	44
5) Bromomethane	1.66	94	1278	0.85	ug/l	90
6) Chloroethane	1.69	64	316	Below Cal	#	44
10) Methyl Iodide	2.52	142	521	4.64	ug/l #	43
11) Tert butyl alcohol	3.07	59	1328	2.74	ug/l #	89
13) Acrolein	2.32	56	57	14.93	ug/l #	13
14) Allyl chloride	2.71	41	1623	0.69	ug/l #	38
16) Acetone	2.45	43	19833	16.93	ug/l	98
18) Methyl Acetate	2.77	43	525	0.21	ug/l #	51
25) 2-Butanone	4.73	43	3974	3.02	ug/l	99
29) Tetrahydrofuran	5.18	42	2340	2.89	ug/l	95
31) Cyclohexane	5.68	56	2884	1.62	ug/l #	42
36) 1,1-Dichloropropene	5.68	75	8347	4.49	ug/l #	48
37) Ethyl Acetate	4.73	43	3974	1.56	ug/l #	69
38) Carbon Tetrachloride	5.67	117	10645	5.45	ug/l #	16
40) Benzene	6.15	78	3605	0.67	ug/l	97
51) 4-Methyl-2-Pentanone	8.67	43	1926	0.66	ug/l	91
68) m/p-Xylenes	10.37	106	1148	0.38	ug/l	87
69) o-Xylene	10.71	106	762	0.26	ug/l	85
74) N-amyl acetate	6.45	43	25	Below Cal	#	59
76) 1,2,3-Trichloropropane	11.15	75	52340	22.71	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.15	75	52340	73.52	ug/l #	9
84) 1,2,4-Trimethylbenzene	11.82	105	1262	0.20	ug/l	90
86) p-Isopropyltoluene	12.07	119	4817	0.73	ug/l	88
95) Naphthalene	13.85	128	5379	0.61	ug/l	97

(#)=qualifier out of range (m)=manual integration (+)=signals summed

Data File : VX000523.D

Acq On : 29 Mar 2018 19:48

Operator : JC/MD

Sample : J2098-01

Misc : 5.0mL/MSVOA_X/WATER

ALS Vial : 19 Sample Multiplier: 1

Instrument :

MSVOA_X

ClientSampleId :

MW-5


Quant Time: Mar 30 06:56:09 2018


Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M

Quant Title : SW846 8260

QLast Update : Wed Mar 21 04:52:42 2018

Response via : Initial Calibration




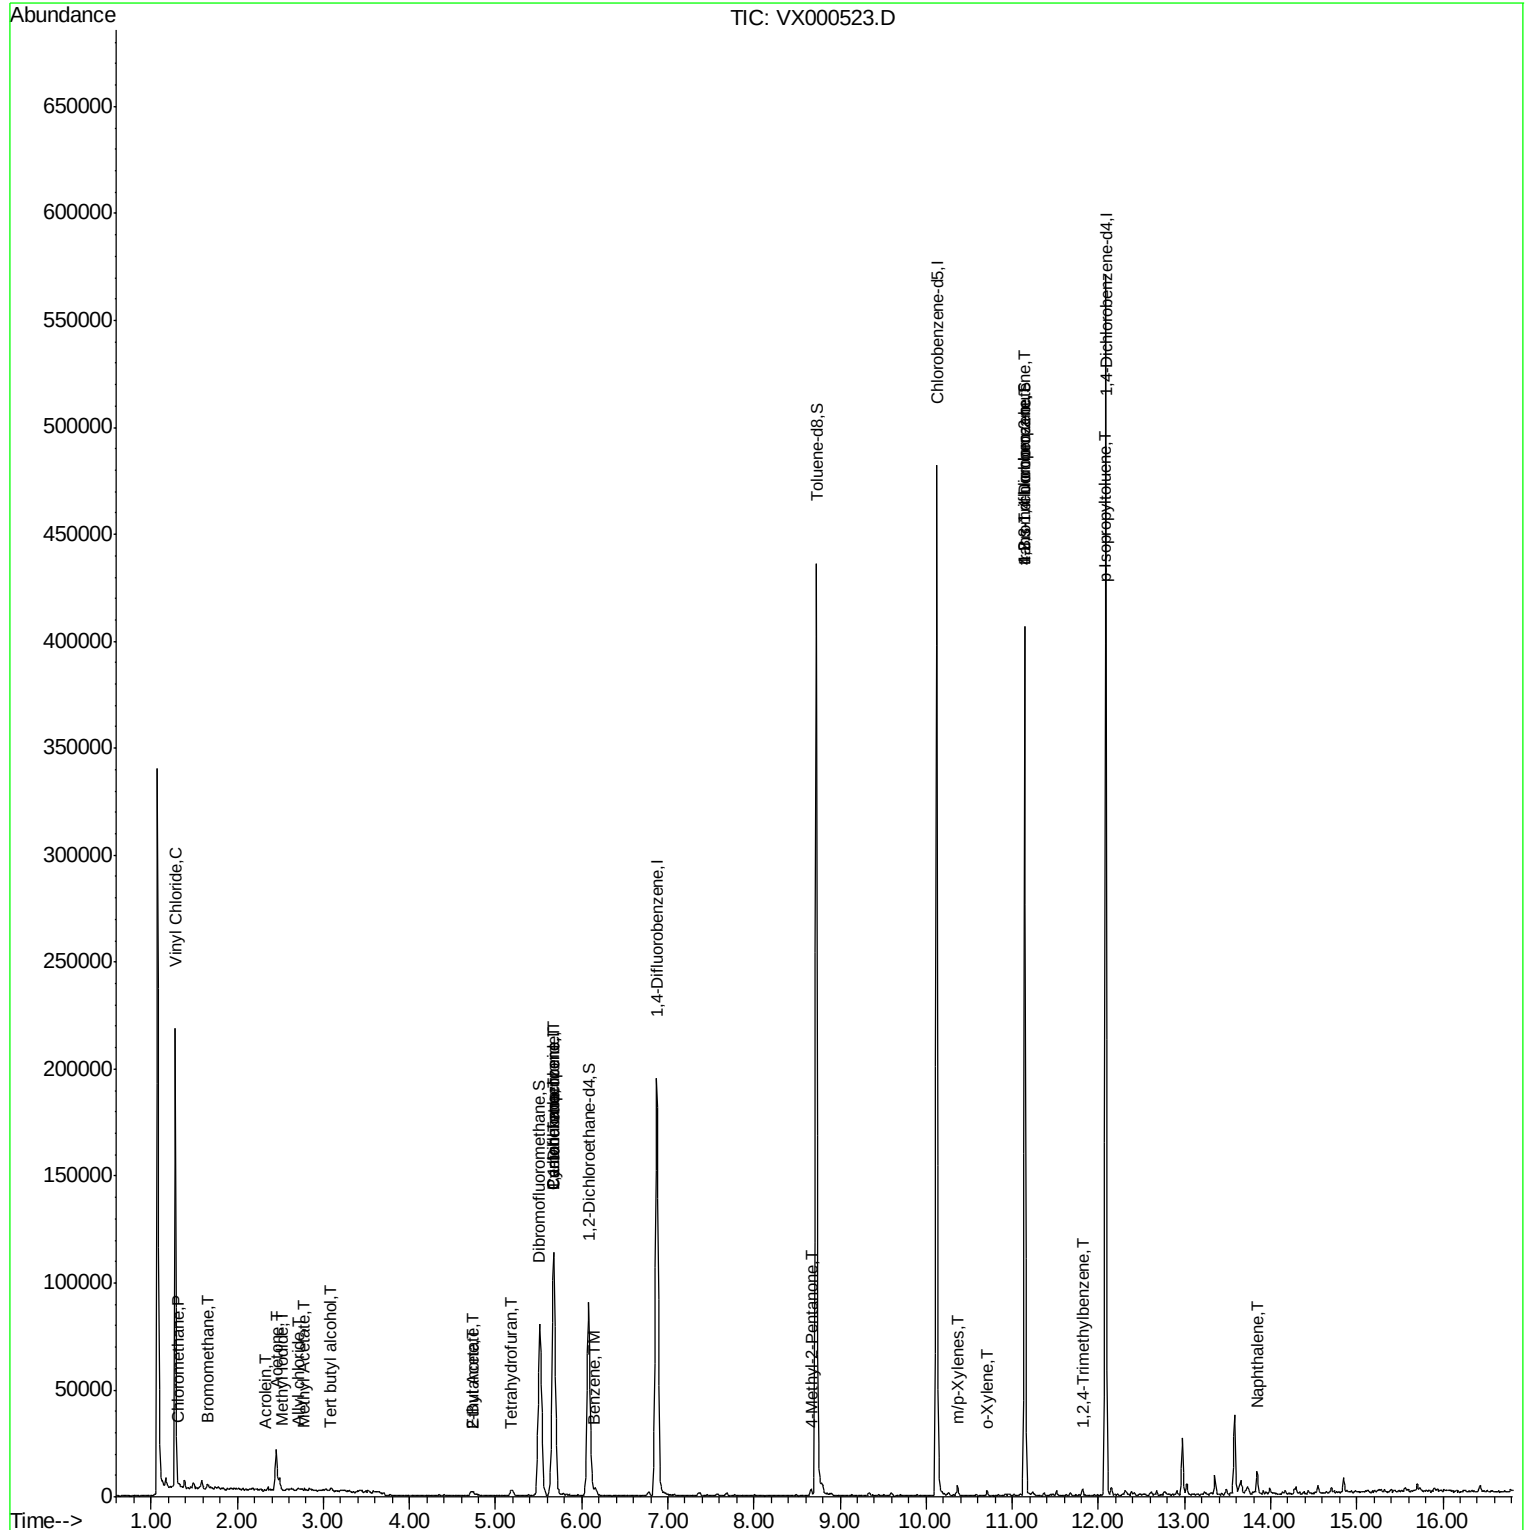




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.68 min Scan# 835
Delta R.T. 0.00 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48




Instrument :
MSVOA_X
ClientSampled :
MW-5


Tgt Ion: 168 Resp: 107881
Ion Ratio Lower Upper
168 100
99 50.3 45.8 68.6

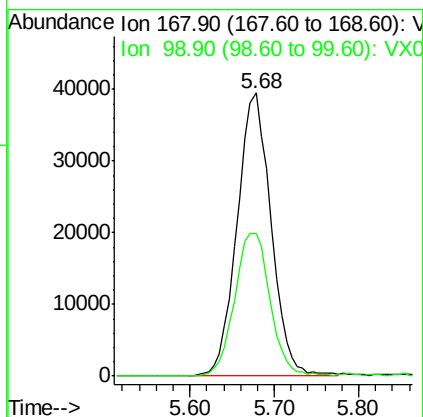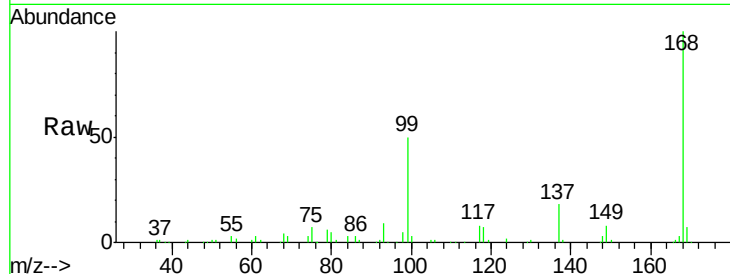

#3
Chloromethane
Concen: 0.27 ug/l
RT: 1.32 min Scan# 121
Delta R.T. 0.00 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48

Tgt Ion: 50 Resp: 333
Ion Ratio Lower Upper
50 100
52 72.5 27.5 41.3#

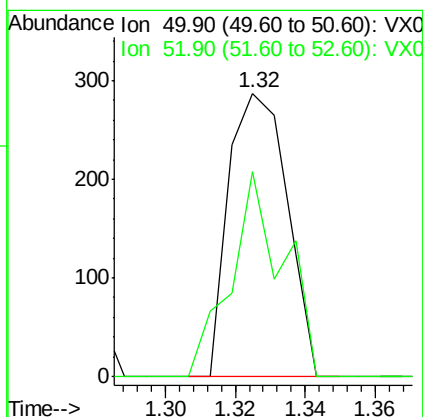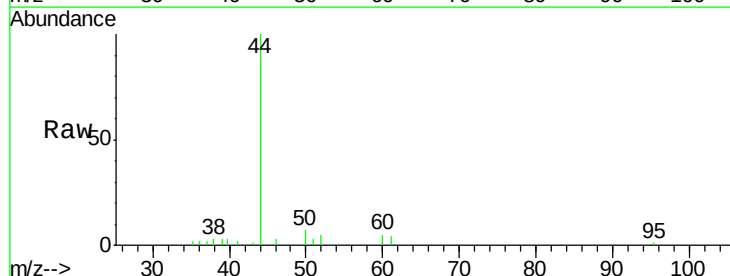



#4

Vinyl Chloride

Concen: 1.23 ug/l

RT: 1.28 min Scan# 114

Delta R.T. -0.13 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampled :





MW-5

Tgt Ion: 62 Resp: 1625

Ion Ratio Lower Upper

62 100

64 0.0 24.8 37.2#

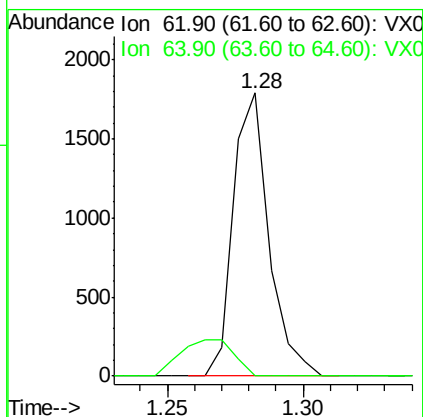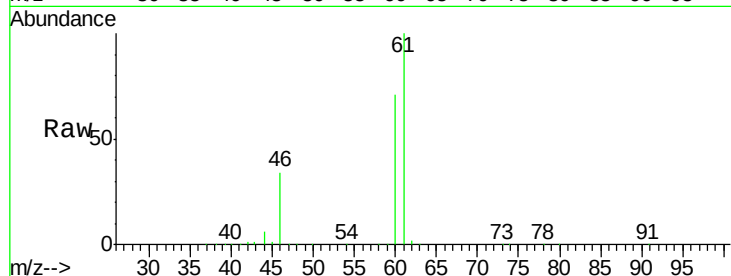

#5

Bromomethane

Concen: 0.85 ug/l

RT: 1.66 min Scan# 176

Delta R.T. 0.02 min

Lab File: VX000523.D




Acq: 29 Mar 2018 19:48


Tgt Ion: 94 Resp: 1278

Ion Ratio Lower Upper

94 100

96 86.8 77.7 116.5

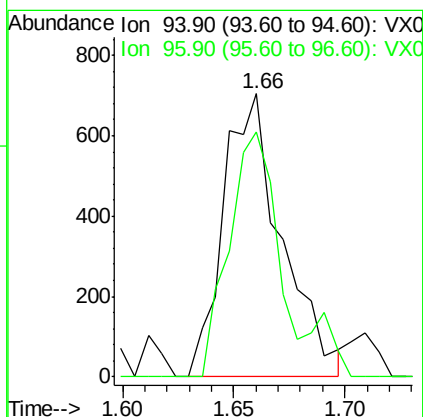

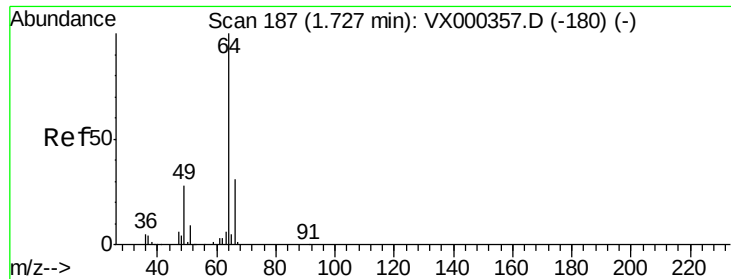

#6

Chloroethane

Concen: Below Cal

RT: 1.69 min Scan# 181

Delta R.T. -0.04 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampled :





MW-5

Tgt Ion: 64 Resp: 316

Ion Ratio Lower Upper

64 100

66 0.0 24.8 37.2#

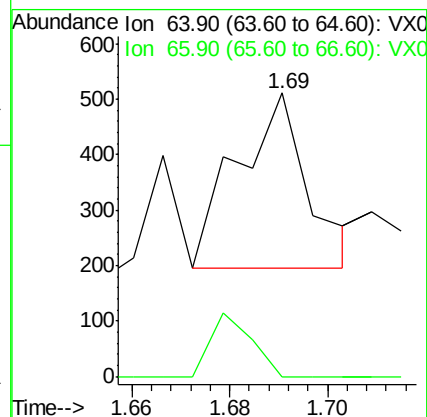

#10

Methyl Iodide

Concen: 4.64 ug/l

RT: 2.52 min Scan# 317

Delta R.T. 0.00 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48




Tgt Ion: 142 Resp: 521


Ion Ratio Lower Upper

142 100

127 6.1 39.2 58.8#

141 0.0 11.7 17.5#



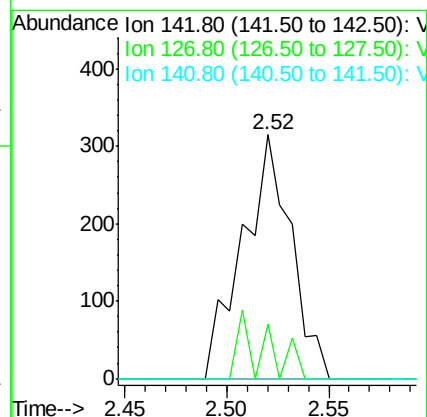





#11
Tert butyl alcohol
Concen: 2.74 ug/l
RT: 3.07 min Scan# 408
Delta R.T. 0.00 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48




Instrument :
MSVOA_X
ClientSampled :
MW-5


Tgt Ion: 59 Resp: 1328
Ion Ratio Lower Upper
59 100
57 6.5 8.4 12.6#

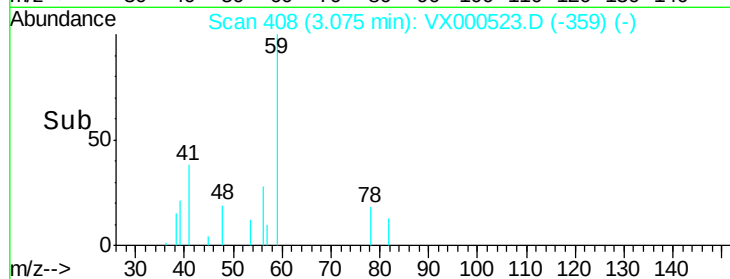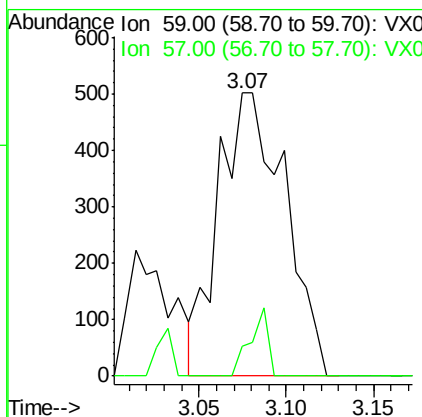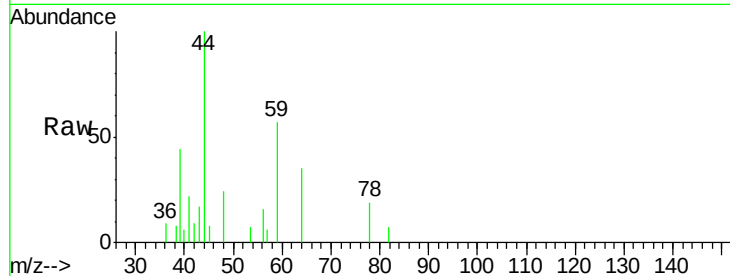

#13
Acrolein
Concen: 14.93 ug/l
RT: 2.32 min Scan# 285
Delta R.T. 0.02 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48

Tgt Ion: 56 Resp: 57
Ion Ratio Lower Upper
56 100
55 0.0 58.8 88.2#

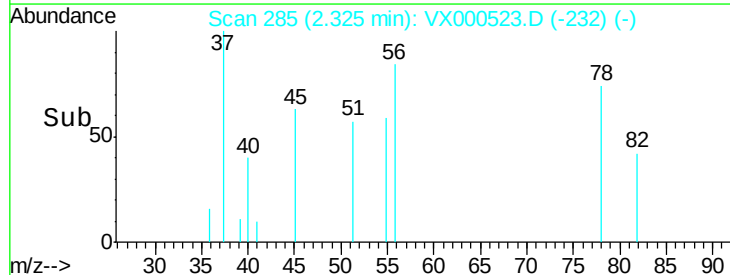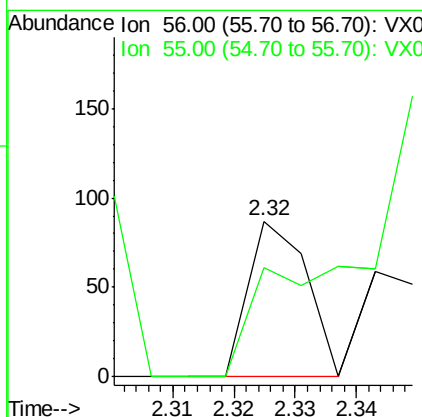

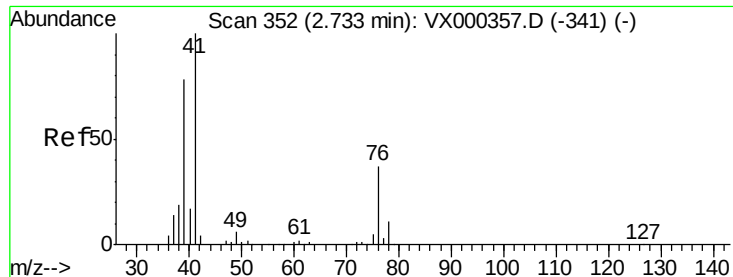

#14

Allyl chloride

Concen: 0.69 ug/l

RT: 2.71 min Scan# 349

Delta R.T. -0.02 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampled :

MW-5


Tgt Ion: 41 Resp: 1623

Ion Ratio Lower Upper

41 100

39 19.8 57.6 86.4#




76 0.0 27.3 40.9#

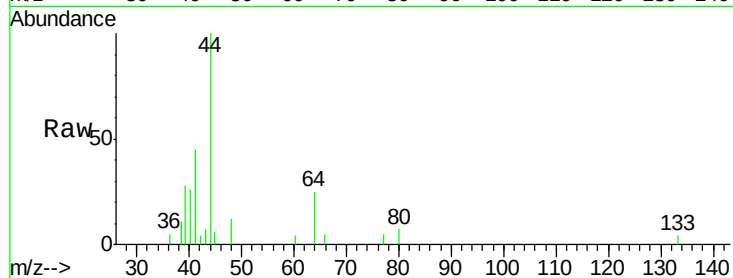

Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

Ion 75.90 (75.60 to 76.60): VX0

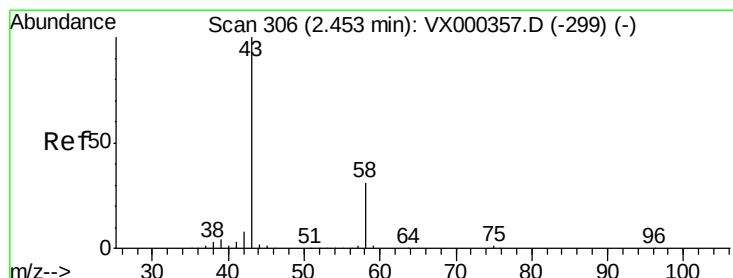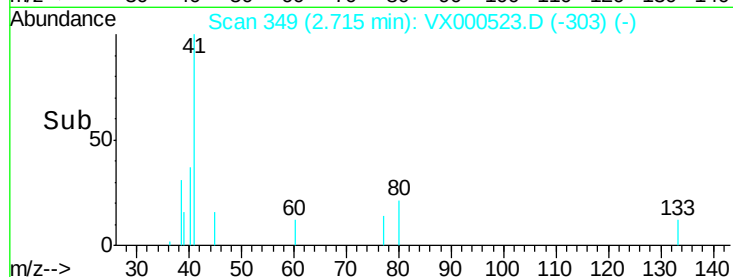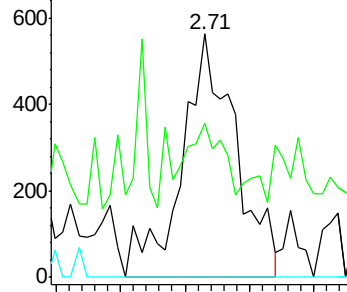

#16

Acetone

Concen: 16.93 ug/l

RT: 2.45 min Scan# 306

Delta R.T. 0.00 min

Lab File: VX000523.D


Acq: 29 Mar 2018 19:48

Tgt Ion: 43 Resp: 19833

Ion Ratio Lower Upper



43 100


58 31.9 24.7 37.1

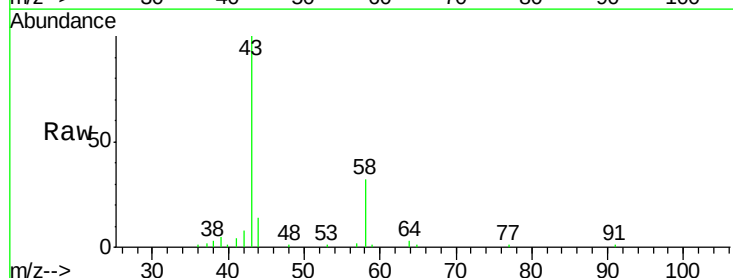

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



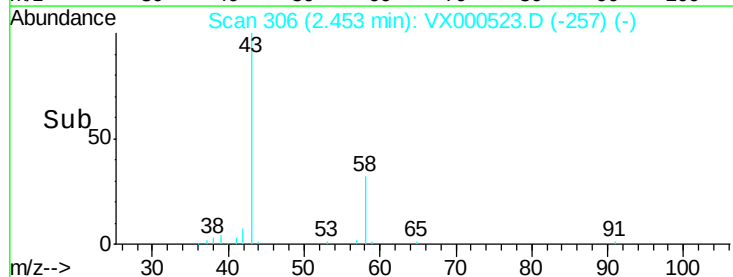
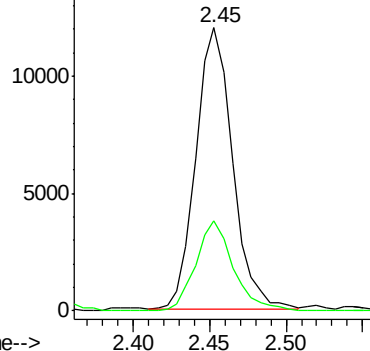


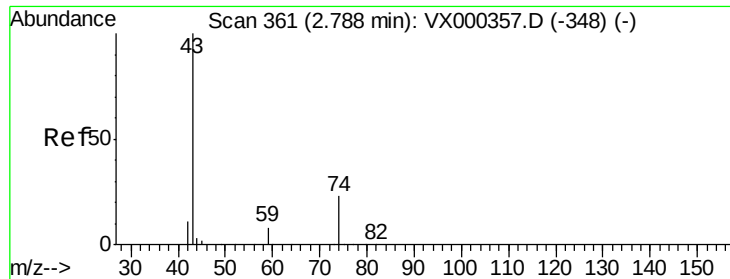

#18
Methyl Acetate
Concen: 0.21 ug/l
RT: 2.77 min Scan# 358
Delta R.T. -0.02 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48




Instrument :
MSVOA_X
ClientSampled :
MW-5


Tgt Ion: 43 Resp: 525
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.2#

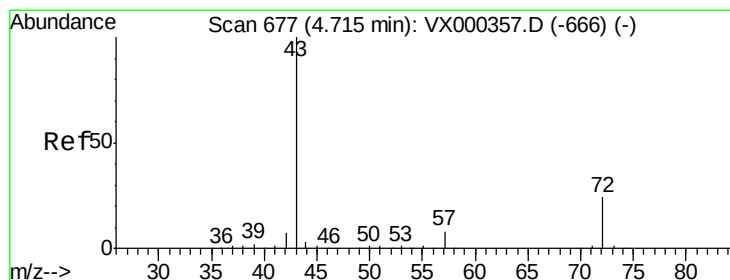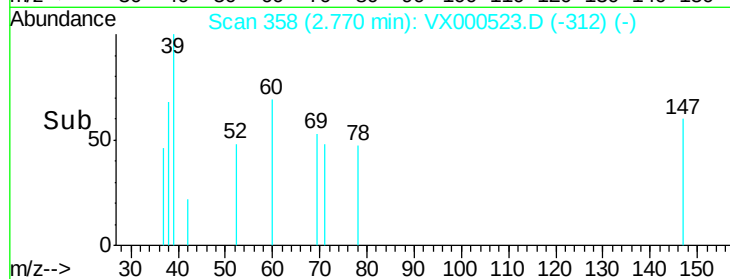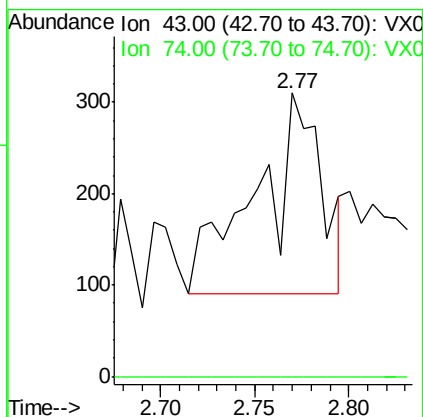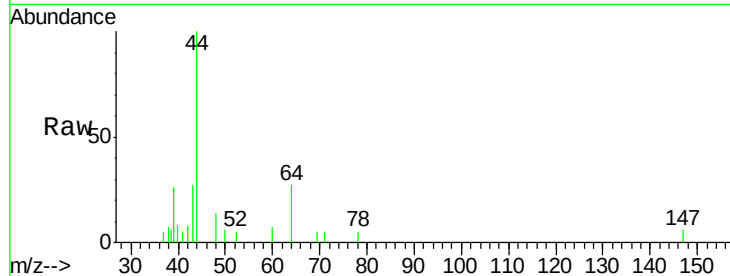

#25
2-Butanone
Concen: 3.02 ug/l
RT: 4.73 min Scan# 680
Delta R.T. 0.02 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48

Tgt Ion: 43 Resp: 3974
Ion Ratio Lower Upper
43 100
72 26.7 21.0 31.6

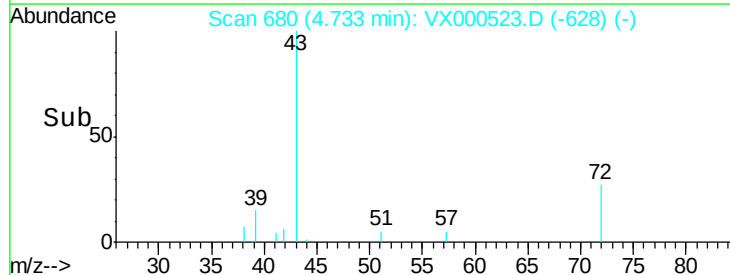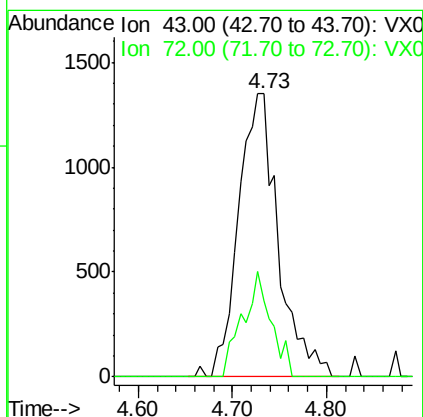



#29

Tetrahydrofuran

Concen: 2.89 ug/l

RT: 5.18 min Scan# 754

Delta R.T. 0.01 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampleId :

MW-5


Tgt Ion: 42 Resp: 2340

Ion Ratio Lower Upper

42 100

72 42.2 37.9 56.9




71 43.8 34.4 51.6



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

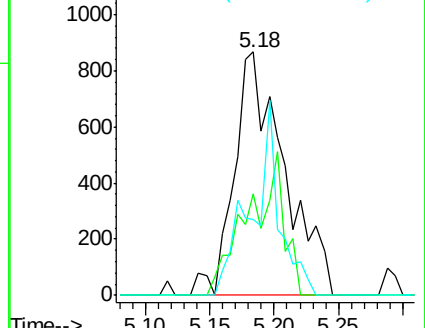

#31

Cyclohexane

Concen: 1.62 ug/l

RT: 5.68 min Scan# 835

Delta R.T. 0.09 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48


Tgt Ion: 56 Resp: 2884

Ion Ratio Lower Upper

56 100

69 103.4 23.4 35.0#



84 117.8 71.0 106.4#




Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

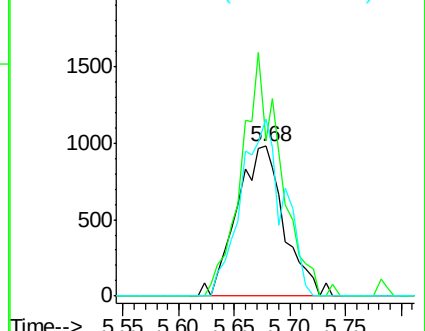

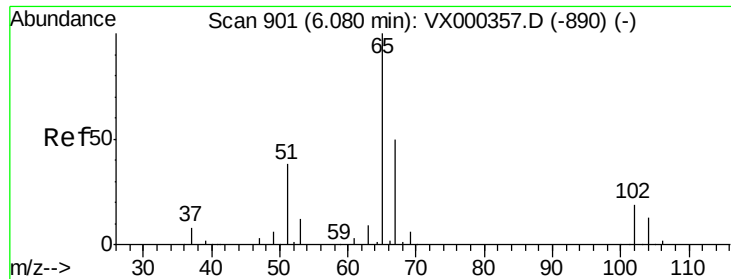

#33

1,2-Dichloroethane-d4

Concen: 56.37 ug/l

RT: 6.08 min Scan# 901

Delta R.T. 0.00 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampleId :


MW-5

Tgt Ion: 65 Resp: 79375

Ion Ratio Lower Upper




65 100

67 51.1 0.0 103.2

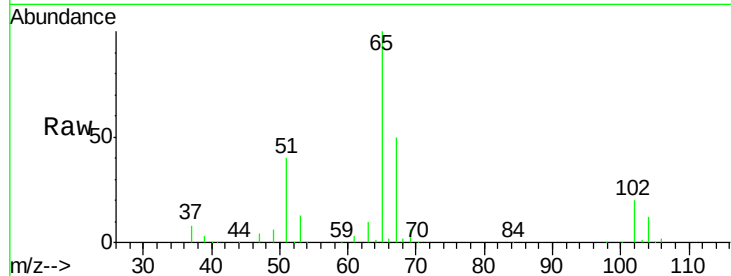

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

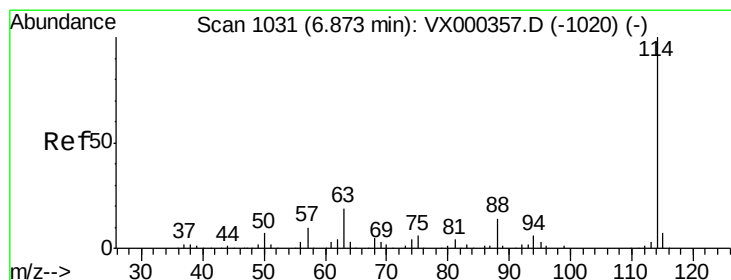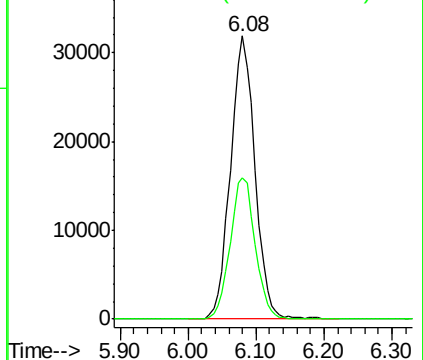

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48


Tgt Ion: 114 Resp: 198588

Ion Ratio Lower Upper

114 100

63 19.0 0.0 38.4



88 14.6 0.0 27.0




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

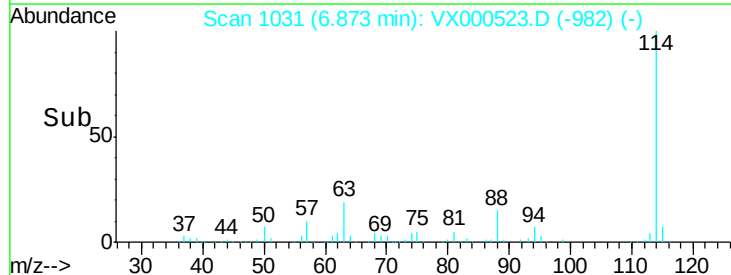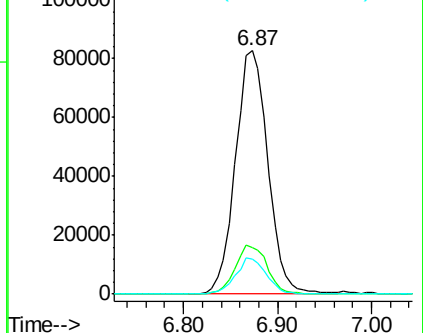



#35

Dibromofluoromethane

Concen: 48.93 ug/l

RT: 5.52 min Scan# 809

Delta R.T. 0.01 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampleId :

MW-5


Tgt Ion:113 Resp: 61227

Ion Ratio Lower Upper

113 100

111 103.9 82.4 123.6




192 20.7 15.8 23.6

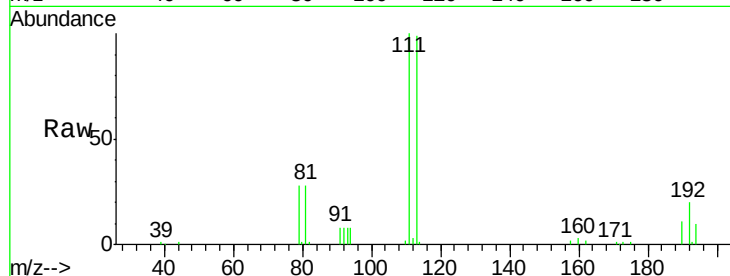

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

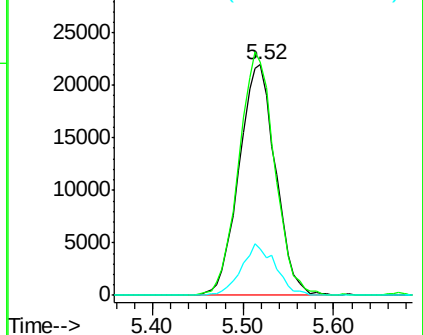

#36

1,1-Dichloropropene

Concen: 4.49 ug/l

RT: 5.68 min Scan# 835

Delta R.T. -0.13 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48


Tgt Ion: 75 Resp: 8347

Ion Ratio Lower Upper

75 100

110 6.9 17.9 53.7#



77 0.0 24.0 36.0#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

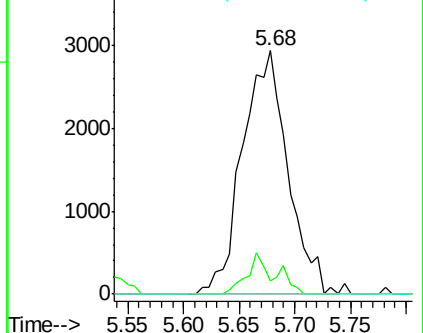

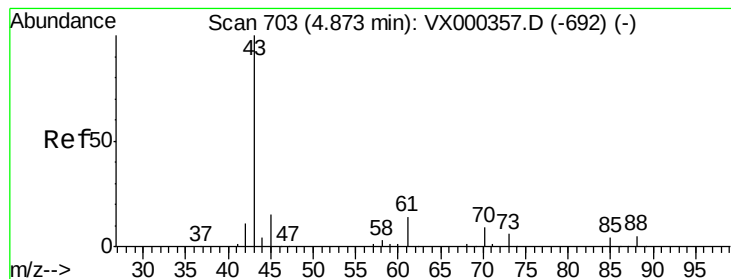

#37

Ethyl Acetate

Concen: 1.56 ug/l

RT: 4.73 min Scan# 680

Delta R.T. -0.14 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampleId :

MW-5


Tgt Ion: 43 Resp: 3974

Ion Ratio Lower Upper

43 100

61 0.0 11.1 16.7#




70 0.0 7.7 11.5#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

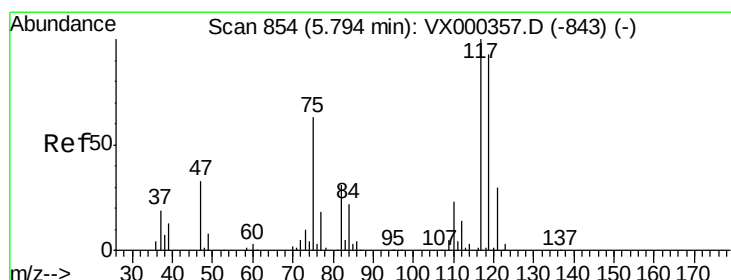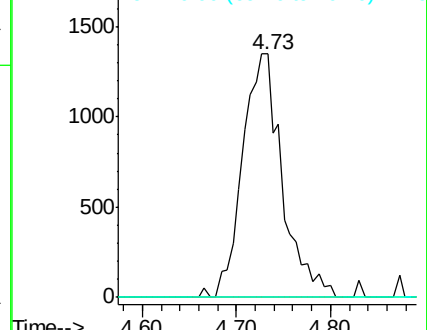

#38

Carbon Tetrachloride

Concen: 5.45 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.12 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48


Tgt Ion: 117 Resp: 10645

Ion Ratio Lower Upper

117 100

119 5.7 77.4 116.2#



121 0.0 24.8 37.2#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

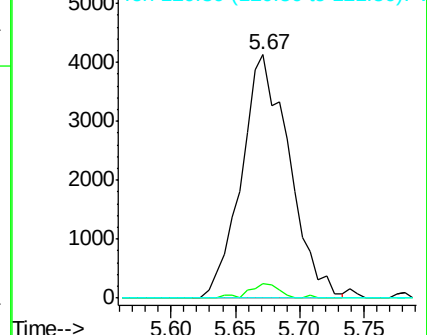

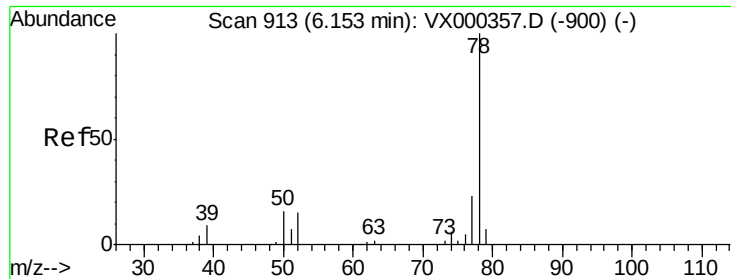

#40

Benzene

Concen: 0.67 ug/l

RT: 6.15 min Scan# 913

Delta R.T. 0.00 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampled :





MW-5

Tgt Ion: 78 Resp: 3605

Ion Ratio Lower Upper

78 100

77 24.8 18.7 28.1

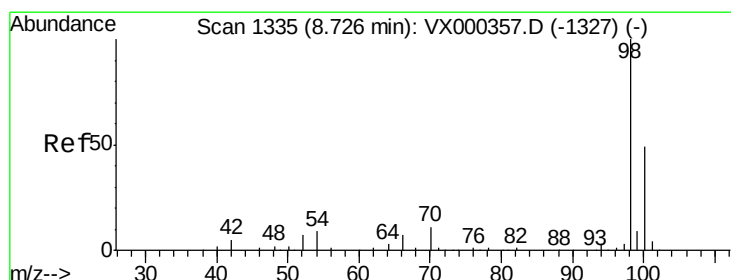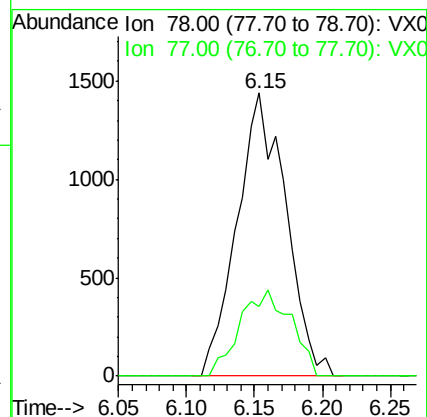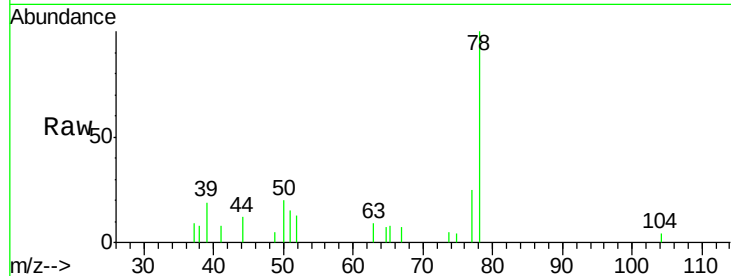

#50

Toluene-d8

Concen: 49.01 ug/l

RT: 8.73 min Scan# 1335

Delta R.T. 0.00 min

Lab File: VX000523.D




Acq: 29 Mar 2018 19:48


Tgt Ion: 98 Resp: 253971

Ion Ratio Lower Upper

98 100

100 63.0 51.2 76.8



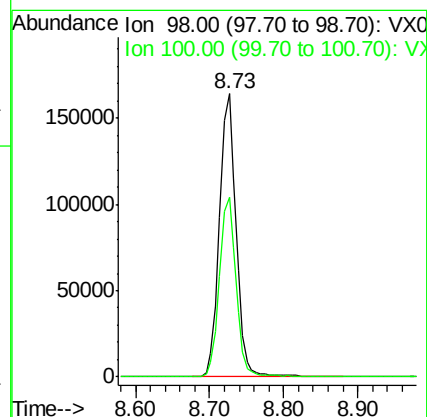



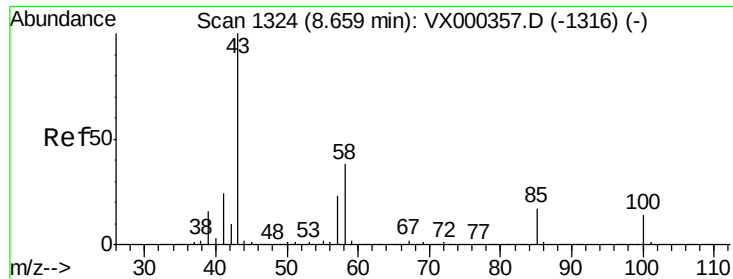

#51
4-Methyl-2-Pentanone
Concen: 0.66 ug/l
RT: 8.67 min Scan# 1325
Delta R.T. 0.01 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48




Instrument :
MSVOA_X
ClientSampled :
MW-5


Tgt Ion: 43 Resp: 1926
Ion Ratio Lower Upper
43 100
58 43.0 30.3 45.5

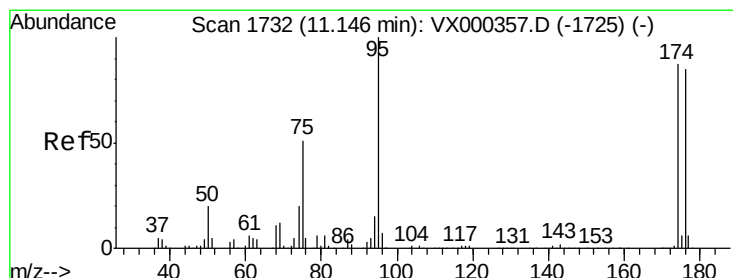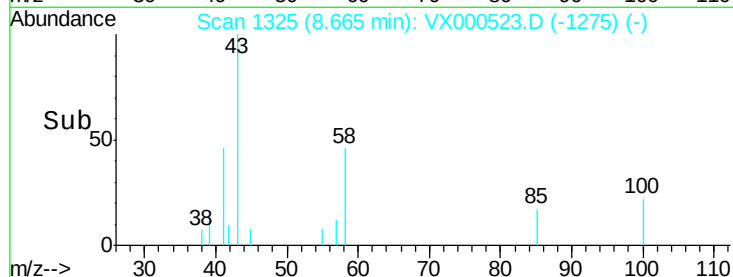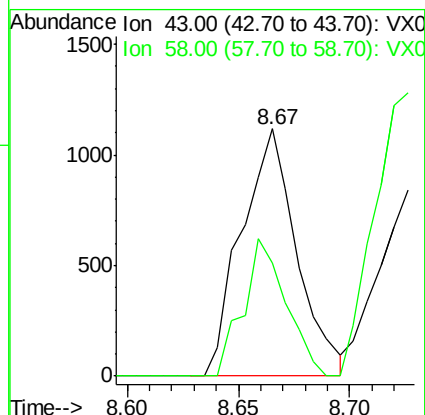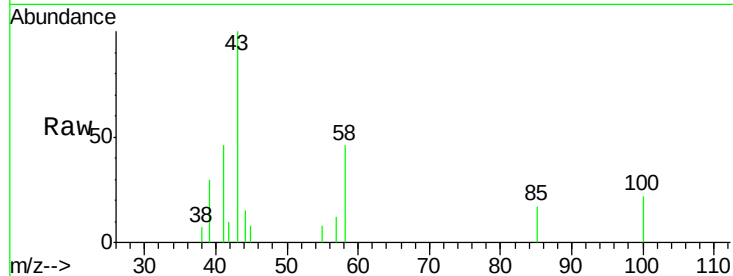

#62
4-Bromofluorobenzene
Concen: 42.74 ug/l
RT: 11.15 min Scan# 1732
Delta R.T. 0.00 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48

Tgt Ion: 95 Resp: 91368
Ion Ratio Lower Upper
95 100
174 89.5 0.0 173.6
176 85.6 0.0 164.6


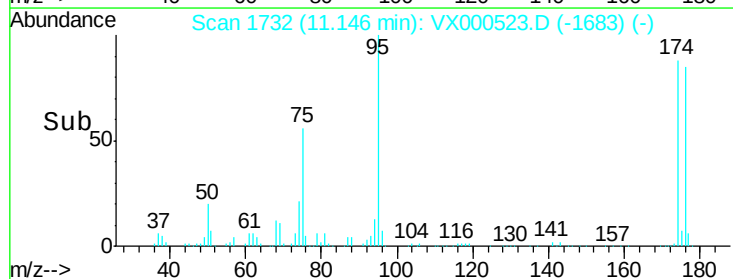
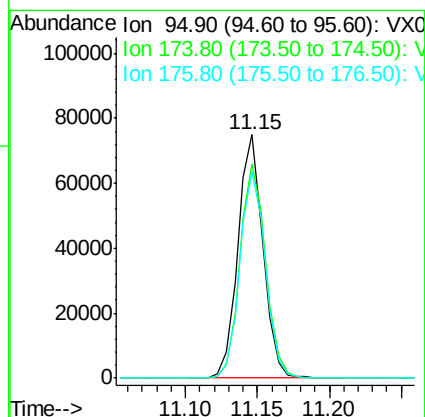
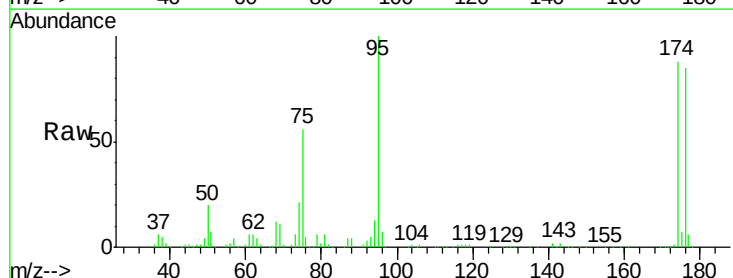


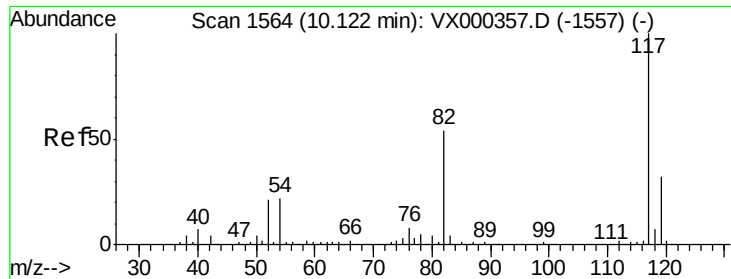

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. 0.00 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48




Instrument :
MSVOA_X
ClientSampled :
MW-5


Tgt Ion:117 Resp: 201314
Ion Ratio Lower Upper
117 100
82 54.8 43.8 65.8
119 33.2 24.9 37.3

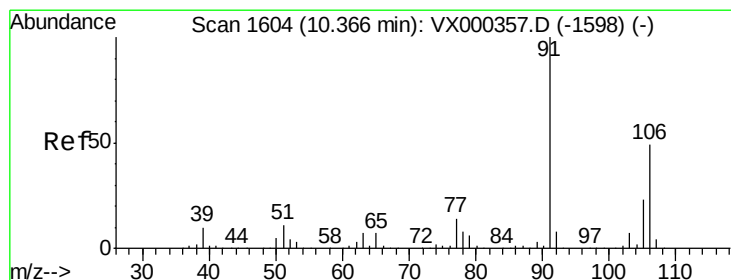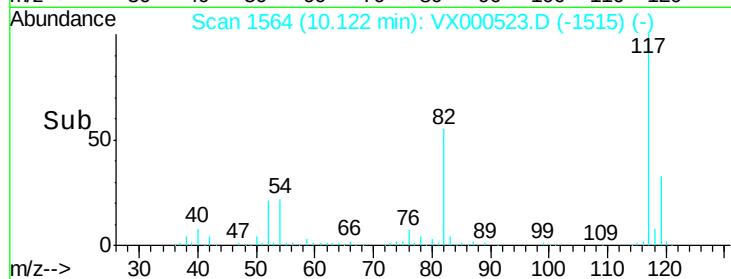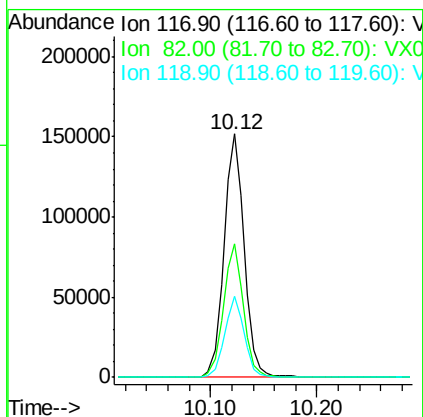

#68
m/p-Xylenes
Concen: 0.38 ug/l
RT: 10.37 min Scan# 1604
Delta R.T. 0.00 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48

Tgt Ion:106 Resp: 1148
Ion Ratio Lower Upper
106 100
91 184.8 163.4 245.2

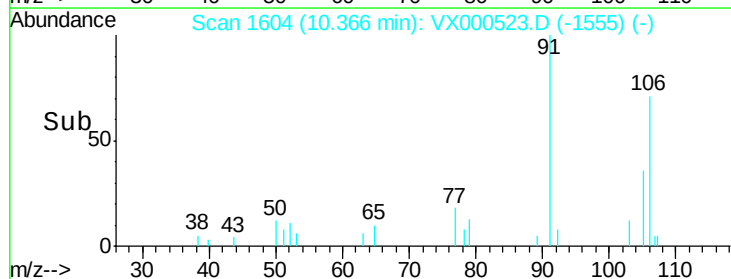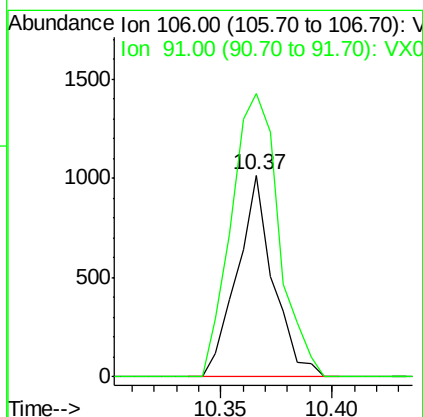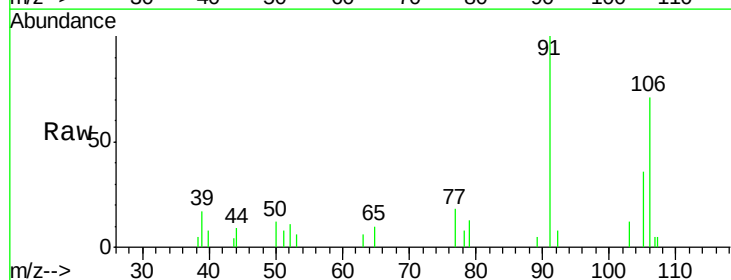


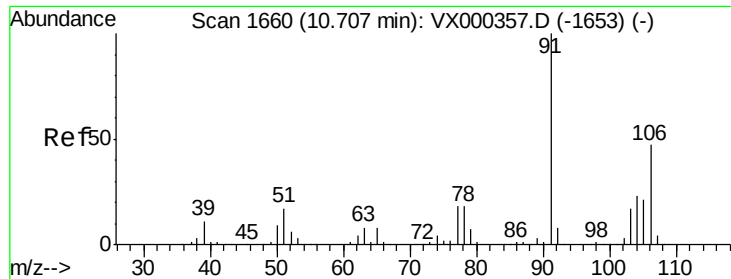




#69
o-Xylene
Concen: 0.26 ug/l
RT: 10.71 min Scan# 1661
Delta R.T. 0.01 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48

Instrument :
MSVOA_X
ClientSampled :
MW-5

Tgt Ion:106 Resp: 762
Ion Ratio Lower Upper
106 100
91 190.2 106.5 319.6




Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0

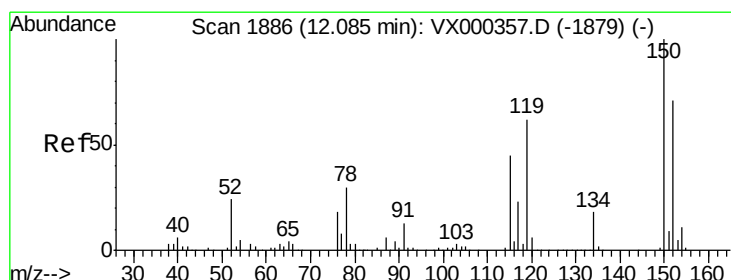
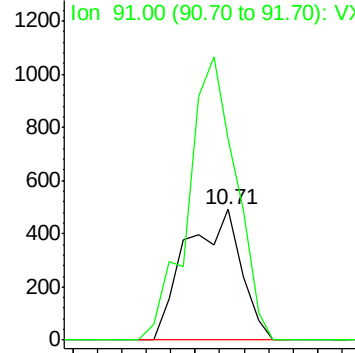



#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. 0.00 min
Lab File: VX000523.D
Acq: 29 Mar 2018 19:48

Tgt Ion:152 Resp: 107255
Ion Ratio Lower Upper
152 100
115 55.4 39.8 119.3
150 156.8 0.0 344.4

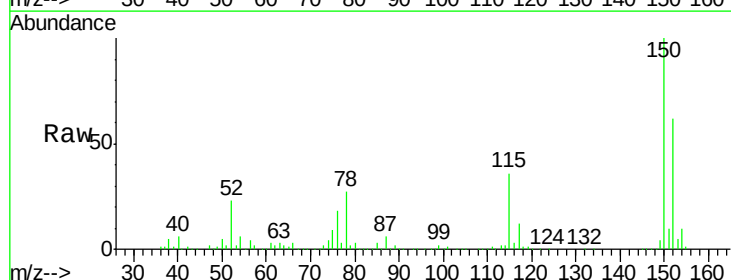

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

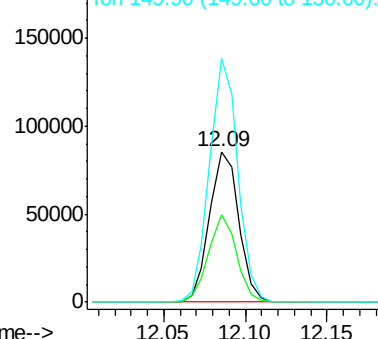



#74

N-amyI acetate

Concen: Below Cal

RT: 6.45 min Scan# 962

Delta R.T. -0.02 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampled :

MW-5

Tgt Ion: 43 Resp: 25


Ion Ratio Lower Upper

43 100

70 0.0 0.0 0.0

55 0.0 0.0 0.0

61 0.0 14.4 21.6#

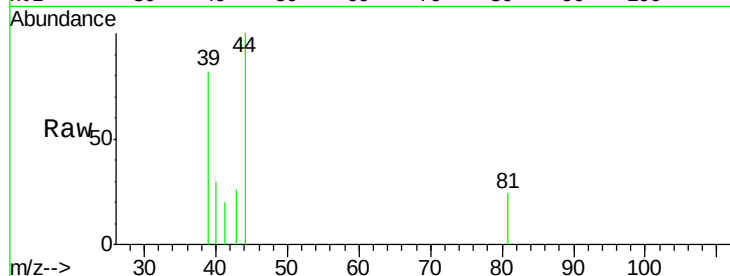


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Time--> 6.43 6.44 6.45 6.46 6.47



#76

1,2,3-Trichloropropane

Concen: 22.71 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. -0.16 min

Lab File: VX000523.D


Acq: 29 Mar 2018 19:48

Tgt Ion: 75 Resp: 52340

Ion Ratio Lower Upper


75 100

77 1.0 21.4 64.2#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0







Time--> 11.10 11.15 11.20

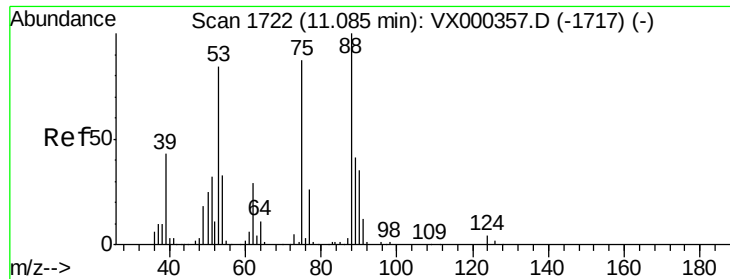

#81
 trans-1,4-Dichloro-2-butene
 Concen: 73.52 ug/l
 RT: 11.15 min Scan# 1732
 Delta R.T. 0.06 min
 Lab File: VX000523.D
 Acq: 29 Mar 2018 19:48




Instrument :
 MSVOA_X
 ClientSampled :
 MW-5


Tgt Ion: 75 Resp: 52340
 Ion Ratio Lower Upper
 75 100
 53 0.0 80.7 121.1#
 89 0.0 39.4 59.0#

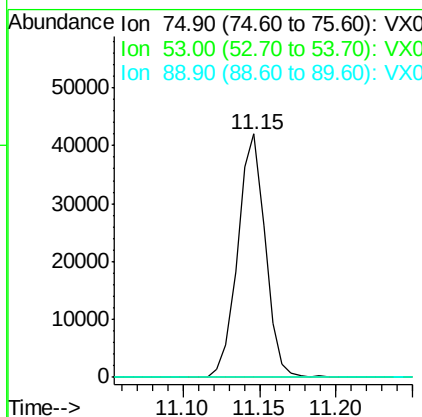

#84
 1,2,4-Trimethylbenzene
 Concen: 0.20 ug/l
 RT: 11.82 min Scan# 1842
 Delta R.T. 0.00 min
 Lab File: VX000523.D
 Acq: 29 Mar 2018 19:48

Tgt Ion: 105 Resp: 1262
 Ion Ratio Lower Upper
 105 100
 120 38.4 22.4 67.3

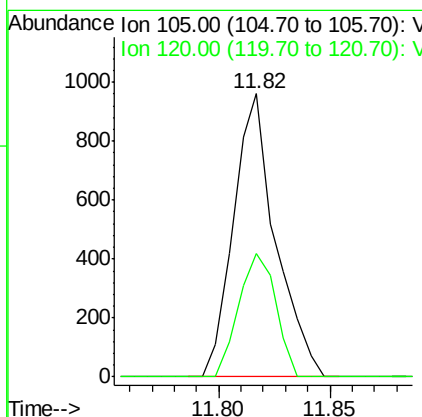



#86

p-Isopropyltoluene

Concen: 0.73 ug/l

RT: 12.07 min Scan# 1884

Delta R.T. 0.00 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48

Instrument :

MSVOA_X

ClientSampled :

MW-5


Tgt Ion:119 Resp: 4817

Ion Ratio Lower Upper

119 100

134 32.0 13.3 39.9




91 30.7 12.0 36.1



Abundance Ion 119.00 (118.70 to 119.70): V

Ion 134.00 (133.70 to 134.70): V

Ion 91.00 (90.70 to 91.70): V

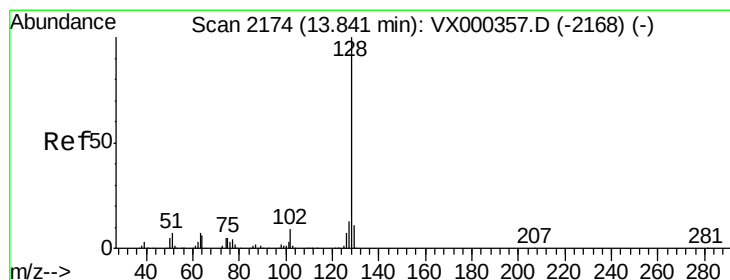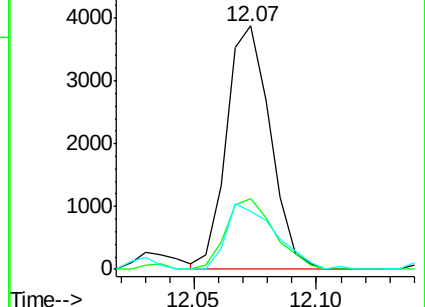

#95

Naphthalene

Concen: 0.61 ug/l

RT: 13.85 min Scan# 2175

Delta R.T. 0.01 min

Lab File: VX000523.D

Acq: 29 Mar 2018 19:48


Tgt Ion:128 Resp: 5379

Ion Ratio Lower Upper

128 100

127 15.2 10.6 15.8

129 10.5 8.9 13.3



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

