

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX032918\
 Data File : VX000545.D
 Acq On : 30 Mar 2018 06:01
 Operator : JC/MD
 Sample : J2127-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRIP-BLANK

Quant Time: Mar 30 08:35:49 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 21 04:52:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	107536	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	187790	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	191911	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	101363	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	77663	55.33	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.66%	
35) Dibromofluoromethane	5.51	113	61376	51.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.74%	
50) Toluene-d8	8.73	98	244726	49.94	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.88%	
62) 4-Bromofluorobenzene	11.15	95	85105	42.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	84.40%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX032918\
Data File : VX000545.D
Acq On : 30 Mar 2018 06:01
Operator : JC/MD
Sample : J2127-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Quant Time: Mar 30 08:35:49 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 21 04:52:42 2018
Response via : Initial Calibration

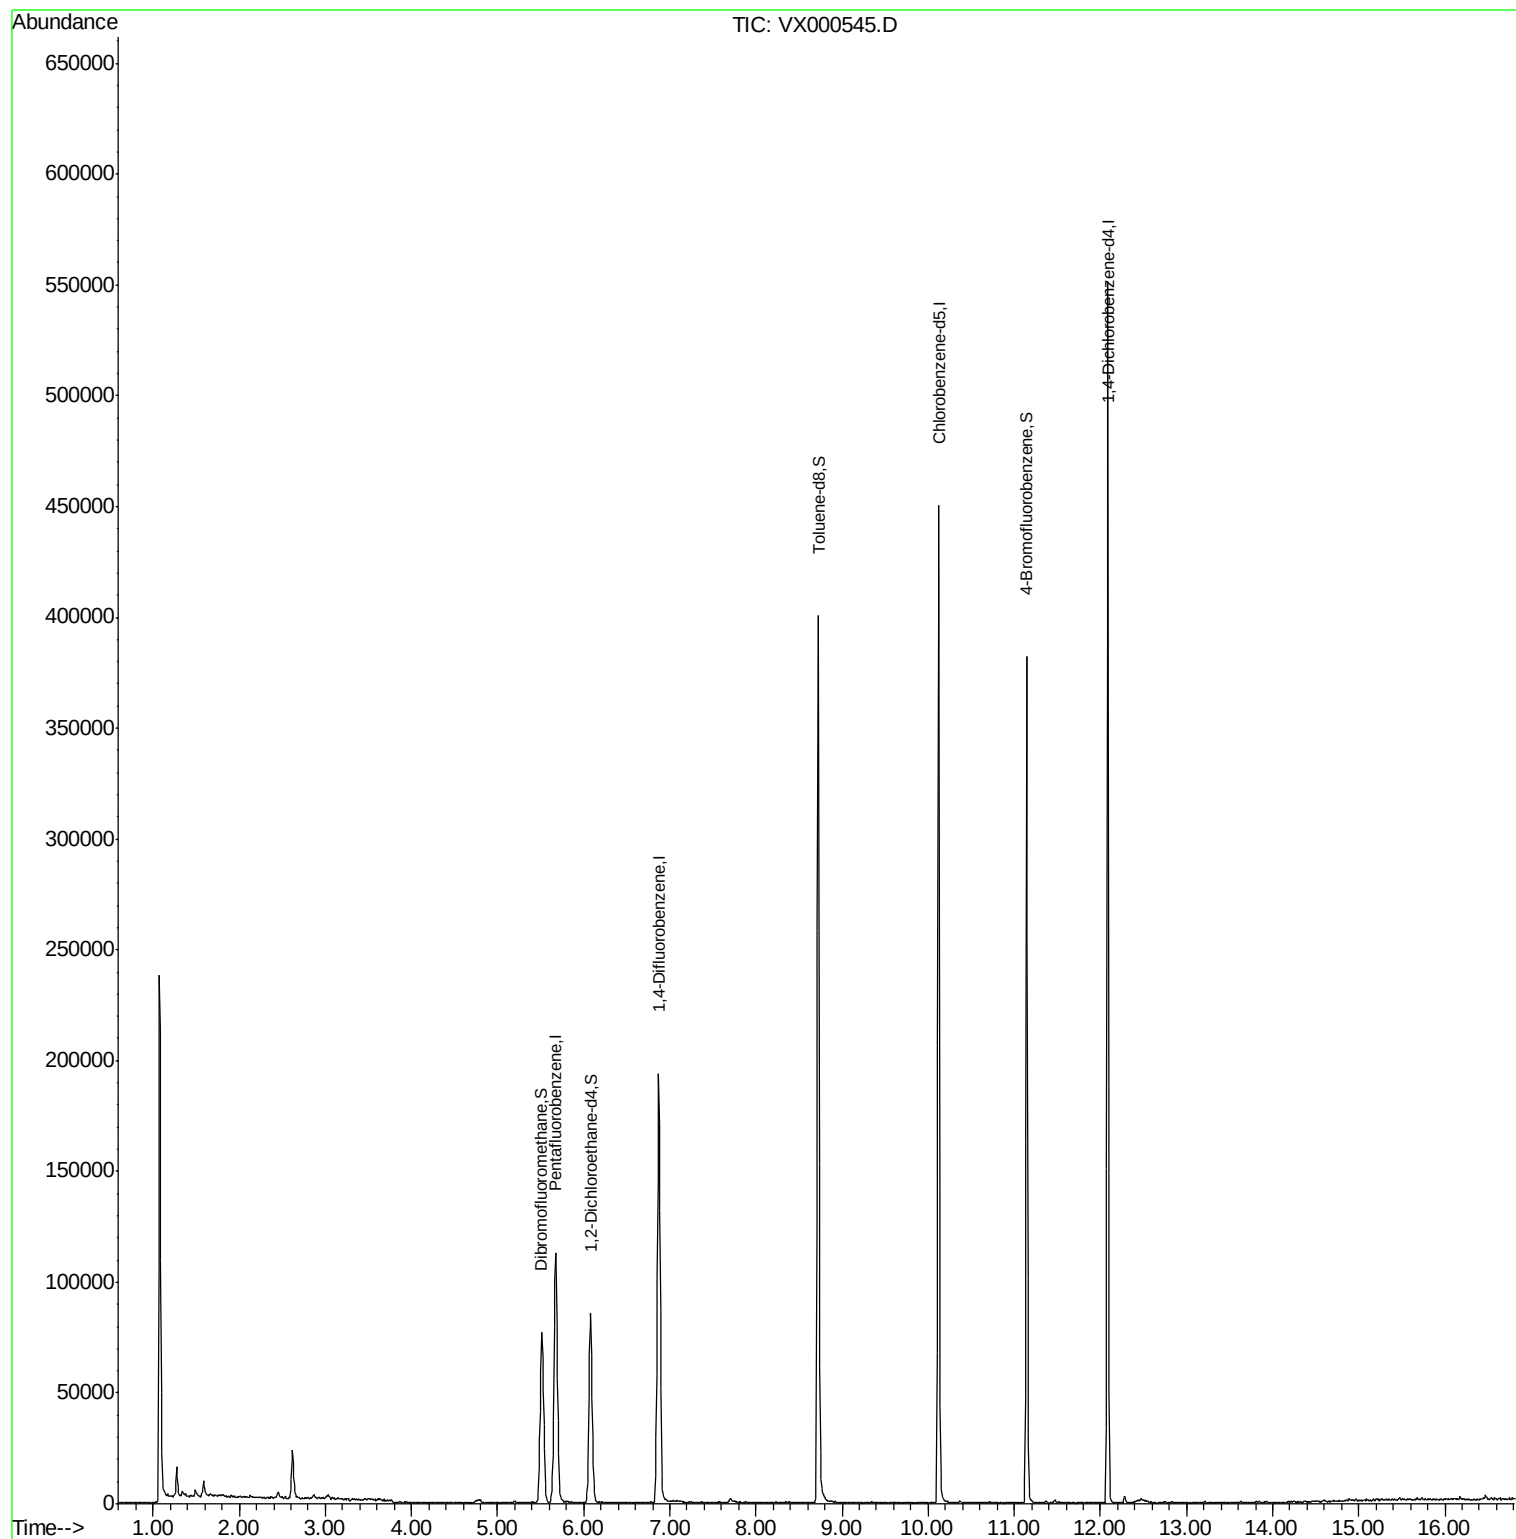

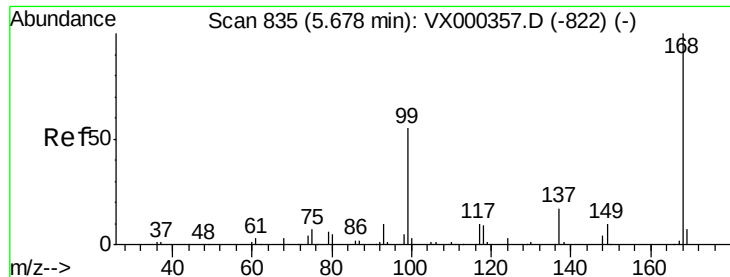

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.01 min

Lab File: VX000545.D

Acq: 30 Mar 2018 06:01

Instrument :

MSVOA_X

ClientSampled :


TRIP-BLANK

Tot Ion:168 Resp: 107536

Ion Ratio Lower Upper




168 100

99 52.1 45.8 68.6

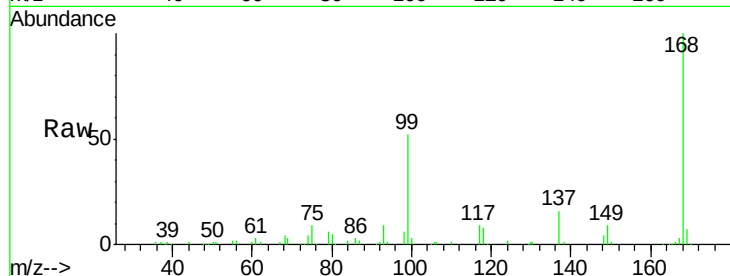

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

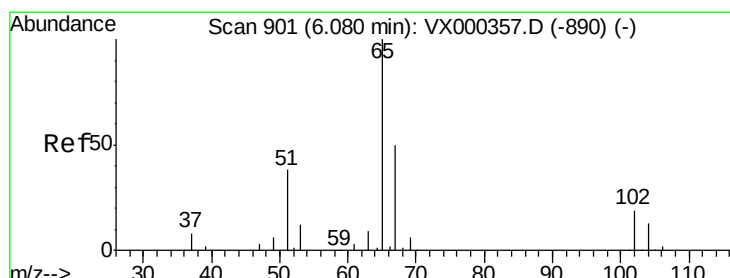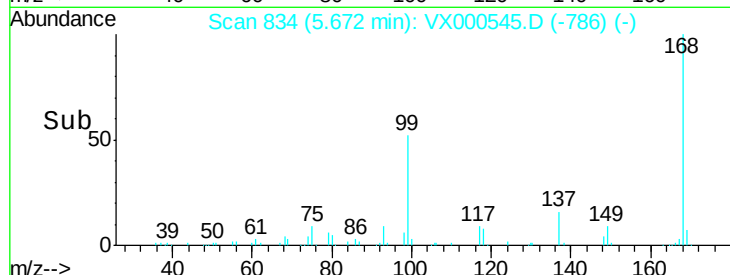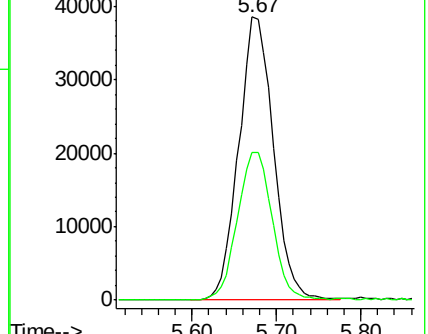

#33

1,2-Dichloroethane-d4

Concen: 55.33 ug/l

RT: 6.08 min Scan# 901

Delta R.T. 0.00 min

Lab File: VX000545.D


Acq: 30 Mar 2018 06:01

Tgt Ion: 65 Resp: 77663

Ion Ratio Lower Upper



65 100


67 50.6 0.0 103.2

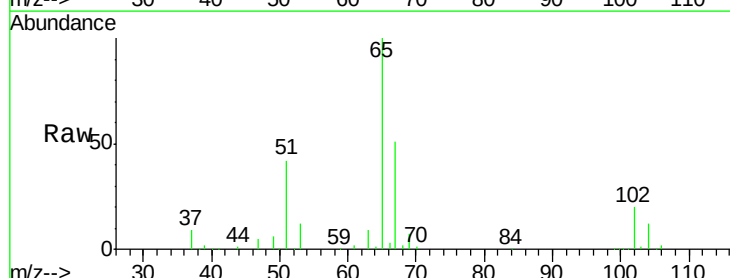

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

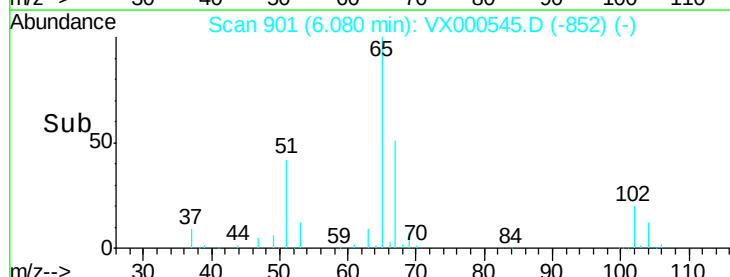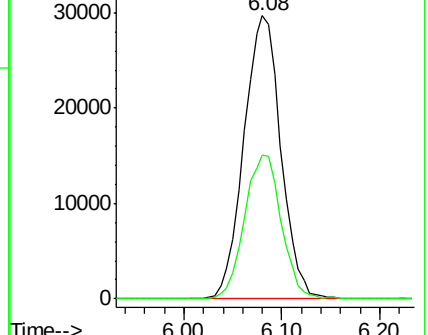

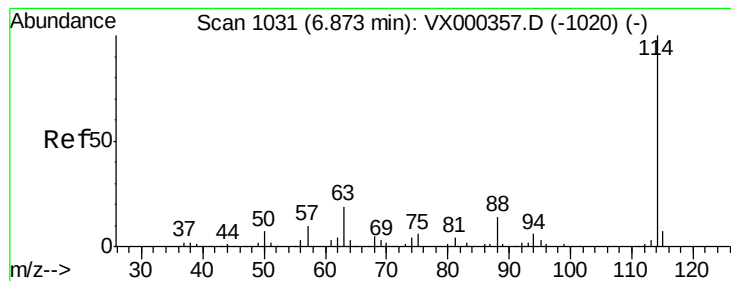

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1031

Delta R.T. -0.00 min

Lab File: VX000545.D

Acq: 30 Mar 2018 06:01

Instrument :

MSVOA_X

ClientSampleId :

TRIP-BLANK


Tot Ion:114 Resp: 187790

Ion Ratio Lower Upper

114 100

63 19.7 0.0 38.4




88 14.8 0.0 27.0

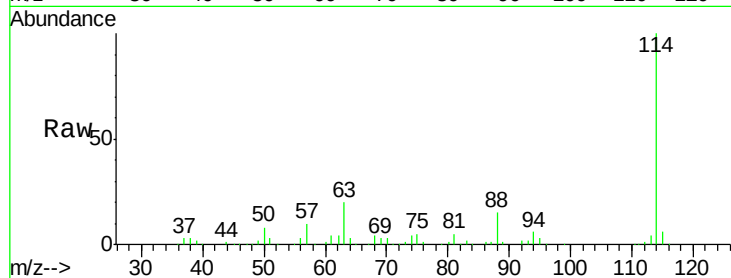

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

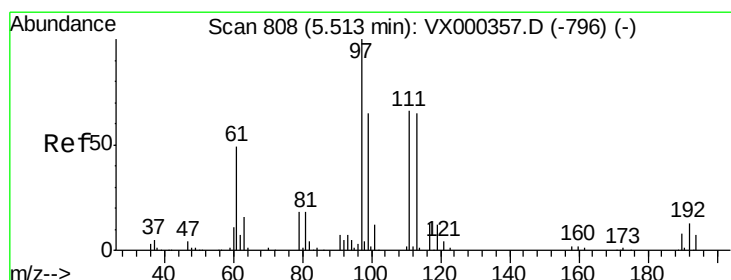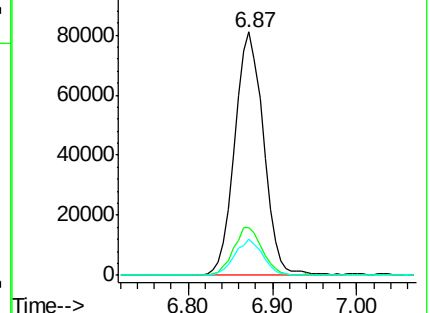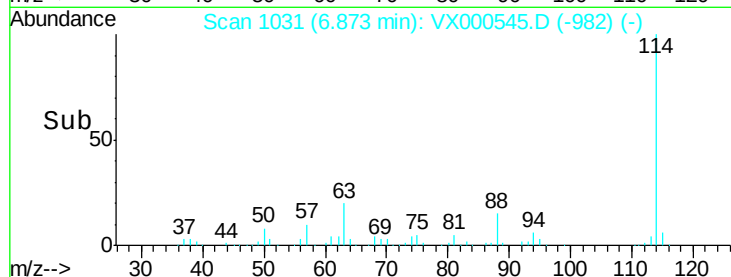

#35

Dibromofluoromethane

Concen: 51.87 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX000545.D

Acq: 30 Mar 2018 06:01


Tgt Ion:113 Resp: 61376

Ion Ratio Lower Upper

113 100

111 98.6 82.4 123.6



192 19.4 15.8 23.6

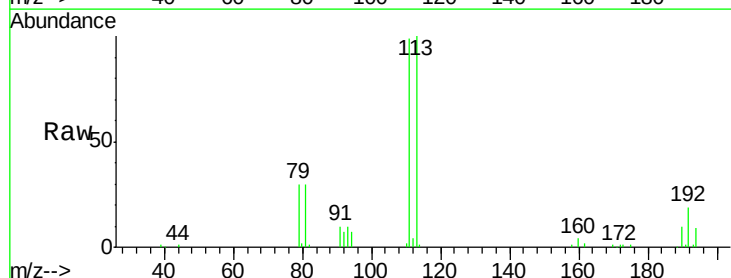


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



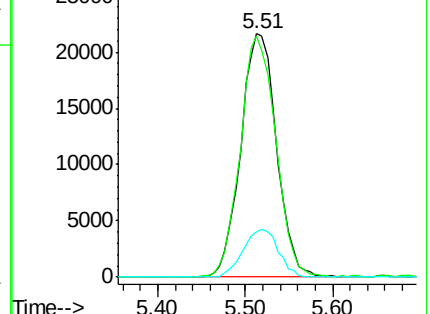
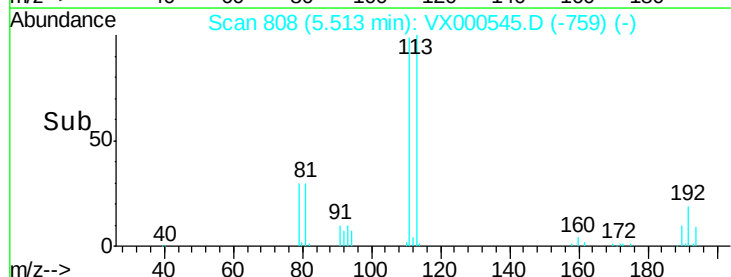


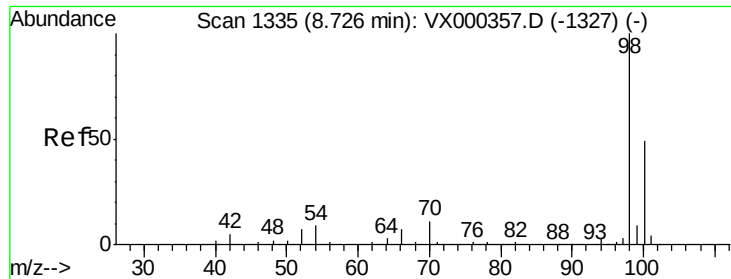

#50
Toluene-d8
Concen: 49.94 ug/l
RT: 8.73 min Scan# 1335
Delta R.T. -0.00 min
Lab File: VX000545.D
Acq: 30 Mar 2018 06:01




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tot Ion: 98 Resp: 244726
Ion Ratio Lower Upper
98 100
100 62.8 51.2 76.8

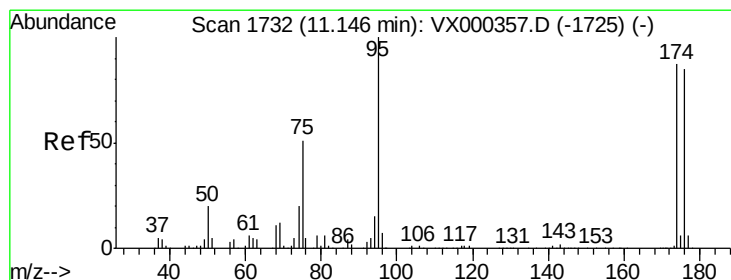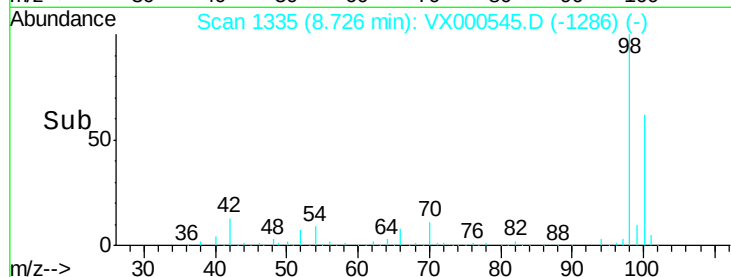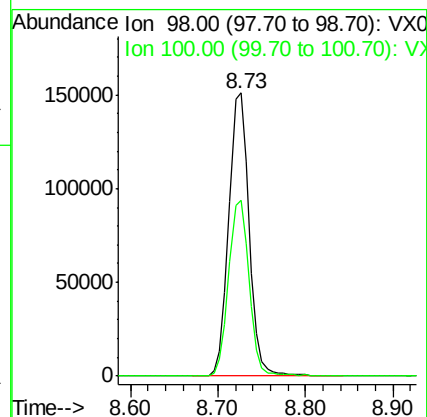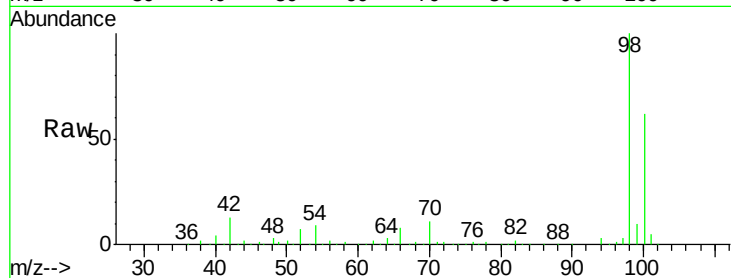

#62
4-Bromofluorobenzene
Concen: 42.20 ug/l
RT: 11.15 min Scan# 1732
Delta R.T. 0.00 min
Lab File: VX000545.D
Acq: 30 Mar 2018 06:01

Tgt Ion: 95 Resp: 85105
Ion Ratio Lower Upper
95 100
174 90.9 0.0 173.6
176 88.7 0.0 164.6

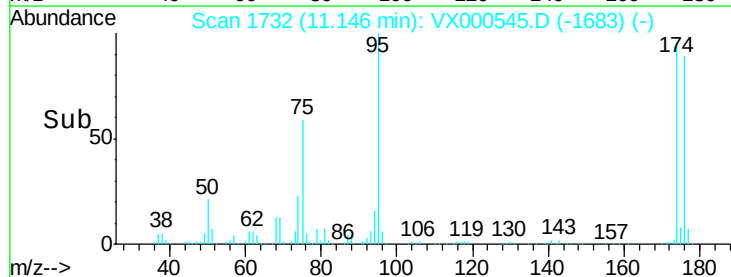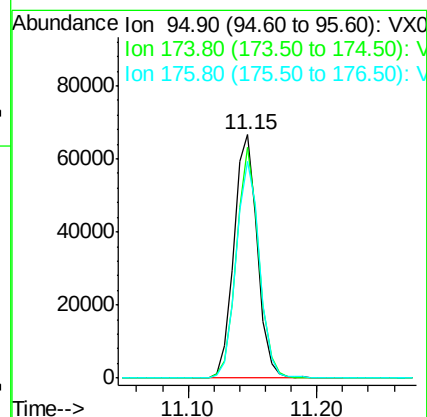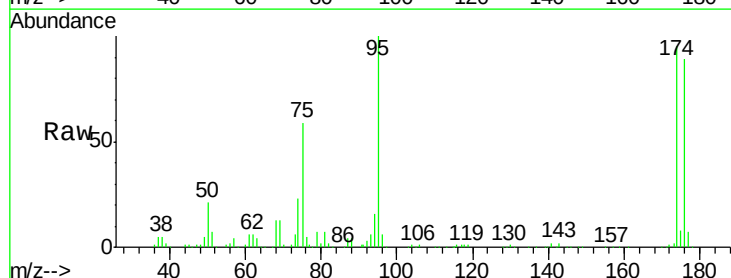


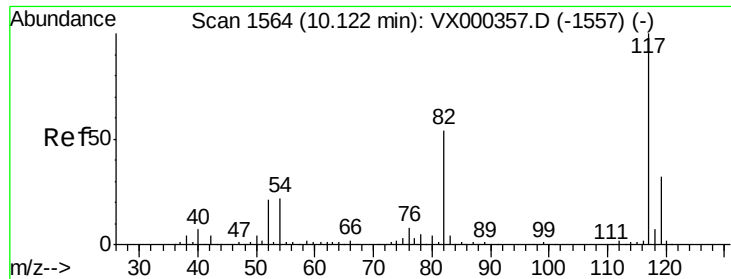




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. -0.00 min
Lab File: VX000545.D
Acq: 30 Mar 2018 06:01

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Tot Ion:117 Resp: 191911
Ion Ratio Lower Upper
117 100
82 53.9 43.8 65.8
119 32.4 24.9 37.3

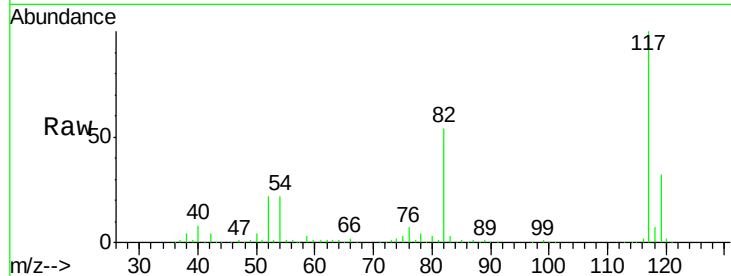


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

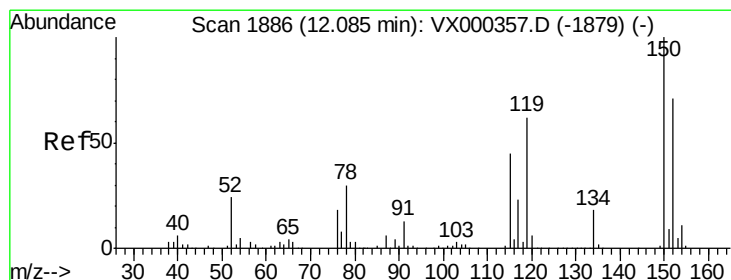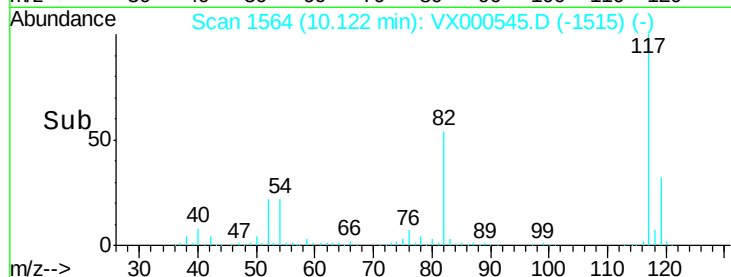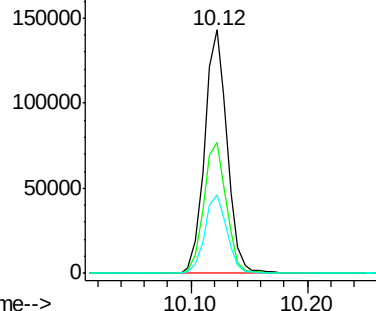

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX000545.D
Acq: 30 Mar 2018 06:01

Tgt Ion:152 Resp: 101363
Ion Ratio Lower Upper
152 100
115 58.4 39.8 119.3
150 157.6 0.0 344.4

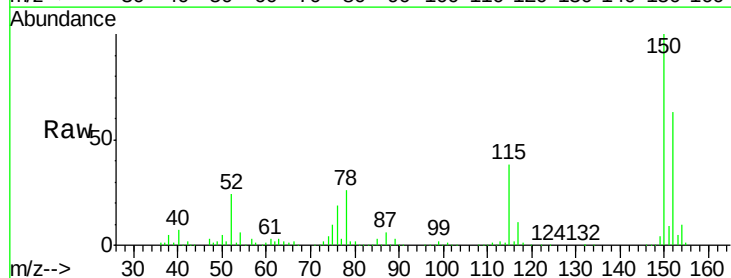

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

