

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX032918\
 Data File : VX000525.D
 Acq On : 29 Mar 2018 20:40
 Operator : JC/MD
 Sample : J2098-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LIP-22

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	93	rBV	564215	646823	99.51%	14.818%
2	1.270	108	112	122	rBV	56910	84889	13.06%	1.945%
3	3.215	425	431	438	rVB4	3503	8834	1.36%	0.202%
4	5.513	797	808	820	rBV	73451	208933	32.14%	4.786%
5	5.672	824	834	846	rBV2	106041	297714	45.80%	6.820%
6	6.080	891	901	916	rBV	84374	216491	33.31%	4.959%
7	6.873	1021	1031	1044	rBV2	182076	438035	67.39%	10.035%
8	8.726	1328	1335	1352	rBV	411974	650012	100.00%	14.891%
9	10.122	1557	1564	1573	rBV	444086	590786	90.89%	13.534%
10	11.146	1726	1732	1737	rBV	383064	467814	71.97%	10.717%
11	12.085	1881	1886	1892	rBV	522901	637214	98.03%	14.597%
12	12.725	1985	1991	1995	rBV5	8673	13334	2.05%	0.305%
13	12.902	2013	2020	2026	rVB2	12762	21309	3.28%	0.488%
14	12.987	2031	2034	2038	rVB2	6131	7337	1.13%	0.168%
15	13.359	2090	2095	2100	rVB3	7475	10574	1.63%	0.242%
16	13.749	2157	2159	2166	rVB7	5938	7507	1.15%	0.172%
17	13.816	2166	2170	2175	rBV2	6170	9970	1.53%	0.228%
18	13.993	2195	2199	2203	rBV2	9329	11207	1.72%	0.257%
19	14.042	2203	2207	2214	rVB5	3760	6701	1.03%	0.154%
20	14.548	2286	2290	2295	rBV5	6794	10313	1.59%	0.236%
21	14.859	2334	2341	2344	rBV4	6550	12349	1.90%	0.283%
22	15.255	2400	2406	2412	rBV9	3475	7112	1.09%	0.163%


Sum of corrected areas: 4365258

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX032918\
Data File : VX000525.D
Acq On : 29 Mar 2018 20:40
Operator : JC/MD
Sample : J2098-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LIP-22

Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

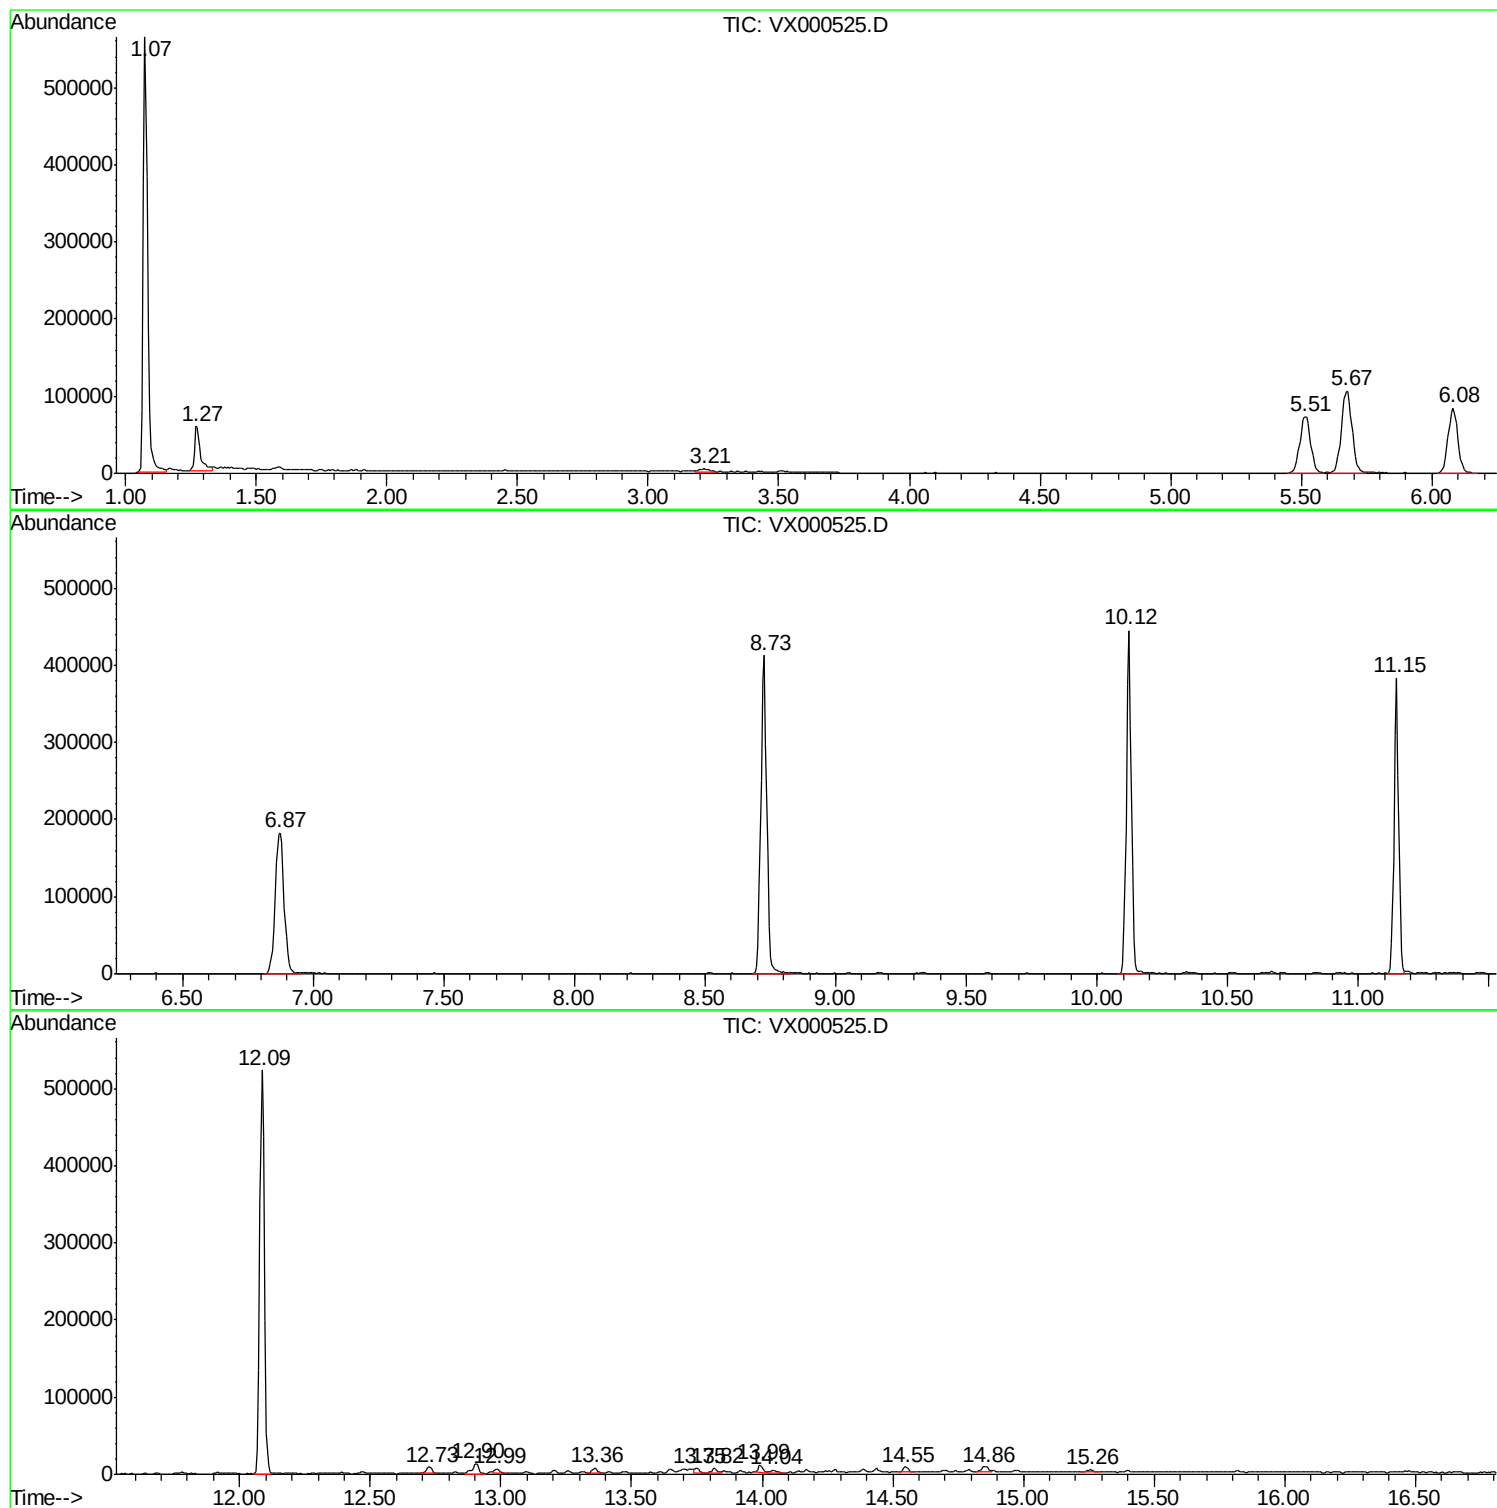

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX032918\
Data File : VX000525.D
Acq On : 29 Mar 2018 20:40
Operator : JC/MD
Sample : J2098-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LIP-22










Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.27	14.26 ug/l	84889	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Sulfur dioxide	64	O2S	007446-09-5	83
2		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
3		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

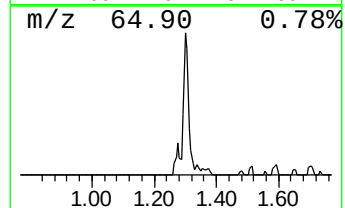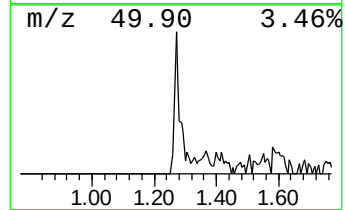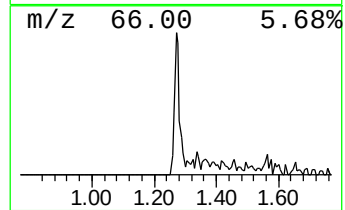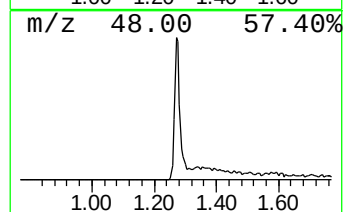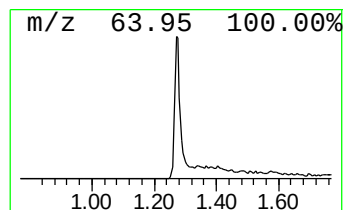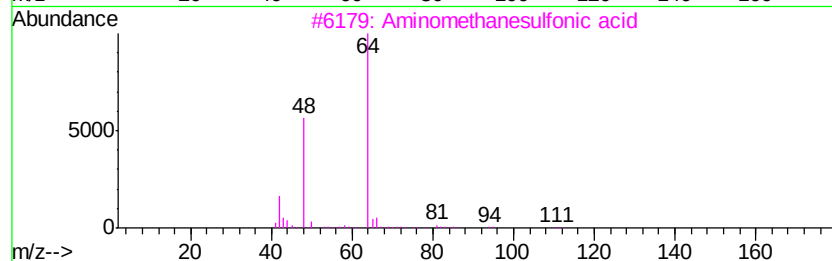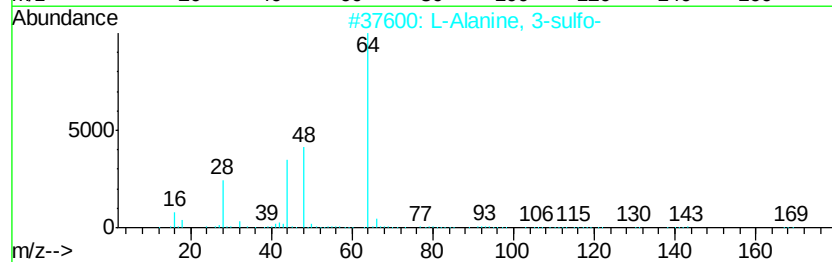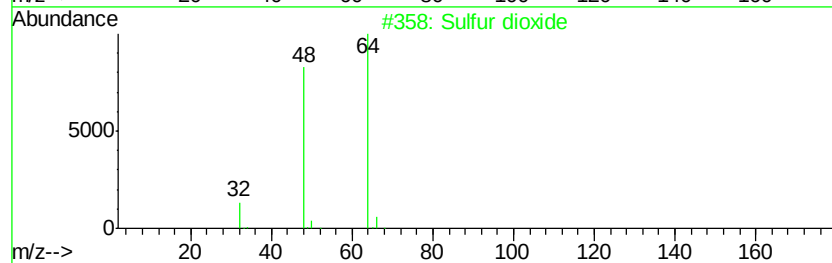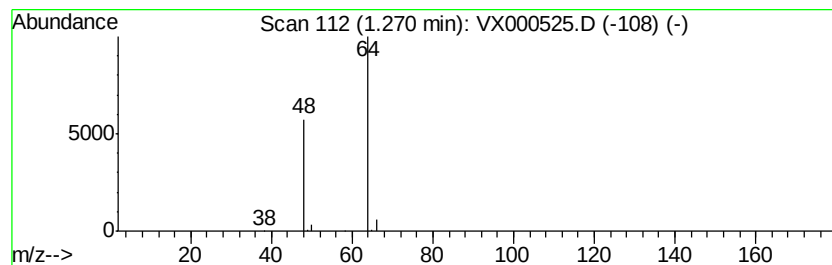

Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX032918\
Data File : VX000525.D
Acq On : 29 Mar 2018 20:40
Operator : JC/MD
Sample : J2098-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LIP-22

Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.27	14.3	ug/l	84889	1	5.67	297714	50.0