


Data Path : W:\HPCHEM1\MSVOA X\DATA\VX032918\  
Data File : VX000530.D  
Acq On : 29 Mar 2018 23:13  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA\_X\METHOD\82X032018W.M  
Title : SW846 8260  
Last Update : Wed Mar 21 04:52:42 2018

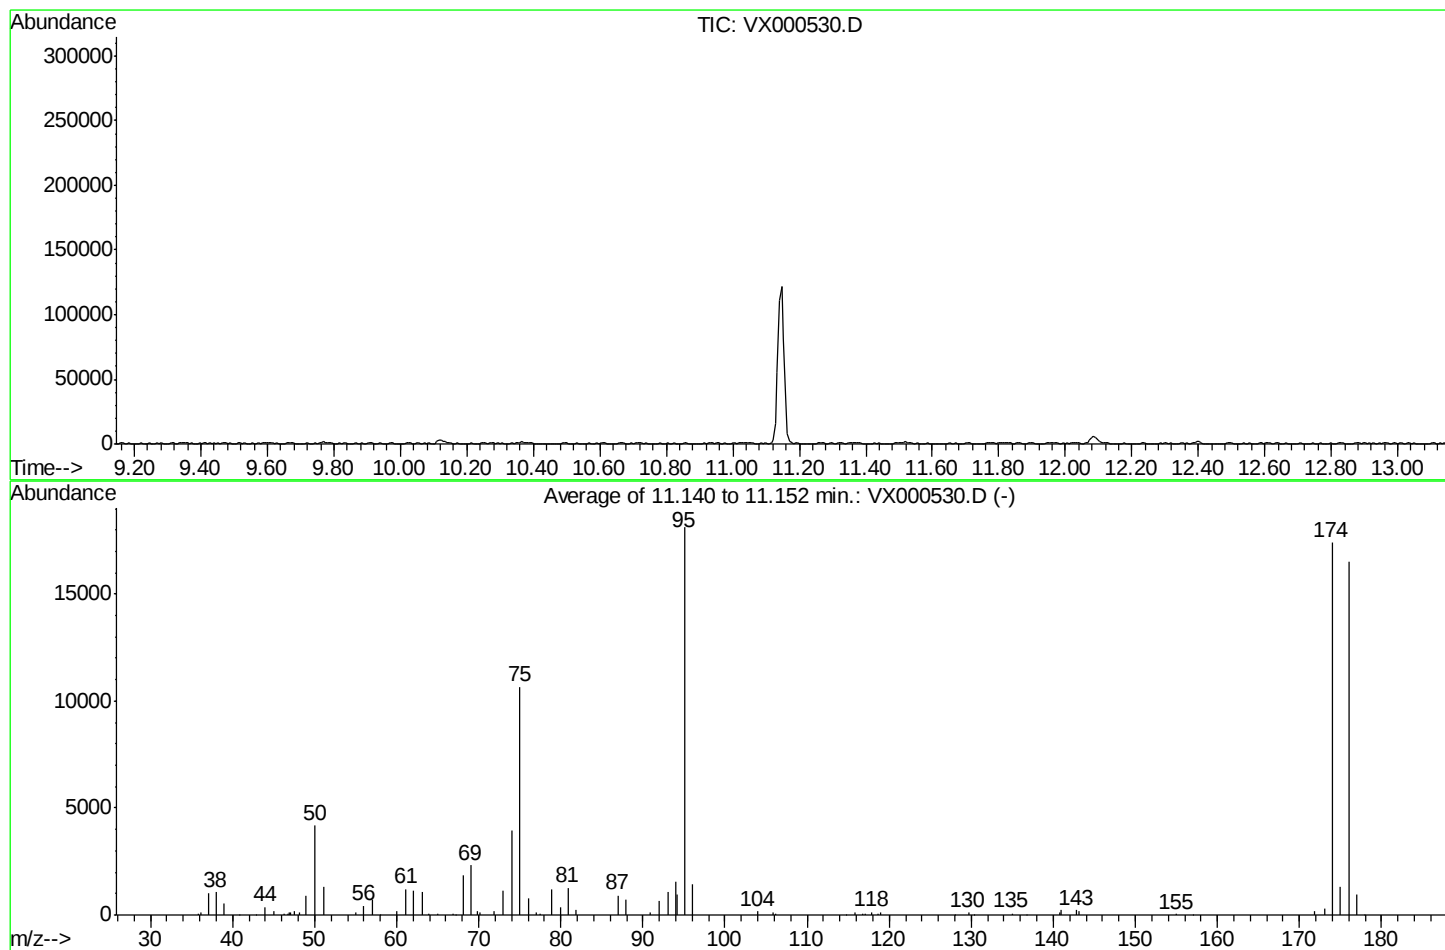

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 23.0      | 4176    | PASS             |
| 75          | 95           | 30           | 60           | 58.9      | 10681   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 18123   | PASS             |
| 96          | 95           | 5            | 9            | 7.9       | 1438    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.6       | 286     | PASS             |
| 174         | 95           | 50           | 100          | 96.0      | 17394   | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 1289    | PASS             |
| 176         | 174          | 95           | 101          | 94.9      | 16510   | PASS             |
| 177         | 176          | 5            | 9            | 5.7       | 943     | PASS             |