

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX033018\
Data File : VX000576.D
Acq On : 30 Mar 2018 22:12
Operator : JC/MD
Sample : J2131-07 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CHRT24482

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	91	rBV	390798	449777	57.83%	8.678%
2	2.453	301	306	311	rVB	7470	12079	1.55%	0.233%
3	2.861	366	373	388	rVB	229928	439196	56.47%	8.474%
4	5.513	797	808	823	rBV2	90145	250565	32.21%	4.835%
5	5.672	823	834	851	rBV2	132388	381617	49.06%	7.363%
6	6.080	891	901	915	rBV	97471	254278	32.69%	4.906%
7	6.873	1021	1031	1046	rBV	222690	524539	67.44%	10.121%
8	8.726	1328	1335	1348	rBV	470242	757029	97.33%	14.607%
9	9.647	1480	1486	1494	rBV	9286	18724	2.41%	0.361%
10	10.122	1558	1564	1578	rBV	519334	703009	90.38%	13.565%
11	11.146	1726	1732	1742	rVB	458577	569764	73.25%	10.994%
12	12.085	1880	1886	1895	rBV	654365	777819	100.00%	15.008%
13	13.841	2169	2174	2181	rVB	28060	35691	4.59%	0.689%
14	14.701	2312	2315	2322	rBV	5710	8606	1.11%	0.166%


Sum of corrected areas: 5182693

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX033018\
Data File : VX000576.D
Acq On : 30 Mar 2018 22:12
Operator : JC/MD
Sample : J2131-07 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CHRT24482

Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

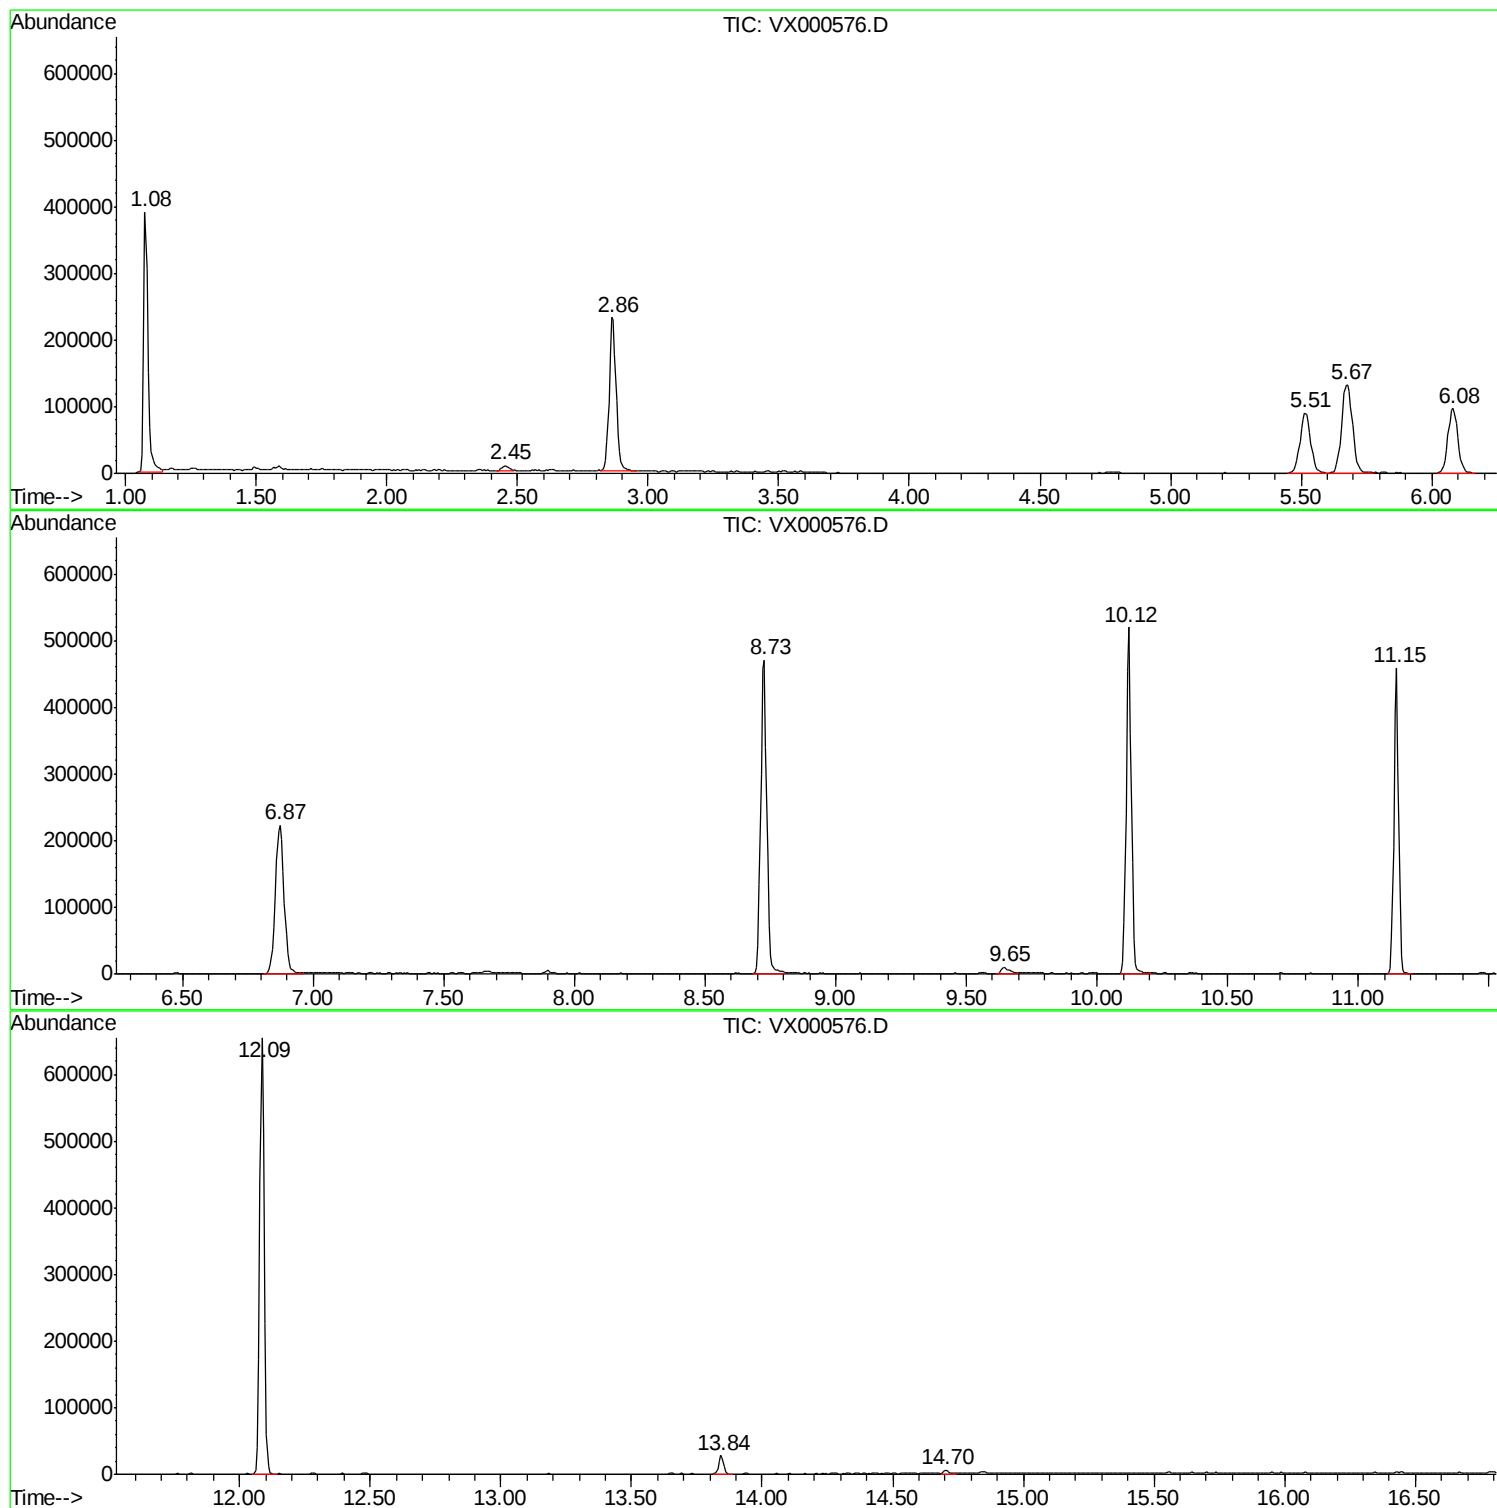

Data_Path : W:\HPCHEM1\MSVOA_X\DATA\VX033018\
Data_File : VX000576.D
Acq_On : 30-Mar-2018 22:122
Operator : JC/MDD
Sample : J2131-07.5XX
Misc : 5.0mL/MSVOA_X/WATER
ALS_Vial : 21 Sample_Multiplier: 11

Instrument :
MSVOA_X
ClientSampleId :
CHRT24482

Quant_Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.MM
Quant_Title : SW846-82600

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
