

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX033118\
 Data File : VX000609.D
 Acq On : 31 Mar 2018 22:57
 Operator : JC/MD
 Sample : VX0331WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Apr 02 06:14:24 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 21 04:52:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	108025	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	178224	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	177159	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	93262	50.00	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	70836	50.23	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.46%	
35) Dibromofluoromethane	5.51	113	55102	49.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.14%	
50) Toluene-d8	8.73	98	220347	47.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.76%	
62) 4-Bromofluorobenzene	11.15	95	78825	41.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	82.66%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX033118\
Data File : VX000609.D
Acq On : 31 Mar 2018 22:57
Operator : JC/MD
Sample : VX0331WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Apr 02 06:14:24 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 21 04:52:42 2018
Response via : Initial Calibration

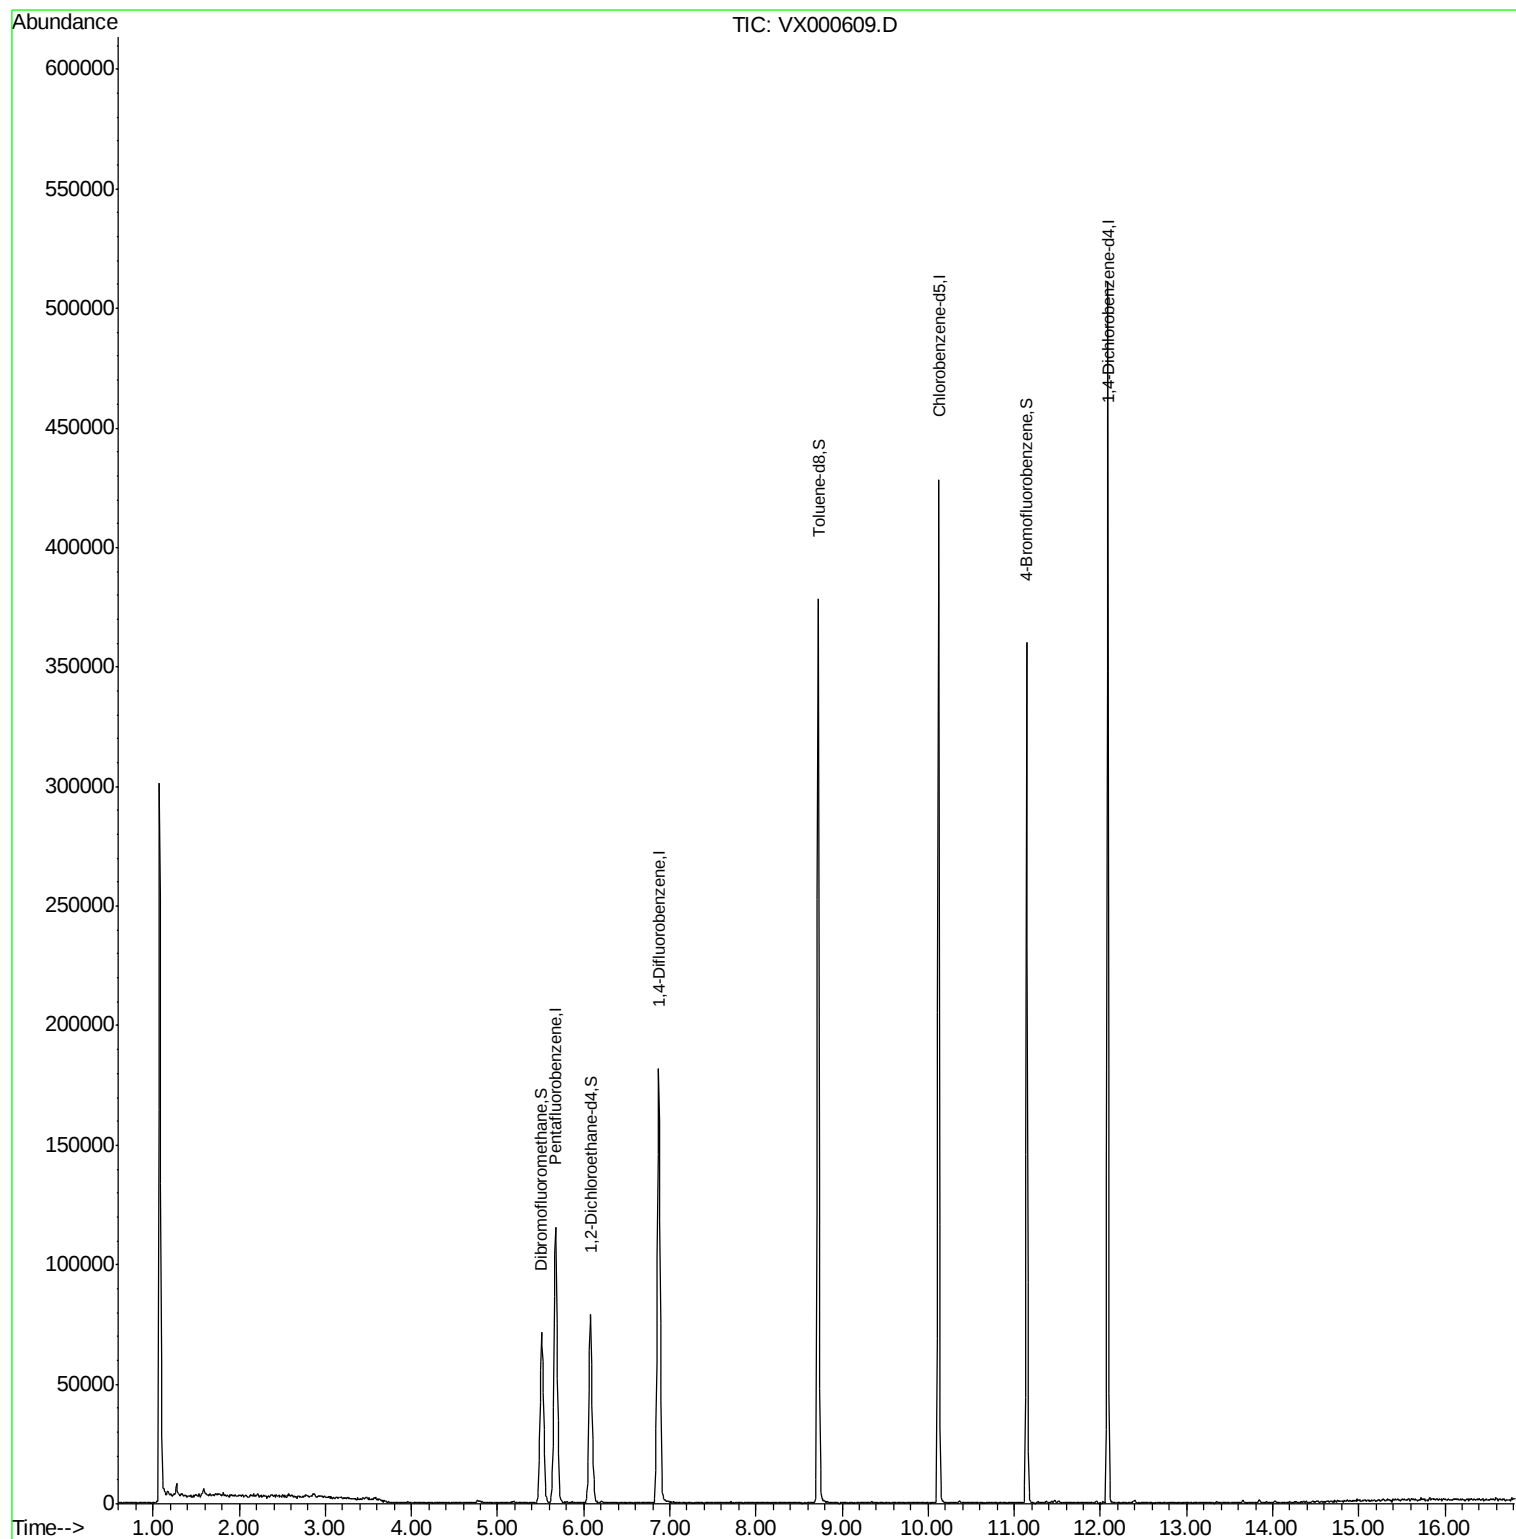

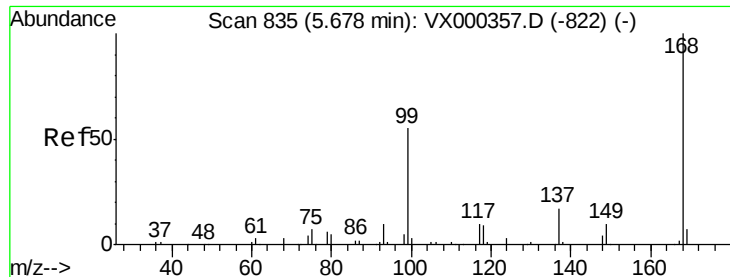

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.01 min

Lab File: VX000609.D


Acq: 31 Mar 2018 22:57

Tot Ion:168 Resp: 108025

Ion Ratio Lower Upper




168 100

99 53.5 45.8 68.6

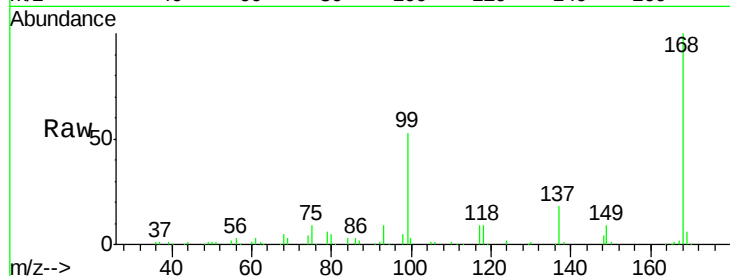

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

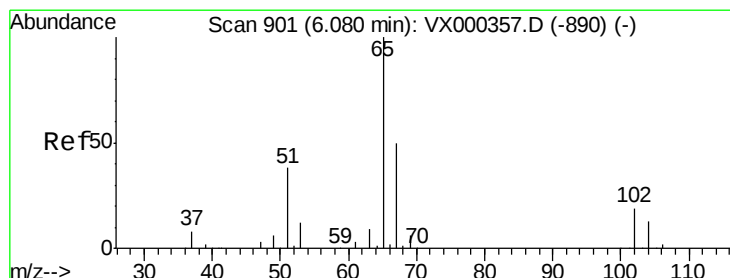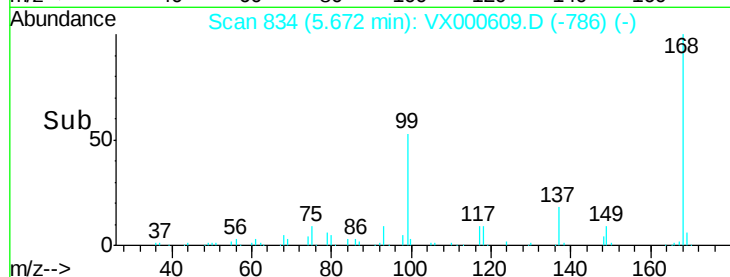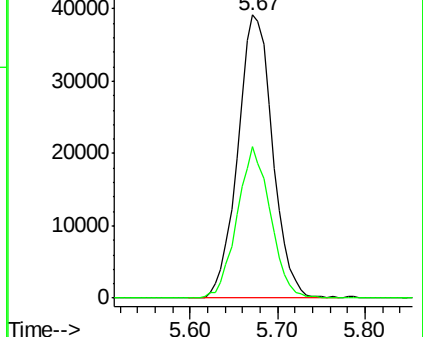

#33

1,2-Dichloroethane-d4

Concen: 50.23 ug/l

RT: 6.08 min Scan# 901

Delta R.T. 0.00 min

Lab File: VX000609.D


Acq: 31 Mar 2018 22:57

Tgt Ion: 65 Resp: 70836

Ion Ratio Lower Upper



65 100


67 53.3 0.0 103.2

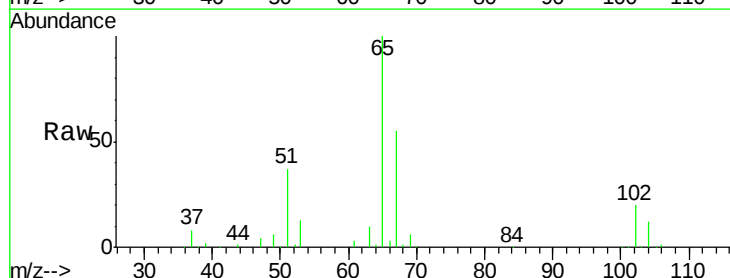

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

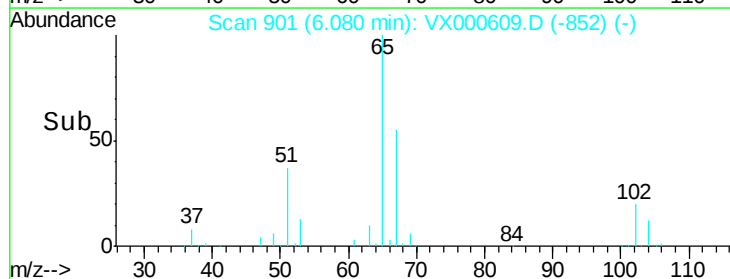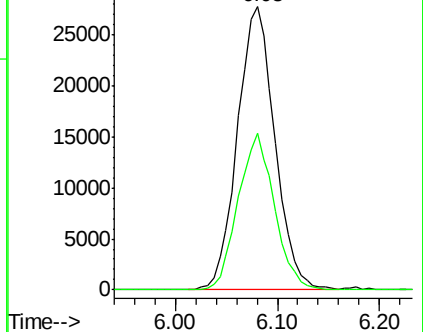

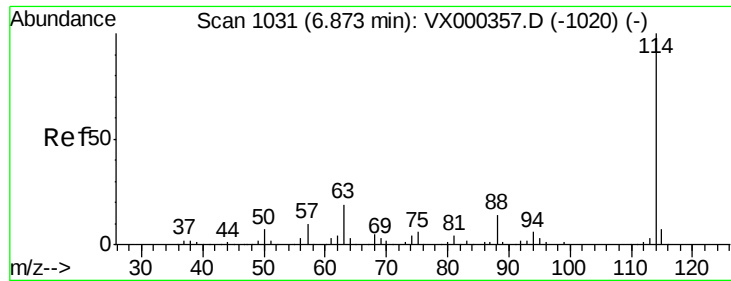

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1031

Delta R.T. -0.00 min

Lab File: VX000609.D

Acq: 31 Mar 2018 22:57


Tot Ion:114 Resp: 178224

Ion Ratio Lower Upper

114 100

63 19.9 0.0 38.4




88 12.7 0.0 27.0

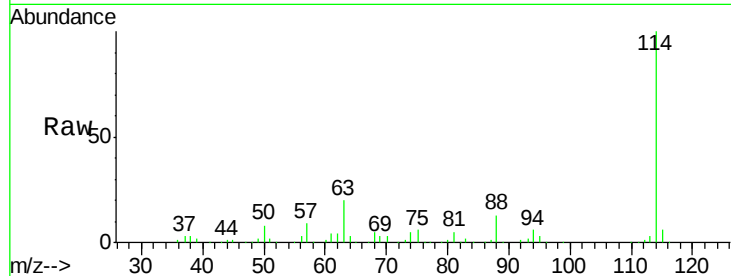

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

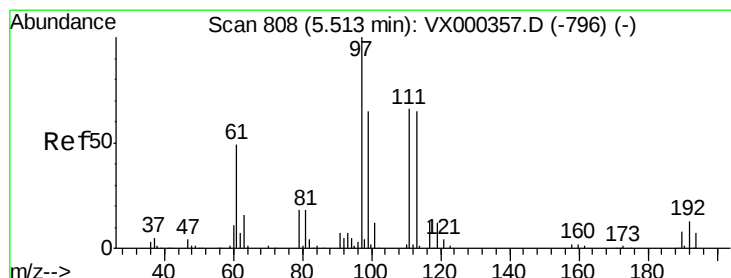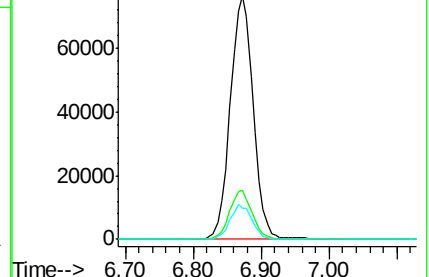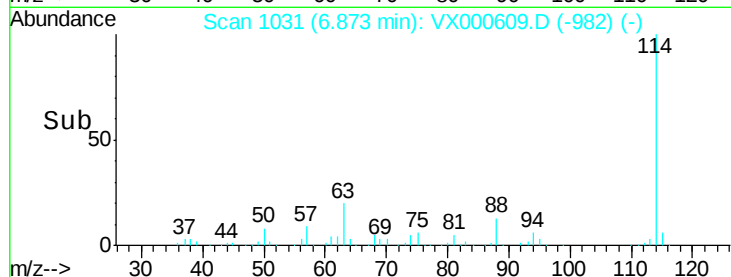

#35

Dibromofluoromethane

Concen: 49.07 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX000609.D

Acq: 31 Mar 2018 22:57


Tgt Ion:113 Resp: 55102

Ion Ratio Lower Upper

113 100

111 103.0 82.4 123.6



192 20.3 15.8 23.6

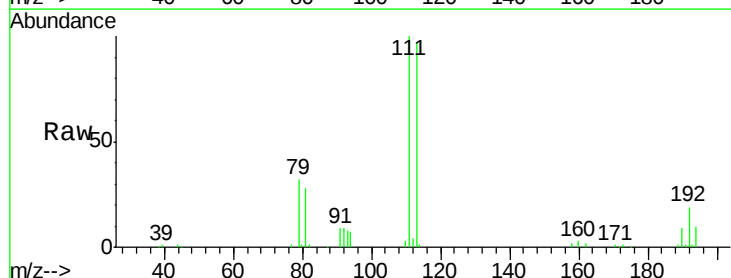


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

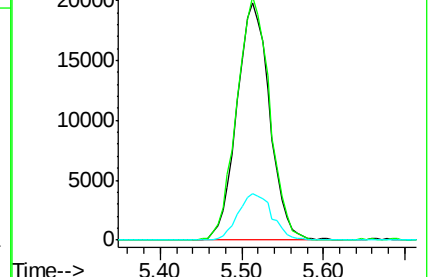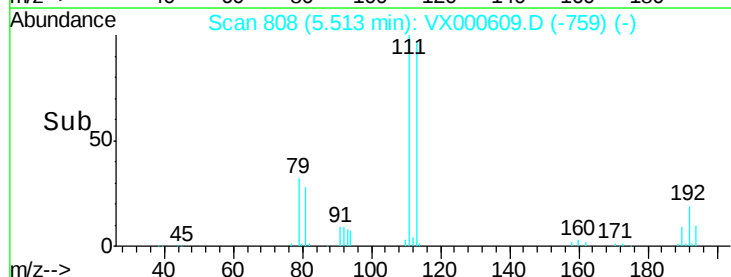

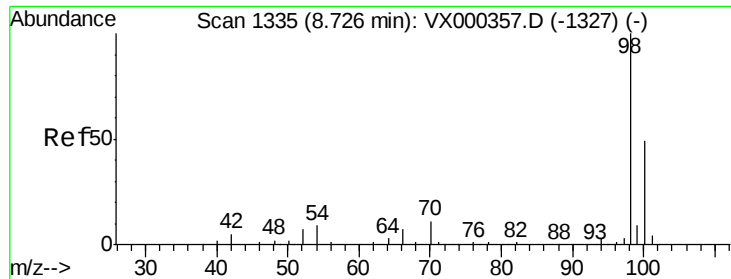

#50

Toluene-d8

Concen: 47.38 ug/l

RT: 8.73 min Scan# 1335

Delta R.T. -0.00 min

Lab File: VX000609.D


Acq: 31 Mar 2018 22:57

Tot Ion: 98 Resp: 220347

Ion Ratio Lower Upper

98 100

100 63.9 51.2 76.8

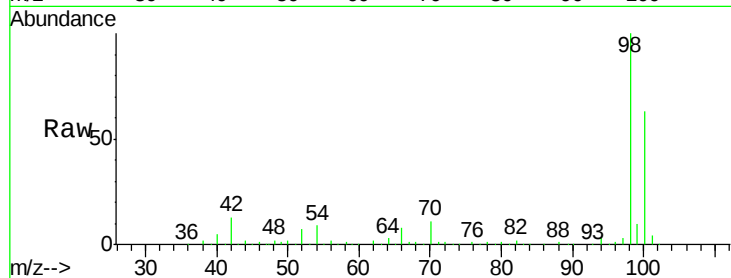

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

150000



100000

50000

0

8.65 8.70 8.75 8.80 8.85

Time-->

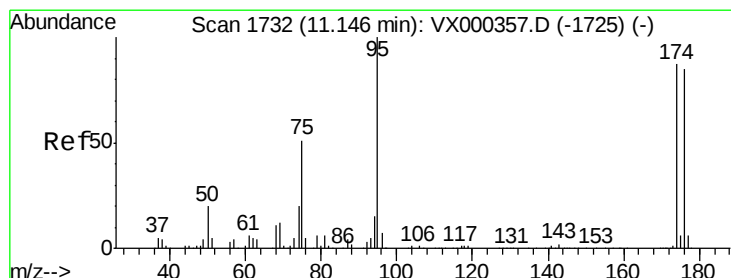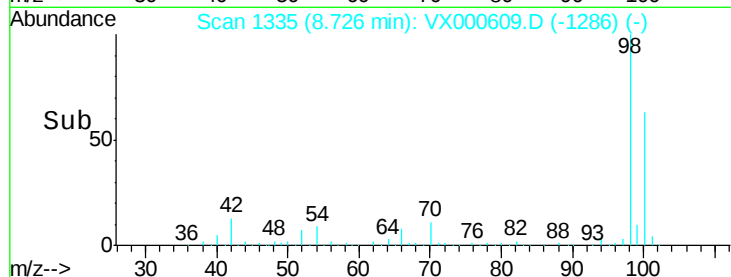

#62

4-Bromofluorobenzene

Concen: 41.33 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. 0.00 min

Lab File: VX000609.D

Acq: 31 Mar 2018 22:57


Tgt Ion: 95 Resp: 78825

Ion Ratio Lower Upper

95 100

174 90.1 0.0 173.6

176 88.1 0.0 164.6

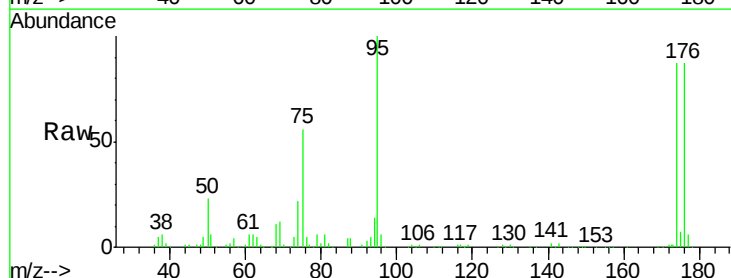

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

80000

60000


40000


20000

0

11.10 11.15 11.20


Time-->

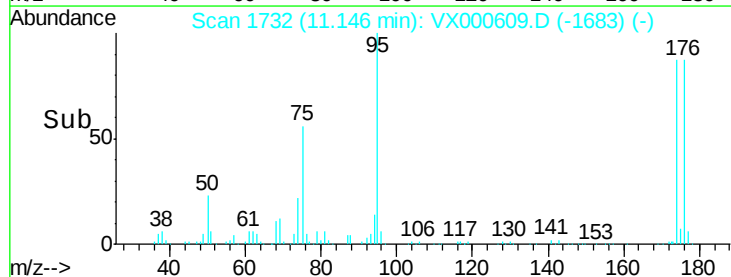



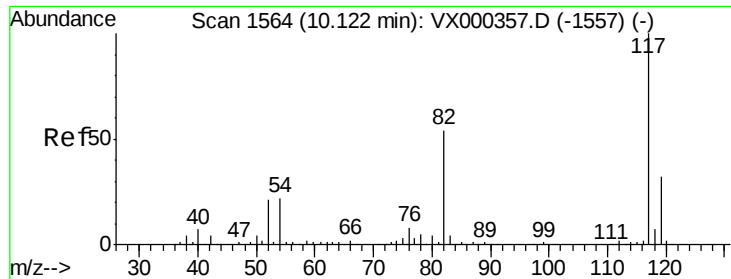


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. -0.00 min
Lab File: VX000609.D
Acq: 31 Mar 2018 22:57

Tot Ion:117 Resp: 177159
Ion Ratio Lower Upper
117 100
82 54.0 43.8 65.8
119 32.5 24.9 37.3

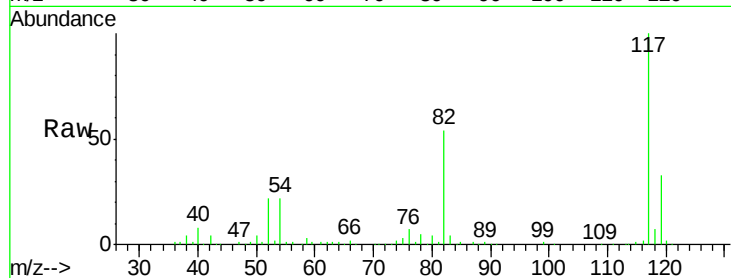


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX
Ion 118.90 (118.60 to 119.60): V

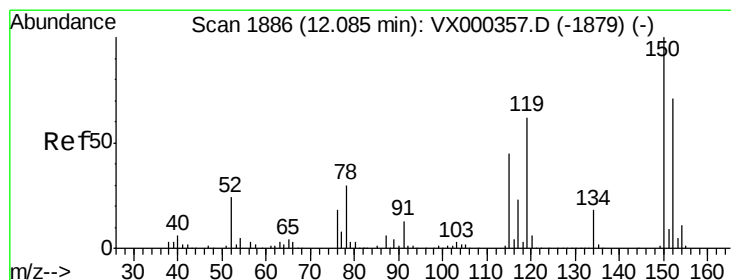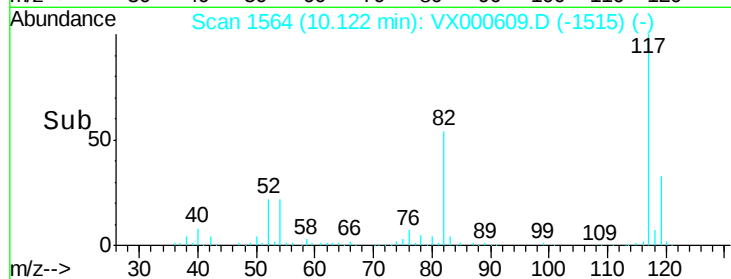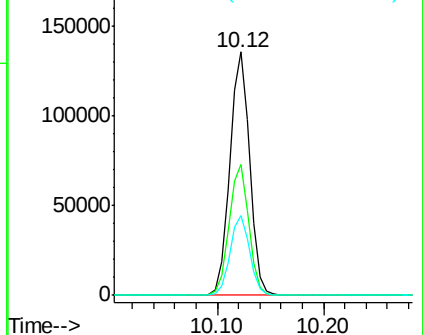

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.09 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX000609.D
Acq: 31 Mar 2018 22:57

Tgt Ion:152 Resp: 93262
Ion Ratio Lower Upper
152 100
115 57.3 39.8 119.3
150 159.8 0.0 344.4

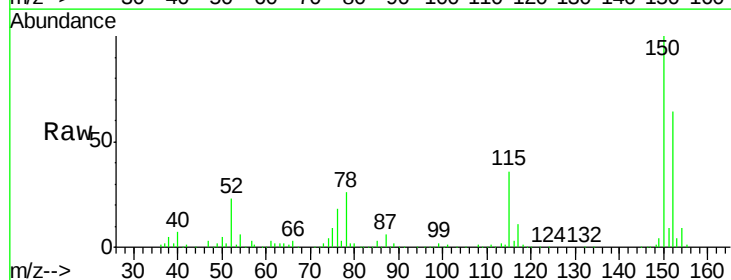

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

