


Data Path : W:\HPCHEM1\MSVOA\_X\Data\VX033118\  
Data File : VX000582.D  
Acq On : 31 Mar 2018 09:10  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA\_X\METHOD\82X032018W.M  
Title : SW846 8260  
Last Update : Wed Mar 21 04:52:42 2018

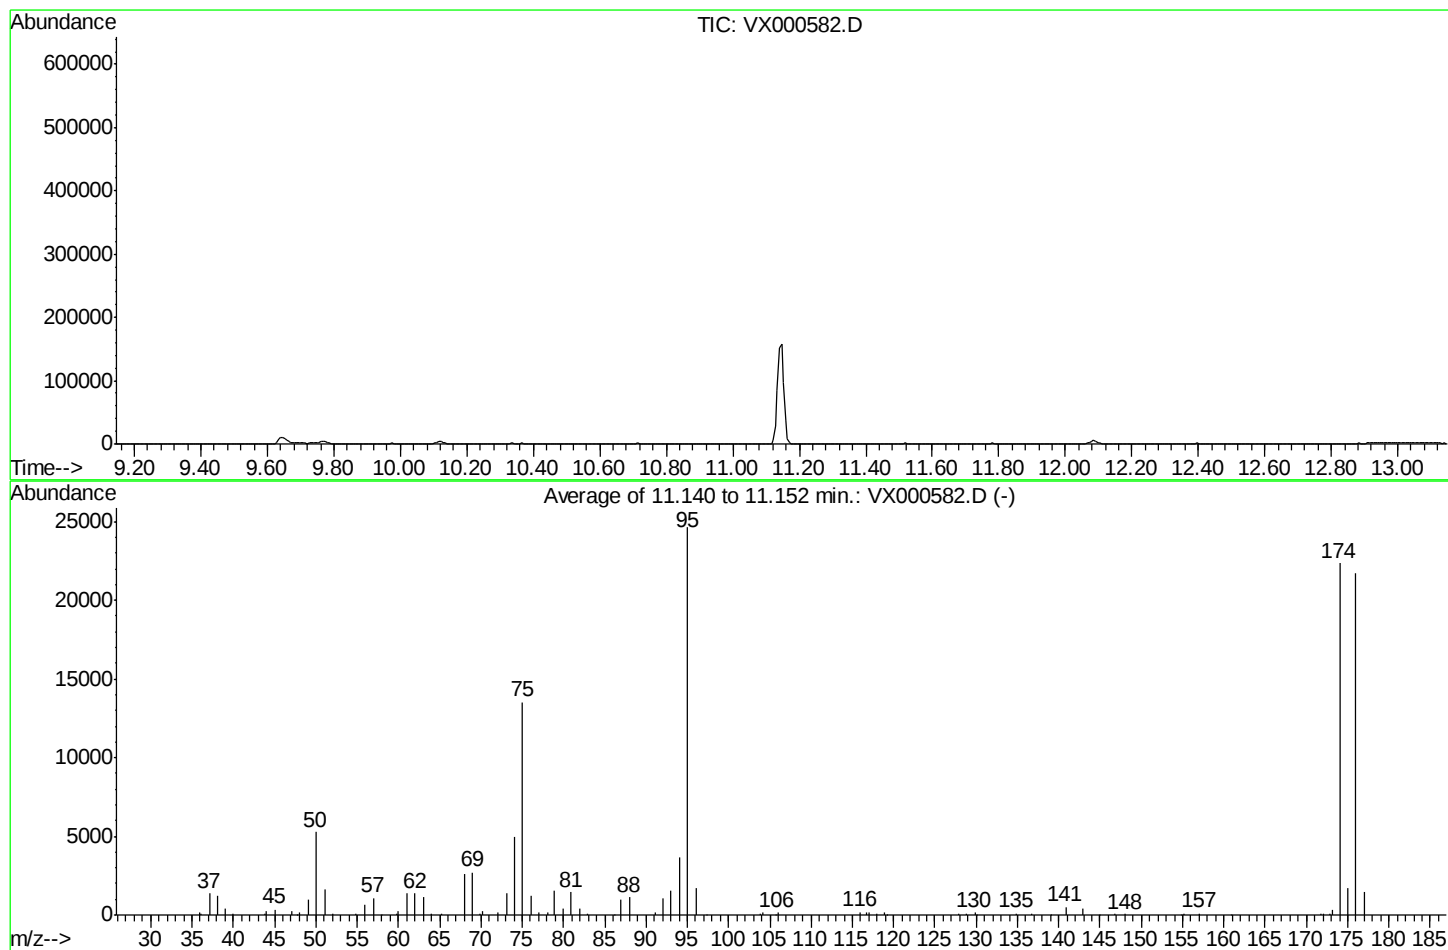

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 21.4      | 5263    | PASS             |
| 75          | 95           | 30           | 60           | 54.9      | 13522   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 24634   | PASS             |
| 96          | 95           | 5            | 9            | 7.1       | 1747    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.5       | 338     | PASS             |
| 174         | 95           | 50           | 100          | 90.7      | 22333   | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 1677    | PASS             |
| 176         | 174          | 95           | 101          | 97.1      | 21693   | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 1477    | PASS             |