


Data Path : W:\HPCHEM1\MSVOA_X\Data\VX033118\
Data File : VX000607.D
Acq On : 31 Mar 2018 21:15
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Title : SW846 8260
Last Update : Wed Mar 21 04:52:42 2018

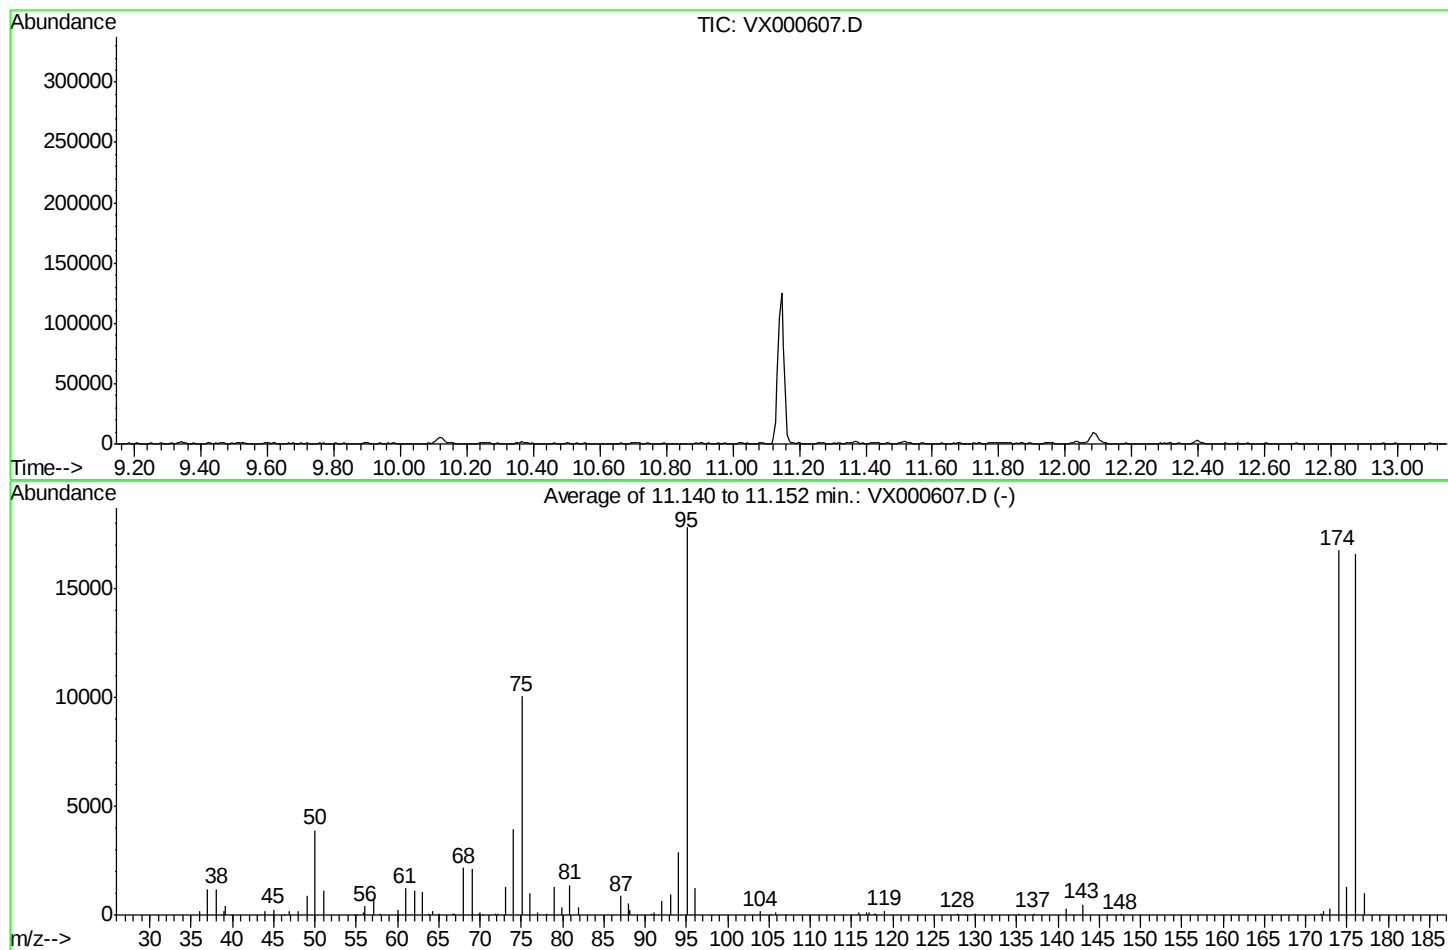

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	3899	PASS
75	95	30	60	56.4	10059	PASS
95	95	100	100	100.0	17821	PASS
96	95	5	9	6.8	1211	PASS
173	174	0.00	2	1.8	307	PASS
174	95	50	100	94.0	16749	PASS
175	174	5	9	7.6	1271	PASS
176	174	95	101	99.2	16609	PASS
177	176	5	9	6.1	1011	PASS