


Data Path : W:\HPCHEM1\MSVOA_X\Data\VX040218\
Data File : VX000632.D
Acq On : 02 Apr 2018 09:46
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X032018W.M
Title : SW846 8260
Last Update : Wed Mar 21 04:52:42 2018

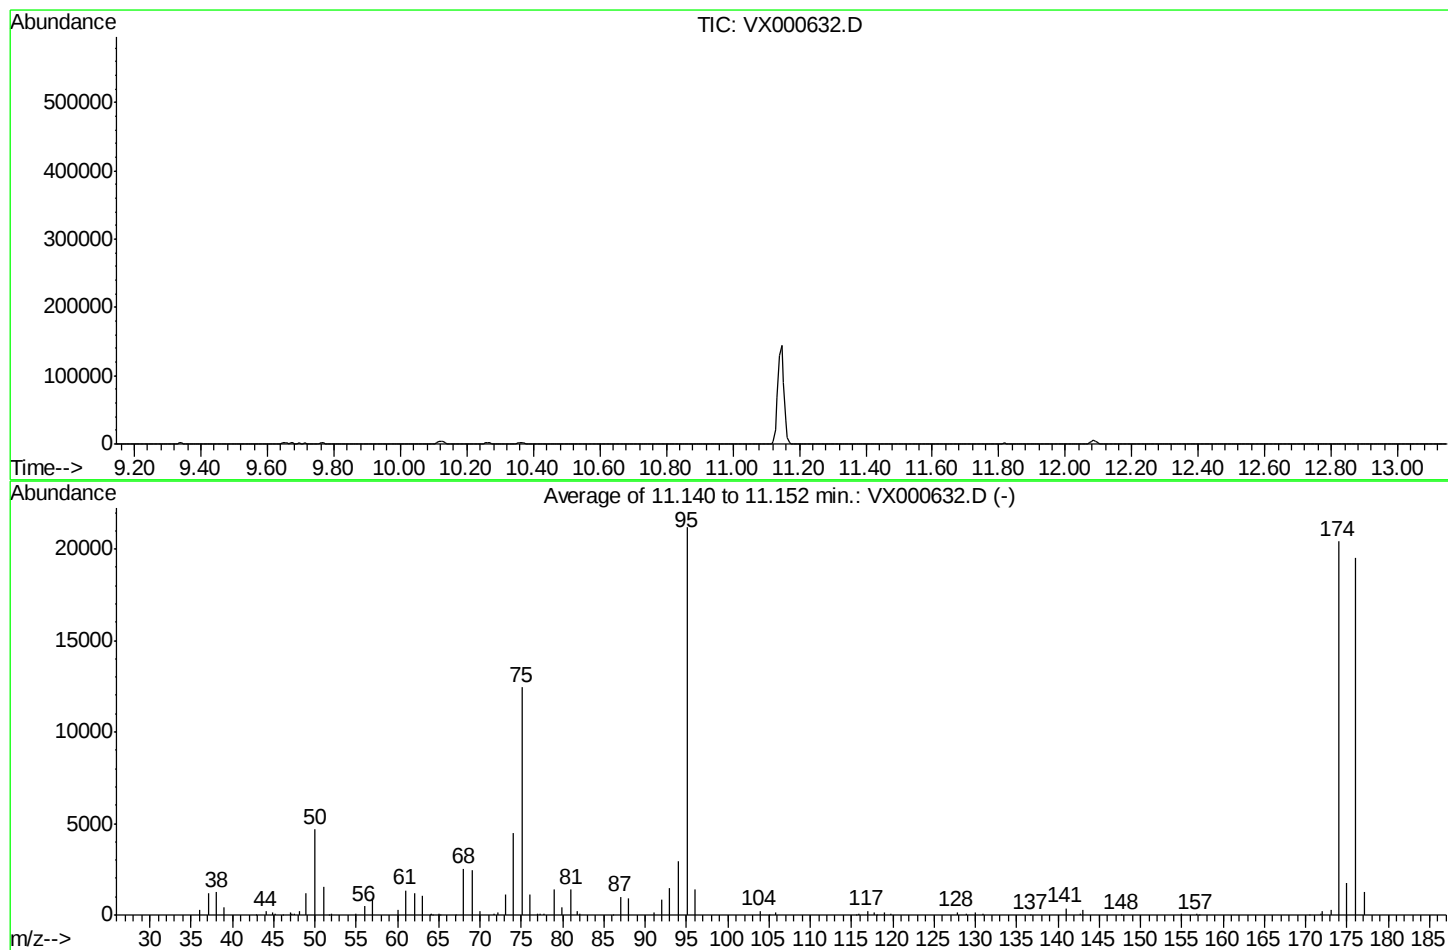

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	4672	PASS
75	95	30	60	58.6	12424	PASS
95	95	100	100	100.0	21186	PASS
96	95	5	9	6.6	1406	PASS
173	174	0.00	2	1.5	298	PASS
174	95	50	100	96.3	20410	PASS
175	174	5	9	8.4	1717	PASS
176	174	95	101	95.7	19541	PASS
177	176	5	9	6.5	1270	PASS