


Data Path : W:\HPCHEM1\MSVOA X\Data\VX040418\
Data File : VX000658.D
Acq On : 04 Apr 2018 14:00
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X040418W.M
Title : SW846 8260
Last Update : Thu Apr 05 03:34:50 2018

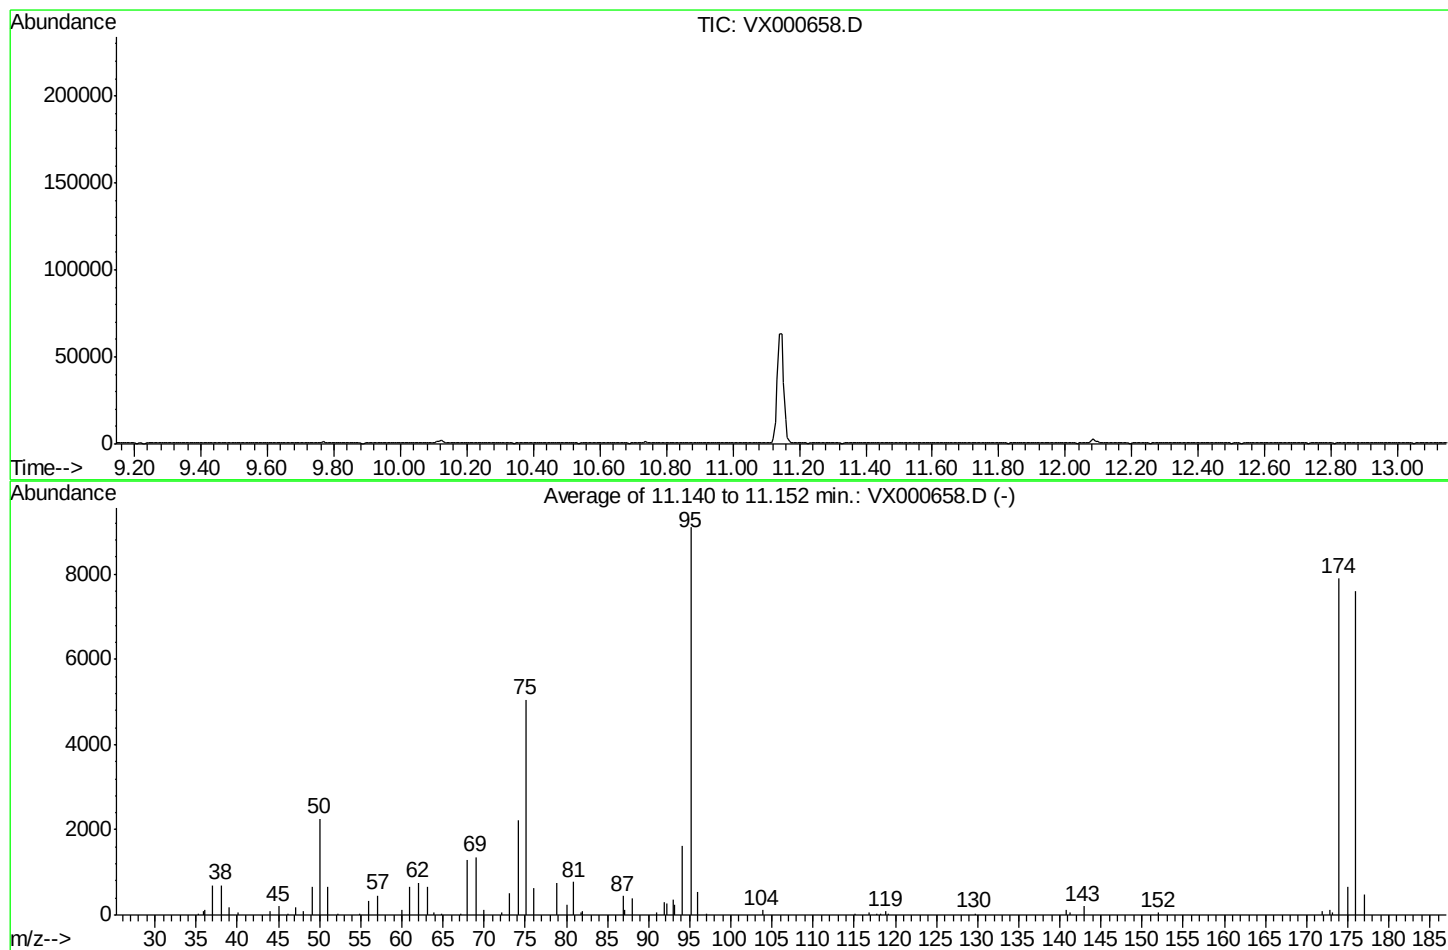

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.9	2267	PASS
75	95	30	60	55.6	5060	PASS
95	95	100	100	100.0	9098	PASS
96	95	5	9	6.0	550	PASS
173	174	0.00	2	1.4	114	PASS
174	95	50	100	86.7	7891	PASS
175	174	5	9	8.5	673	PASS
176	174	95	101	96.2	7593	PASS
177	176	5	9	6.2	474	PASS