




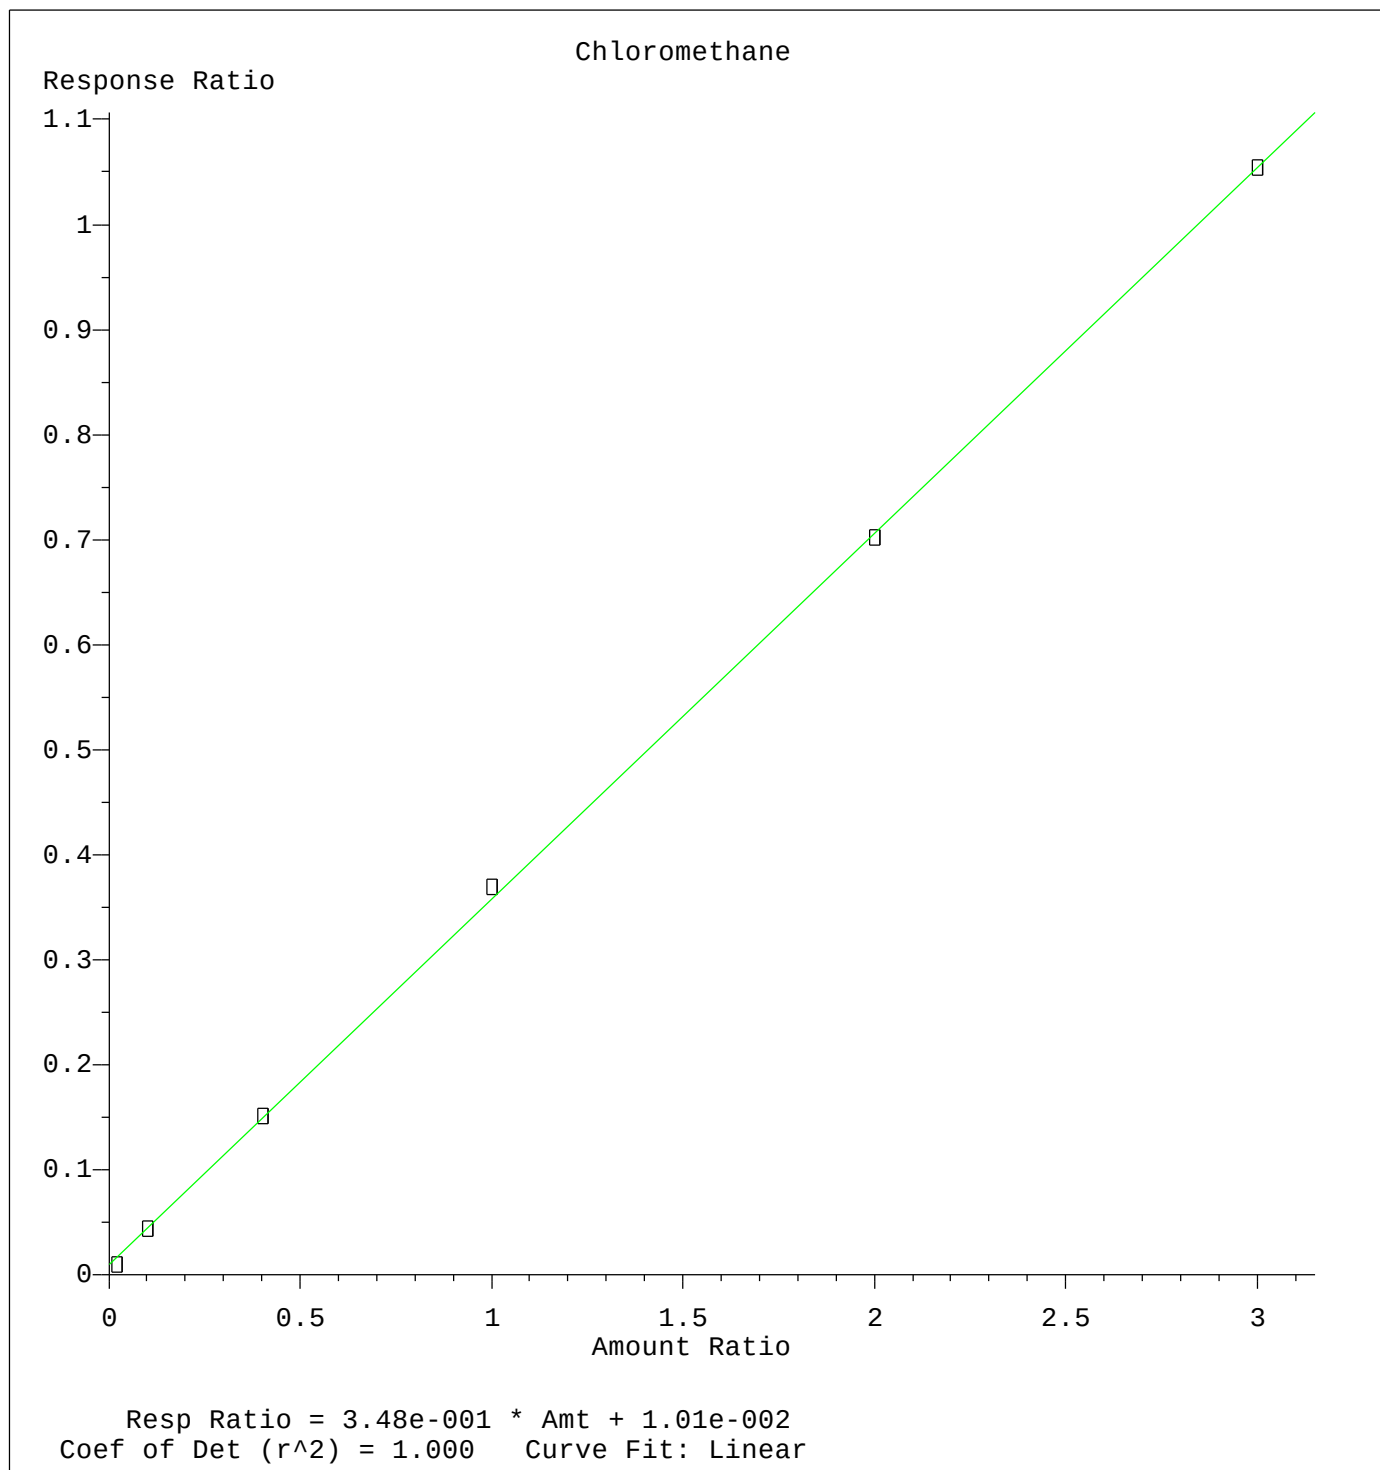


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

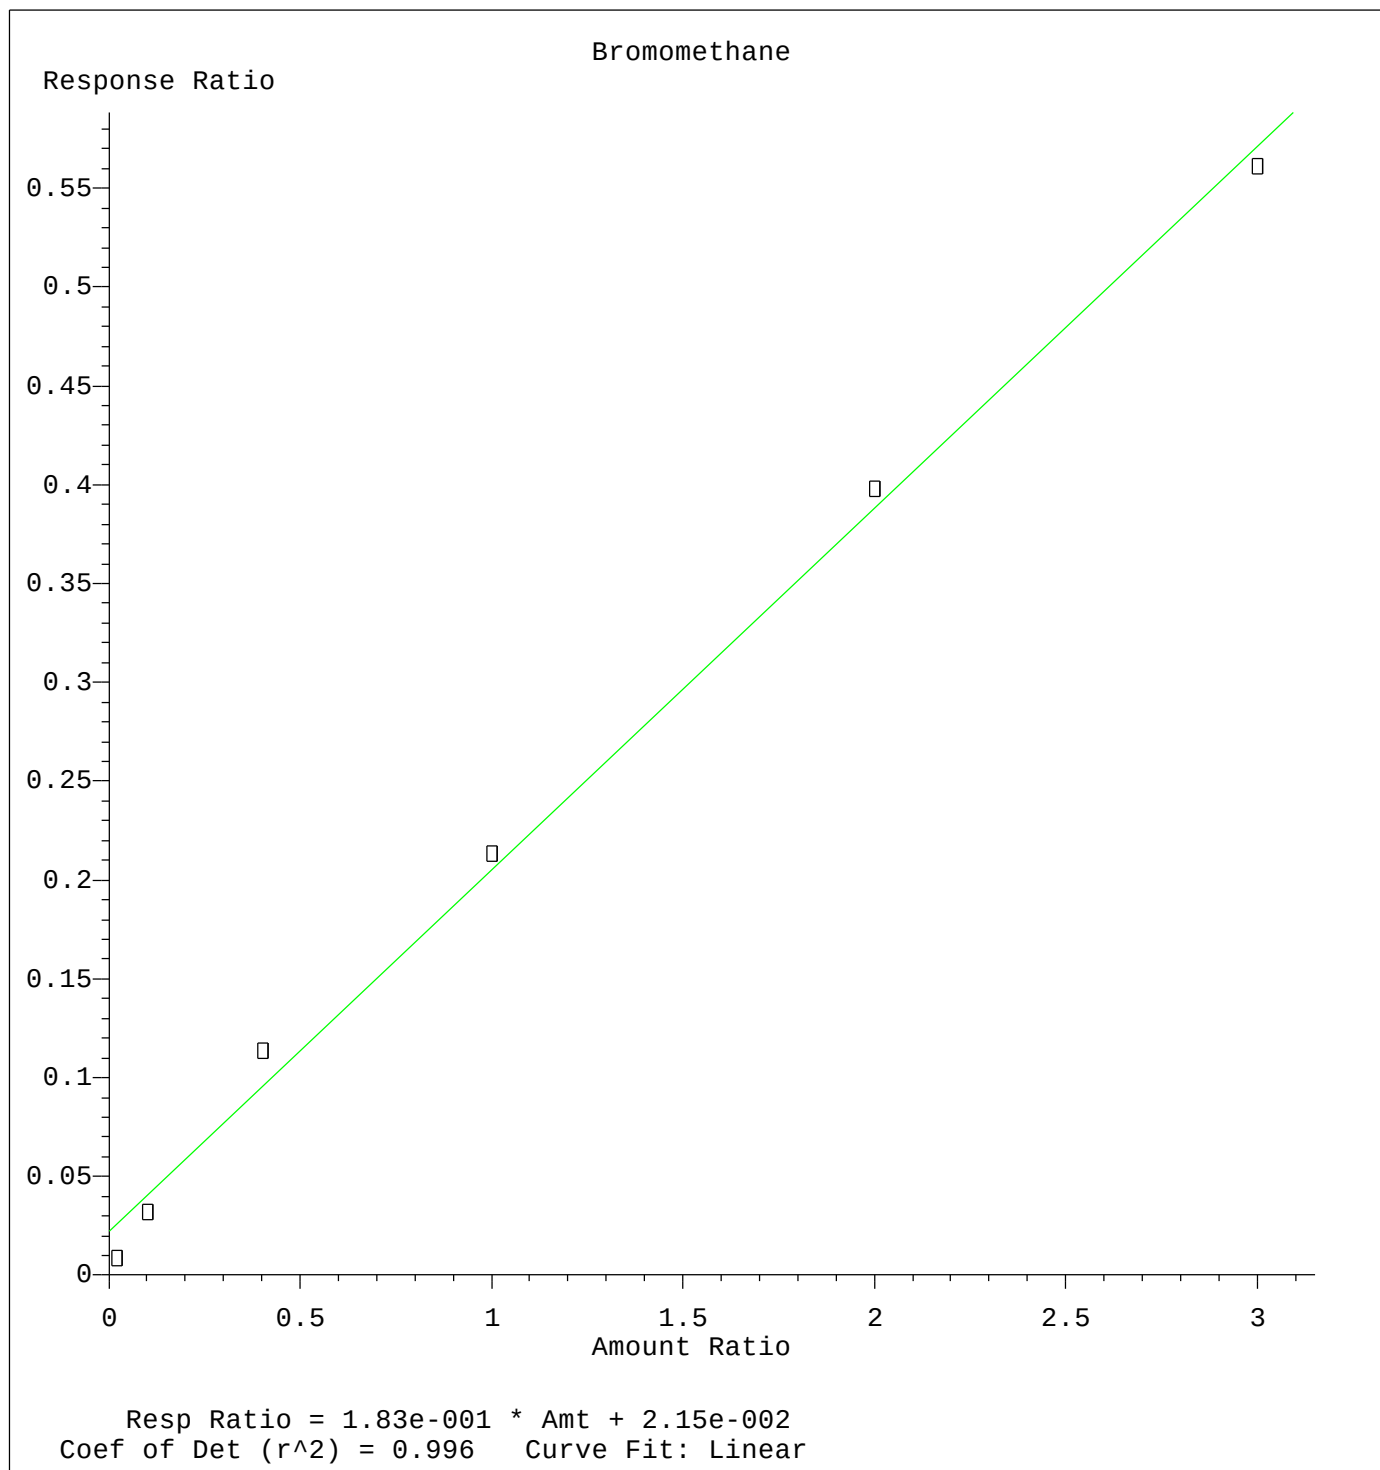


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

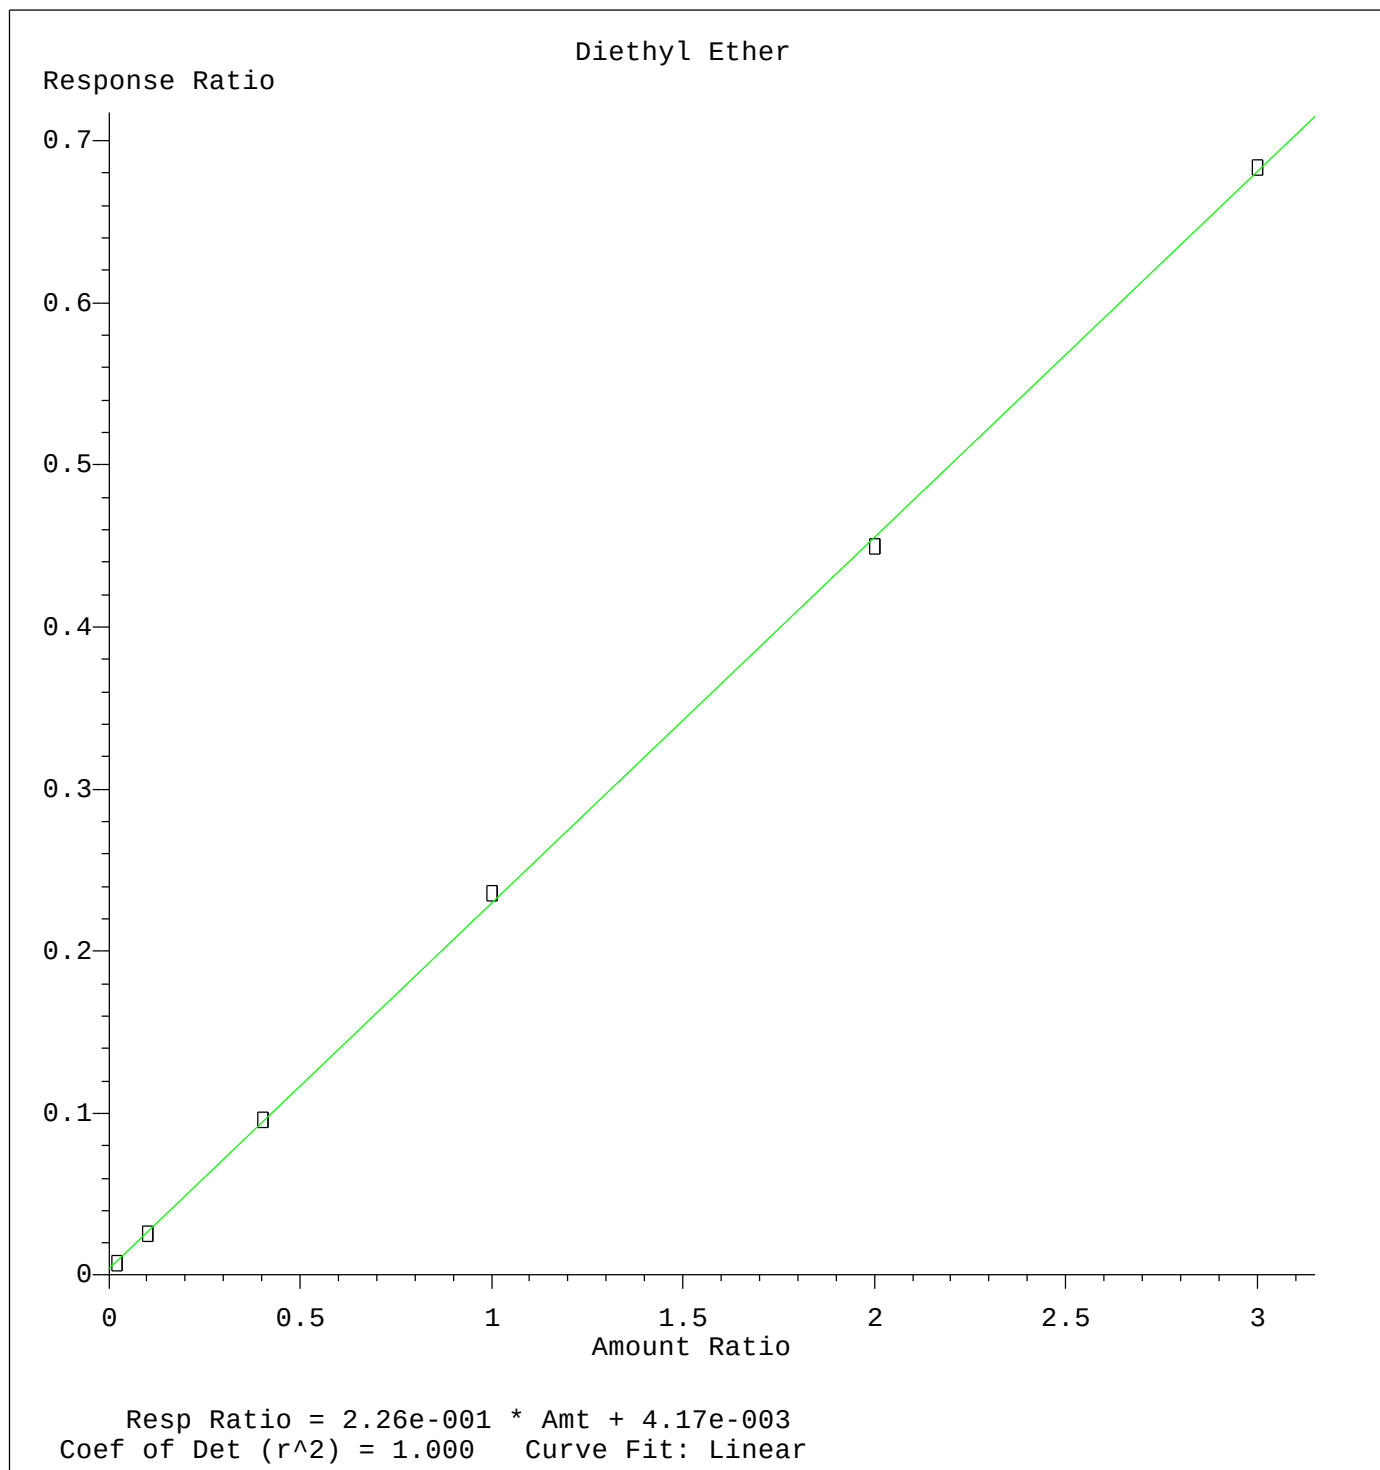


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

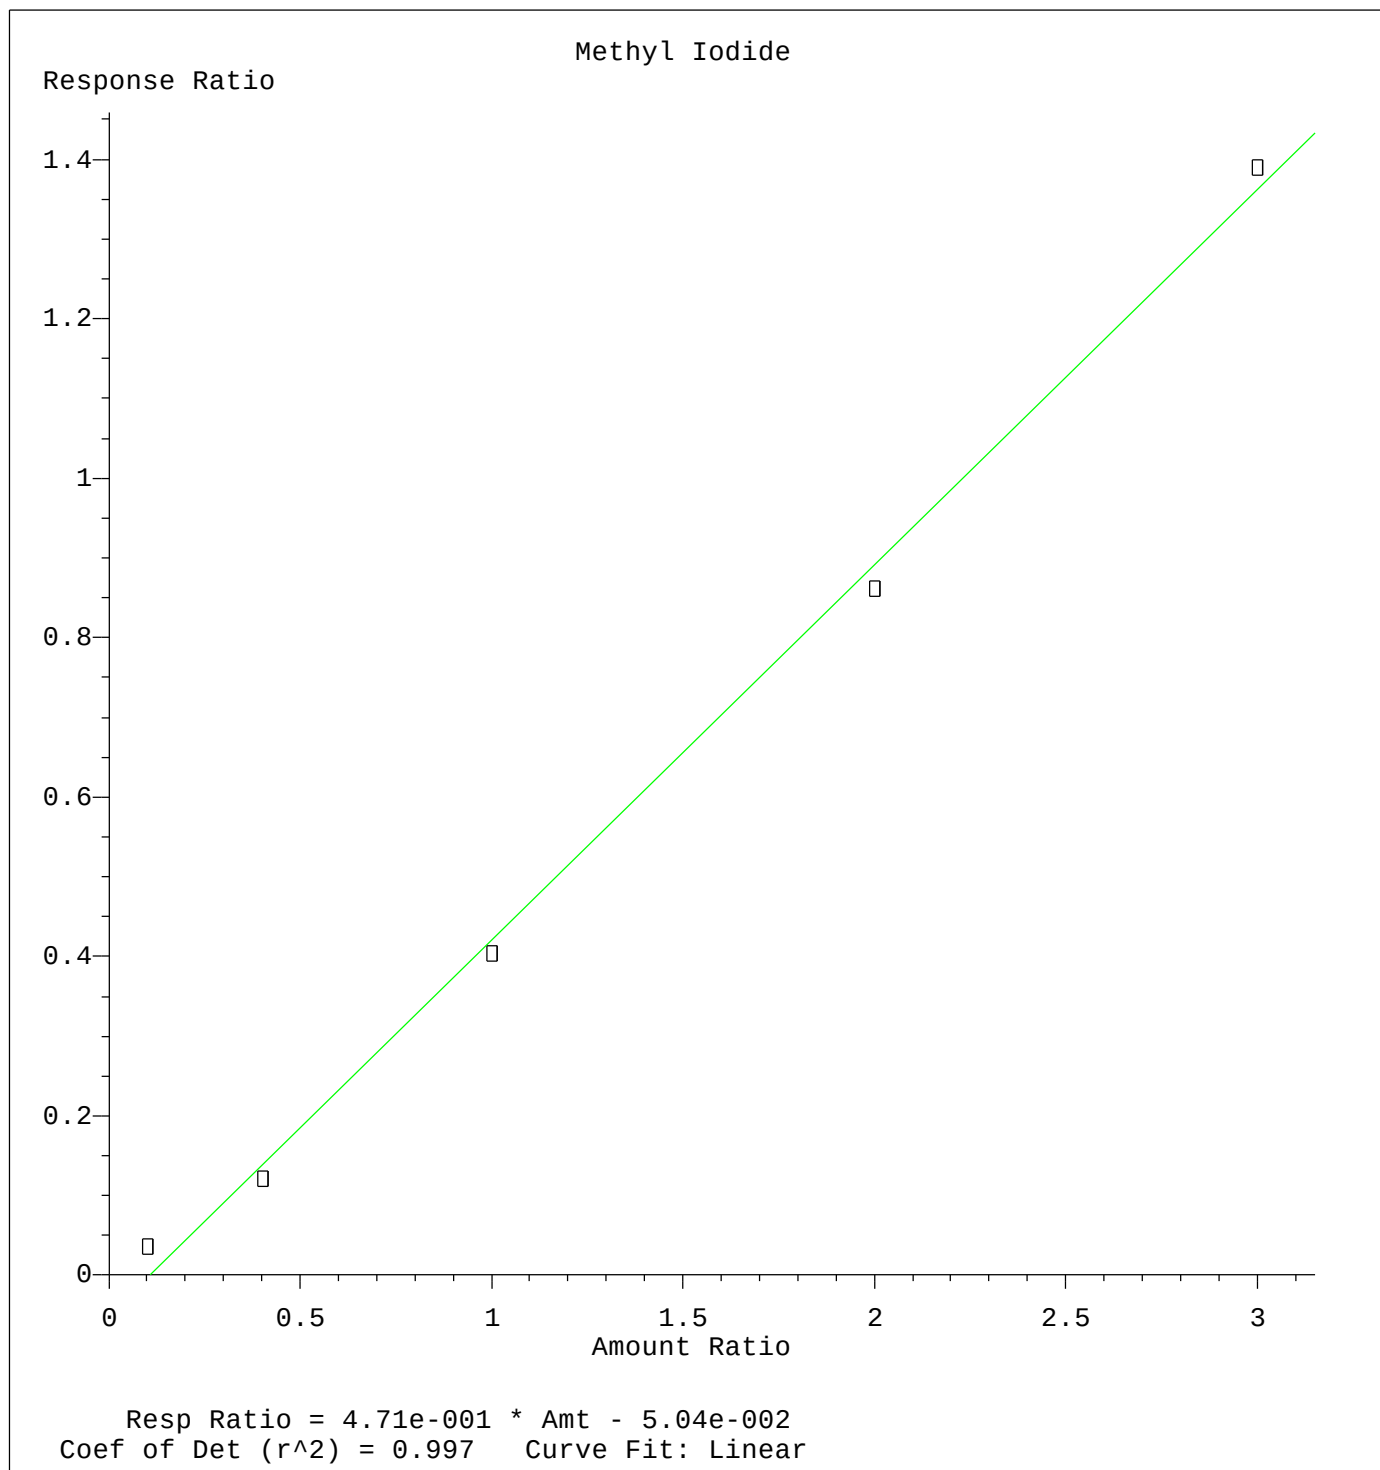


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

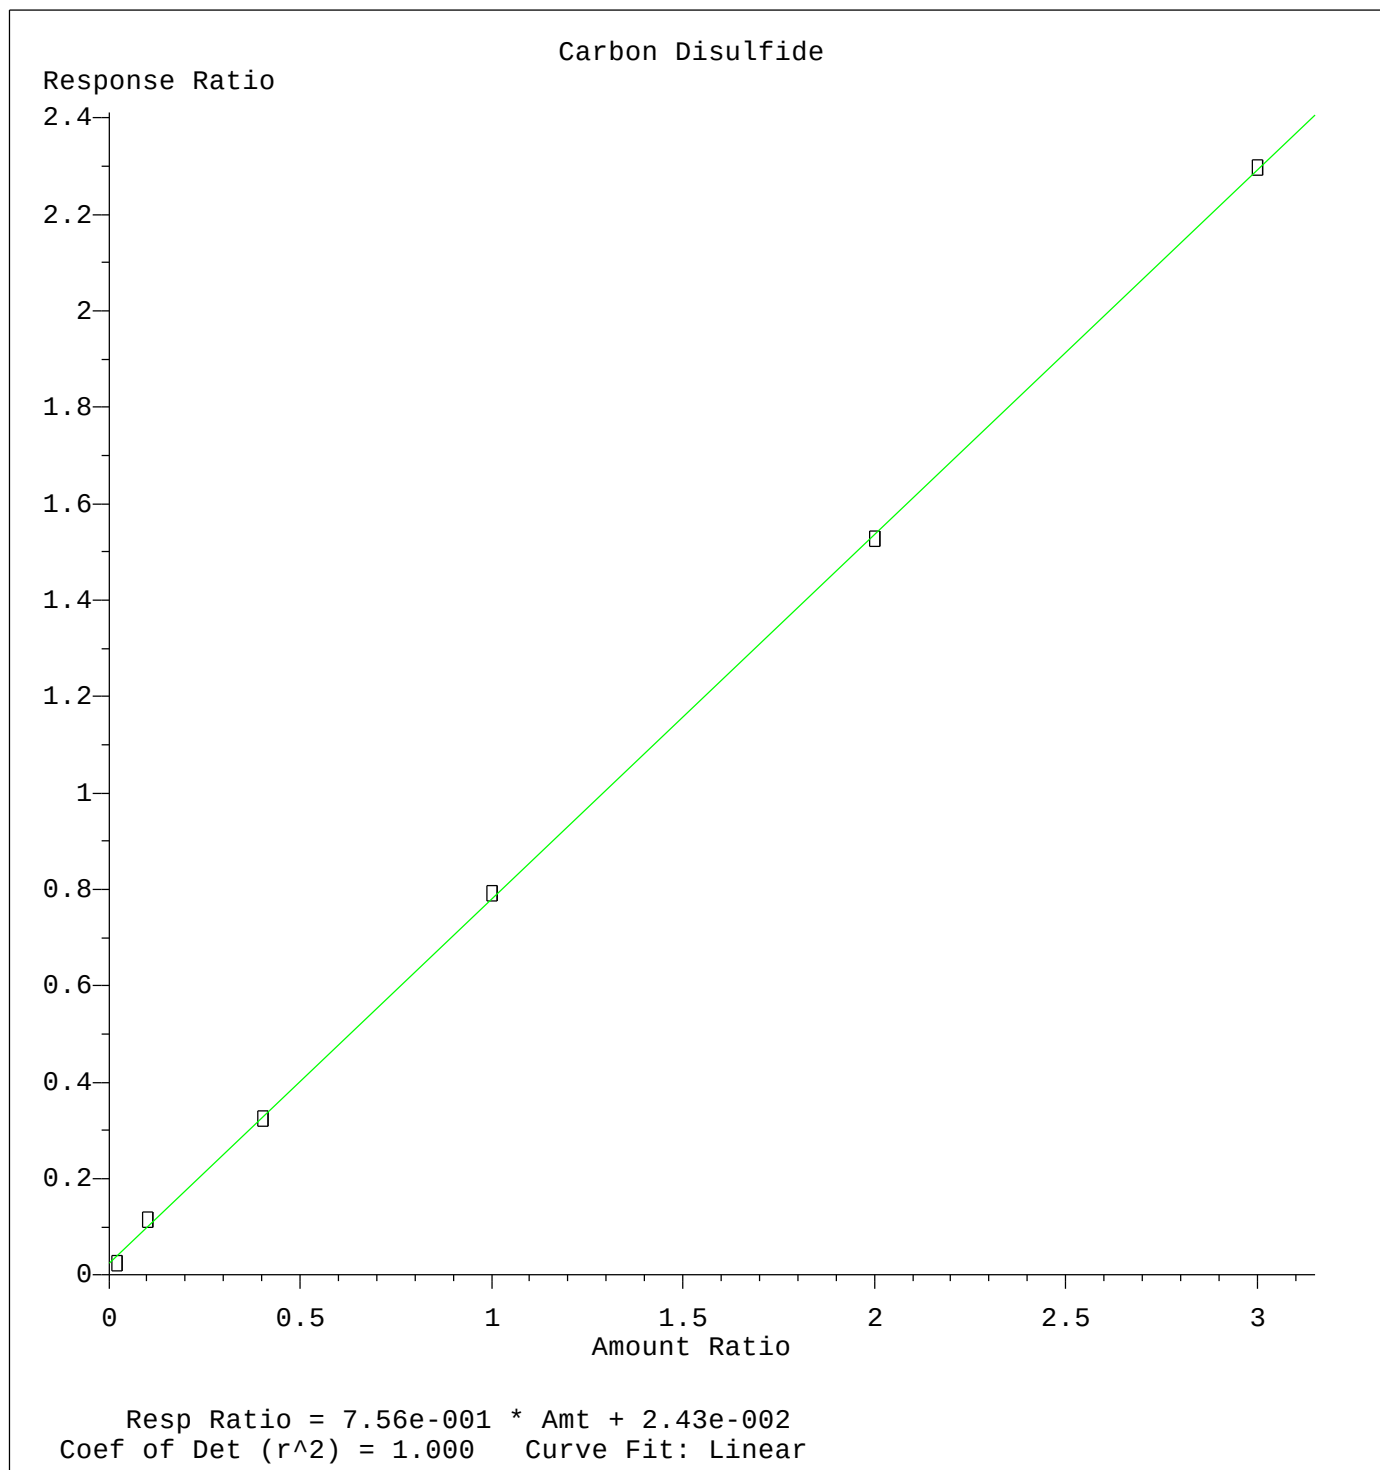

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

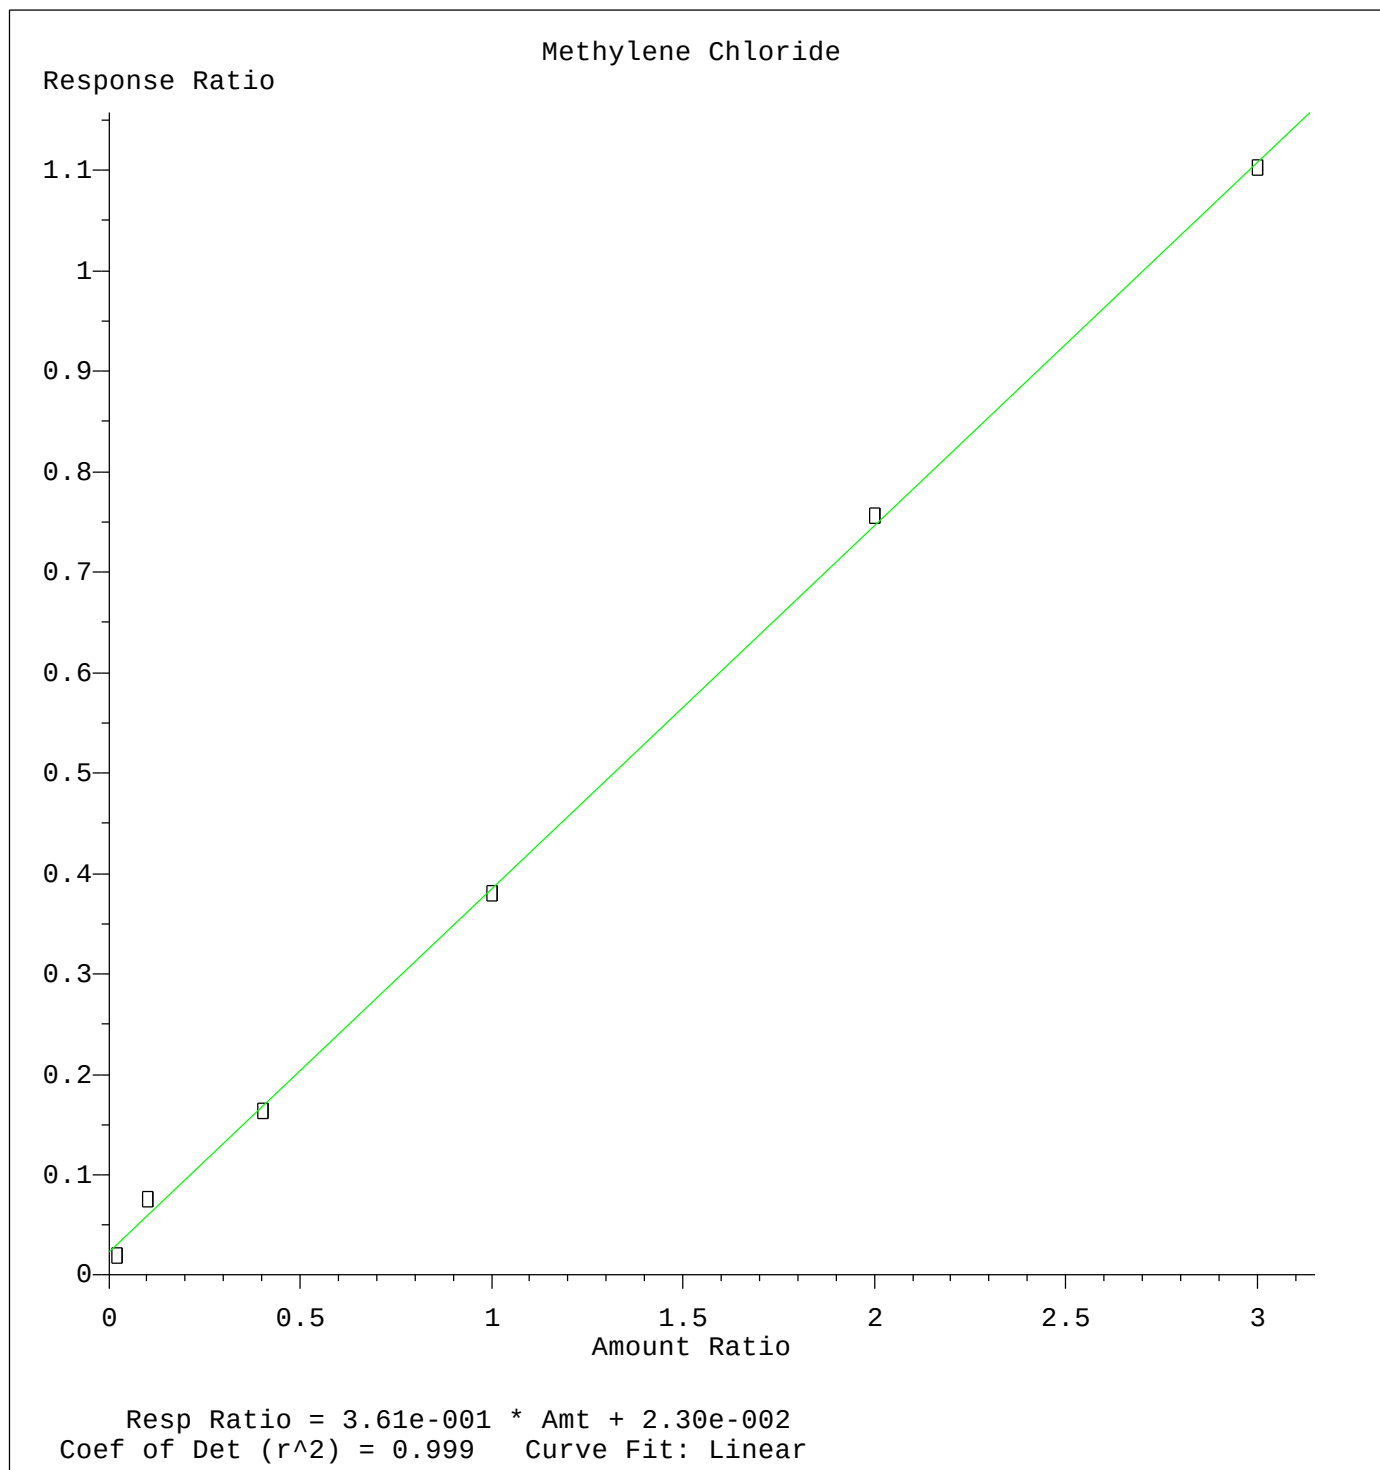


Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

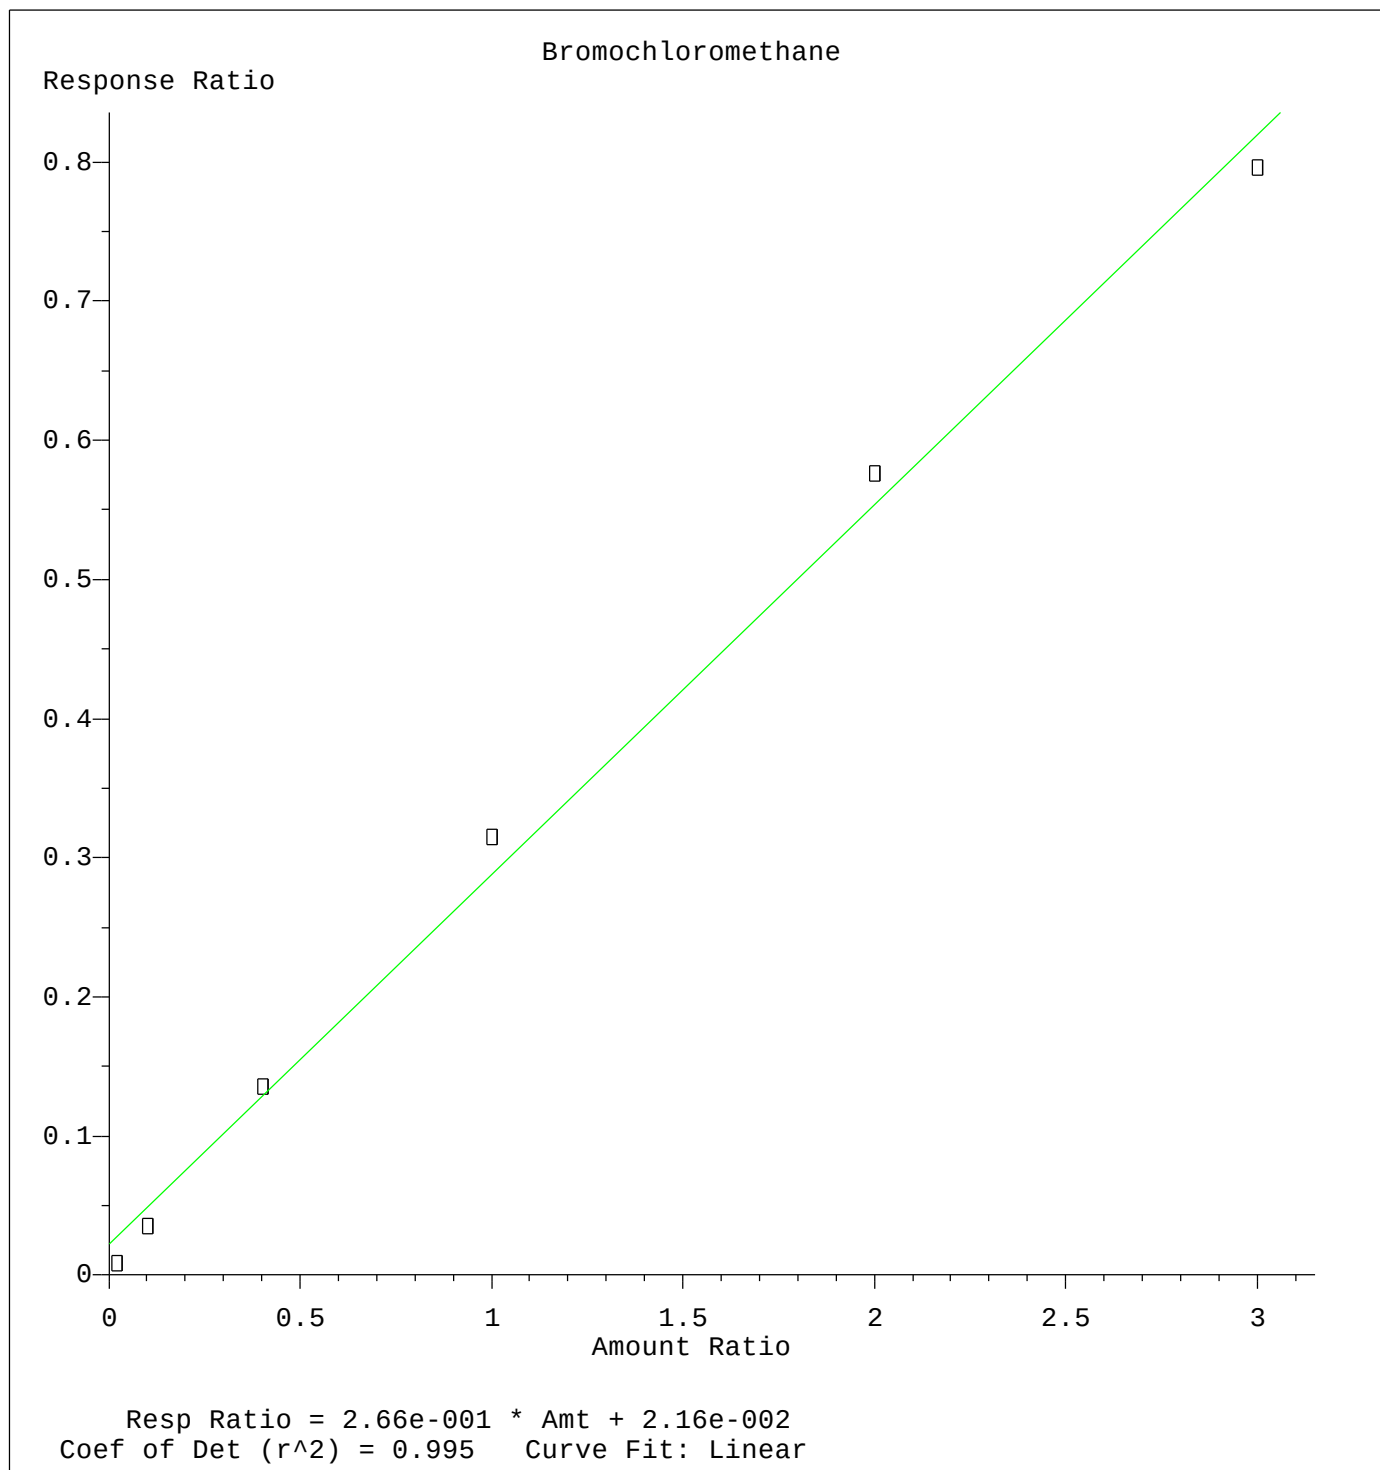

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

Cyclohexane

Response Ratio

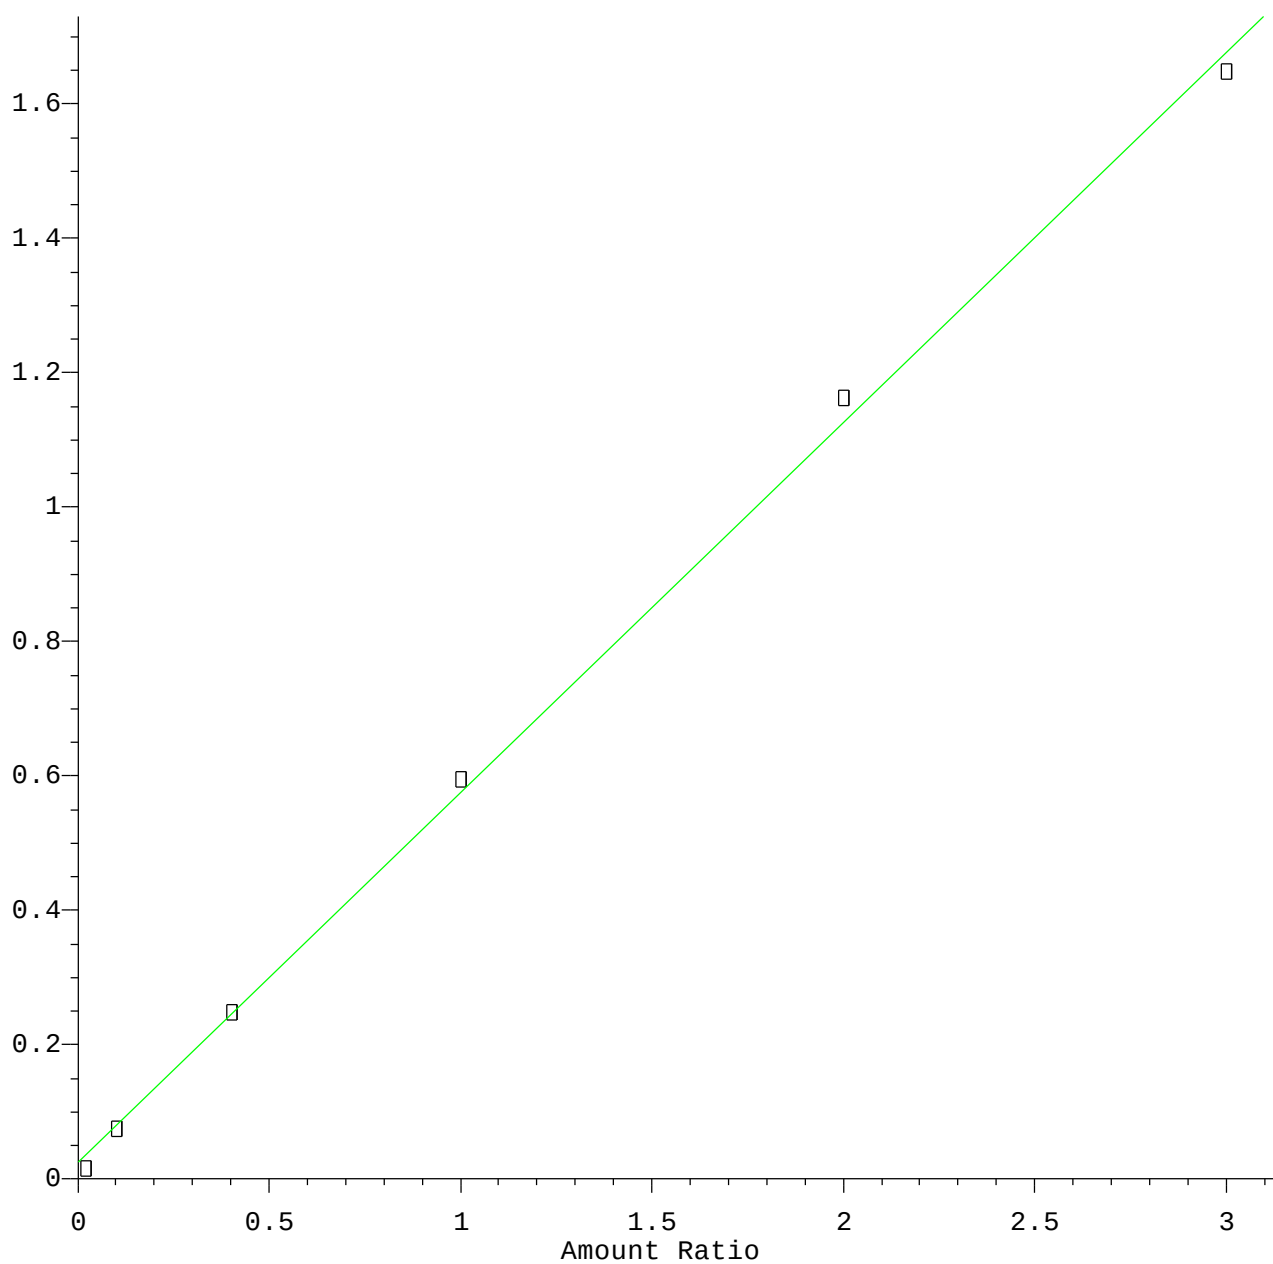


Resp Ratio = $5.51 \times 10^{-1} \times \text{Amt} + 2.53 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

Methylcyclohexane

Response Ratio

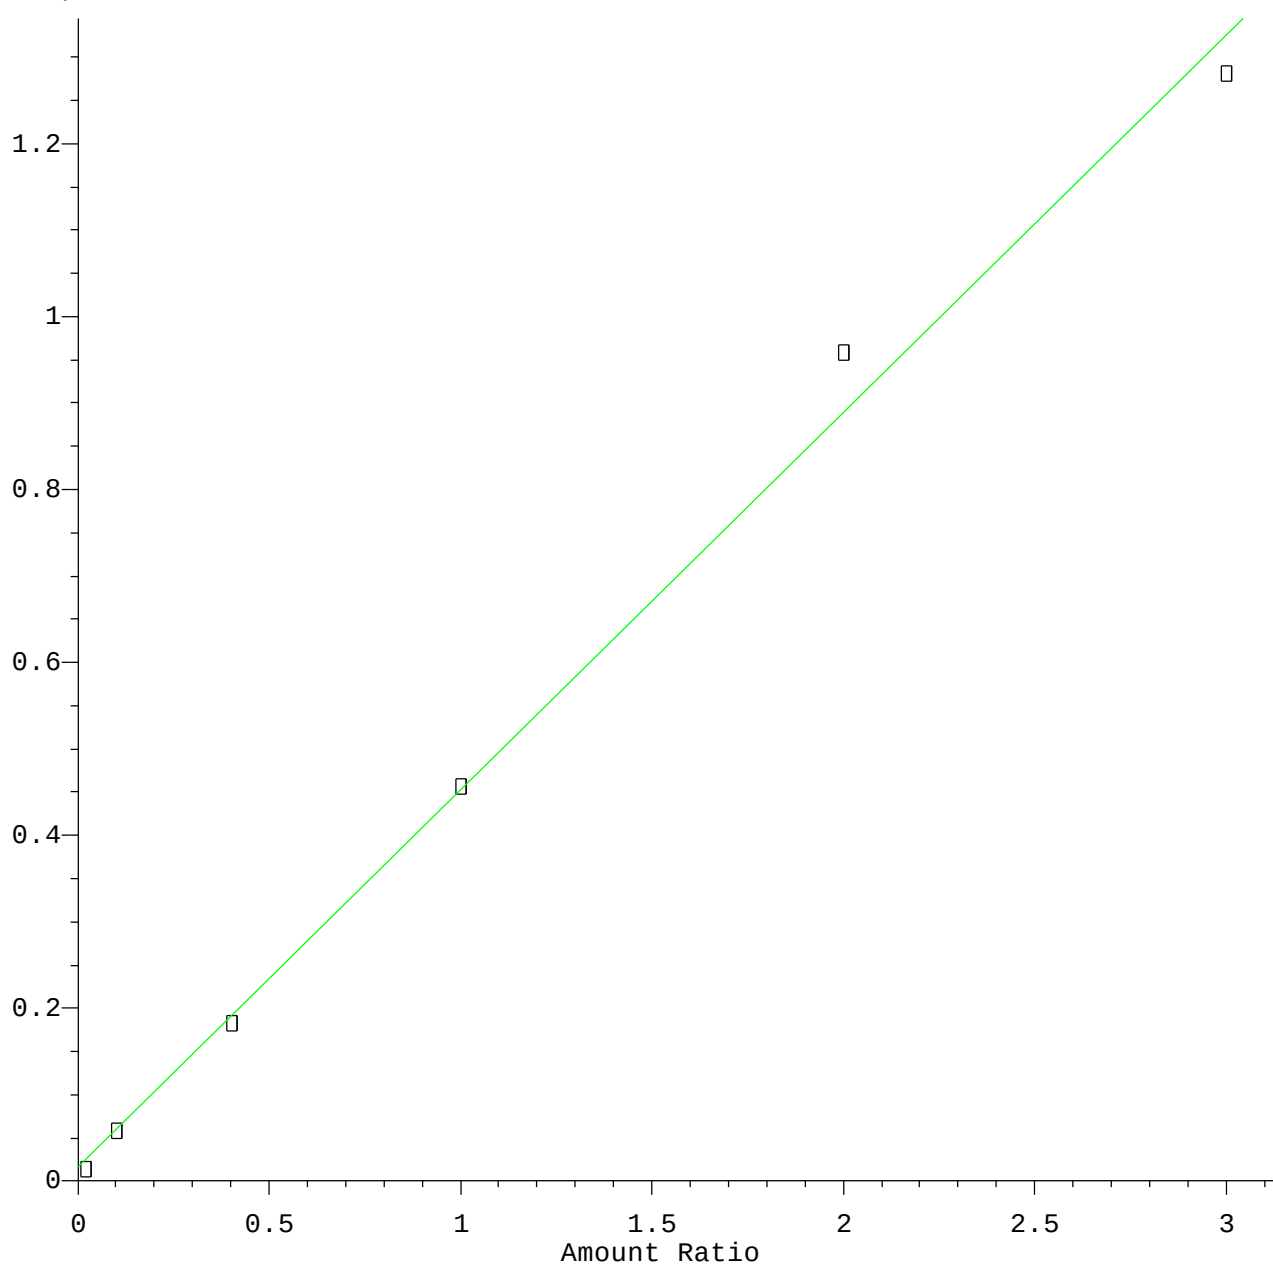


Resp Ratio = $4.36 \times 10^{-1} \times \text{Amt} + 1.69 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018

Methylcyclohexane

Response Ratio

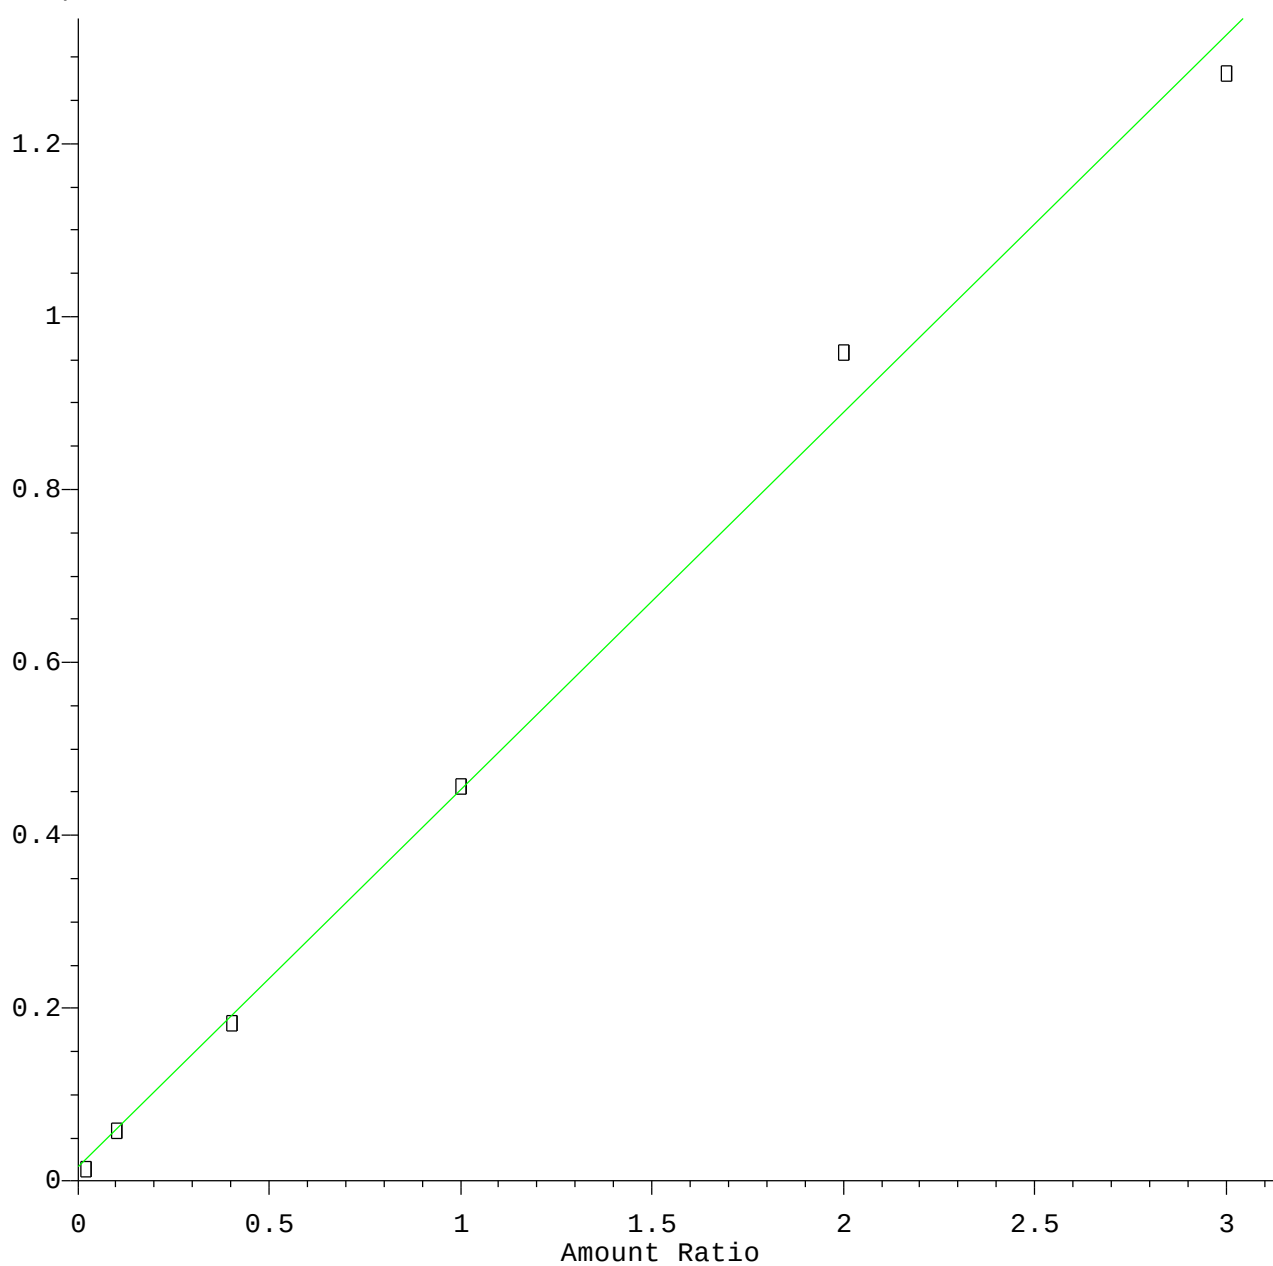

Resp Ratio = $4.36 \times 10^{-1} \times \text{Amt} + 1.69 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Calibration Table Last Updated: Sat Apr 07 17:01:21 2018