

Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX040718\
 Data File : VX000715.D
 Acq On : 07 Apr 2018 13:58
 Operator : JC/MD
 Sample : IBLK01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK01

Quant Time: Apr 09 01:29:53 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
 Quant Title : SW846 8260
 QLast Update : Sat Apr 07 16:39:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0m	50.00	ug/l	-5.68
34) 1,4-Difluorobenzene	0.00	114	0m	50.00	ug/l	-6.87
63) Chlorobenzene-d5	0.00	117	0m	50.00	ug/l	-10.12
72) 1,4-Dichlorobenzene-d4	0.00	152	0m	50.00	ug/l	-12.09

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.00	65	0d	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
35) Dibromofluoromethane	5.49	113	120	0.00	ug/l	-0.02
Spiked Amount	50.000		Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0d	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0d	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX040718\
Data File : VX000715.D
Acq On : 07 Apr 2018 13:58
Operator : JC/MD
Sample : IBLK01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK01

Quant Time: Apr 09 01:29:53 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Quant Title : SW846 8260
QLast Update : Sat Apr 07 16:39:08 2018
Response via : Initial Calibration

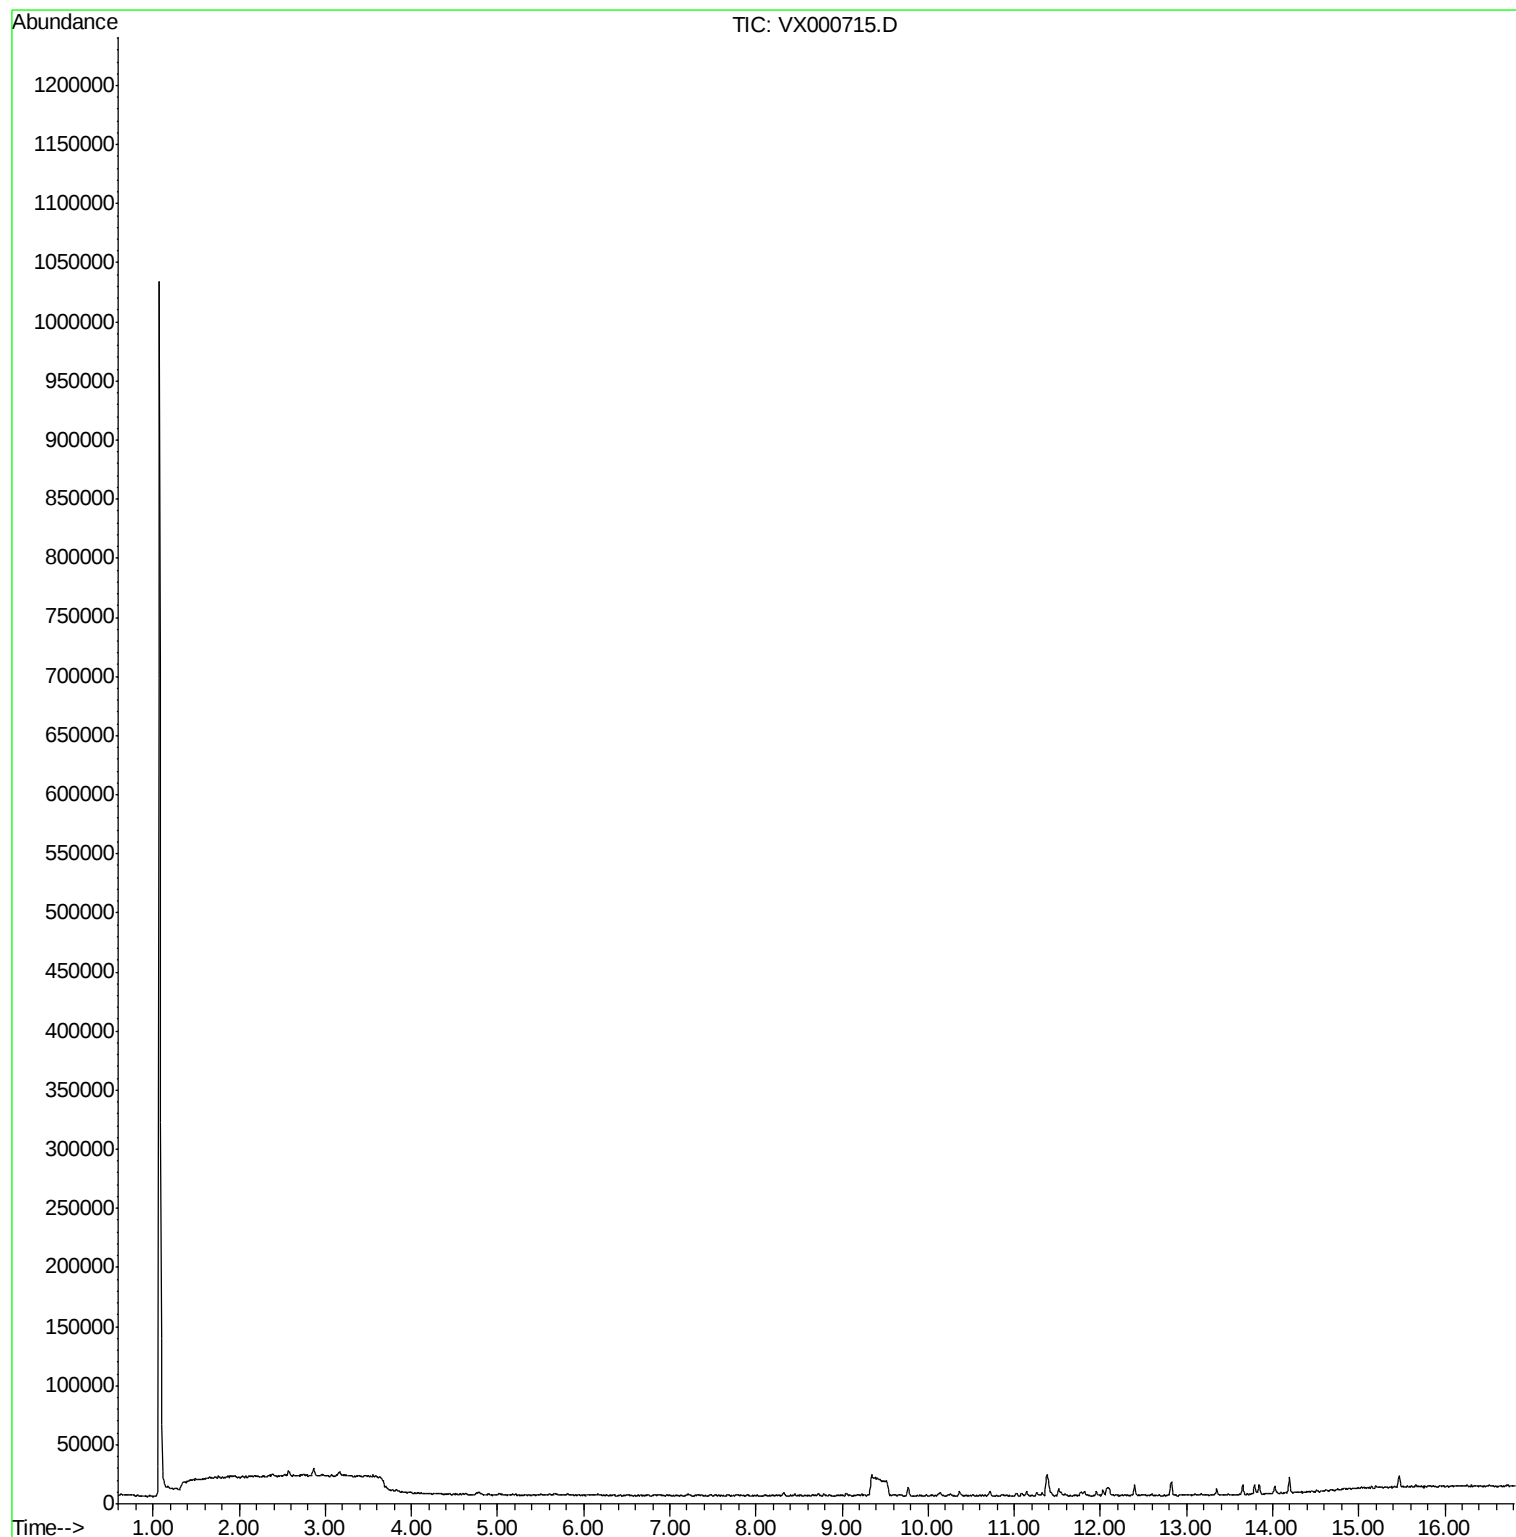


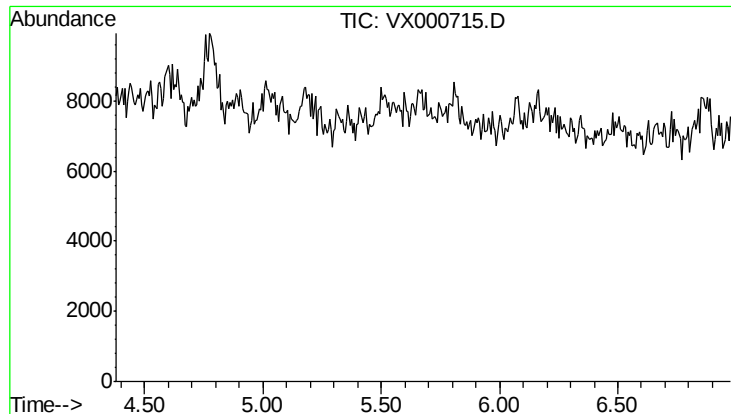


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 5.68 min

Lab File: VX000715.D
Acq: 07 Apr 2018 13:58

Instrument :
MSVOA_X
ClientSampleId :
IBLK01


Tgt Ion: 168
Sig Exp Ratio
168 100
99 46.5

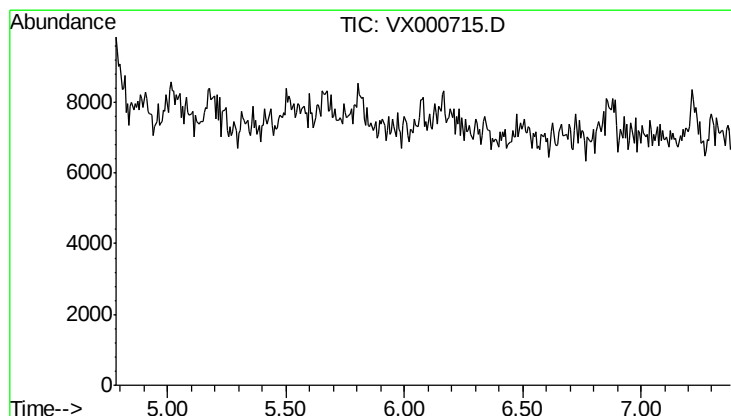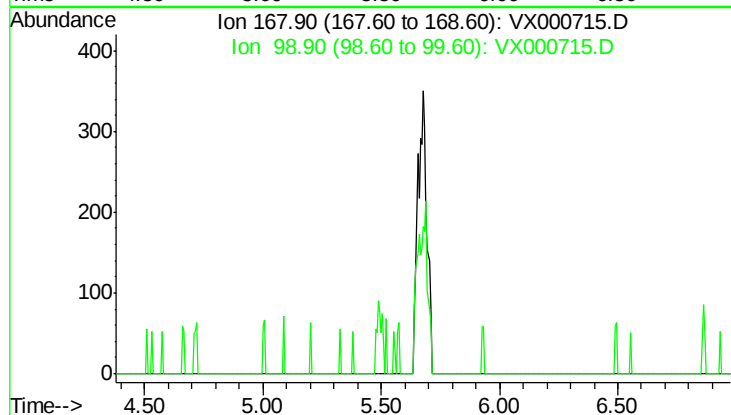


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 6.08 min

Lab File: VX000715.D
Acq: 07 Apr 2018 13:58

Tgt Ion: 65
Sig Exp Ratio
65 100
67 51.3

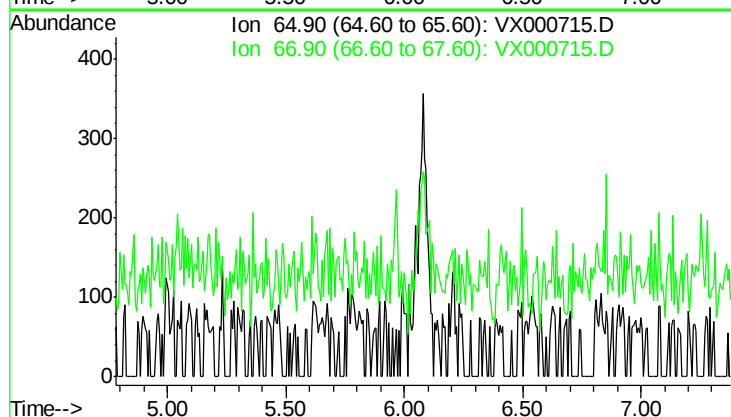

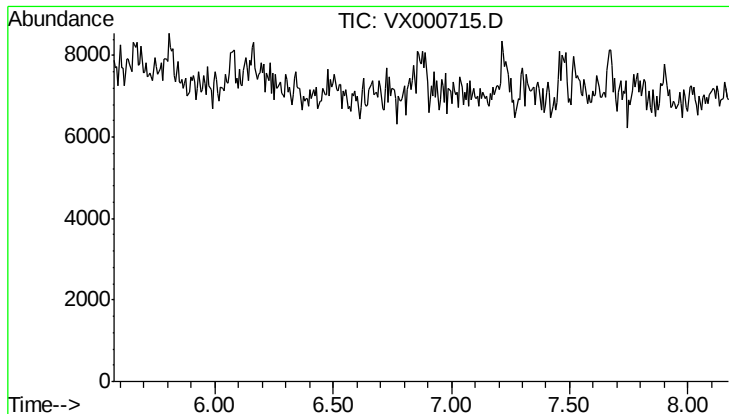

#34

1,4-Difluorobenzene

Concen: 0.000 ug/l

Expected RT: 6.87 min

Lab File: VX000715.D

Acq: 07 Apr 2018 13:58

Instrument :

MSVOA_X

ClientSampleId :

IBLK01



Tgt Ion: 114

Sig Exp Ratio

114 100

63 19.8

88 15.3

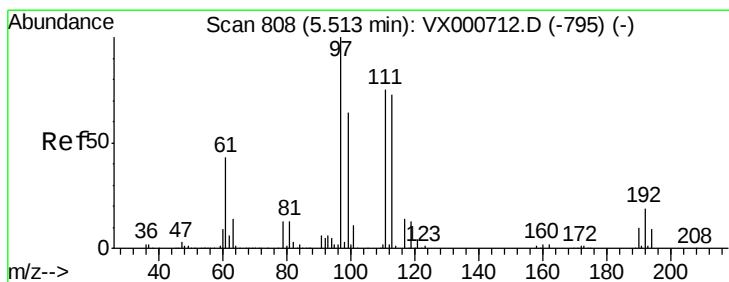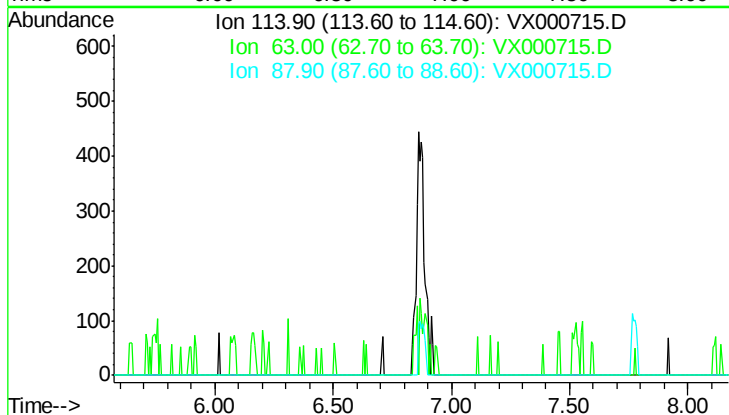

#35

Dibromofluoromethane

Concen: 0.000 ug/l

RT: 5.49 min Scan# 805

Delta R.T. -0.02 min

Lab File: VX000715.D

Acq: 07 Apr 2018 13:58




Tgt Ion: 113 Resp: 120


Ion Ratio Lower Upper

113 100

111 0.0 81.5 122.3#

192 0.0 20.0 30.0#

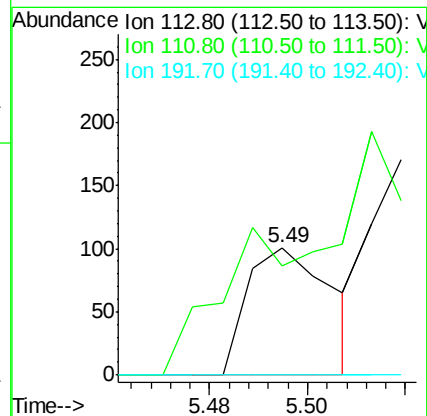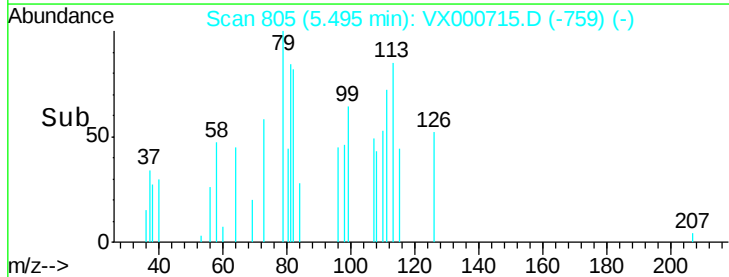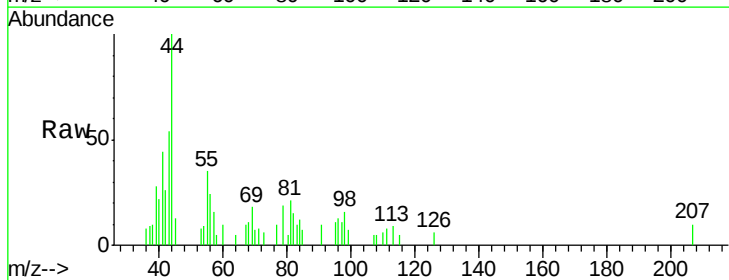


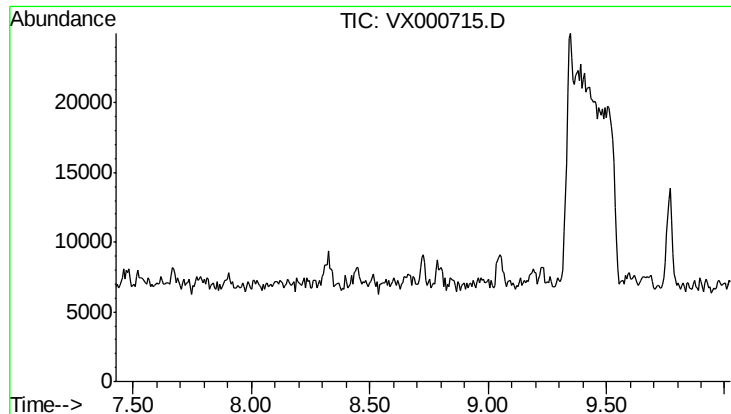


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 8.73 min

Lab File: VX000715.D
Acq: 07 Apr 2018 13:58

Instrument :
MSVOA_X
ClientSampleId :
IBLK01


Tgt Ion: 98
Sig Exp Ratio
98 100
100 65.7

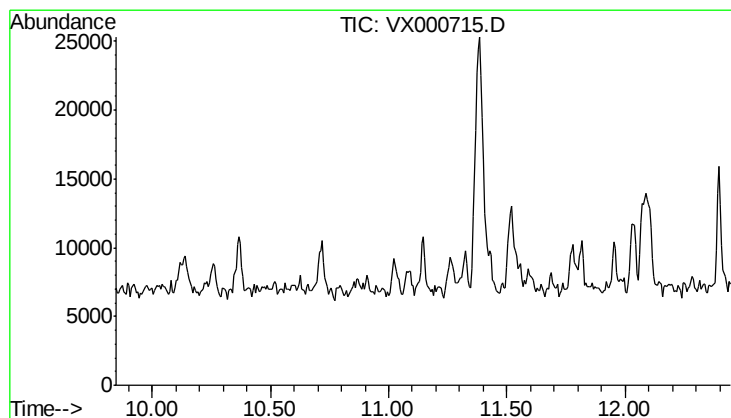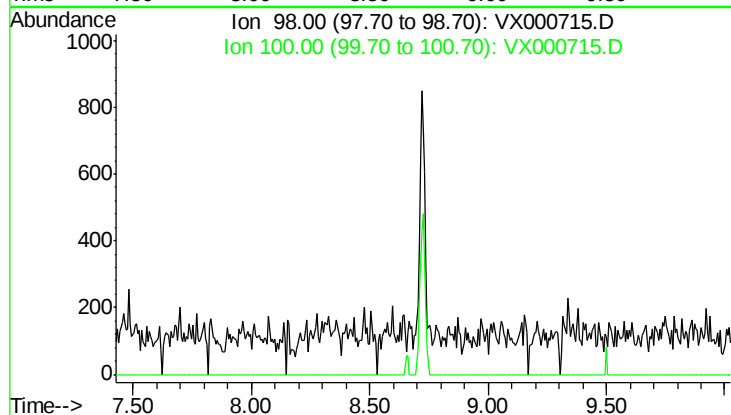


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 11.15 min

Lab File: VX000715.D
Acq: 07 Apr 2018 13:58

Tgt Ion: 95
Sig Exp Ratio
95 100
174 95.8
176 93.5


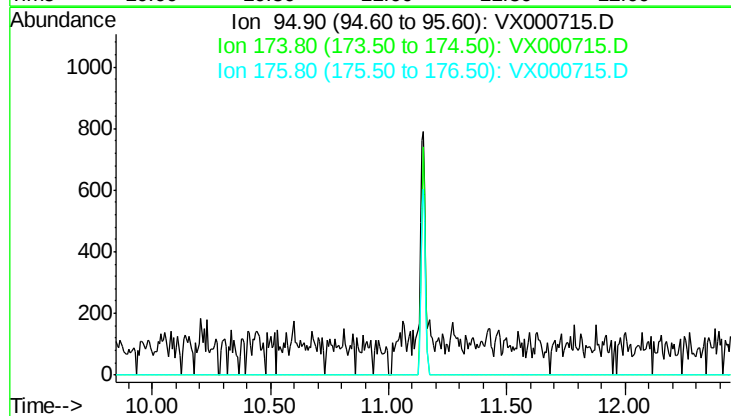


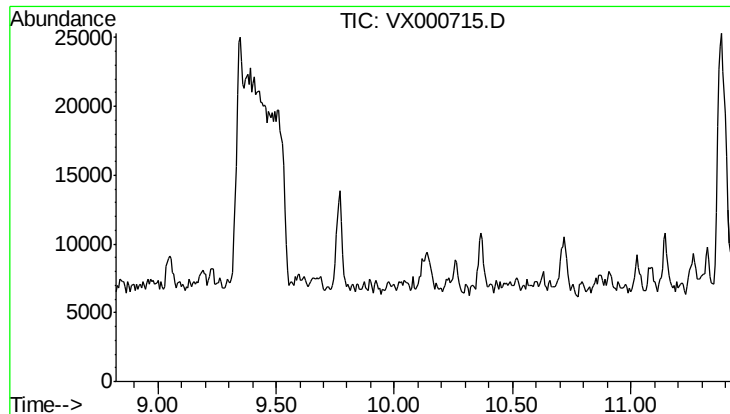

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 10.12 min
 Lab File: VX000715.D
 Acq: 07 Apr 2018 13:58

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK01

Tgt Ion: 117
 Sig Exp Ratio
 117 100
 82 52.4
 119 32.3

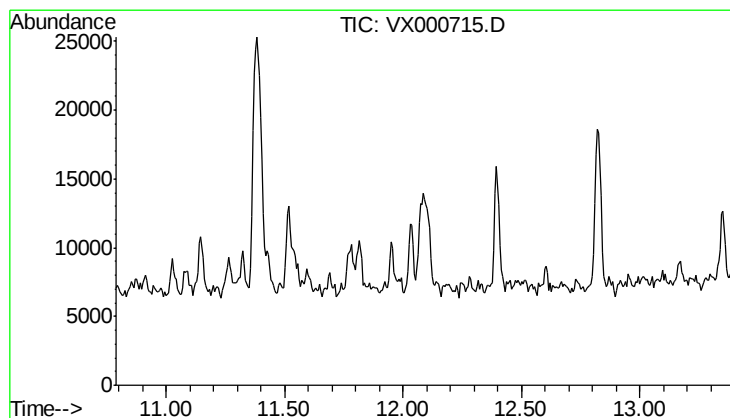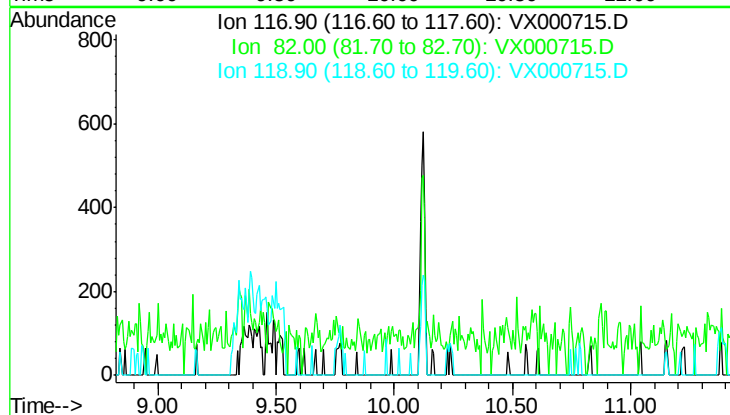

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 12.09 min
 Lab File: VX000715.D
 Acq: 07 Apr 2018 13:58

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 75.4
 150 172.5

