


Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX040718\
Data File : VX000708.D
Acq On : 07 Apr 2018 10:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X040718W.M
Title : SW846 8260
Last Update : Sat Apr 07 17:01:21 2018

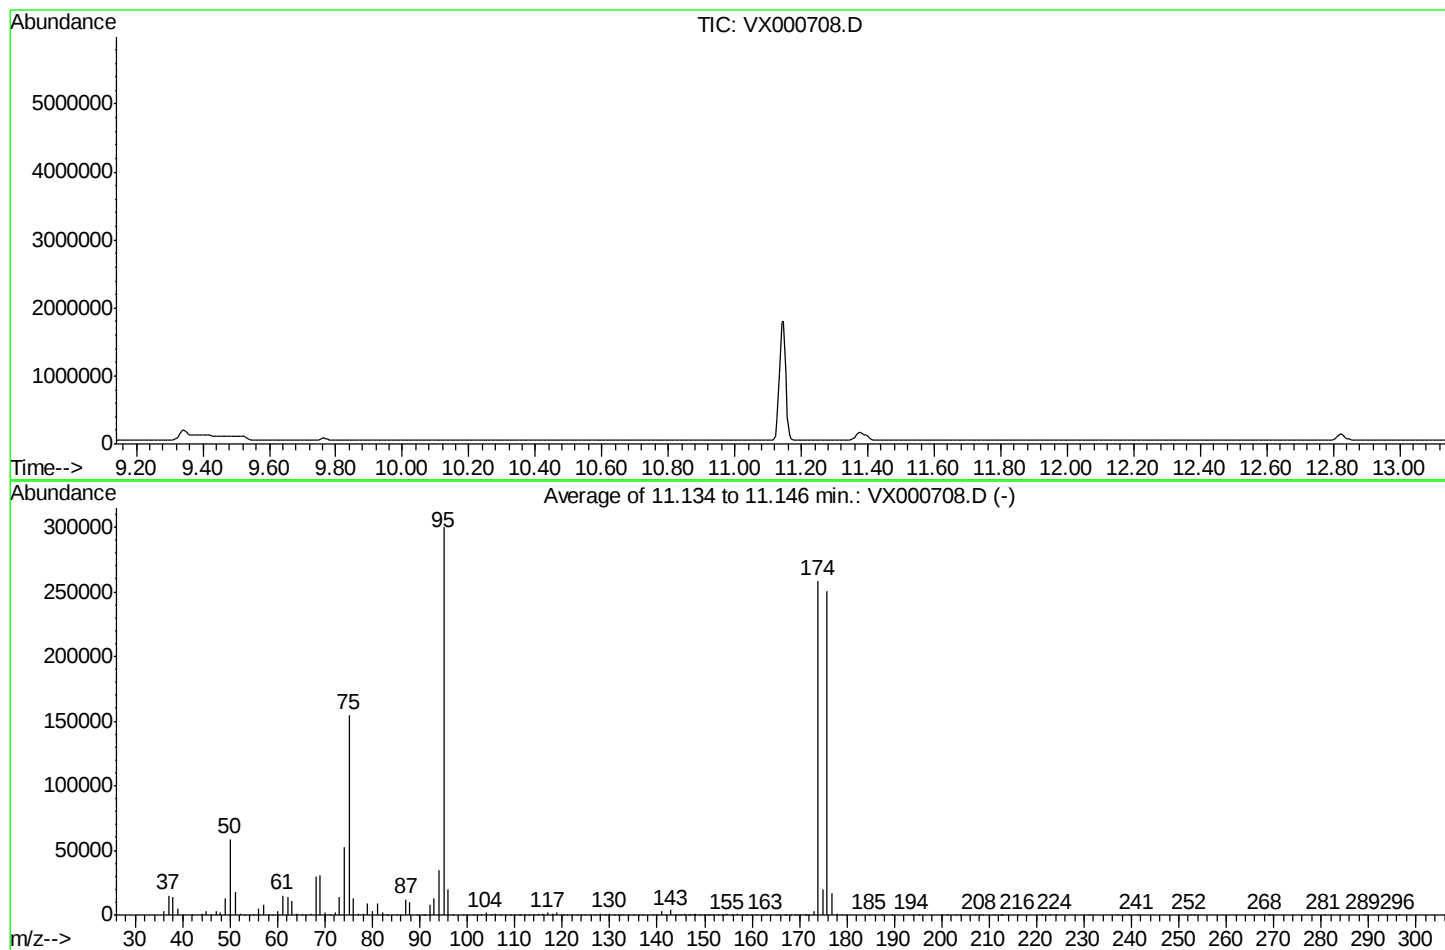

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	58644	PASS
75	95	30	60	51.6	154821	PASS
95	95	100	100	100.0	299875	PASS
96	95	5	9	6.7	20144	PASS
173	174	0.00	2	1.0	2625	PASS
174	95	50	100	86.2	258478	PASS
175	174	5	9	7.7	20012	PASS
176	174	95	101	96.7	250048	PASS
177	176	5	9	6.7	16820	PASS