


Data Path : W:\HPCHEM1\MSVOA X\Data\VX041118\
 Data File : VX000769.D
 Acq On : 11 Apr 2018 09:12
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Title : SW846 8260
 Last Update : Tue Apr 10 15:49:28 2018

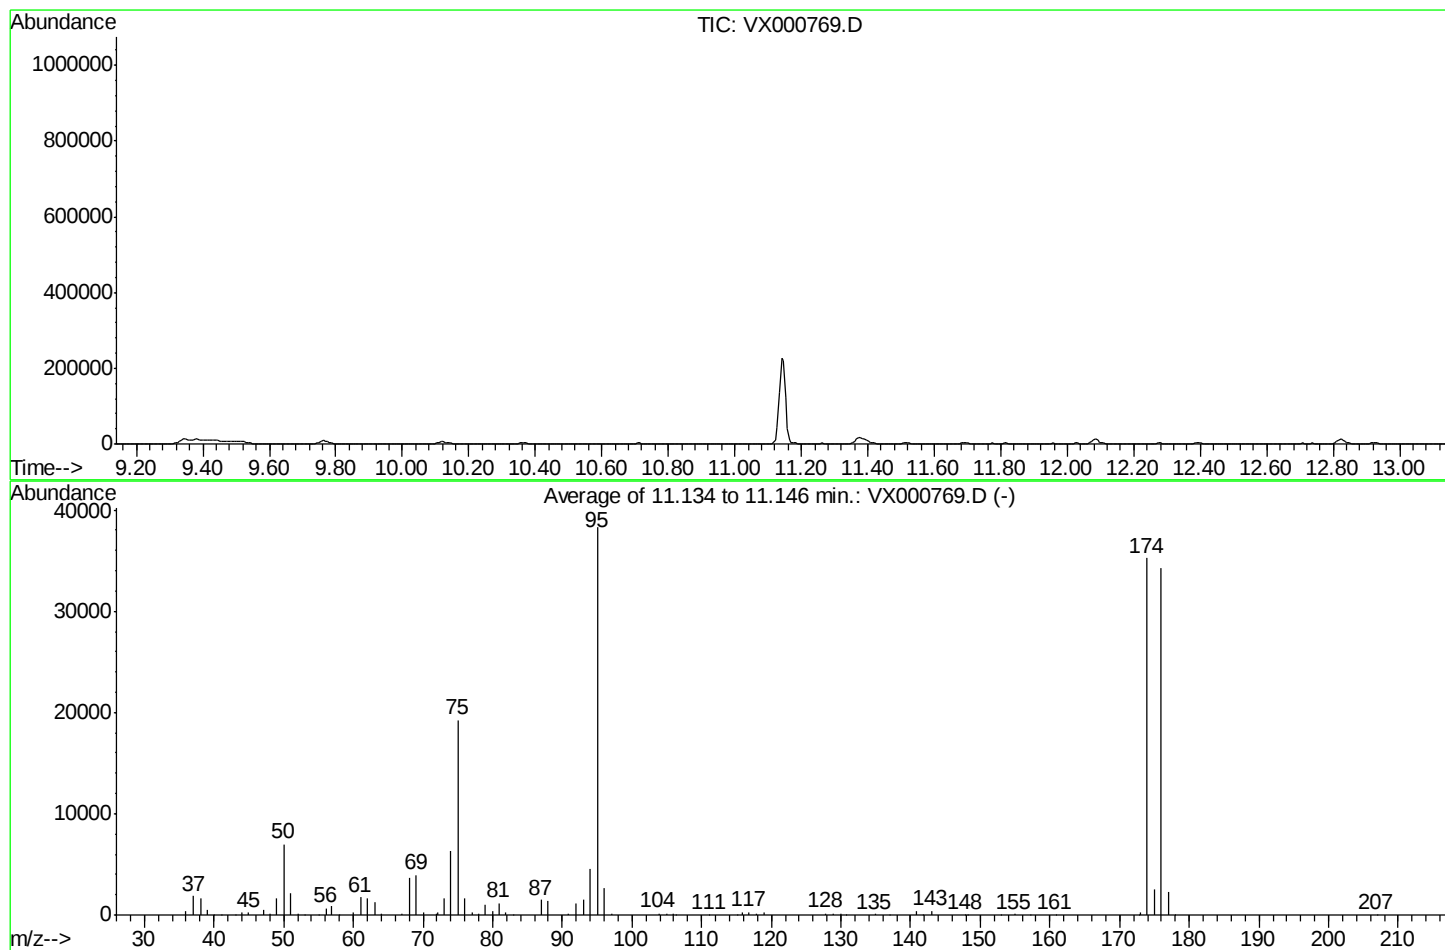

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	7011	PASS
75	95	30	60	50.2	19238	PASS
95	95	100	100	100.0	38285	PASS
96	95	5	9	6.9	2657	PASS
173	174	0.00	2	0.8	291	PASS
174	95	50	100	92.0	35221	PASS
175	174	5	9	7.3	2574	PASS
176	174	95	101	97.1	34216	PASS
177	176	5	9	6.7	2276	PASS