

Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX041218\
 Data File : VX000795.D
 Acq On : 12 Apr 2018 11:52
 Operator : JC/MD
 Sample : VX0412WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Quant Time: Apr 13 07:08:20 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	286454	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	370643	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	323745	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	193910	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	160997	44.57	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.14%	
35) Dibromofluoromethane	5.51	113	133695	46.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.64%	
50) Toluene-d8	8.72	98	500958	47.12	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.24%	
62) 4-Bromofluorobenzene	11.15	95	183425	41.70	ug/l	0.00
Spiked Amount 50.000			Recovery	=	83.40%	
Target Compounds						
36) 1,1-Dichloropropene	5.67	75	17218	4.22	ug/l	Qvalue # 49

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX041218\
Data File : VX000795.D
Acq On : 12 Apr 2018 11:52
Operator : JC/MD
Sample : VX0412WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Quant Time: Apr 13 07:08:20 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 10 15:49:28 2018
Response via : Initial Calibration

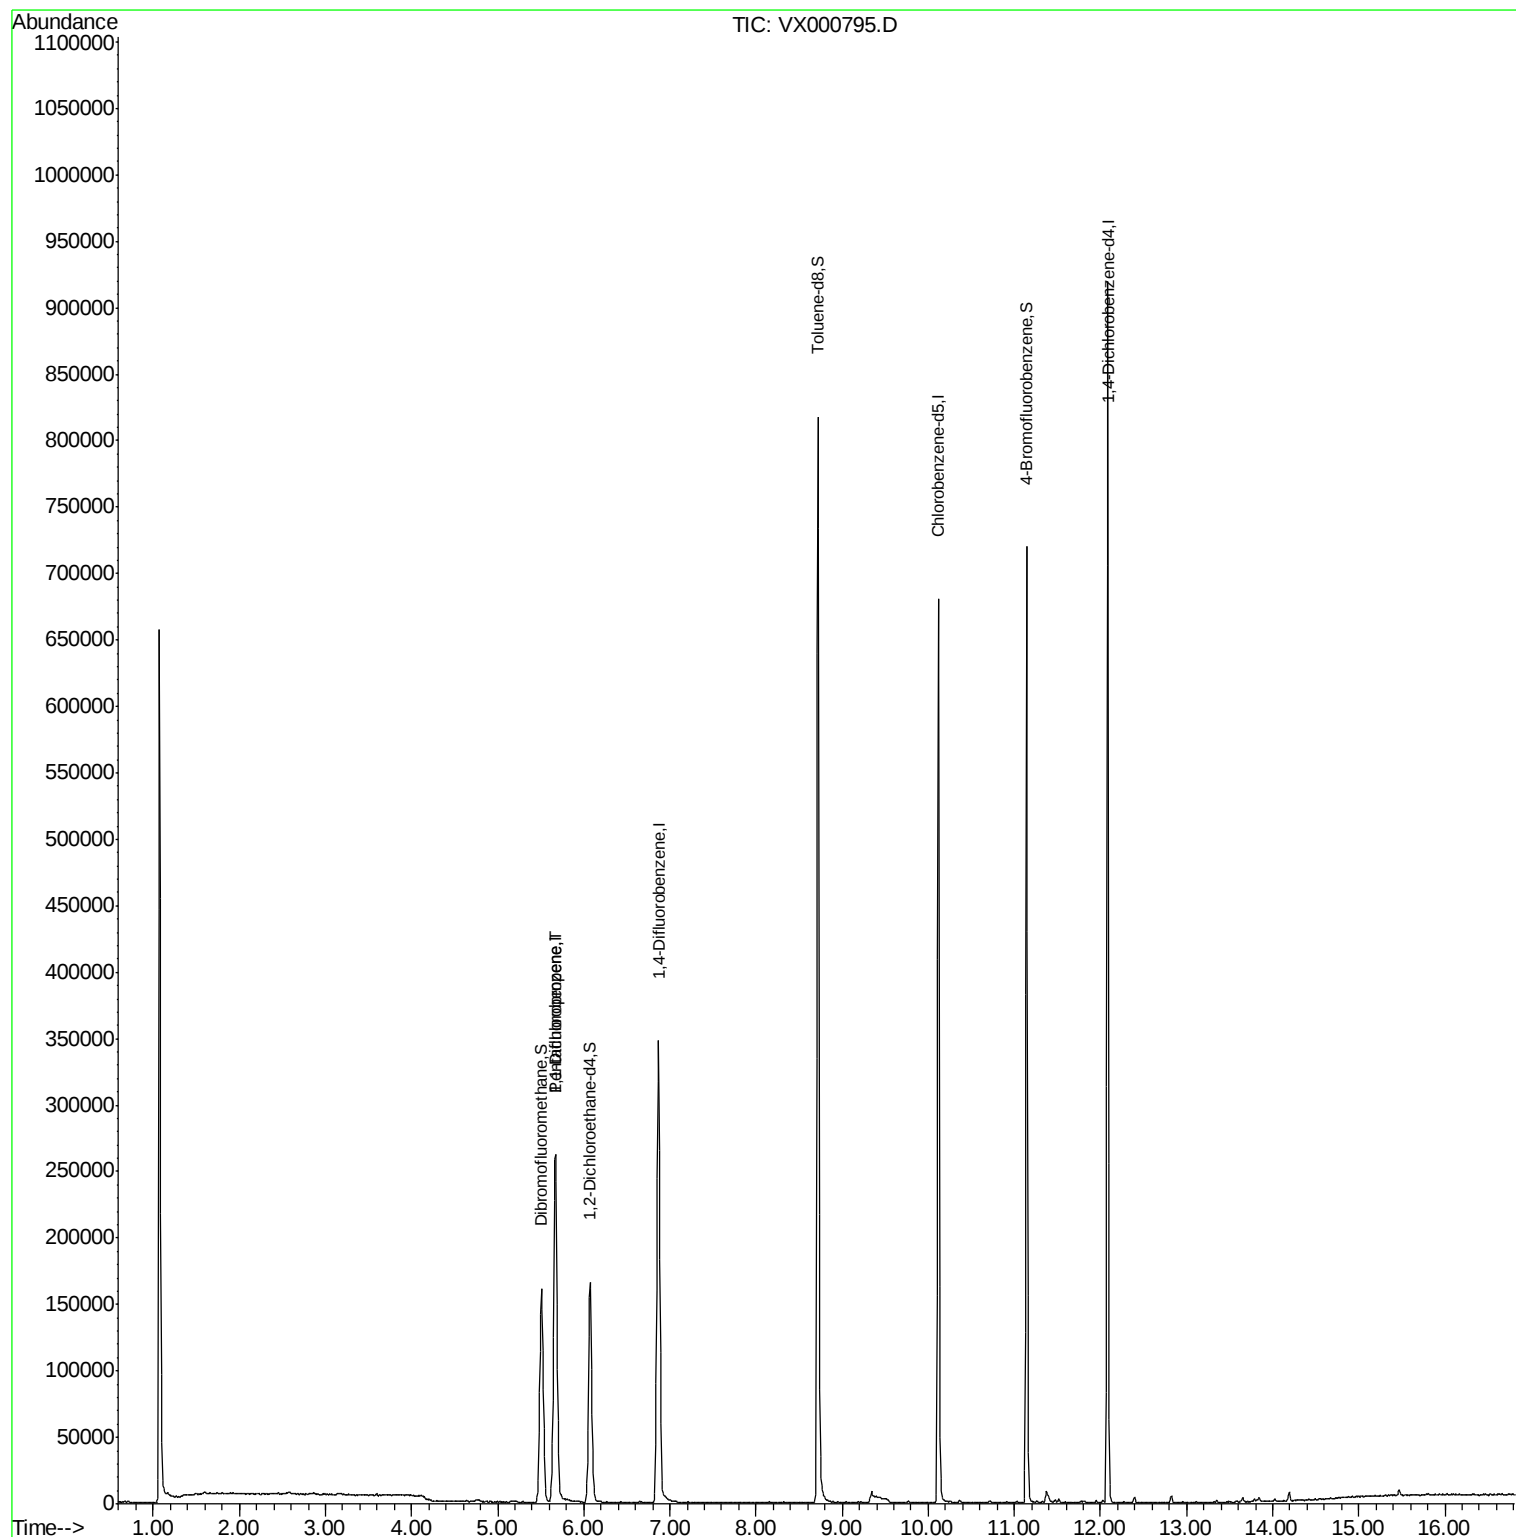



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX000795.D

Acq: 12 Apr 2018 11:52

Instrument :

MSVOA_X

ClientSampleId :


BFB

Tgt Ion:168 Resp: 286454

Ion Ratio Lower Upper




168 100

99 48.2 38.3 57.5

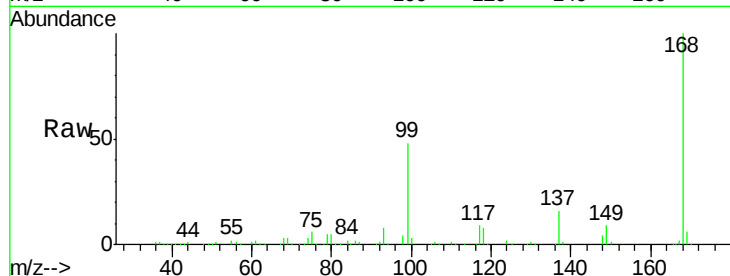

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

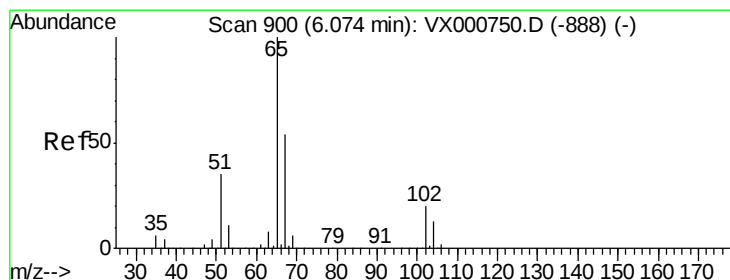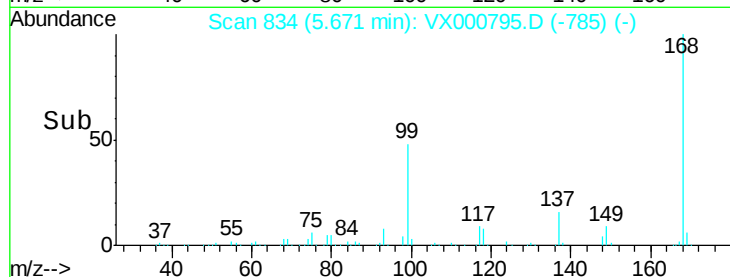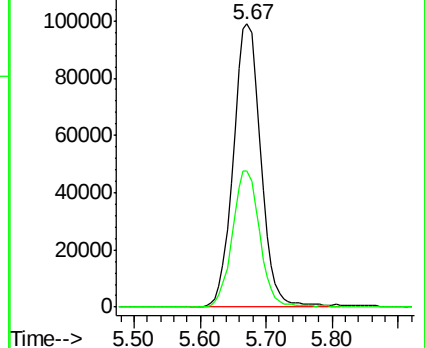

#33

1,2-Dichloroethane-d4

Concen: 44.57 ug/l

RT: 6.07 min Scan# 900

Delta R.T. -0.00 min

Lab File: VX000795.D


Acq: 12 Apr 2018 11:52

Tgt Ion: 65 Resp: 160997

Ion Ratio Lower Upper



65 100


67 52.1 0.0 103.8

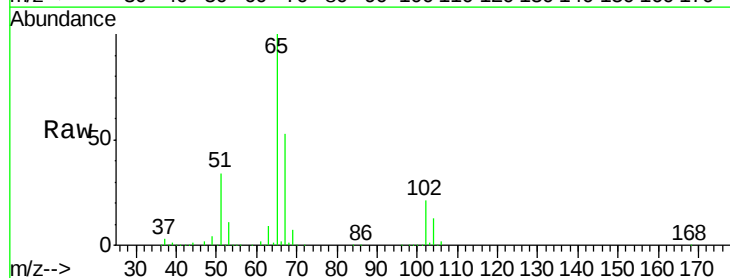

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

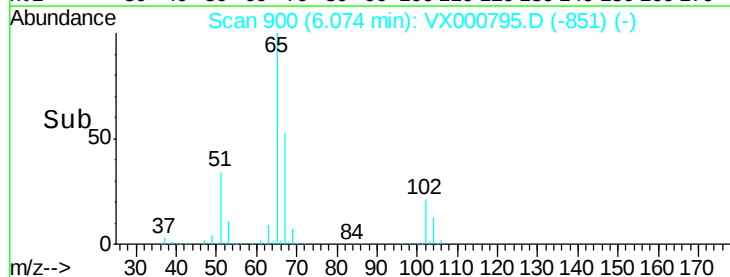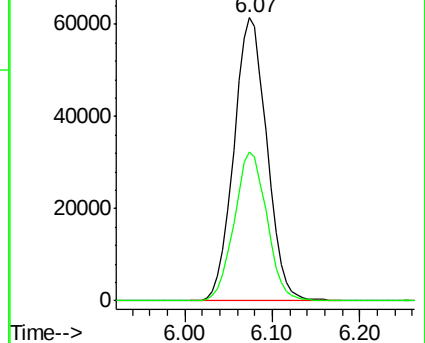

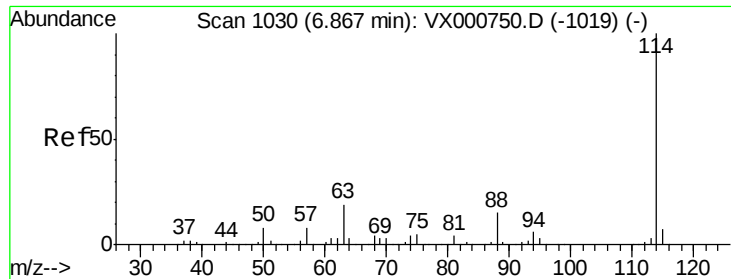

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1030

Delta R.T. -0.00 min

Lab File: VX000795.D


Acq: 12 Apr 2018 11:52

Instrument :

MSVOA_X

ClientSampleId :

BFB

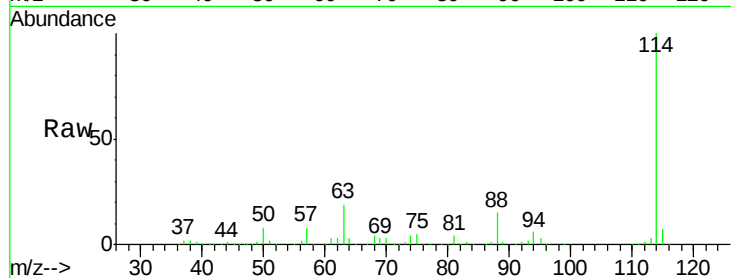

Tgt Ion:114 Resp: 370643

Ion Ratio Lower Upper

114 100

63 19.3 0.0 38.4

88 15.4 0.0 31.0

