

Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX041218\
 Data File : VX000820.D
 Acq On : 12 Apr 2018 23:46
 Operator : JC/MD
 Sample : J2162-04 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EO-01-041118-B

Quant Time: Apr 13 06:59:56 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	273263	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	355747	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	317830	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	209730	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	155283	45.07	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.14%	
35) Dibromofluoromethane	5.51	113	127724	46.60	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.20%	
50) Toluene-d8	8.73	98	488092	47.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.66%	
62) 4-Bromofluorobenzene	11.15	95	188016	44.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.06%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.65	94	349	Below Cal	#	54
6) Chloroethane	1.64	64	1496	0.83	ug/l	69
10) Methyl Iodide	2.52	142	466	8.42	ug/l	88
11) Tert butyl alcohol	3.08	59	290	0.47	ug/l	72
13) Acrolein	2.30	56	281	0.95	ug/l	94
15) Acrylonitrile	3.15	53	846	0.65	ug/l	80
16) Acetone	2.45	43	4488	3.78	ug/l	96
17) Carbon Disulfide	2.57	76	2069	0.27	ug/l	94
20) Methylene Chloride	2.86	84	81717	29.57	ug/l	98
21) trans-1,2-Dichloroethene	3.18	96	650	0.24	ug/l	87
25) 2-Butanone	4.72	43	1502	0.77	ug/l	94
29) Tetrahydrofuran	5.18	42	857	0.69	ug/l	47
38) Carbon Tetrachloride	5.68	117	22992	5.24	ug/l	15
43) Isopropyl Acetate	6.48	43	2240	0.34	ug/l	89
64) Tetrachloroethene	9.34	164	808	0.26	ug/l	79
68) m/p-Xylenes	10.37	106	1583	0.30	ug/l	89
74) N-amyl acetate	6.48	43	2240	0.37	ug/l	91
76) 1,2,3-Trichloropropane	11.15	75	91299	25.24	ug/l	36
81) trans-1,4-Dichloro-2-buten	11.15	75	91299	69.43	ug/l	11
84) 1,2,4-Trimethylbenzene	11.81	105	2907	0.25	ug/l	100
89) n-Butylbenzene	12.40	91	2531	0.22	ug/l	97
93) 1,2,4-Trichlorobenzene	13.65	180	1734	0.29	ug/l	98
94) Hexachlorobutadiene	13.79	225	750	0.26	ug/l	99
95) Naphthalene	13.84	128	35670	2.34	ug/l	99
96) 1,2,3-Trichlorobenzene	14.02	180	1218	0.21	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA_X\DATA\VX041218\
Data File : VX000820.D
Acq On : 12 Apr 2018 23:46
Operator : JC/MD
Sample : J2162-04 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EO-01-041118-B

Quant Time: Apr 13 06:59:56 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 10 15:49:28 2018
Response via : Initial Calibration

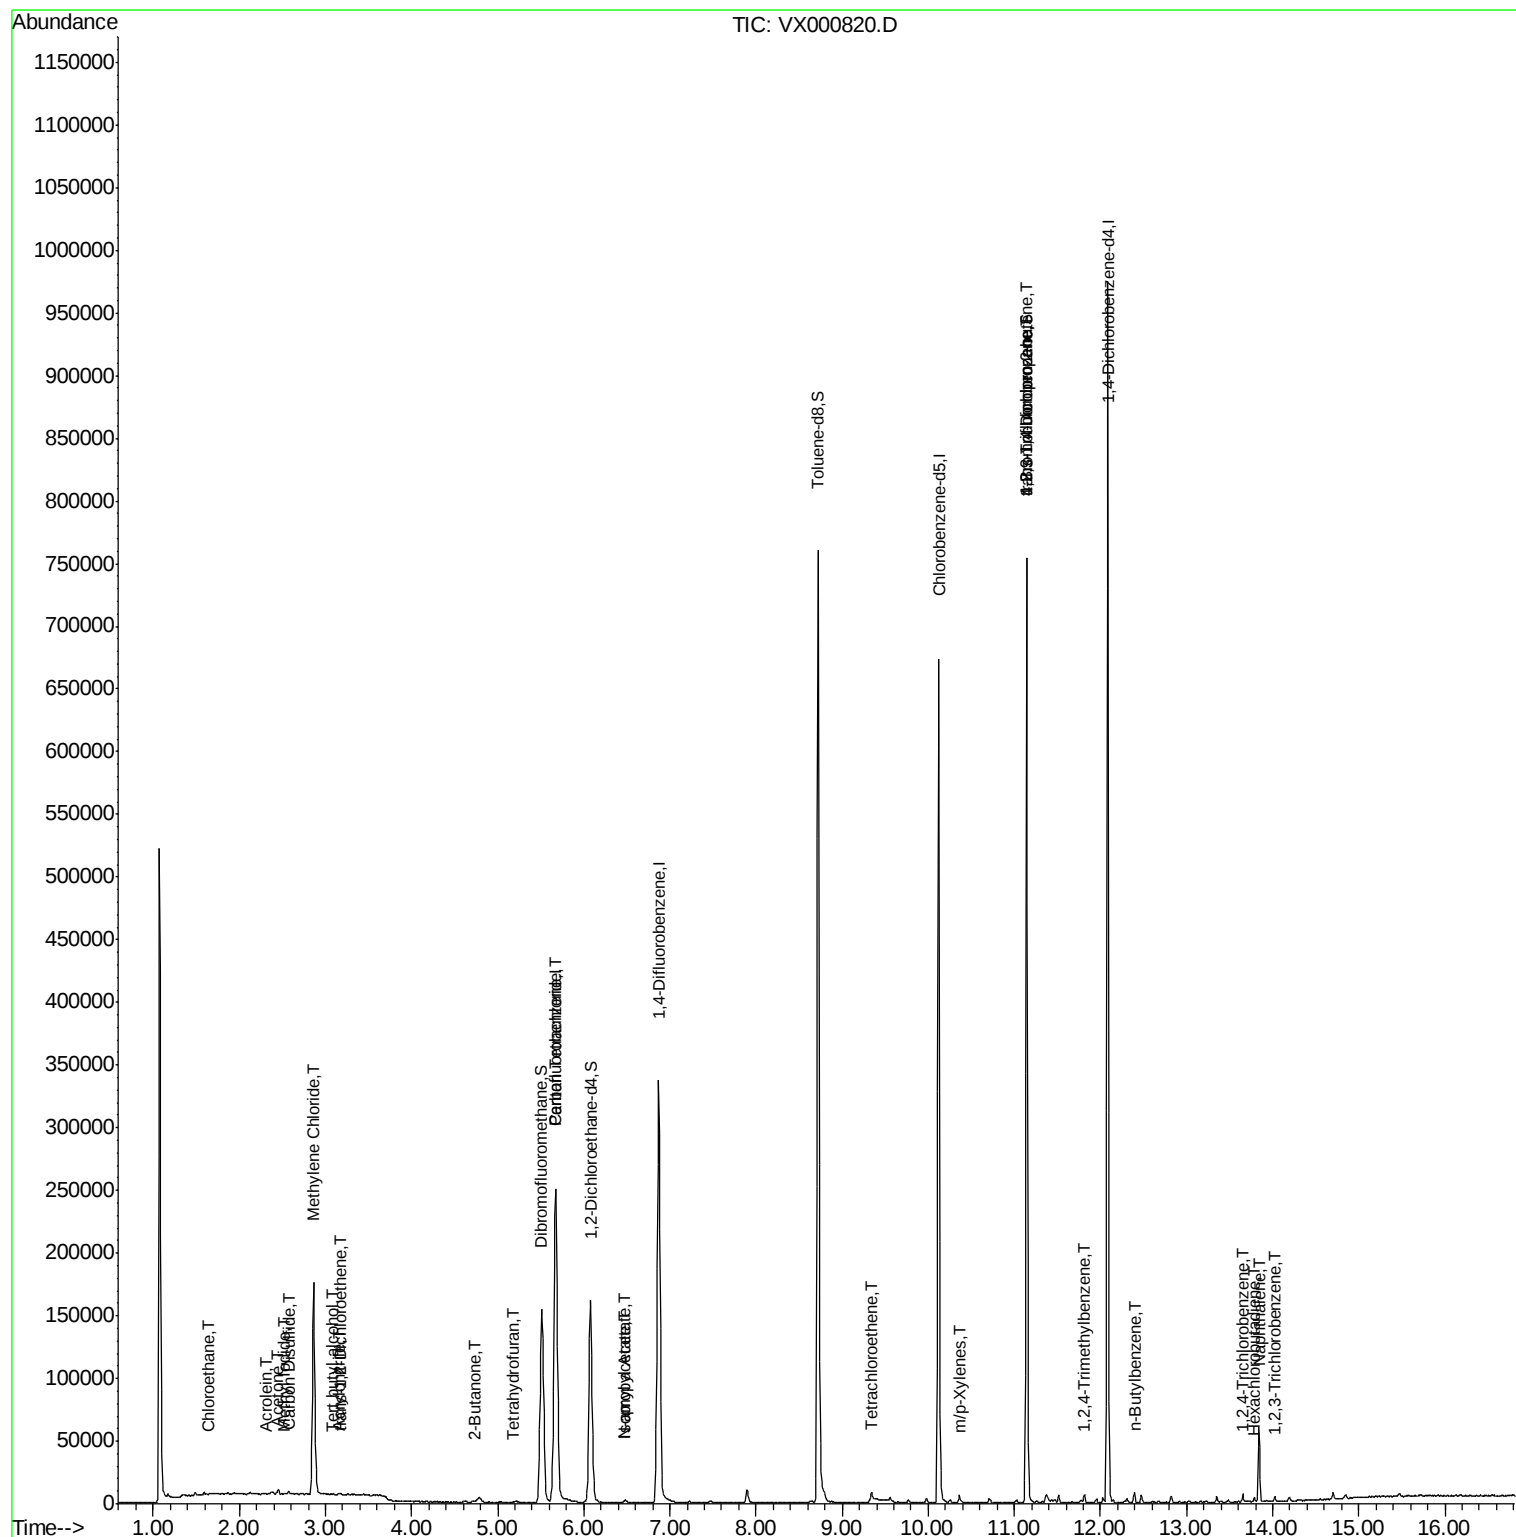



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 834

Delta R.T. -0.00 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :


EO-01-041118-B

Tgt Ion:168 Resp: 273263

Ion Ratio Lower Upper




168 100

99 47.7 38.3 57.5



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

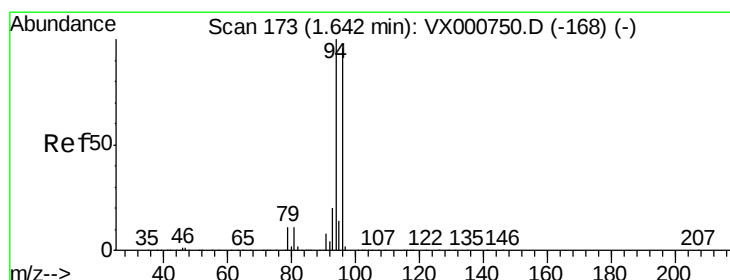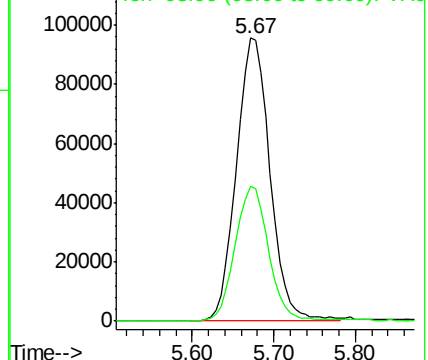

#5

Bromomethane

Concen: Below Cal

RT: 1.65 min Scan# 175

Delta R.T. 0.01 min

Lab File: VX000820.D


Acq: 12 Apr 2018 23:46

Tgt Ion: 94 Resp: 349

Ion Ratio Lower Upper



94 100


96 51.7 77.0 115.6#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

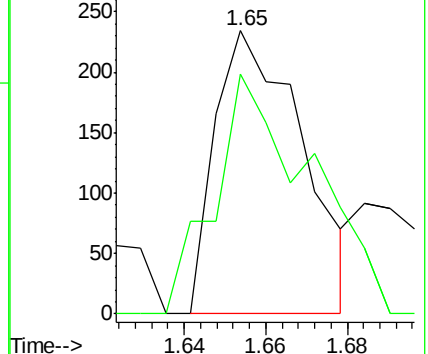



#6

Chloroethane

Concen: 0.83 ug/l

RT: 1.64 min Scan# 173

Delta R.T. -0.09 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :





EO-01-041118-B

Tgt Ion: 64 Resp: 1496

Ion Ratio Lower Upper

64 100

66 14.3 25.3 37.9#

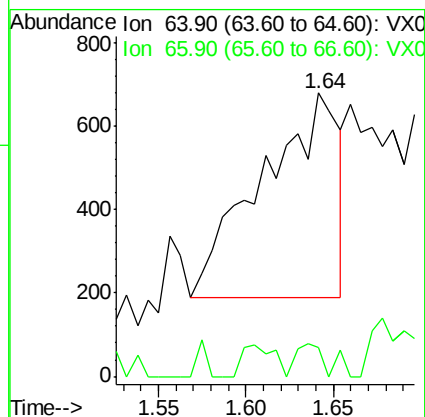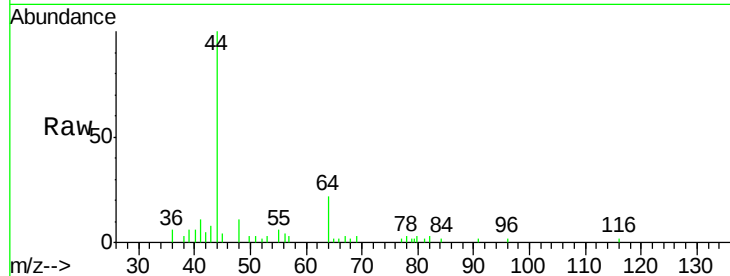

#10

Methyl Iodide

Concen: 8.42 ug/l

RT: 2.52 min Scan# 317

Delta R.T. 0.01 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46




Tgt Ion: 142 Resp: 466


Ion Ratio Lower Upper

142 100

127 38.2 32.6 49.0

141 0.0 11.5 17.3#

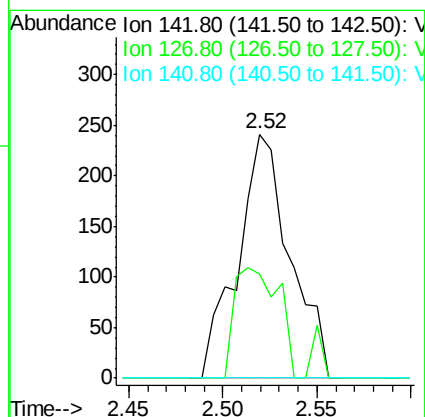



#11

Tert butyl alcohol

Concen: 0.47 ug/l

RT: 3.08 min Scan# 409

Delta R.T. 0.01 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :


EO-01-041118-B

Tgt Ion: 59 Resp: 290

Ion Ratio Lower Upper




59 100

57 0.0 8.4 12.6#



Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

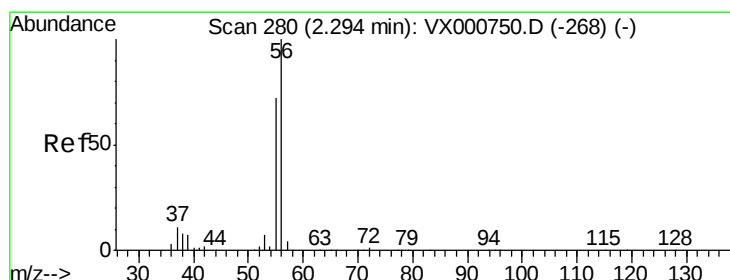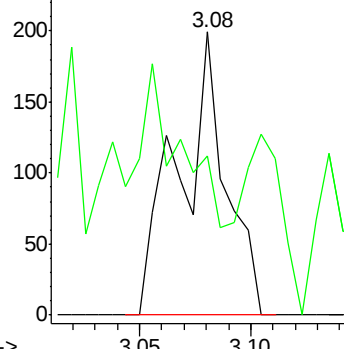

#13

Acrolein

Concen: 0.95 ug/l

RT: 2.30 min Scan# 281

Delta R.T. 0.01 min

Lab File: VX000820.D


Acq: 12 Apr 2018 23:46

Tgt Ion: 56 Resp: 281

Ion Ratio Lower Upper



56 100


55 68.0 58.7 88.1



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

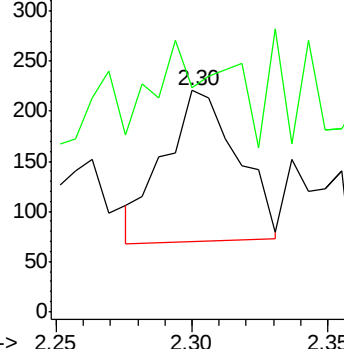



#15

Acrylonitrile

Concen: 0.65 ug/l

RT: 3.15 min Scan# 421

Delta R.T. -0.00 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampled :

EO-01-041118-B


Tgt Ion: 53 Resp: 846

Ion Ratio Lower Upper

53 100

52 81.4 66.5 99.7




51 0.0 28.8 43.2#

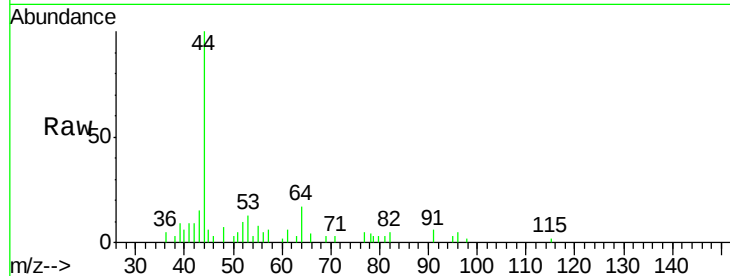

Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

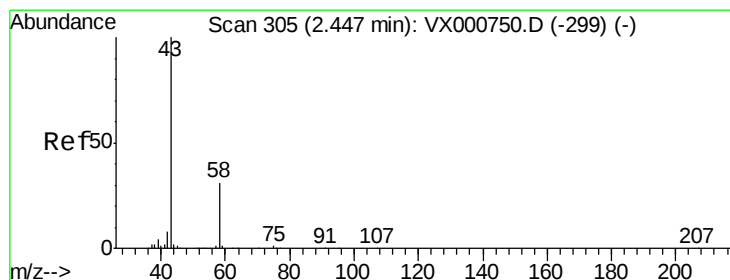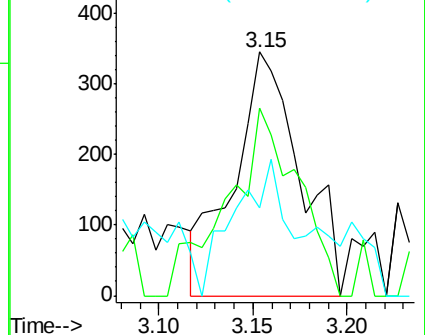

#16

Acetone

Concen: 3.78 ug/l

RT: 2.45 min Scan# 306

Delta R.T. 0.01 min

Lab File: VX000820.D


Acq: 12 Apr 2018 23:46

Tgt Ion: 43 Resp: 4488

Ion Ratio Lower Upper



43 100


58 28.5 24.6 37.0



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




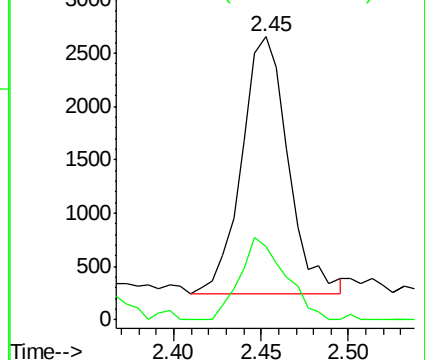




#17
Carbon Disulfide
Concen: 0.27 ug/l
RT: 2.57 min Scan# 326
Delta R.T. -0.00 min
Lab File: VX000820.D
Acq: 12 Apr 2018 23:46




Instrument :
MSVOA_X
ClientSampleId :
EO-01-041118-B


Tgt Ion: 76 Resp: 2069
Ion Ratio Lower Upper
76 100
78 7.2 7.4 11.2#

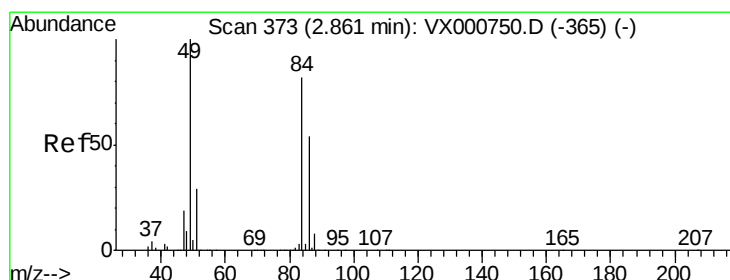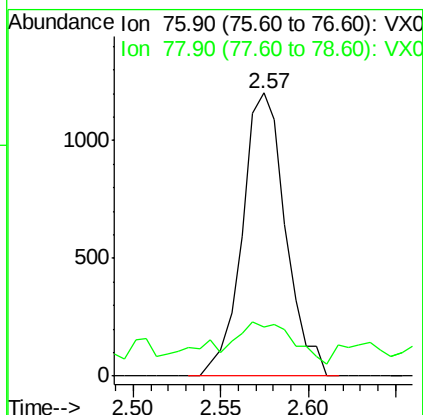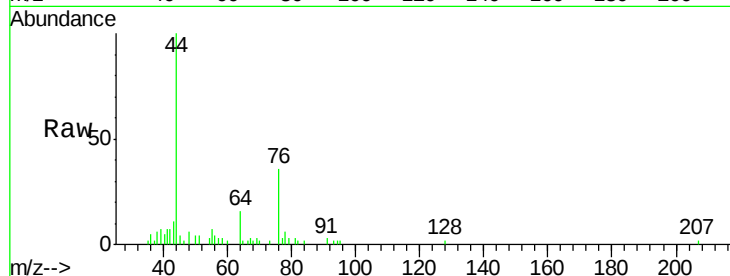

#20
Methylene Chloride
Concen: 29.57 ug/l
RT: 2.86 min Scan# 373
Delta R.T. -0.00 min
Lab File: VX000820.D
Acq: 12 Apr 2018 23:46

Tgt Ion: 84 Resp: 81717
Ion Ratio Lower Upper
84 100
49 119.6 98.1 147.1
51 37.3 28.9 43.3
86 64.8 52.7 79.1

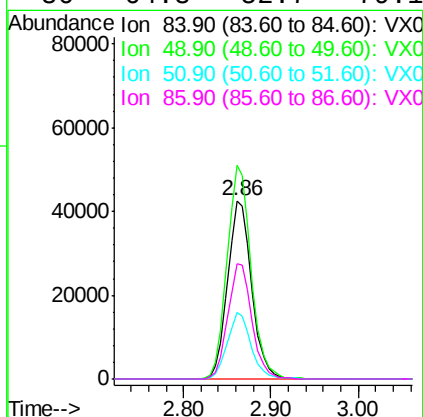

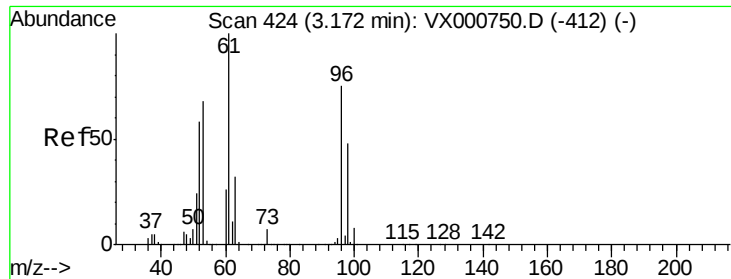

#21

trans-1,2-Dichloroethene

Concen: 0.24 ug/l

RT: 3.18 min Scan# 425

Delta R.T. 0.01 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :

EO-01-041118-B


Tgt Ion: 96 Resp: 650

Ion Ratio Lower Upper

96 100

61 114.6 106.2 159.2




98 70.7 51.2 76.8

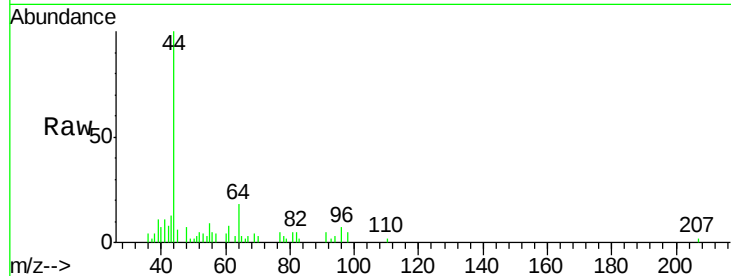

Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

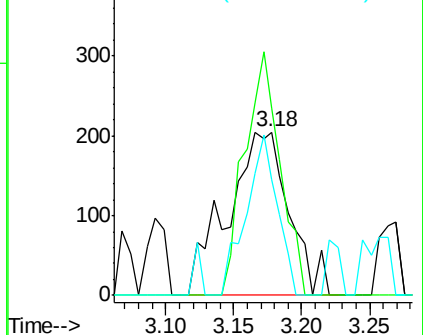

#25

2-Butanone

Concen: 0.77 ug/l

RT: 4.72 min Scan# 678

Delta R.T. 0.01 min

Lab File: VX000820.D


Acq: 12 Apr 2018 23:46

Tgt Ion: 43 Resp: 1502

Ion Ratio Lower Upper



43 100


72 22.2 20.3 30.5



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

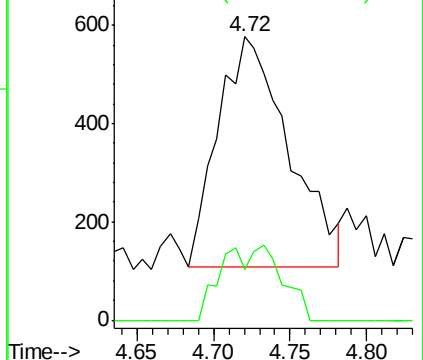



#29

Tetrahydrofuran

Concen: 0.69 ug/l

RT: 5.18 min Scan# 754

Delta R.T. 0.01 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :

EO-01-041118-B


Tgt Ion: 42 Resp: 857

Ion Ratio Lower Upper

42 100

72 3.6 35.1 52.7#




71 14.7 32.8 49.2#

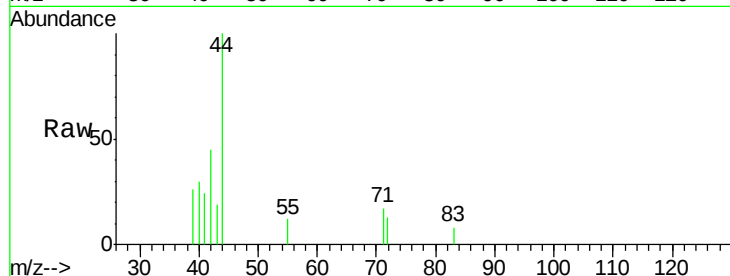

Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

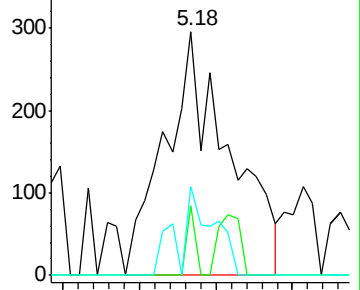

#33

1,2-Dichloroethane-d4

Concen: 45.07 ug/l

RT: 6.08 min Scan# 901

Delta R.T. 0.01 min

Lab File: VX000820.D


Acq: 12 Apr 2018 23:46

Tgt Ion: 65 Resp: 155283

Ion Ratio Lower Upper



65 100


67 51.4 0.0 103.8



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0




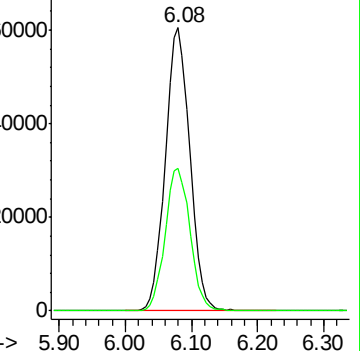


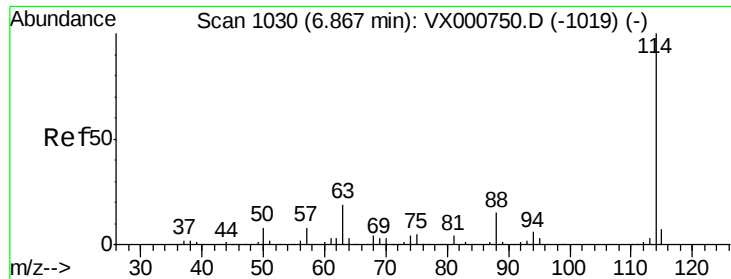

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1031
 Delta R.T. 0.01 min
 Lab File: VX000820.D
 Acq: 12 Apr 2018 23:46




Instrument :
 MSVOA_X
 ClientSampleId :
 EO-01-041118-B


Tgt Ion:114 Resp: 355747
 Ion Ratio Lower Upper
 114 100
 63 19.2 0.0 38.4
 88 15.5 0.0 31.0

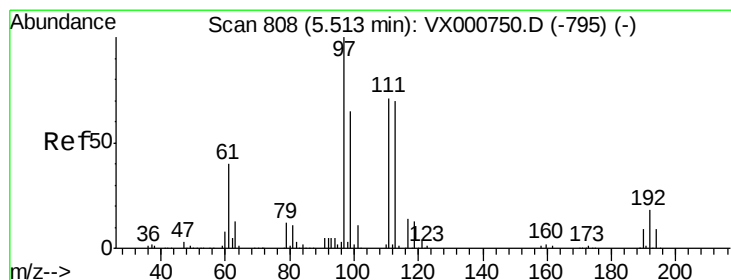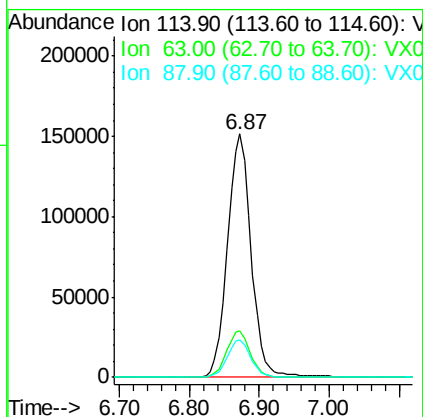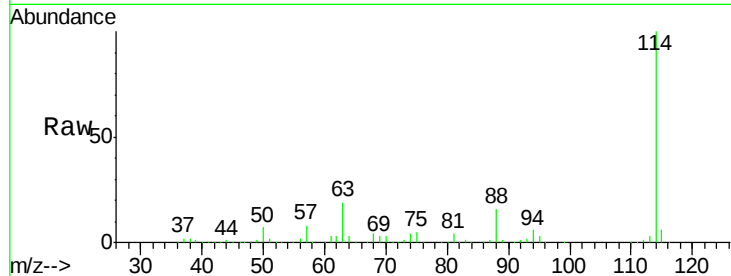

#35
 Dibromofluoromethane
 Concen: 46.60 ug/l
 RT: 5.51 min Scan# 808
 Delta R.T. -0.00 min
 Lab File: VX000820.D
 Acq: 12 Apr 2018 23:46

Tgt Ion:113 Resp: 127724
 Ion Ratio Lower Upper
 113 100
 111 101.5 81.5 122.3
 192 25.8 20.4 30.6

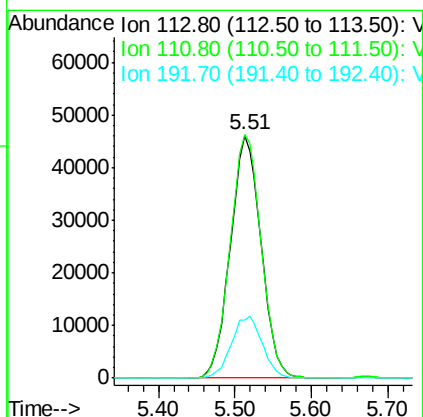







#38
Carbon Tetrachloride
Concen: 5.24 ug/l
RT: 5.68 min Scan# 835
Delta R.T. -0.12 min
Lab File: VX000820.D
Acq: 12 Apr 2018 23:46

Instrument :
MSVOA_X
ClientSampleId :
EO-01-041118-B

Tgt Ion:117 Resp: 22992
Ion Ratio Lower Upper
117 100
119 5.3 78.4 117.6#
121 0.0 25.4 38.0#

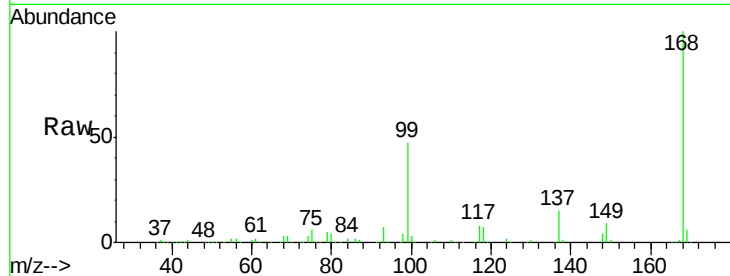


Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V


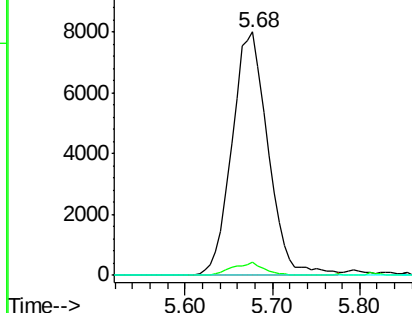



#43
Isopropyl Acetate
Concen: 0.34 ug/l
RT: 6.48 min Scan# 966
Delta R.T. -0.00 min
Lab File: VX000820.D
Acq: 12 Apr 2018 23:46

Tgt Ion: 43 Resp: 2240
Ion Ratio Lower Upper
43 100
61 23.7 15.6 23.4#
87 8.2 10.7 16.1#



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0

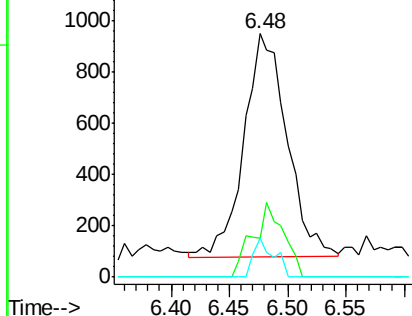

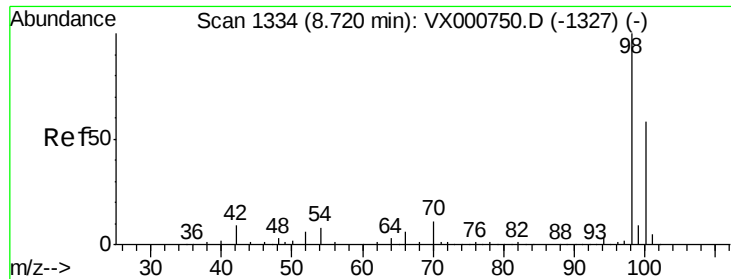

#50

Toluene-d8

Concen: 47.83 ug/l

RT: 8.73 min Scan# 1335

Delta R.T. 0.01 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :


EO-01-041118-B

Tgt Ion: 98 Resp: 488092

Ion Ratio Lower Upper




98 100

100 64.2 52.6 79.0

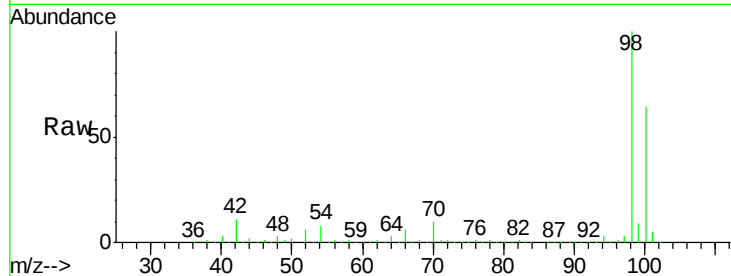

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

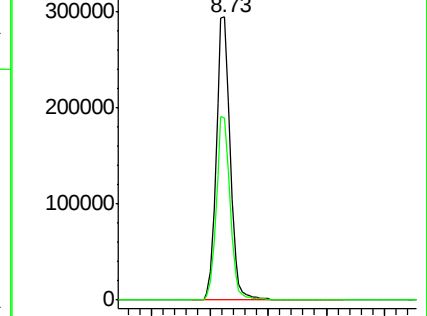

#62

4-Bromofluorobenzene

Concen: 44.53 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. -0.00 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46


Tgt Ion: 95 Resp: 188016

Ion Ratio Lower Upper

95 100

174 97.9 0.0 198.4



176 95.7 0.0 194.4




Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



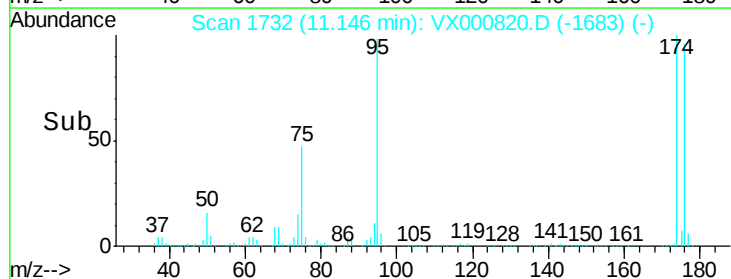
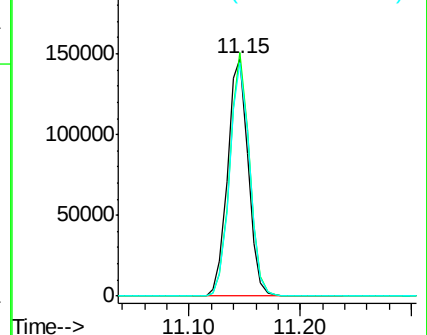


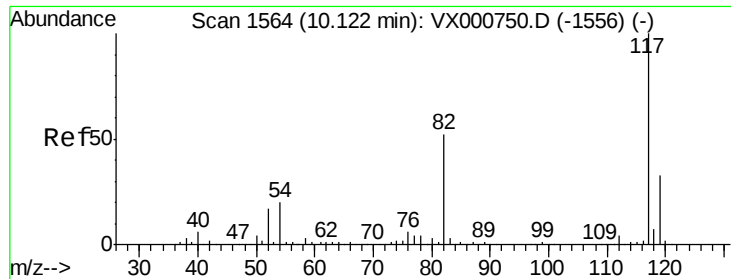

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. -0.00 min
Lab File: VX000820.D
Acq: 12 Apr 2018 23:46




Instrument :
MSVOA_X
ClientSampleId :
EO-01-041118-B


Tgt Ion:117 Resp: 317830
Ion Ratio Lower Upper
117 100
82 52.9 41.9 62.9
119 33.1 26.0 39.0

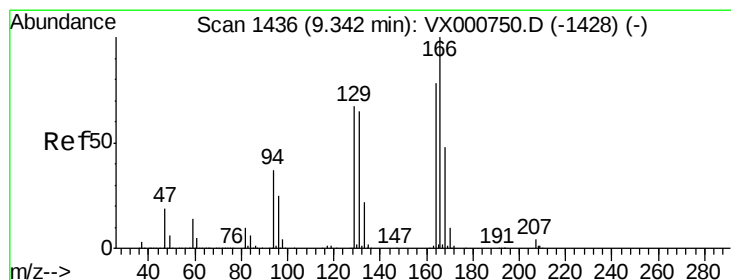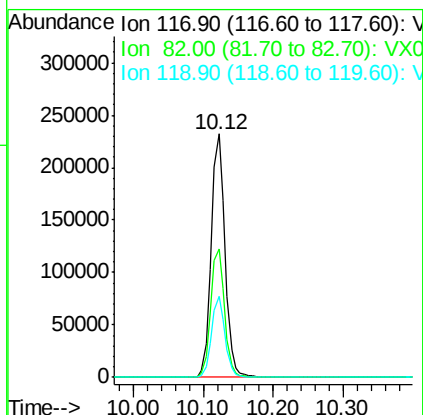

#64
Tetrachloroethene
Concen: 0.26 ug/l
RT: 9.34 min Scan# 1435
Delta R.T. -0.01 min
Lab File: VX000820.D
Acq: 12 Apr 2018 23:46

Tgt Ion:164 Resp: 808
Ion Ratio Lower Upper
164 100
166 99.6 102.8 154.2#
129 69.5 68.5 102.7
131 68.0 66.6 100.0

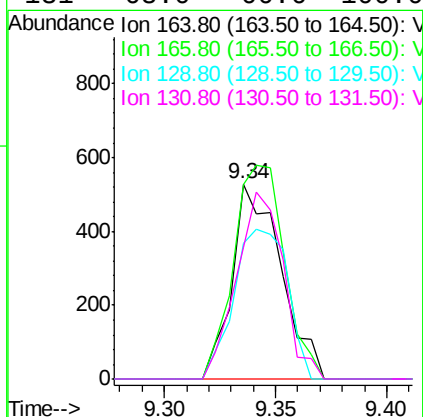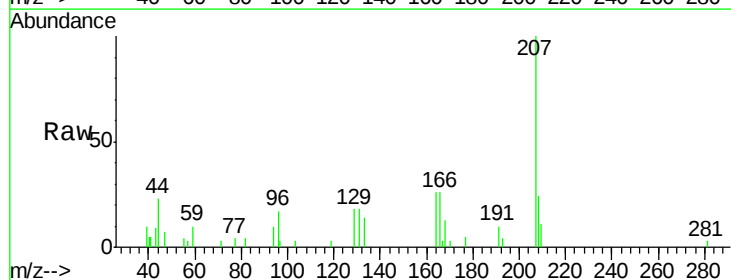


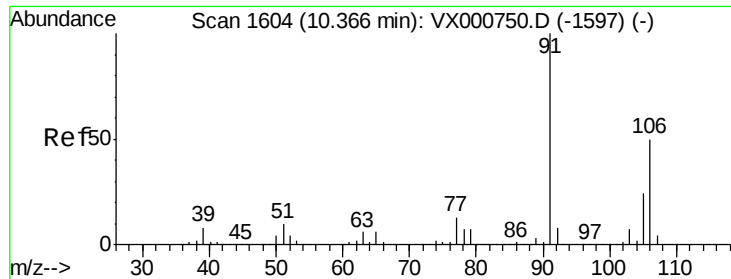




#68
m/p-Xylenes
Concen: 0.30 ug/l
RT: 10.37 min Scan# 1604
Delta R.T. -0.00 min
Lab File: VX000820.D
Acq: 12 Apr 2018 23:46

Instrument :
MSVOA_X
ClientSampleId :
EO-01-041118-B

Tgt Ion:106 Resp: 1583
Ion Ratio Lower Upper
106 100
91 215.5 159.3 238.9

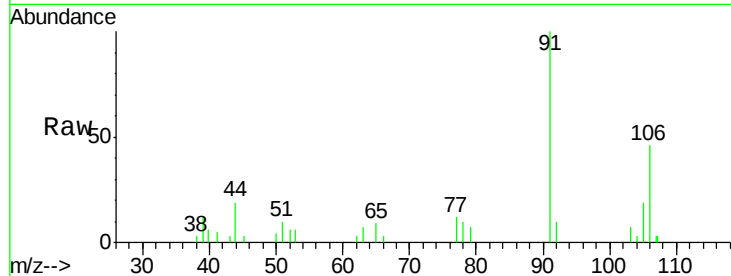


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0


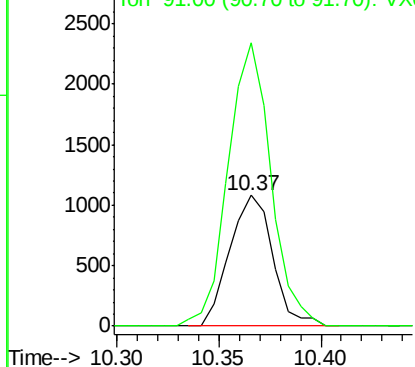



#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX000820.D
Acq: 12 Apr 2018 23:46

Tgt Ion:152 Resp: 209730
Ion Ratio Lower Upper
152 100
115 52.9 37.9 113.7
150 155.2 0.0 348.0



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

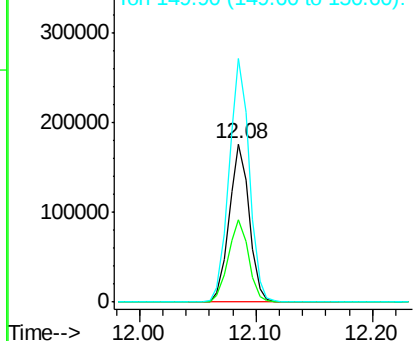



#74

N-amyI acetate

Concen: 0.37 ug/l

RT: 6.48 min Scan# 966

Delta R.T. -0.00 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :

EO-01-041118-B

Tgt Ion: 43 Resp: 2240


Ion Ratio Lower Upper

43 100

70 1.1 0.0 0.0#

55 0.0 0.0 0.0

61 23.7 15.6 23.4#



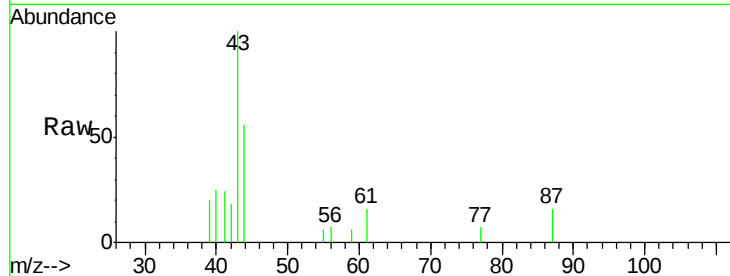


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

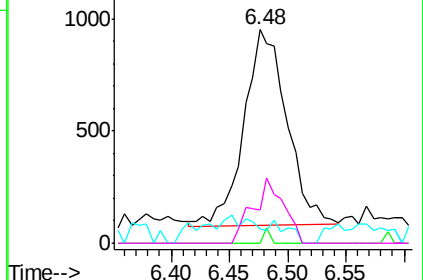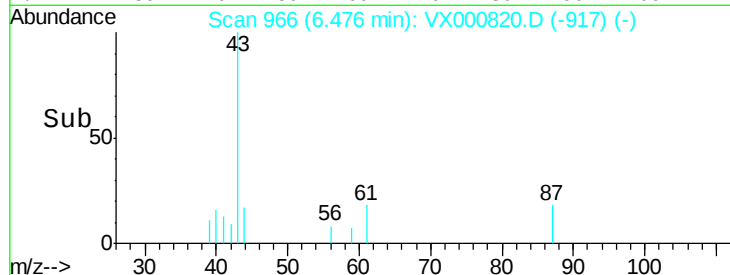

#76

1,2,3-Trichloropropane

Concen: 25.24 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. -0.16 min

Lab File: VX000820.D


Acq: 12 Apr 2018 23:46

Tgt Ion: 75 Resp: 91299

Ion Ratio Lower Upper



75 100


77 1.1 20.5 61.5#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

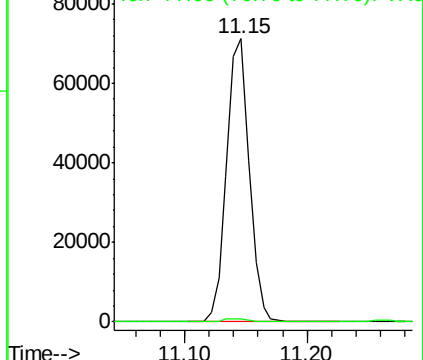



#81

trans-1,4-Dichloro-2-butene

Concen: 69.43 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. 0.07 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :

EO-01-041118-B


Tgt Ion: 75 Resp: 91299

Ion Ratio Lower Upper

75 100

53 0.0 75.4 113.0#




89 0.0 40.9 61.3#

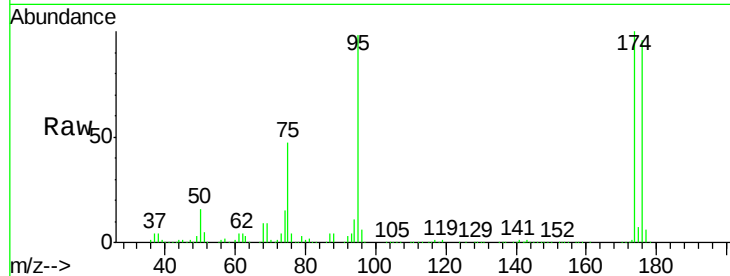

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

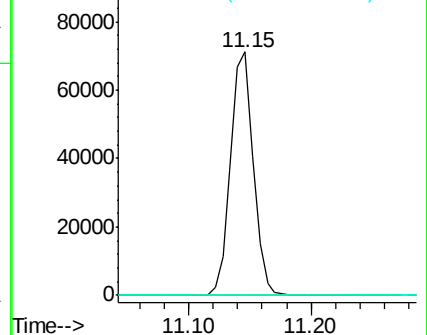

#84

1,2,4-Trimethylbenzene

Concen: 0.25 ug/l

RT: 11.81 min Scan# 1841

Delta R.T. -0.00 min

Lab File: VX000820.D


Acq: 12 Apr 2018 23:46

Tgt Ion: 105 Resp: 2907

Ion Ratio Lower Upper



105 100


120 46.4 23.1 69.3



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

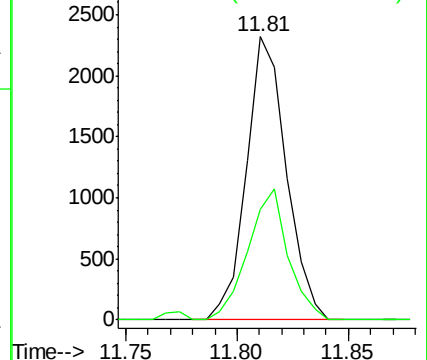

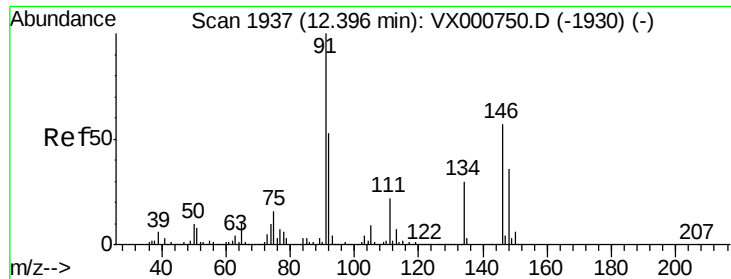

#89

n-Butylbenzene

Concen: 0.22 ug/l

RT: 12.40 min Scan# 1937

Delta R.T. -0.00 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :

EO-01-041118-B





Tgt Ion: 91 Resp: 2531

Ion Ratio Lower Upper

91 100

92 50.3 26.5 79.5

134 29.8 14.5 43.5

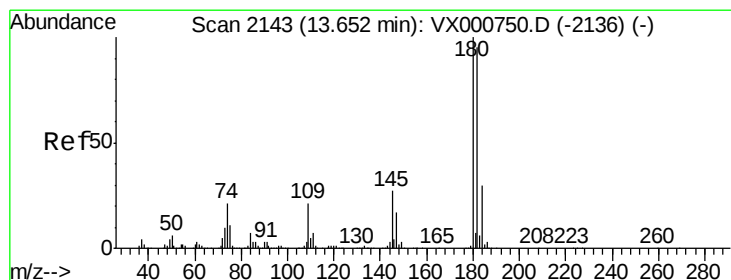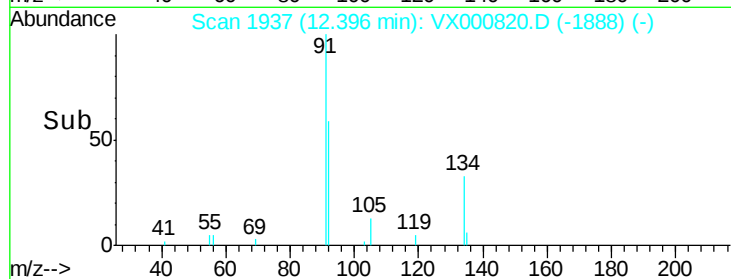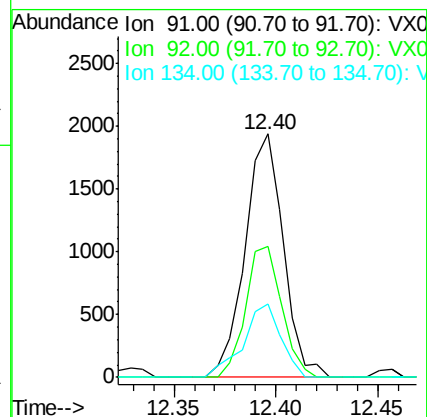

#93

1,2,4-Trichlorobenzene

Concen: 0.29 ug/l

RT: 13.65 min Scan# 2143

Delta R.T. -0.00 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46




Tgt Ion: 180 Resp: 1734


Ion Ratio Lower Upper

180 100

182 96.6 47.5 142.5

145 28.8 13.8 41.4

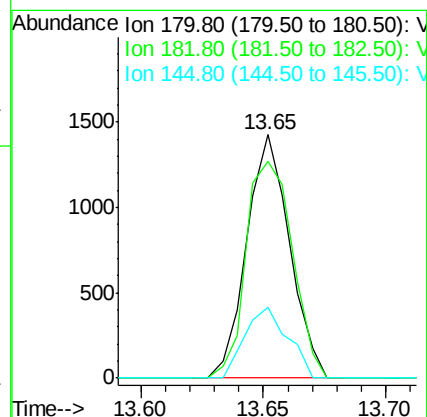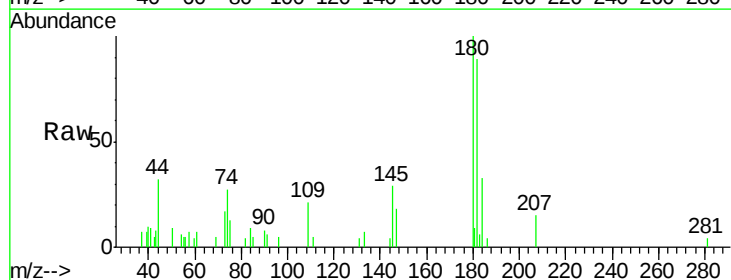



#94

Hexachlorobutadiene

Concen: 0.26 ug/l

RT: 13.79 min Scan# 2166

Delta R.T. 0.01 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46

Instrument :

MSVOA_X

ClientSampleId :

EO-01-041118-B


Tgt Ion:225 Resp: 750

Ion Ratio Lower Upper




225 100

223 63.3 31.2 93.6

227 64.7 32.3 96.9



Abundance Ion 224.70 (224.40 to 225.40): V
Ion 222.70 (222.40 to 223.40): V
Ion 226.70 (226.40 to 227.40): V

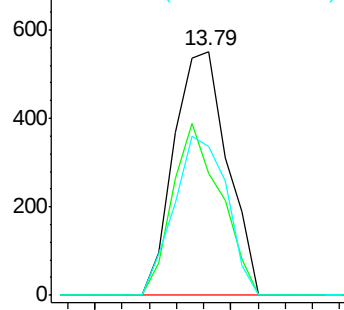

#95

Naphthalene

Concen: 2.34 ug/l

RT: 13.84 min Scan# 2174

Delta R.T. -0.00 min

Lab File: VX000820.D

Acq: 12 Apr 2018 23:46


Tgt Ion:128 Resp: 35670

Ion Ratio Lower Upper



128 100


127 13.5 10.4 15.6

129 11.1 8.7 13.1



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

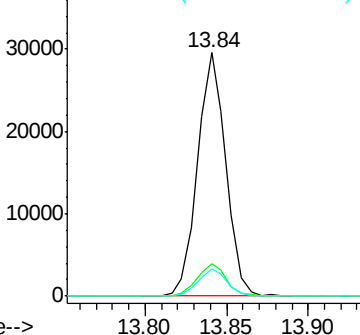


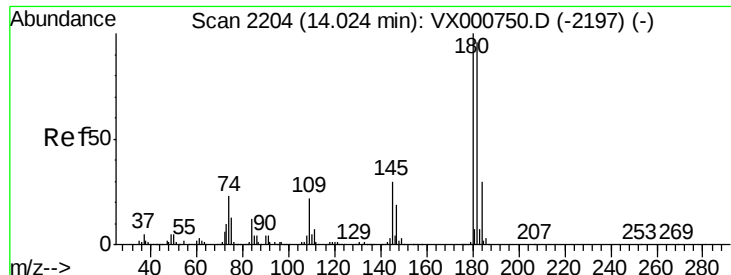

#96
 1,2,3-Trichlorobenzene
 Concen: 0.21 ug/l
 RT: 14.02 min Scan# 2204
 Delta R.T. -0.00 min
 Lab File: VX000820.D
 Acq: 12 Apr 2018 23:46

Instrument :
 MSVOA_X
 ClientSampleId :
 EO-01-041118-B

Tgt Ion	Ratio	Lower	Upper
180	100		
182	97.5	48.4	145.2
145	33.7	14.6	43.8

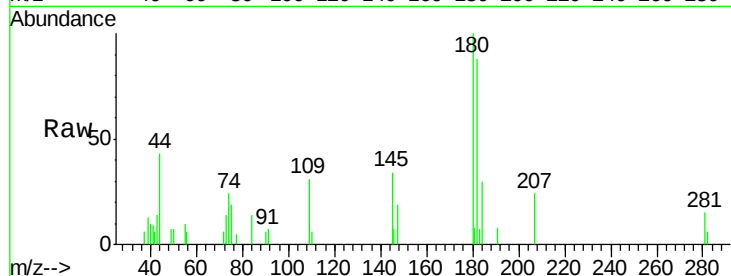

Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.90 (144.60 to 145.60): V

