


Data Path : W:\HPCHEM1\MSVOA X\Data\VX041218\
Data File : VX000815.D
Acq On : 12 Apr 2018 21:13
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Title : SW846 8260
Last Update : Tue Apr 10 15:49:28 2018

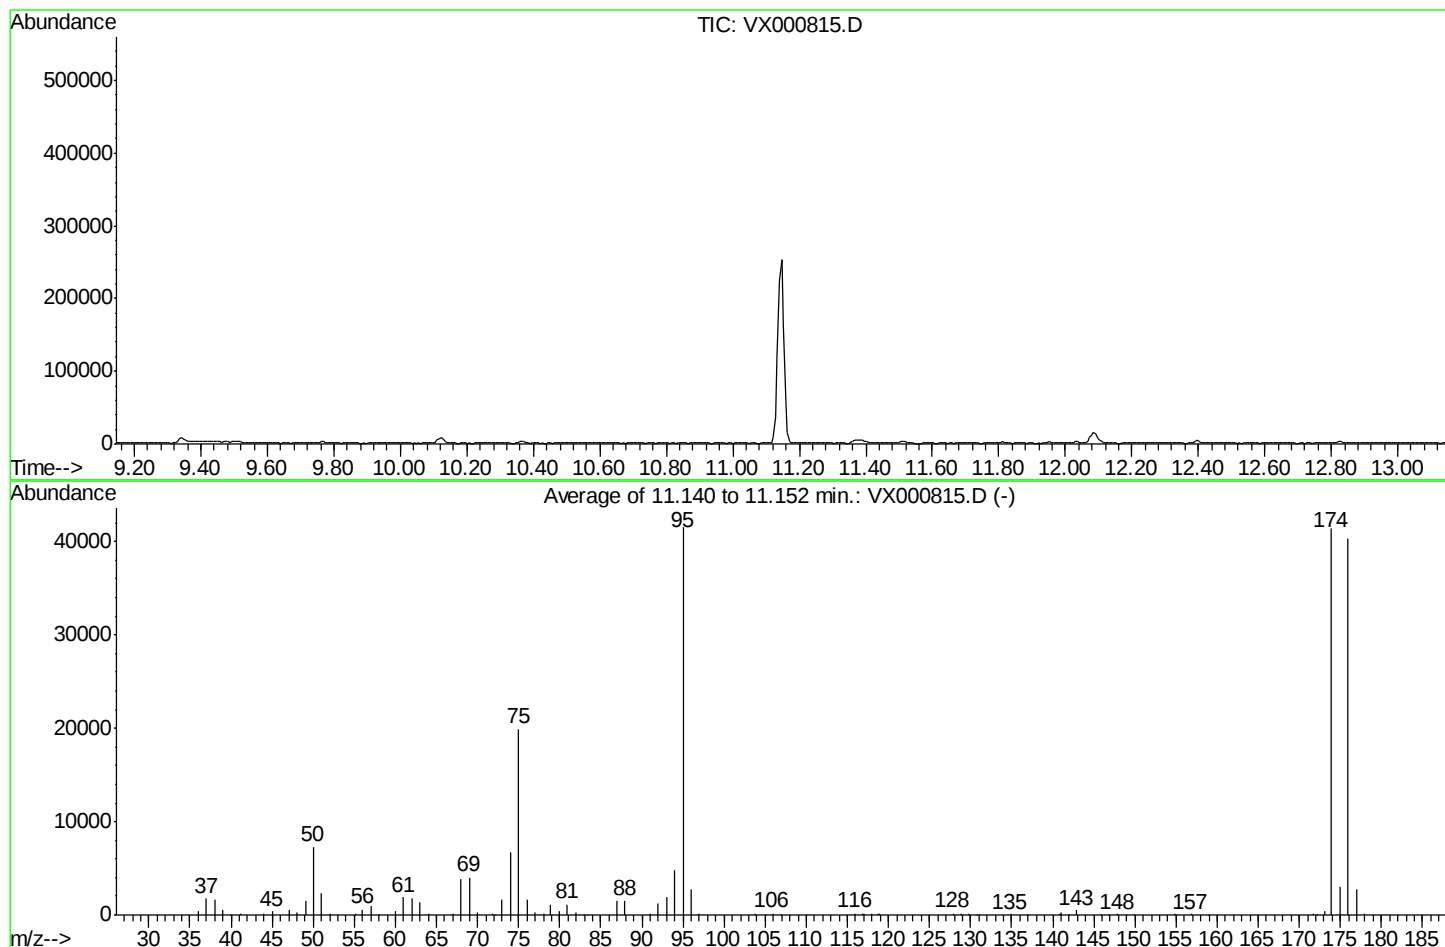

AutoFind: Scans 1731, 1732, 1733; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	7314	PASS
75	95	30	60	48.0	19916	PASS
95	95	100	100	100.0	41528	PASS
96	95	5	9	6.6	2726	PASS
173	174	0.00	2	1.1	462	PASS
174	95	50	100	99.9	41482	PASS
175	174	5	9	7.2	2980	PASS
176	174	95	101	97.1	40274	PASS
177	176	5	9	6.8	2732	PASS