

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041318\
 Data File : VX000853.D
 Acq On : 13 Apr 2018 16:51
 Operator : JC/MD
 Sample : PB108205TB 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB108205TB

Quant Time: Apr 14 05:27:11 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.68	168	252712	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	326153	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	294785	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	190956	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	141361	44.36	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.72%	
35) Dibromofluoromethane	5.51	113	115567	45.99	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.98%	
50) Toluene-d8	8.73	98	452143	48.33	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.66%	
62) 4-Bromofluorobenzene	11.15	95	170651	44.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.18%	
Target Compounds						
20) Methylene Chloride	2.87	84	7791	3.05	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041318\
Data File : VX000853.D
Acq On : 13 Apr 2018 16:51
Operator : JC/MD
Sample : PB108205TB 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB108205TB

Quant Time: Apr 14 05:27:11 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 10 15:49:28 2018
Response via : Initial Calibration

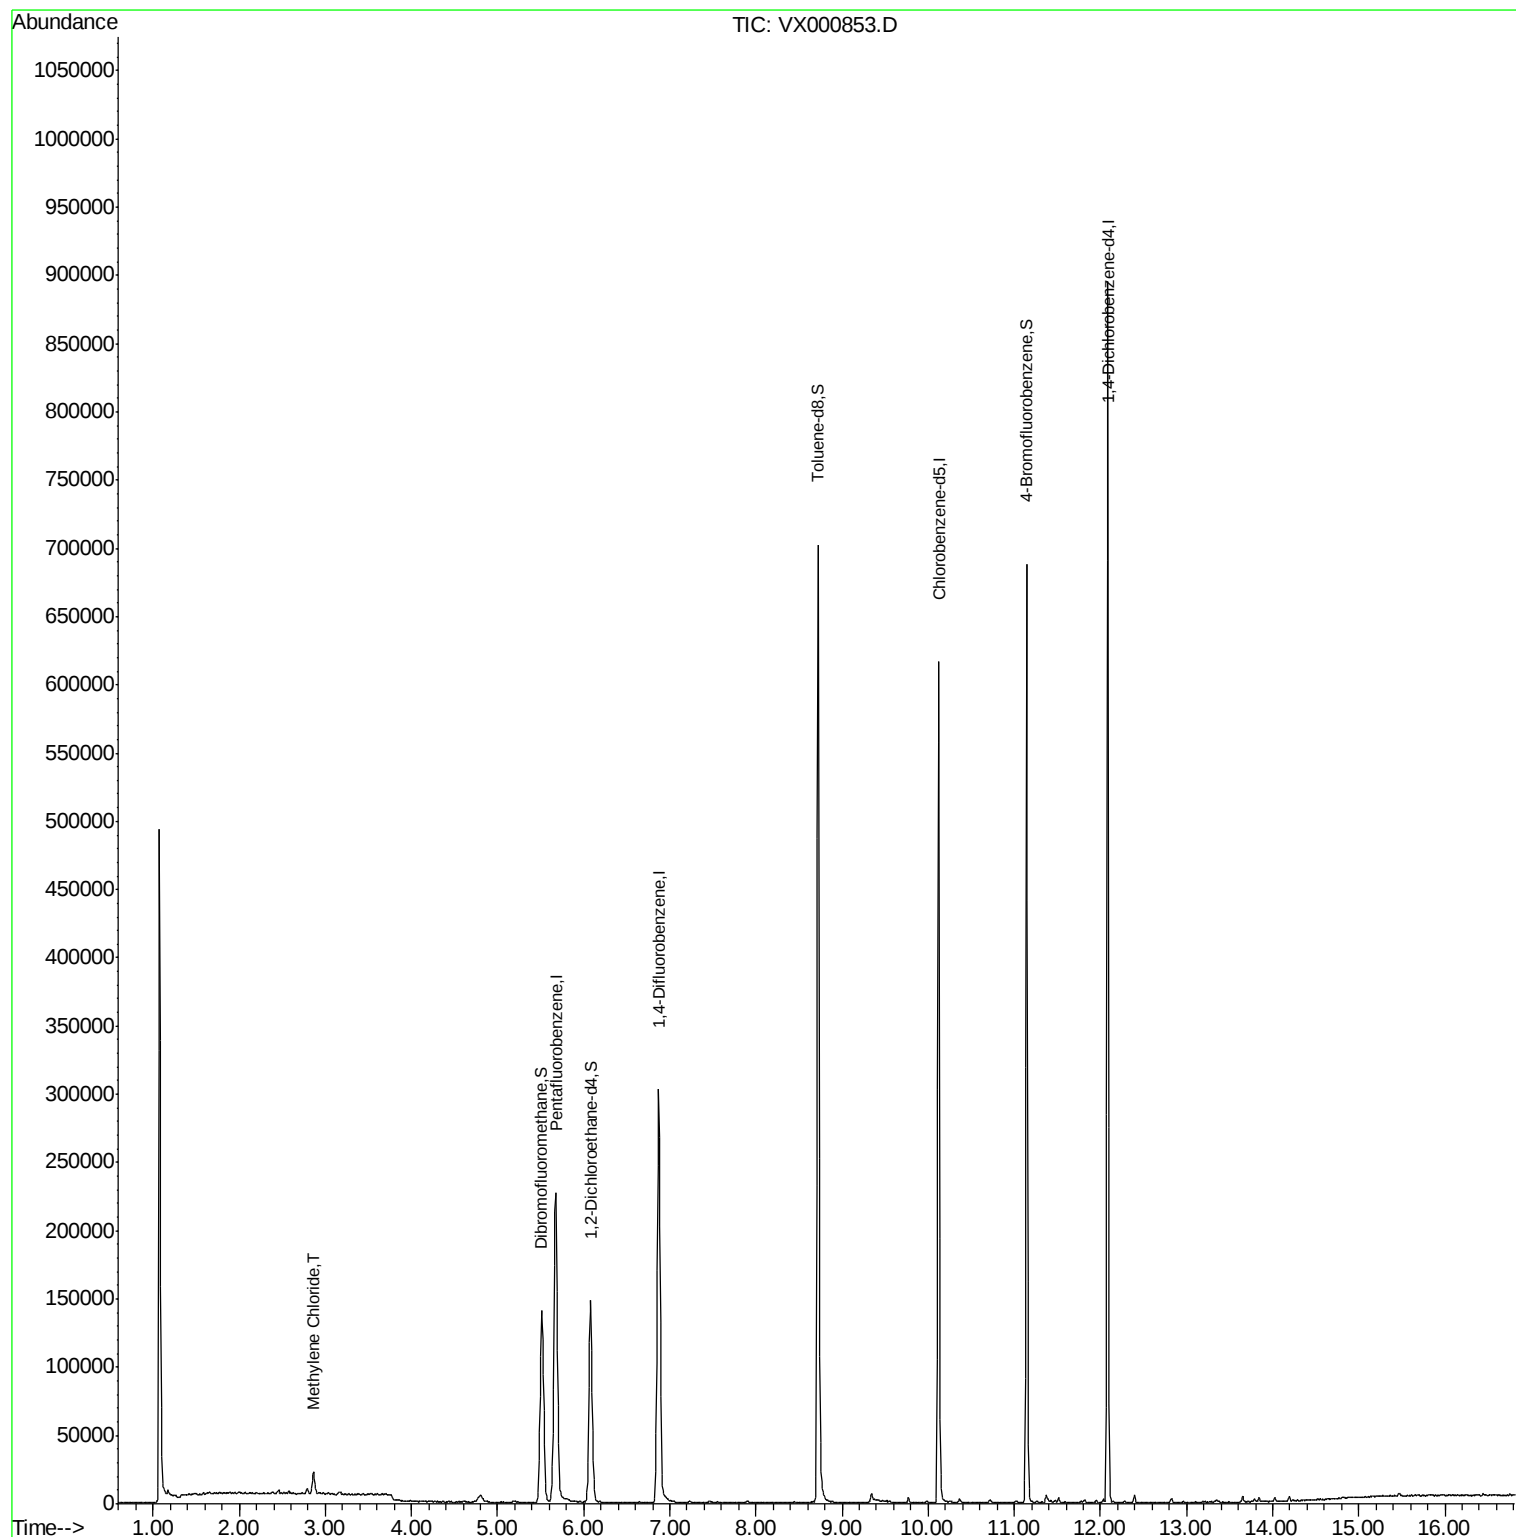

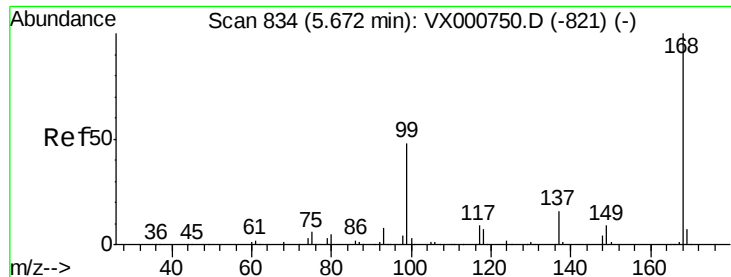

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.68 min Scan# 835

Delta R.T. 0.01 min

Lab File: VX000853.D

Acq: 13 Apr 2018 16:51

Instrument :

MSVOA_X

ClientSampleId :


PB108205TB

Tot Ion:168 Resp: 252712

Ion Ratio Lower Upper

168 100

99 46.2 38.3 57.5

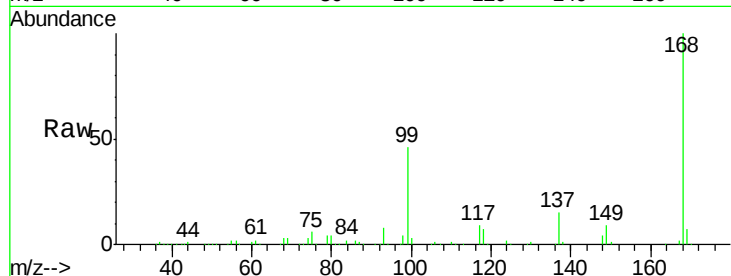

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.68

80000



60000

40000

20000

0

Time-->

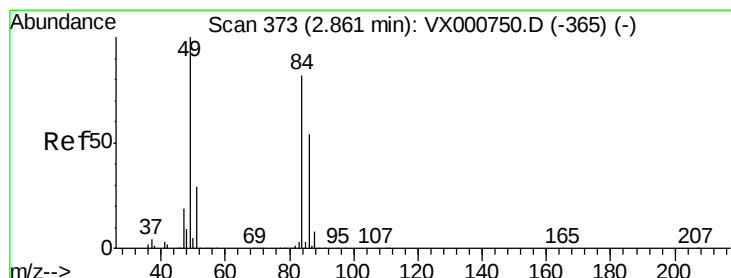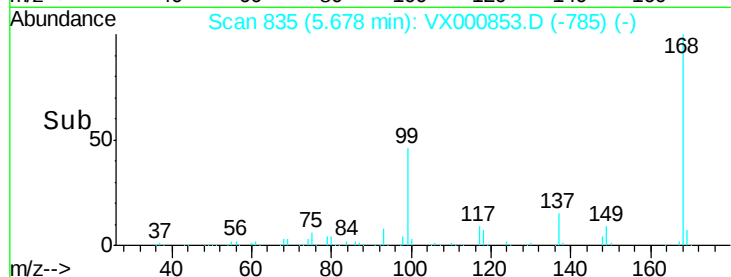

#20

Methylene Chloride

Concen: 3.05 ug/l

RT: 2.87 min Scan# 374

Delta R.T. 0.01 min

Lab File: VX000853.D

Acq: 13 Apr 2018 16:51

Tgt Ion: 84 Resp: 7791


Ion Ratio Lower Upper

84 100

49 115.4 98.1 147.1

51 39.8 28.9 43.3

86 67.8 52.7 79.1

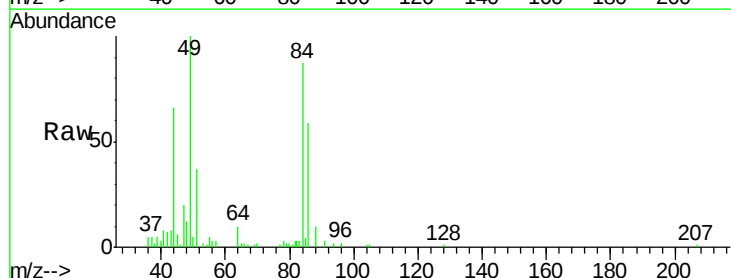

Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

2.87


6000


4000

2000

0

Time-->

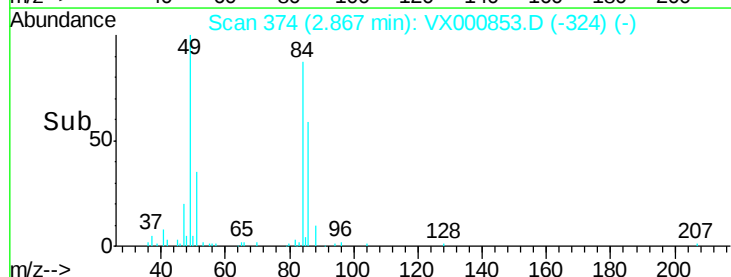

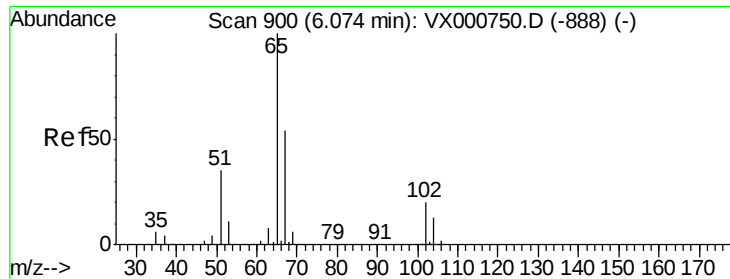

#33

1,2-Dichloroethane-d4

Concen: 44.36 ug/l

RT: 6.08 min Scan# 901

Delta R.T. 0.01 min

Lab File: VX000853.D

Acq: 13 Apr 2018 16:51

Instrument :

MSVOA_X

ClientSampleId :


PB108205TB

Tot Ion: 65 Resp: 141361

Ion Ratio Lower Upper




65 100

67 52.0 0.0 103.8

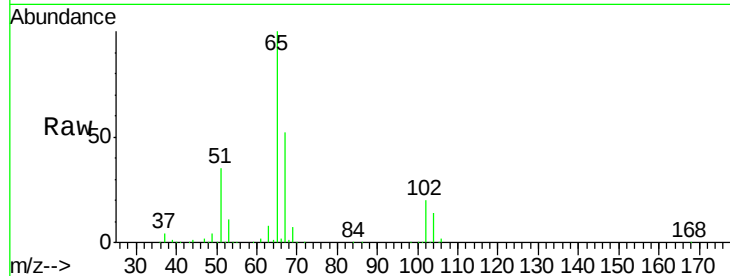

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

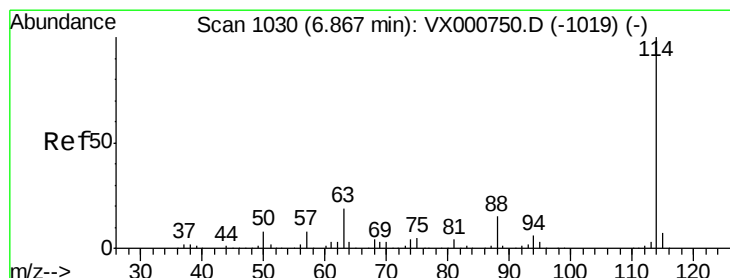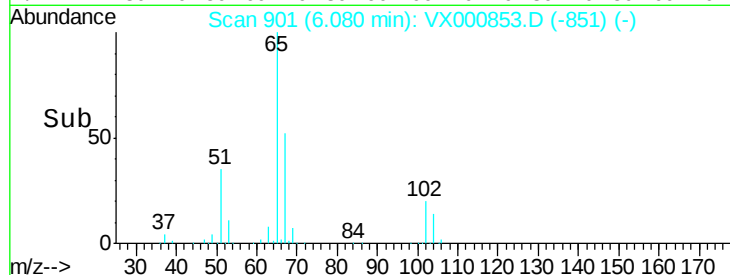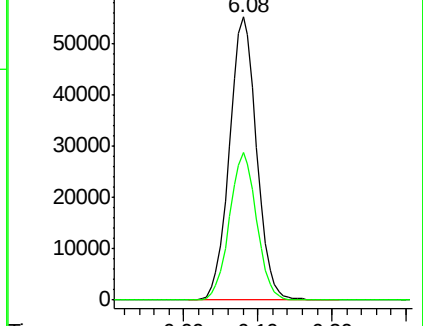

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.87 min Scan# 1031

Delta R.T. 0.01 min

Lab File: VX000853.D

Acq: 13 Apr 2018 16:51


Tgt Ion: 114 Resp: 326153

Ion Ratio Lower Upper

114 100

63 19.3 0.0 38.4



88 15.5 0.0 31.0

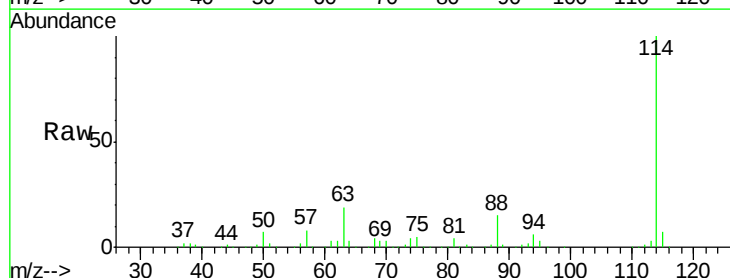


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

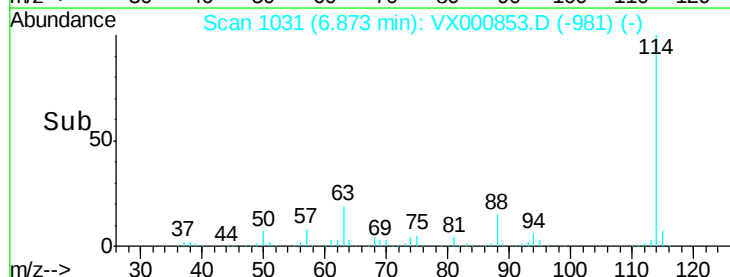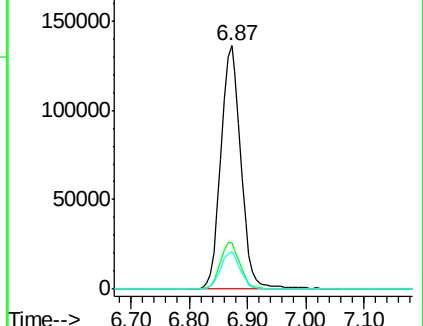

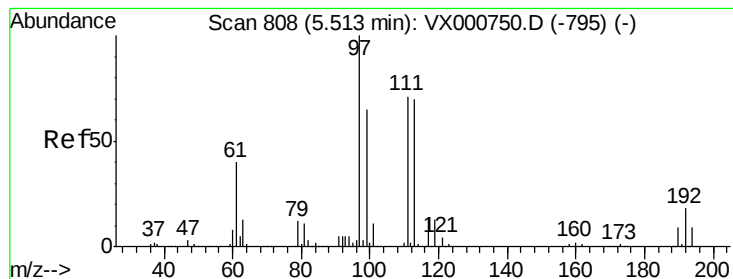

#35

Dibromofluoromethane

Concen: 45.99 ug/l

RT: 5.51 min Scan# 808

Delta R.T. -0.00 min

Lab File: VX000853.D

Acq: 13 Apr 2018 16:51

Instrument :

MSVOA_X

ClientSampleId :

PB108205TB


Tot Ion:113 Resp: 115567

Ion Ratio Lower Upper

113 100

111 102.5 81.5 122.3




192 25.7 20.4 30.6

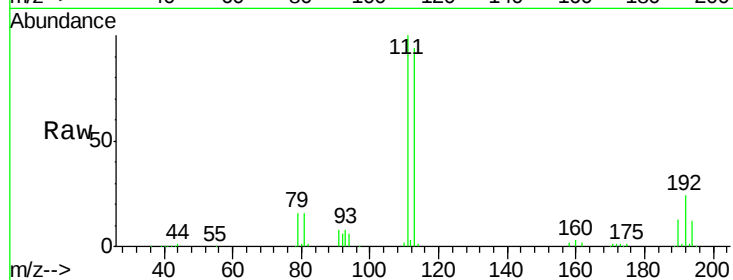

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

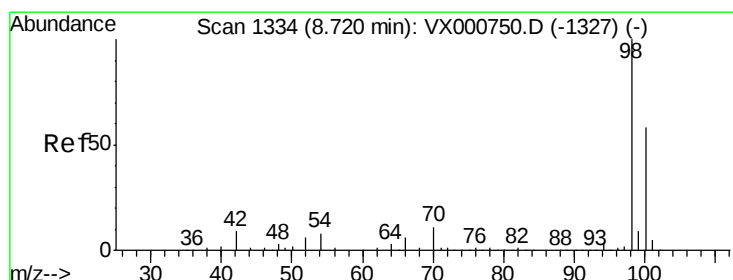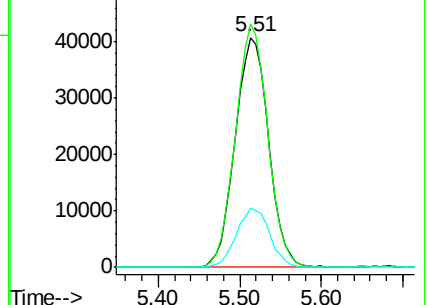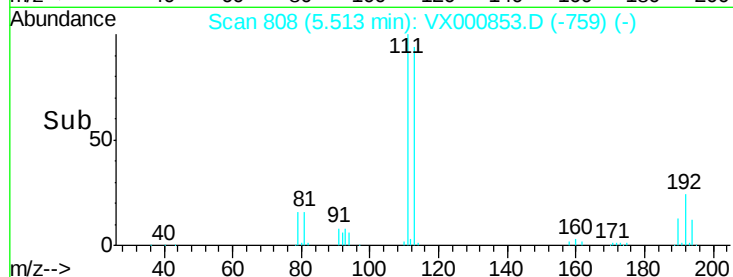

#50

Toluene-d8

Concen: 48.33 ug/l

RT: 8.73 min Scan# 1335

Delta R.T. 0.01 min

Lab File: VX000853.D


Acq: 13 Apr 2018 16:51

Tgt Ion: 98 Resp: 452143

Ion Ratio Lower Upper



98 100


100 64.0 52.6 79.0

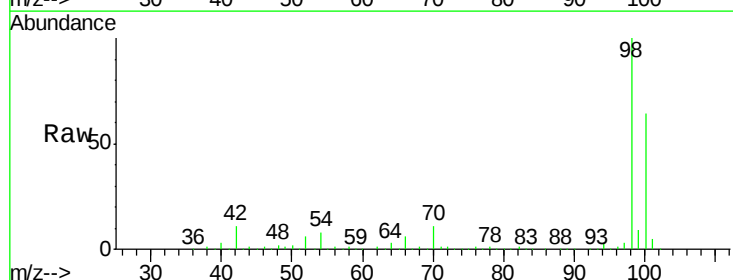

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

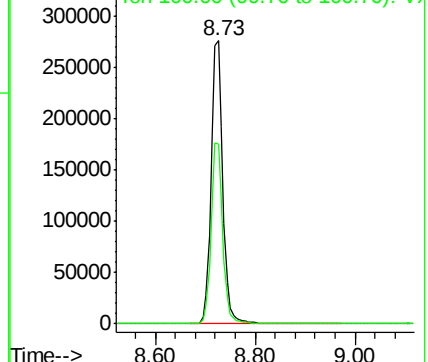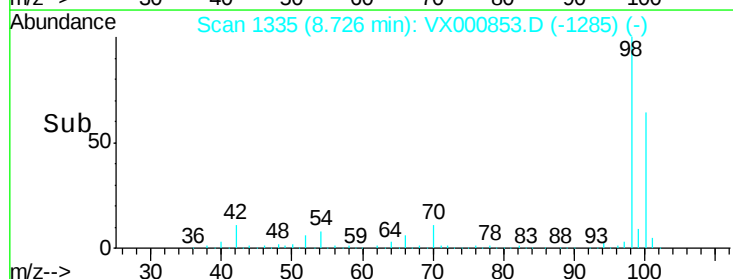

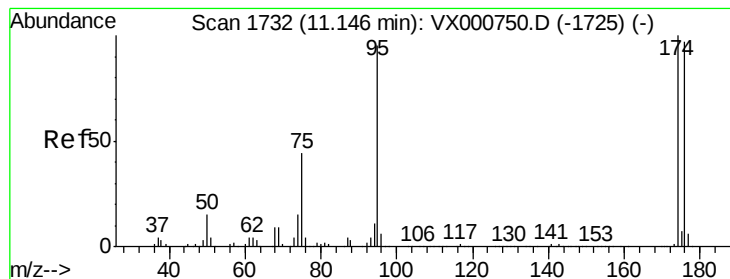

#62

4-Bromofluorobenzene

Concen: 44.09 ug/l

RT: 11.15 min Scan# 1732

Delta R.T. -0.00 min

Lab File: VX000853.D

Acq: 13 Apr 2018 16:51

Instrument :

MSVOA_X

ClientSampleId :

PB108205TB


Tot Ion: 95 Resp: 170651

Ion Ratio Lower Upper

95 100

174 98.3 0.0 198.4




176 96.5 0.0 194.4

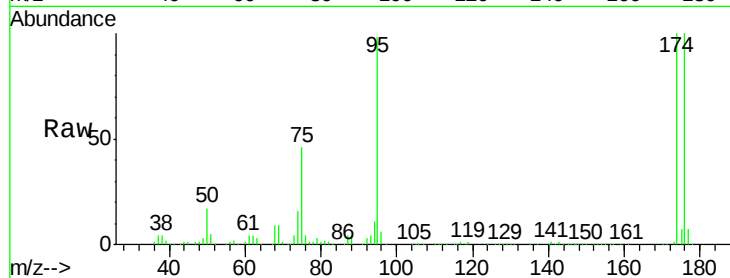

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

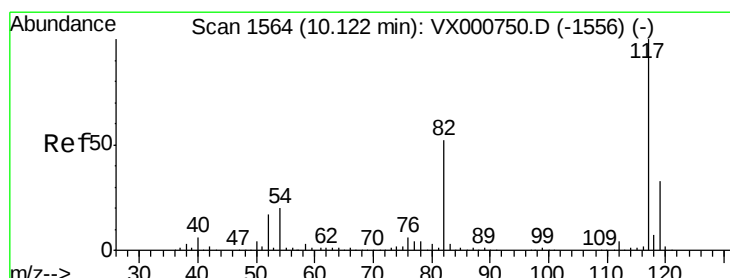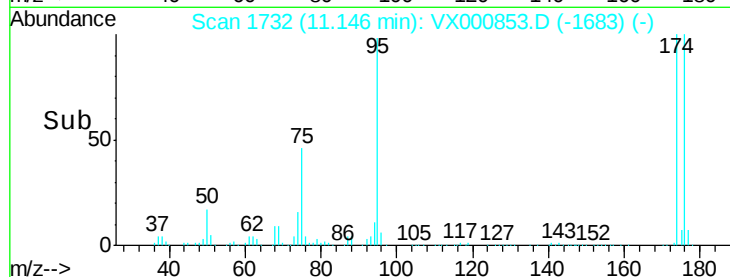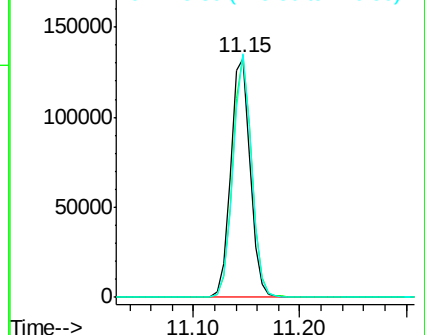

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 10.12 min Scan# 1564

Delta R.T. -0.00 min

Lab File: VX000853.D

Acq: 13 Apr 2018 16:51


Tgt Ion: 117 Resp: 294785

Ion Ratio Lower Upper

117 100

82 51.4 41.9 62.9



119 32.2 26.0 39.0

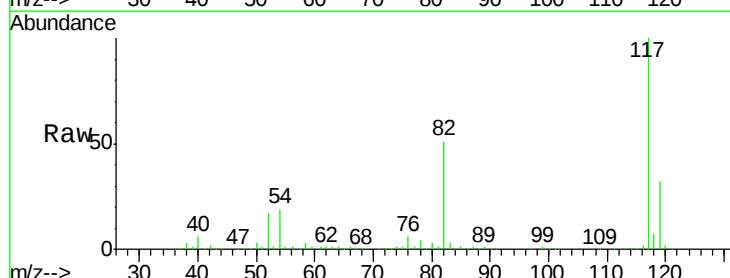


Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

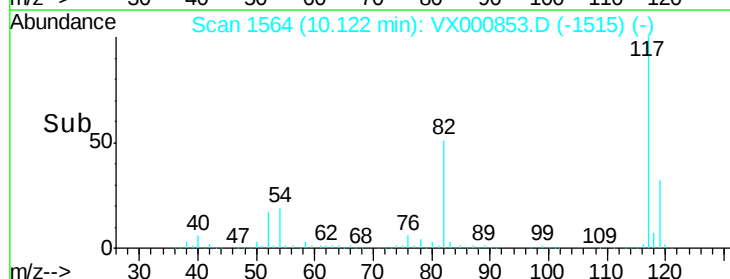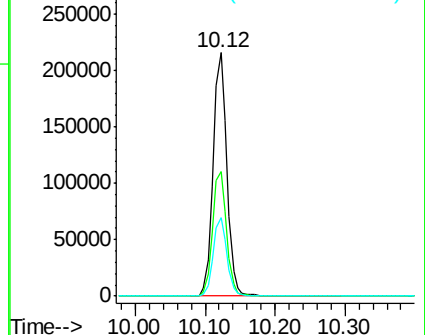

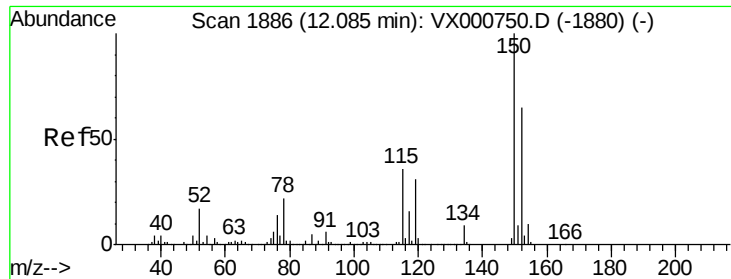

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. -0.00 min

Lab File: VX000853.D

Acq: 13 Apr 2018 16:51

Instrument :

MSVOA_X

ClientSampleId :

PB108205TB


Tot Ion:152 Resp: 190956

Ion Ratio Lower Upper

152 100

115 53.2 37.9 113.7

150 156.0 0.0 348.0

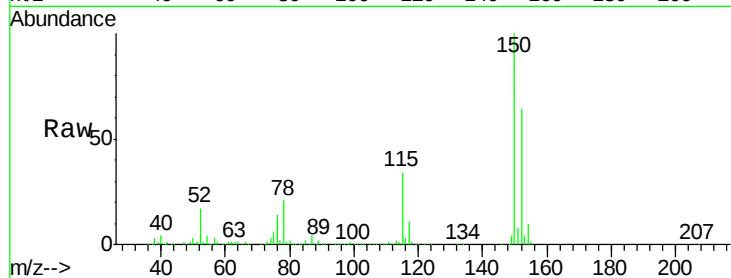

Abundance Ion 151.90 (151.60 to 152.60): V

300000

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

200000

100000

0

