

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041318\
 Data File : VX000862.D
 Acq On : 13 Apr 2018 20:43
 Operator : JC/MD
 Sample : J2348-10 5X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 281

Quant Time: Apr 14 05:44:34 2018
 Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 10 15:49:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.68	168	244655	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	319982	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	290498	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.09	152	179552	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.08	65	141021	45.71	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.42%	
35) Dibromofluoromethane	5.51	113	114529	46.46	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.92%	
50) Toluene-d8	8.73	98	443843	48.35	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.70%	
62) 4-Bromofluorobenzene	11.15	95	167715	44.16	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.32%	
Target Compounds						
16) Acetone	2.45	43	25957	24.40	ug/l	98
18) Methyl Acetate	2.79	43	4872	1.77	ug/l	98
20) Methylene Chloride	2.86	84	19771	7.99	ug/l	98
95) Naphthalene	13.84	128	92766	7.10	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA X\DATA\VX041318\
Data File : VX000862.D
Acq On : 13 Apr 2018 20:43
Operator : JC/MD
Sample : J2348-10 5X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
281

Quant Time: Apr 14 05:44:34 2018
Quant Method : W:\HPCHEM1\MSVOA_X\METHOD\82X041018W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 10 15:49:28 2018
Response via : Initial Calibration

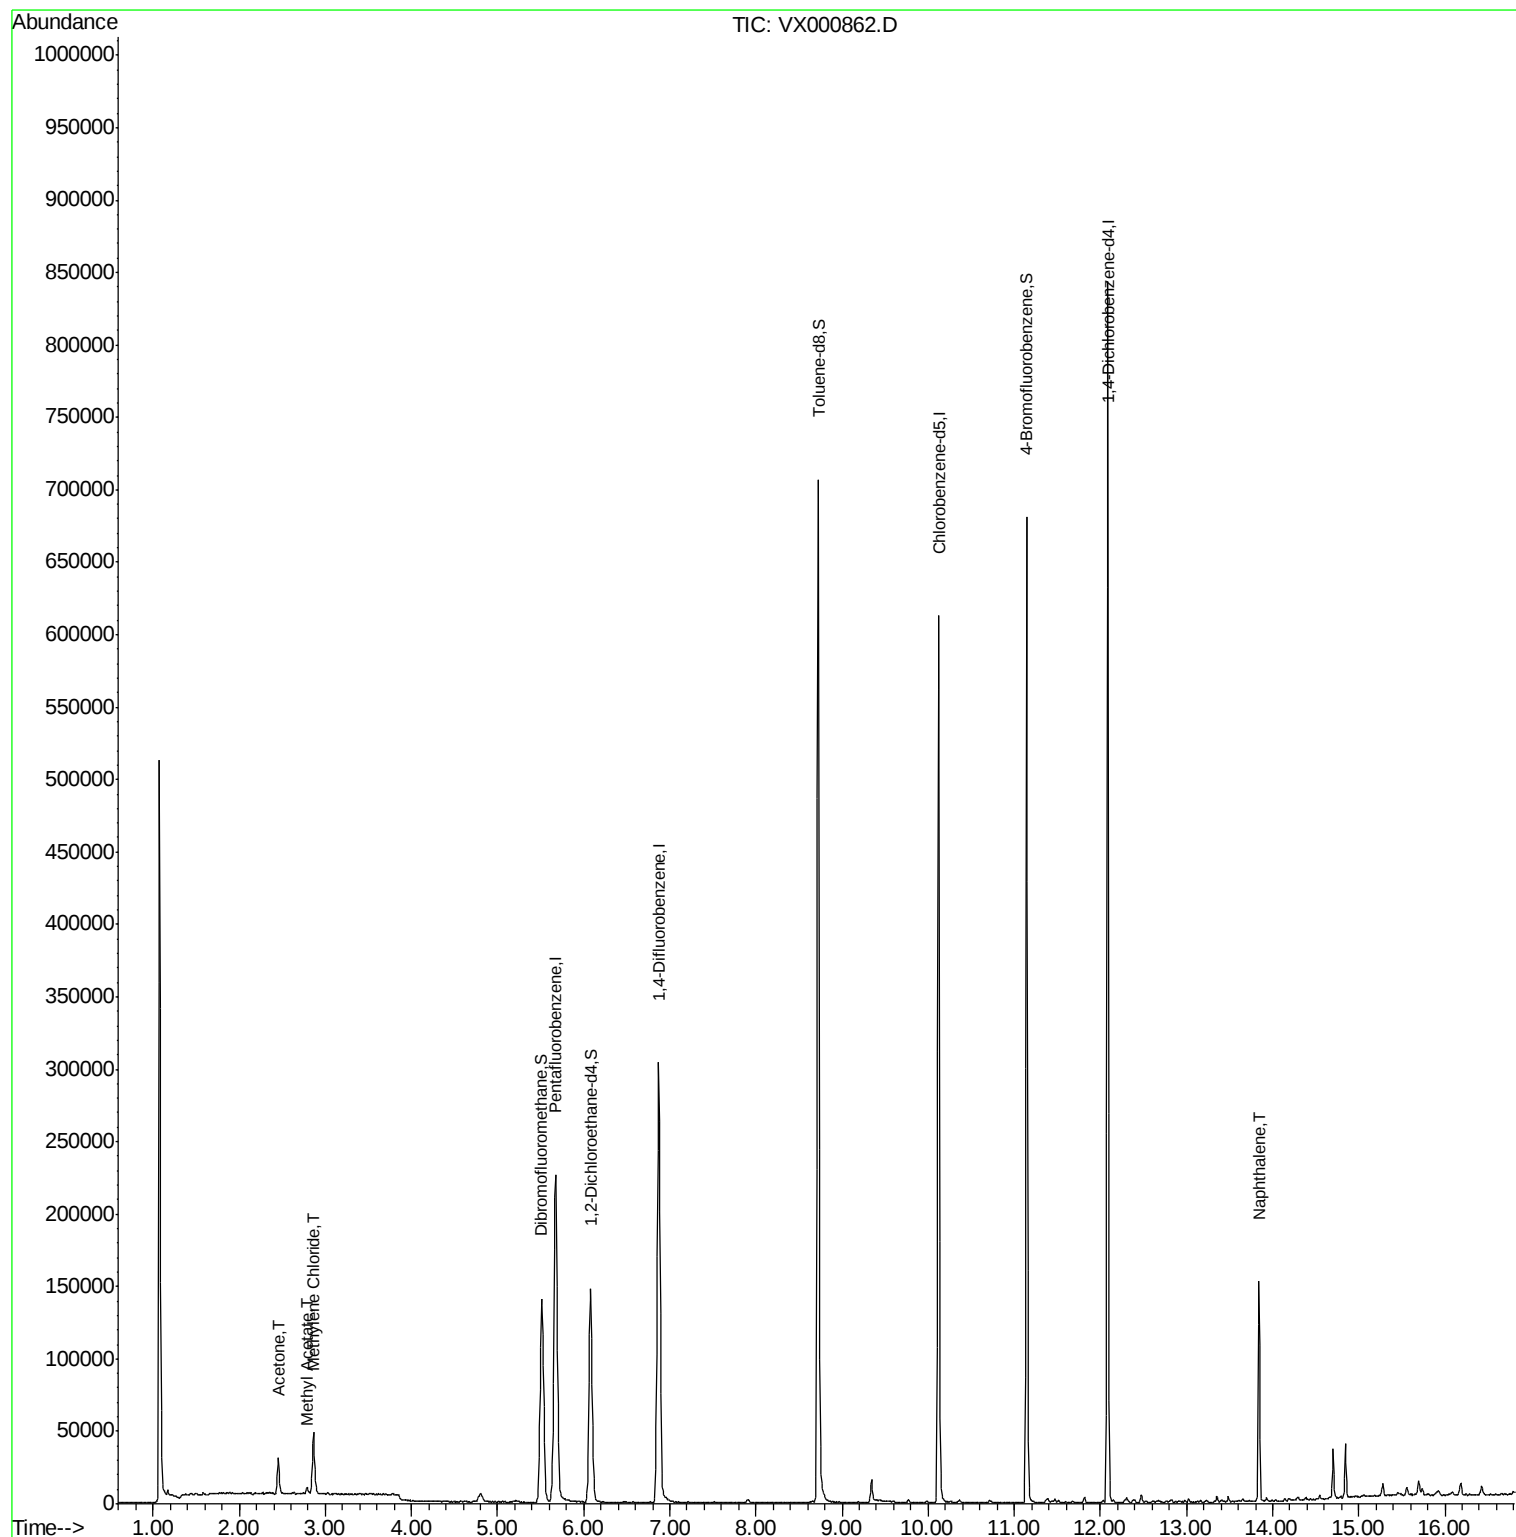



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.68 min Scan# 835

Delta R.T. 0.01 min

Lab File: VX000862.D

Acq: 13 Apr 2018 20:43

Instrument :

MSVOA_X

ClientSampleId :


281

Tot Ion:168 Resp: 244655

Ion Ratio Lower Upper

168 100

99 46.7 38.3 57.5

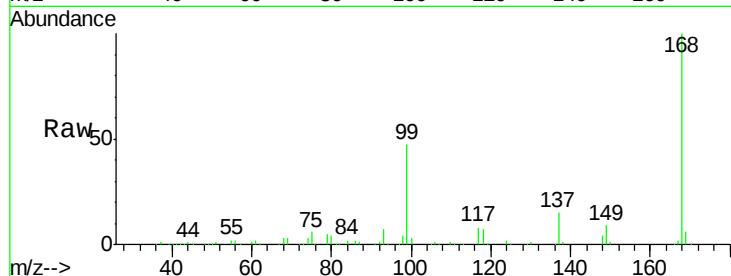

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.68

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

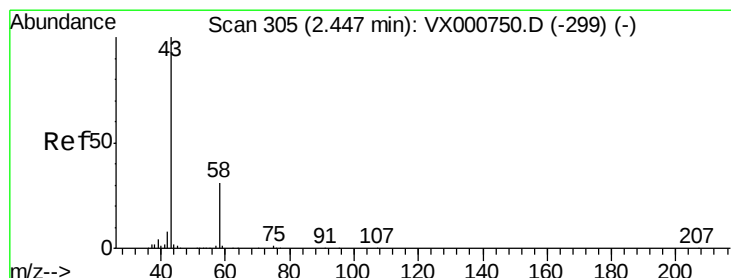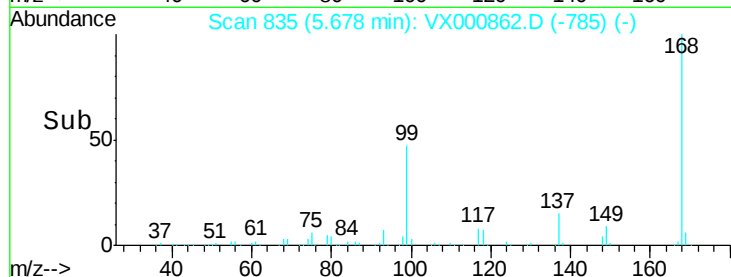

#16

Acetone

Concen: 24.40 ug/l

RT: 2.45 min Scan# 306

Delta R.T. 0.01 min

Lab File: VX000862.D


Acq: 13 Apr 2018 20:43

Tgt Ion: 43 Resp: 25957

Ion Ratio Lower Upper

43 100

58 29.5 24.6 37.0

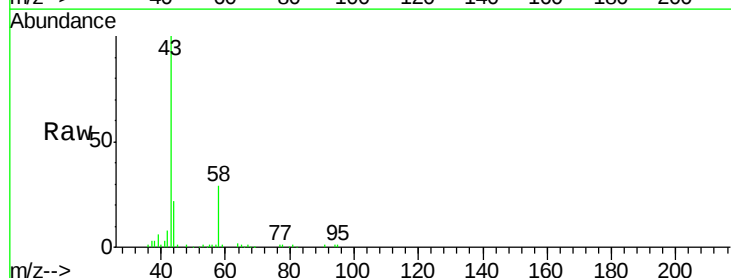

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45


15000


10000

5000

0

Time--> 2.35 2.40 2.45 2.50 2.55




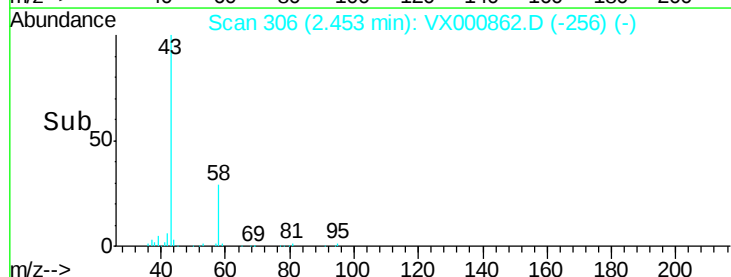


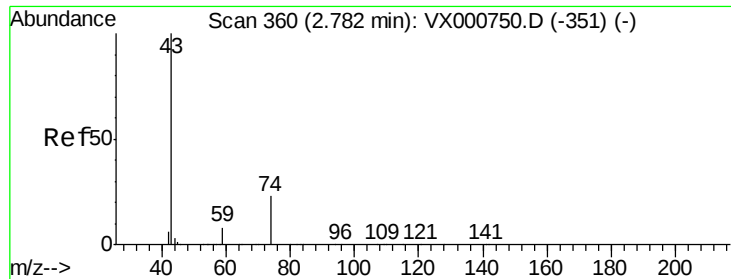

#18
Methvl Acetate
Concen: 1.77 ug/l
RT: 2.79 min Scan# 361
Delta R.T. 0.01 min
Lab File: VX000862.D
Acq: 13 Apr 2018 20:43




Instrument :
MSVOA_X
ClientSampleId :
281


Tot Ion: 43 Resp: 4872
Ion Ratio Lower Upper
43 100
74 25.0 19.1 28.7

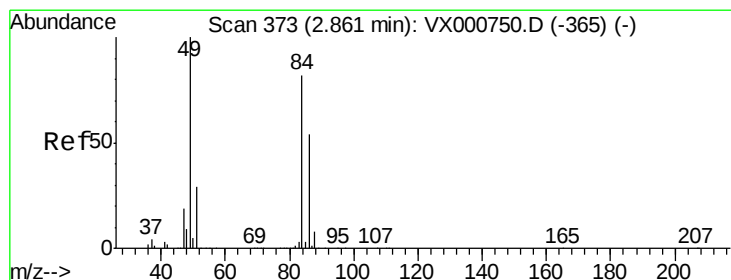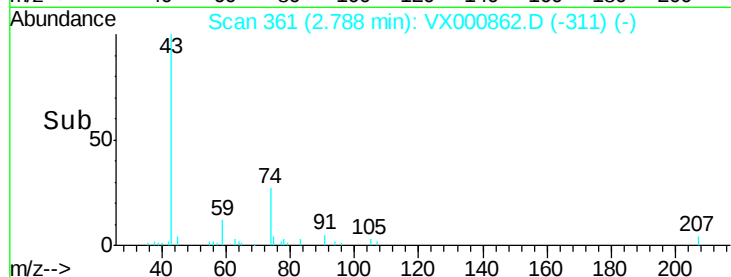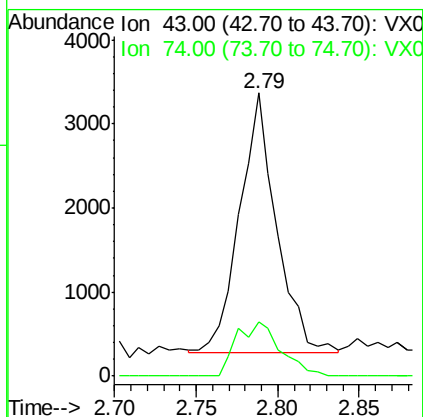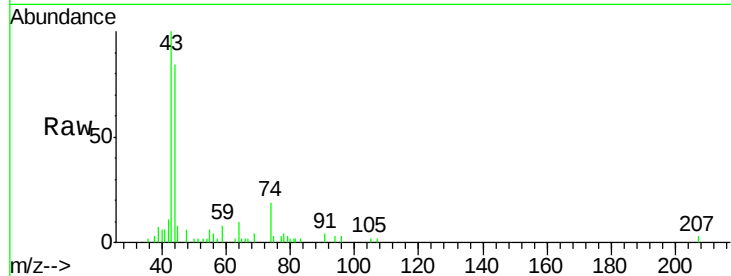

#20
Methylene Chloride
Concen: 7.99 ug/l
RT: 2.86 min Scan# 373
Delta R.T. 0.00 min
Lab File: VX000862.D
Acq: 13 Apr 2018 20:43

Tgt Ion: 84 Resp: 19771
Ion Ratio Lower Upper
84 100
49 121.2 98.1 147.1
51 37.3 28.9 43.3
86 63.7 52.7 79.1


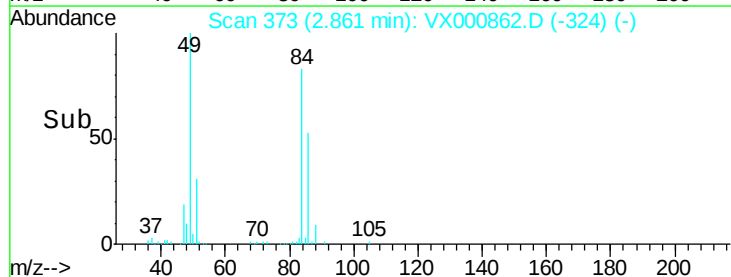
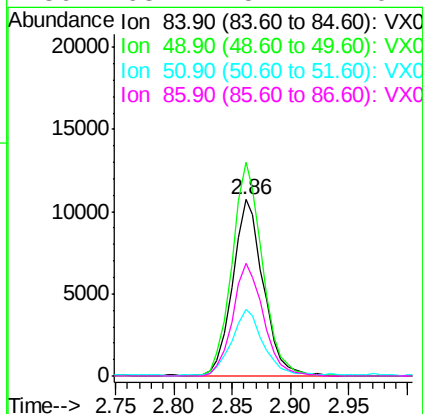
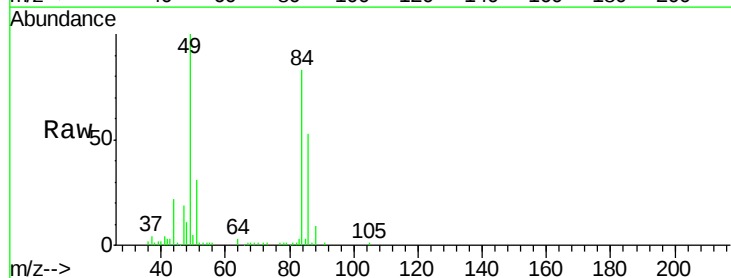


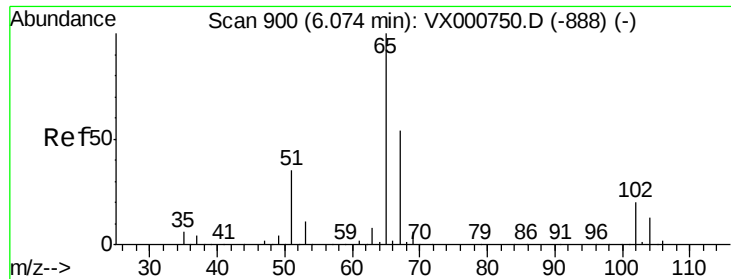

#33
 1,2-Dichloroethane-d4
 Concen: 45.71 ug/l
 RT: 6.08 min Scan# 901
 Delta R.T. 0.01 min
 Lab File: VX000862.D
 Acq: 13 Apr 2018 20:43




Instrument :
 MSVOA_X
 ClientSampleId :
 281


Tot Ion: 65 Resp: 141021
 Ion Ratio Lower Upper
 65 100
 67 52.3 0.0 103.8

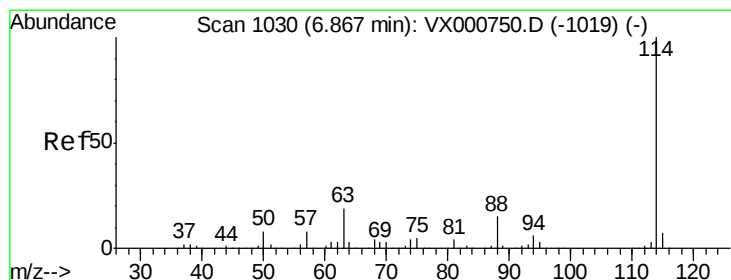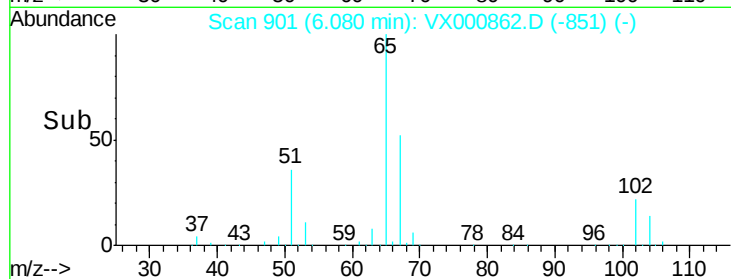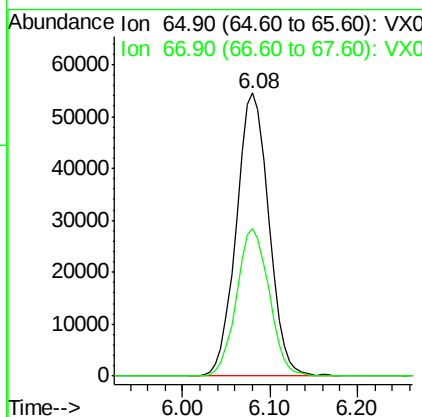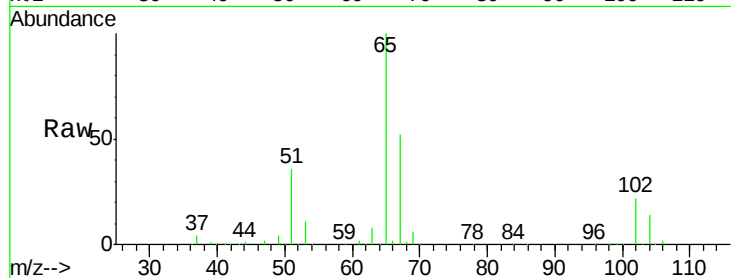

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1031
 Delta R.T. 0.01 min
 Lab File: VX000862.D
 Acq: 13 Apr 2018 20:43

Tgt Ion: 114 Resp: 319982
 Ion Ratio Lower Upper
 114 100
 63 19.5 0.0 38.4
 88 15.1 0.0 31.0

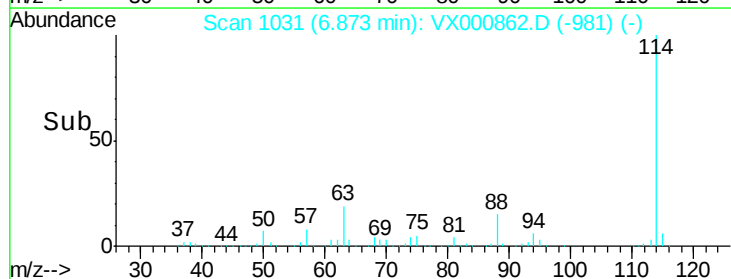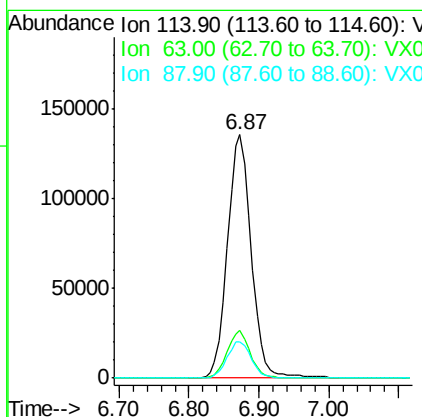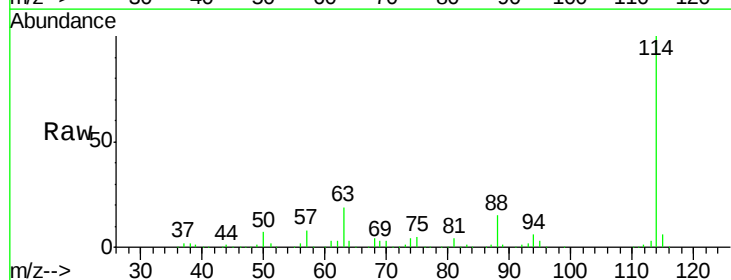

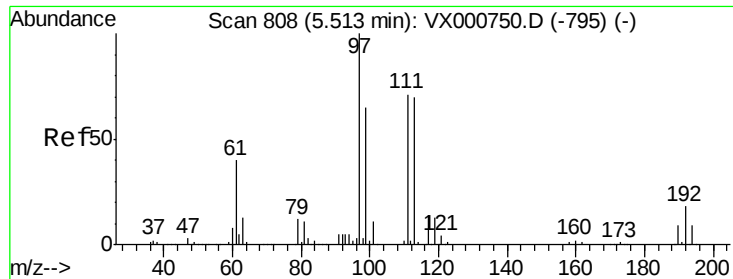

#35

Dibromofluoromethane

Concen: 46.46 ug/l

RT: 5.51 min Scan# 808

Delta R.T. 0.00 min

Lab File: VX000862.D

Acq: 13 Apr 2018 20:43

Instrument :
MSVOA_X
ClientSampleId :
281


Tot Ion:113 Resp: 114529

Ion Ratio Lower Upper




113 100

111 102.6 81.5 122.3

192 25.8 20.4 30.6

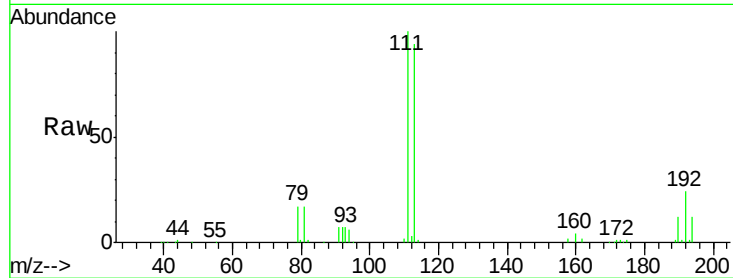

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

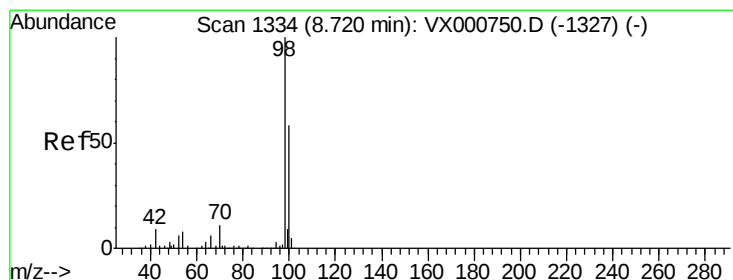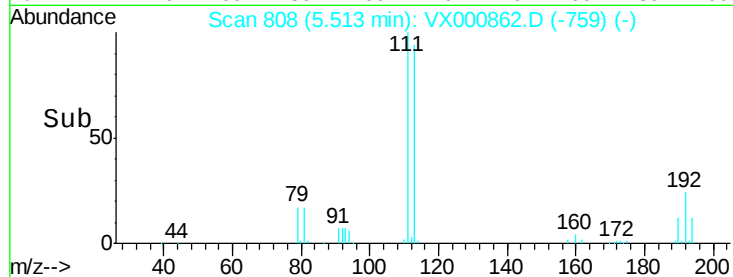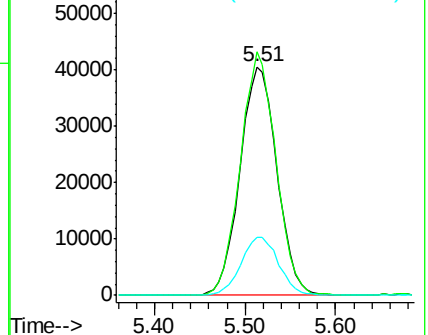

#50

Toluene-d8

Concen: 48.35 ug/l

RT: 8.73 min Scan# 1335

Delta R.T. 0.01 min

Lab File: VX000862.D


Acq: 13 Apr 2018 20:43

Tgt Ion: 98 Resp: 443843



Ion Ratio Lower Upper


98 100

100 64.7 52.6 79.0

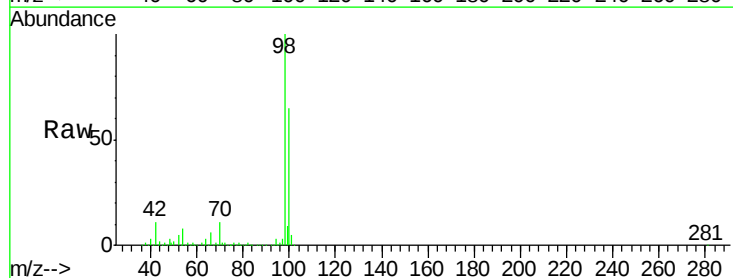

Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): V



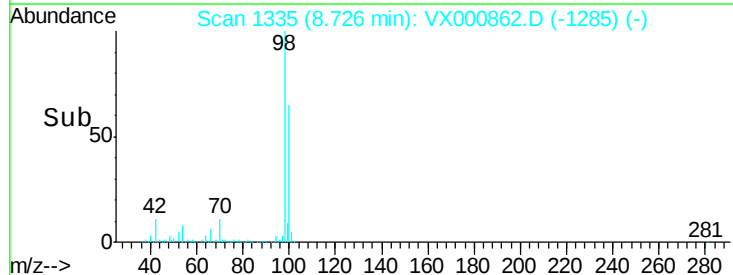
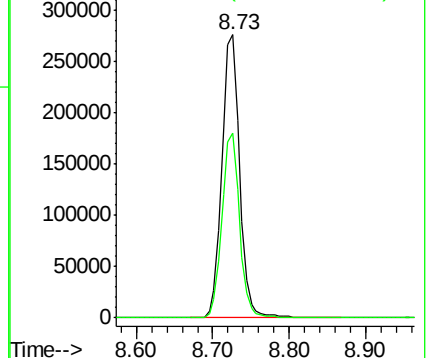


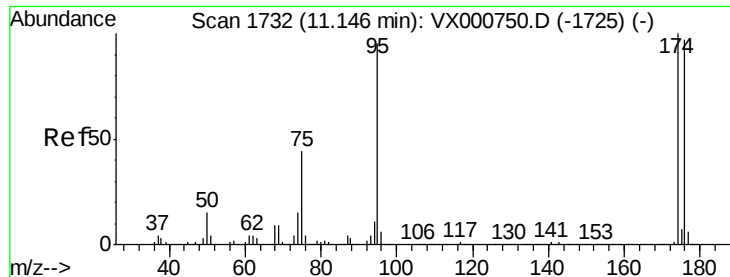

#62
4-Bromofluorobenzene
Concen: 44.16 ug/l
RT: 11.15 min Scan# 1732
Delta R.T. 0.00 min
Lab File: VX000862.D
Acq: 13 Apr 2018 20:43




Instrument :
MSVOA_X
ClientSampleId :
281


Tot Ion: 95 Resp: 167715
Ion Ratio Lower Upper
95 100
174 96.7 0.0 198.4
176 94.1 0.0 194.4

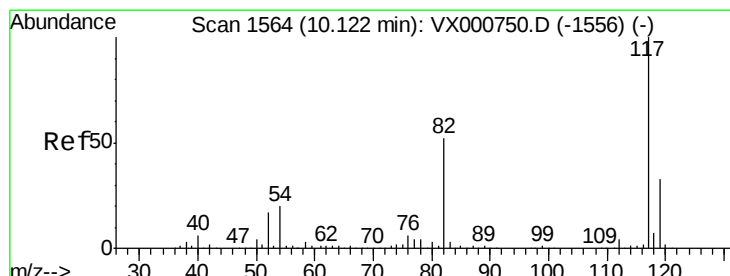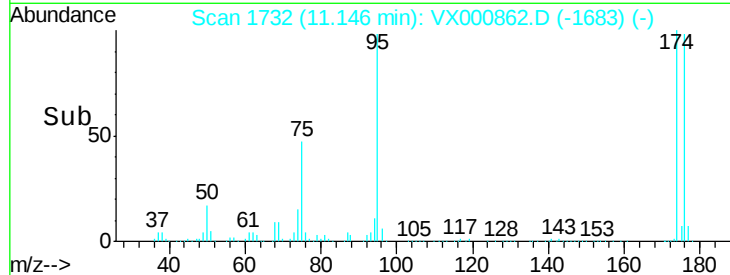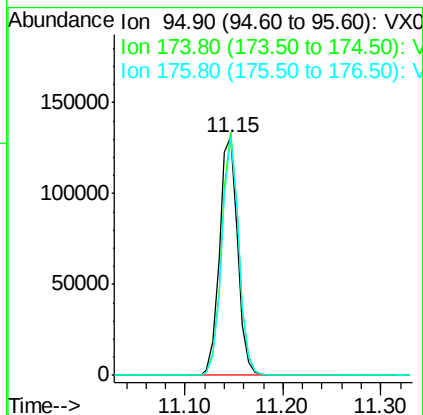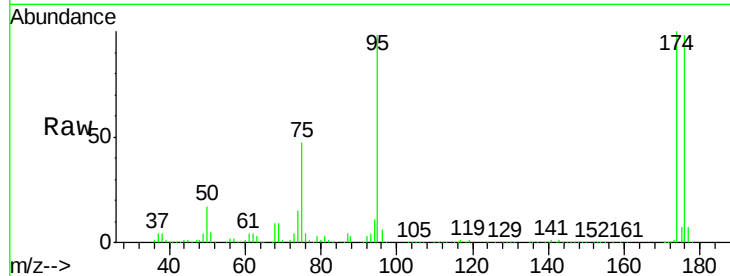

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1564
Delta R.T. 0.00 min
Lab File: VX000862.D
Acq: 13 Apr 2018 20:43

Tgt Ion: 117 Resp: 290498
Ion Ratio Lower Upper
117 100
82 51.8 41.9 62.9
119 32.9 26.0 39.0

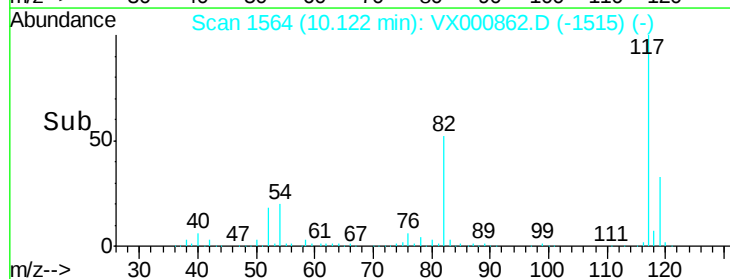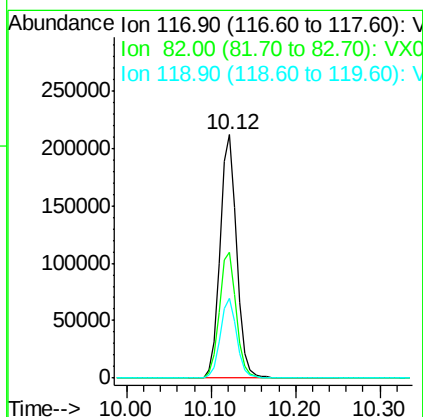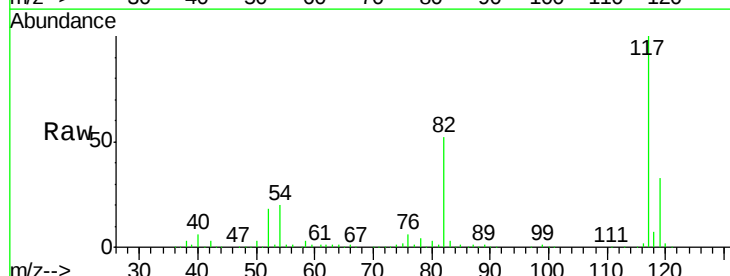

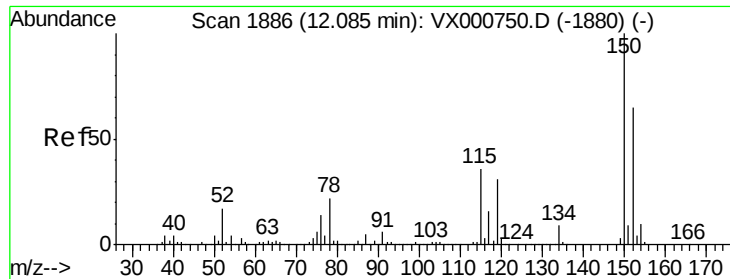

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.09 min Scan# 1886

Delta R.T. 0.00 min

Lab File: VX000862.D

Acq: 13 Apr 2018 20:43

Instrument :

MSVOA_X

ClientSampleId :

281


Tot Ion:152 Resp: 179552

Ion Ratio Lower Upper




152 100

115 53.2 37.9 113.7

150 154.9 0.0 348.0

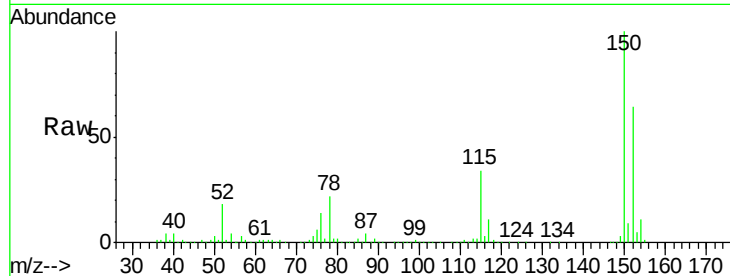

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

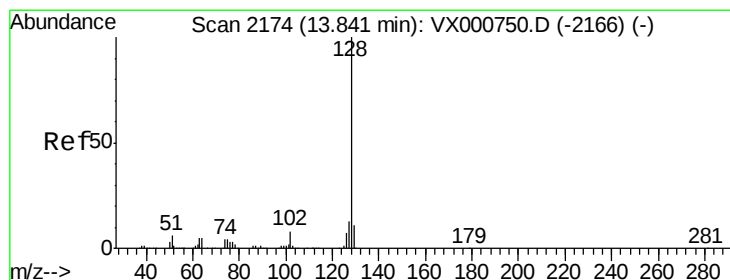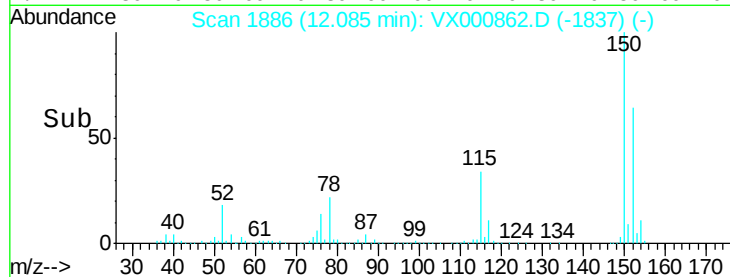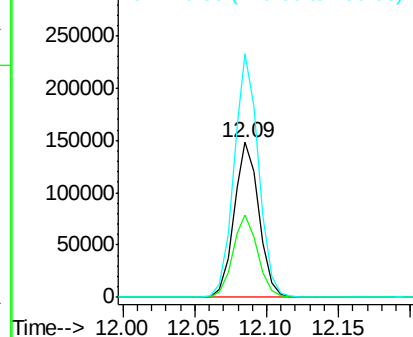

#95

Naphthalene

Concen: 7.10 ug/l

RT: 13.84 min Scan# 2174

Delta R.T. 0.00 min

Lab File: VX000862.D

Acq: 13 Apr 2018 20:43


Tgt Ion:128 Resp: 92766

Ion Ratio Lower Upper

128 100

127 13.0 10.4 15.6

129 10.7 8.7 13.1

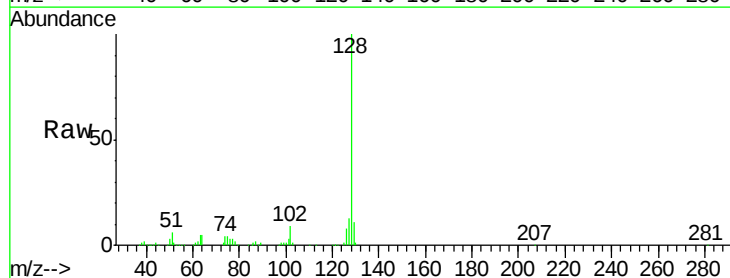

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

